
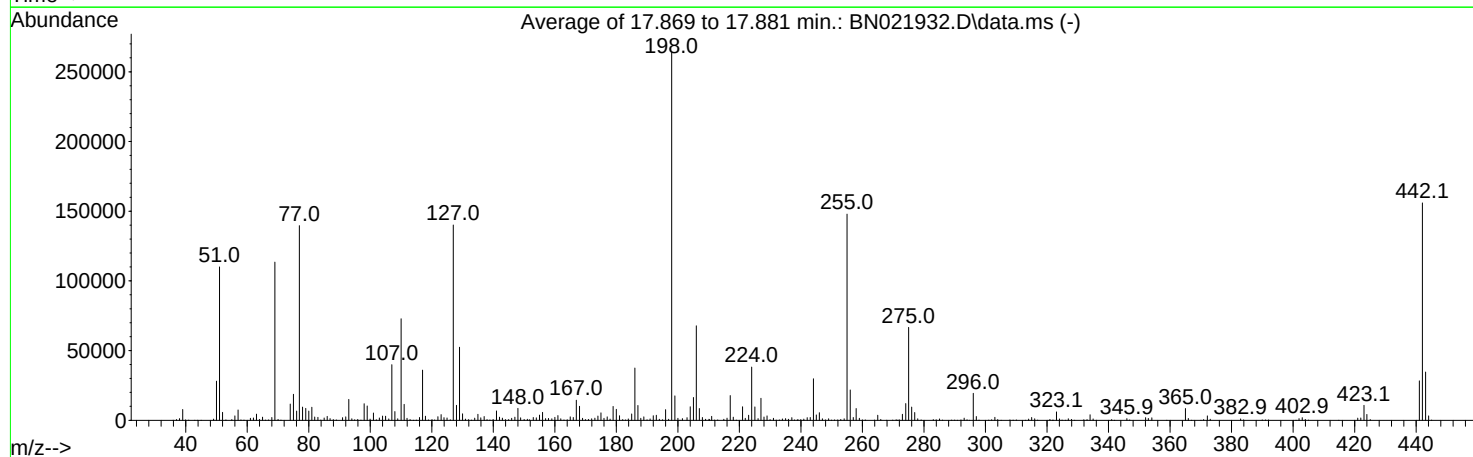


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092822\
 Data File : BN021932.D
 Acq On : 27 Sep 2022 13:04
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN091422.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Sep 28 04:21:32 2022

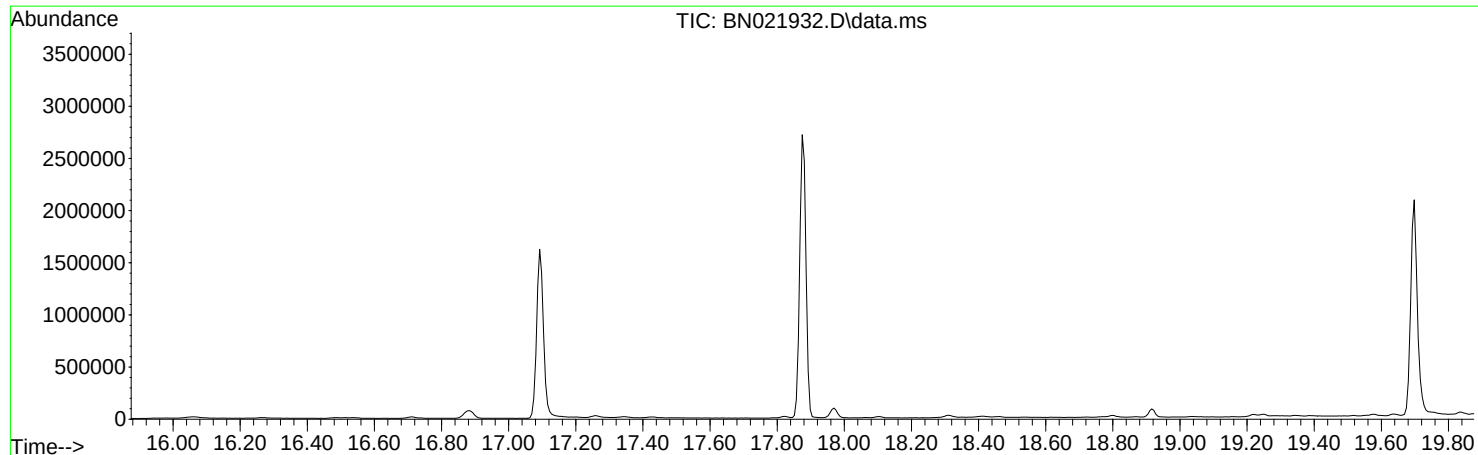




AutoFind: Scans 2479, 2480, 2481; Background Corrected with Scan 2472

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.7	110064	PASS
68	69	0.00	2	1.7	1968	PASS
69	198	0.00	100	43.0	113493	PASS
70	69	0.00	2	0.6	680	PASS
127	198	10	80	53.1	140075	PASS
197	198	0.00	2	0.3	782	PASS
198	198	100	100	100.0	263893	PASS
199	198	5	9	6.6	17493	PASS
275	198	10	60	25.3	66640	PASS
365	198	1	100	3.2	8398	PASS
441	198	0.01	100	10.7	28323	PASS
442	442	50	100	100.0	155955	PASS
443	442	15	24	22.2	34613	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092822\
 Data File : BN021932.D
 Acq On : 27 Sep 2022 13:04
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Sep 28 07:03:57 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 28 07:03:52 2022
 Response via : Initial Calibration

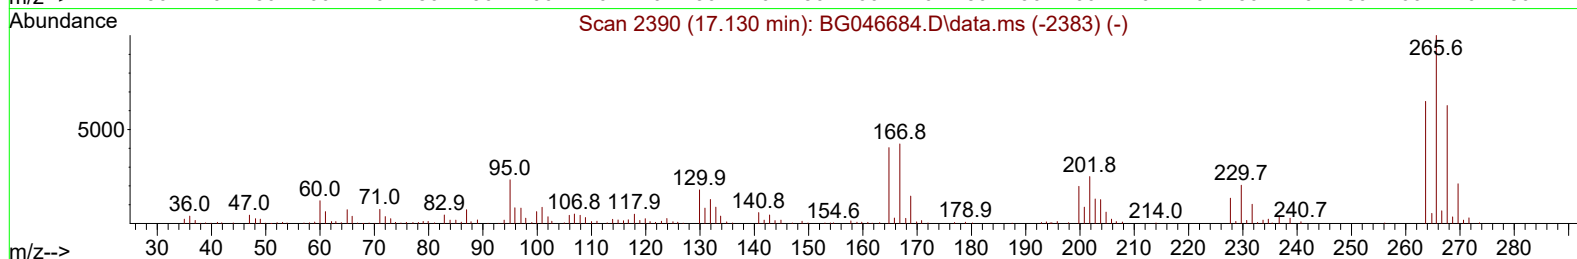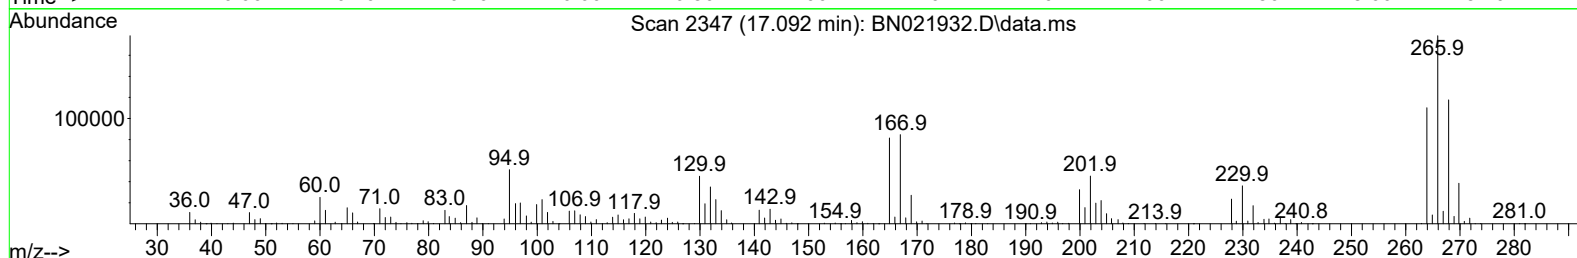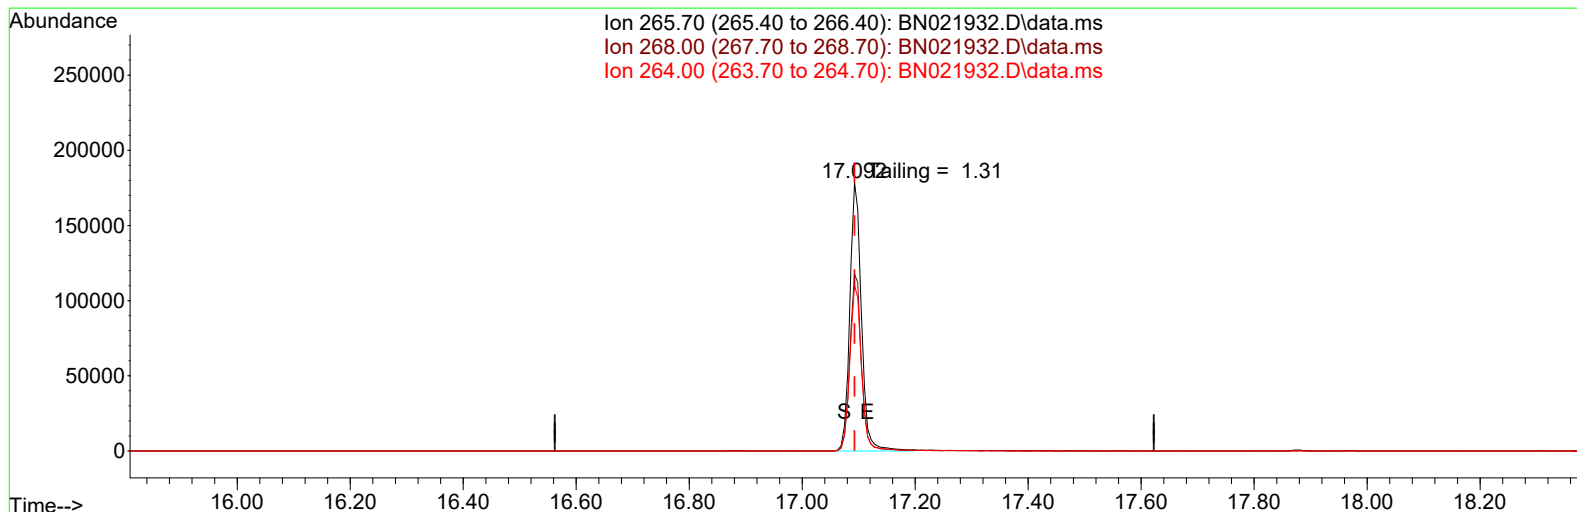

TIC: BN021932.D\data.ms

(70) Pentachlorophenol (C)

17.092min (0.000) 41659.27 ng




response 257622

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.92
264.00	61.60	61.73
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092822\
Data File : BN021932.D
Acq On : 27 Sep 2022 13:04
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 28 07:03:57 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 28 07:03:52 2022
Response via : Initial Calibration

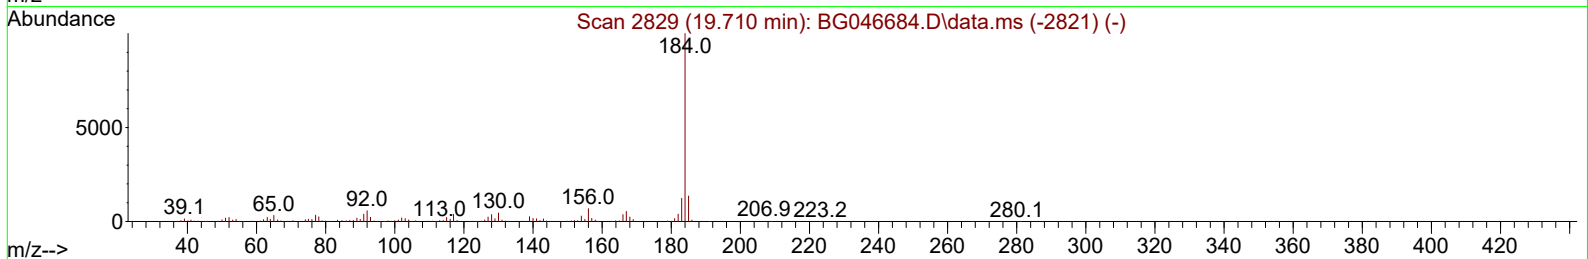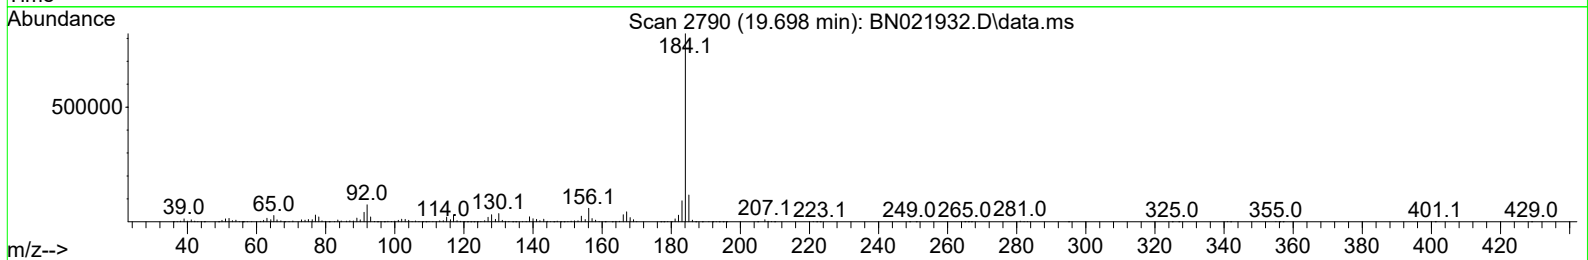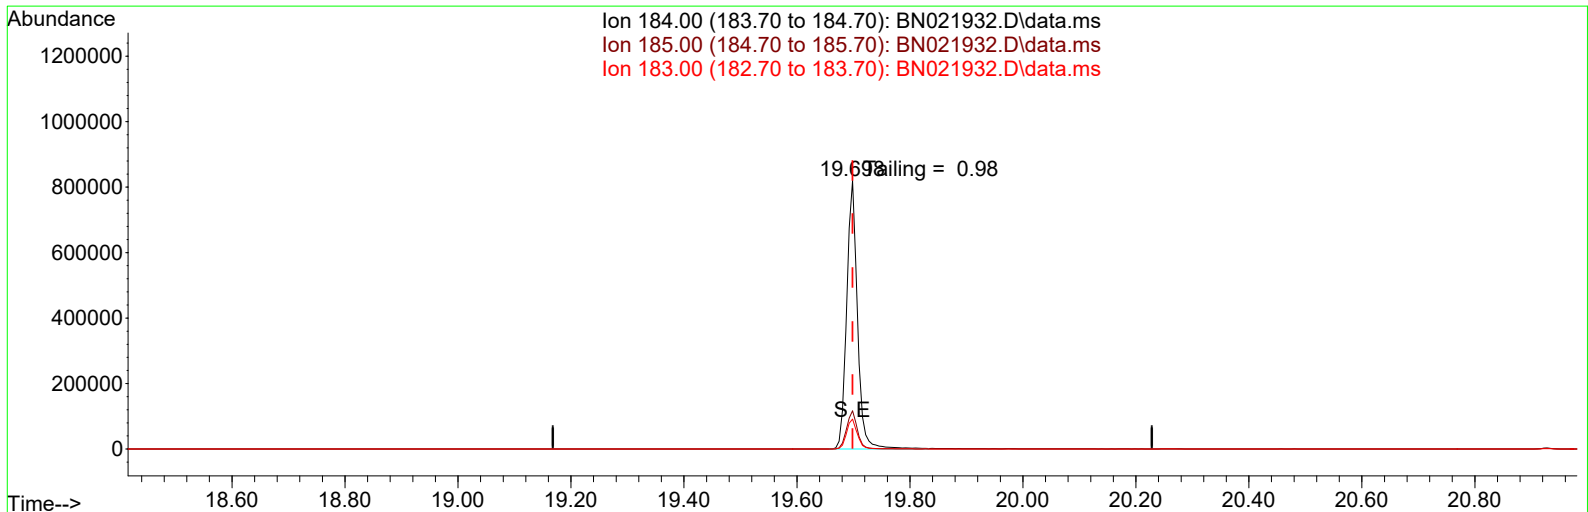

TIC: BN021932.D\data.ms

(77) Benzidine

19.698min (0.000) 62954.60 ng

response 1098379

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.26
183.00	13.20	11.18
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/28/2022	BNA_N	<u>BN021932.D</u>
Compound Name	Response	Retention Time
DDT	760888	20.928
DDD	45099	20.486
DDE	11409	19.975
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
56508	817396	6.91

Instrument :
BNA_N
ClientSampleId :
DFTPP