
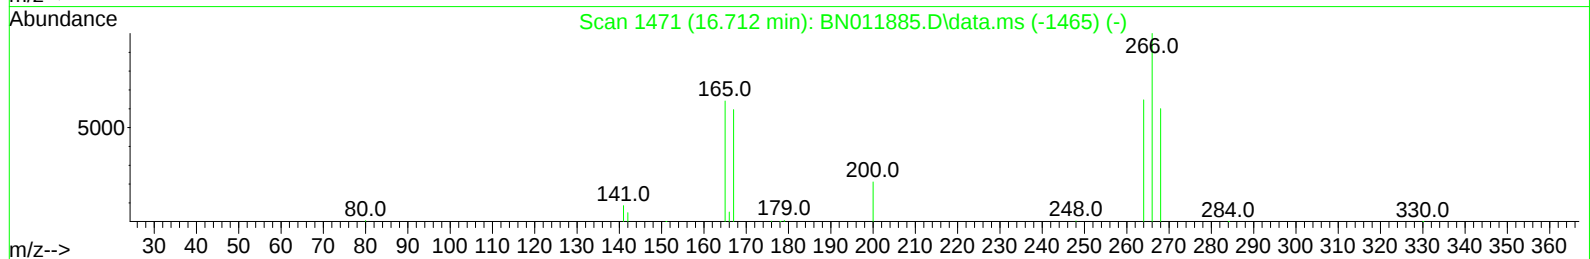
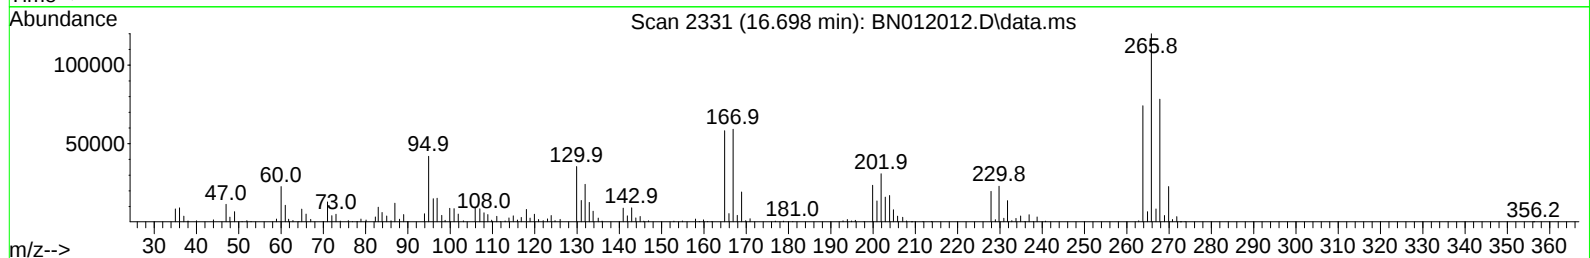


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092920\
Data File : BN012012.D
Acq On : 29 Sep 2020 09:22
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 30 04:58:27 2020
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN092320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 29 10:58:58 2020
Response via : Initial Calibration

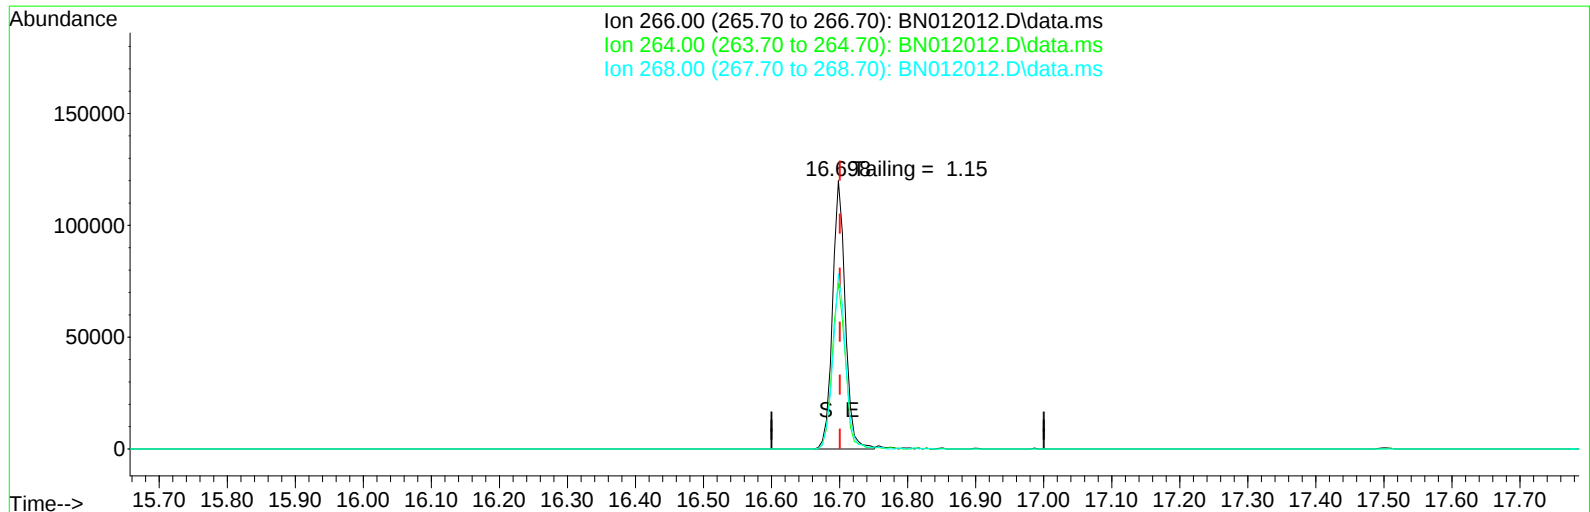

TIC: BN012012.D\data.ms

(24) Pentachlorophenol

16.698min (-0.002) 0.00 ng

response 157370

Ion	Exp%	Act%
266.00	100.00	100.00
264.00	64.00	63.39
268.00	65.50	64.98
0.00	0.00	0.00