
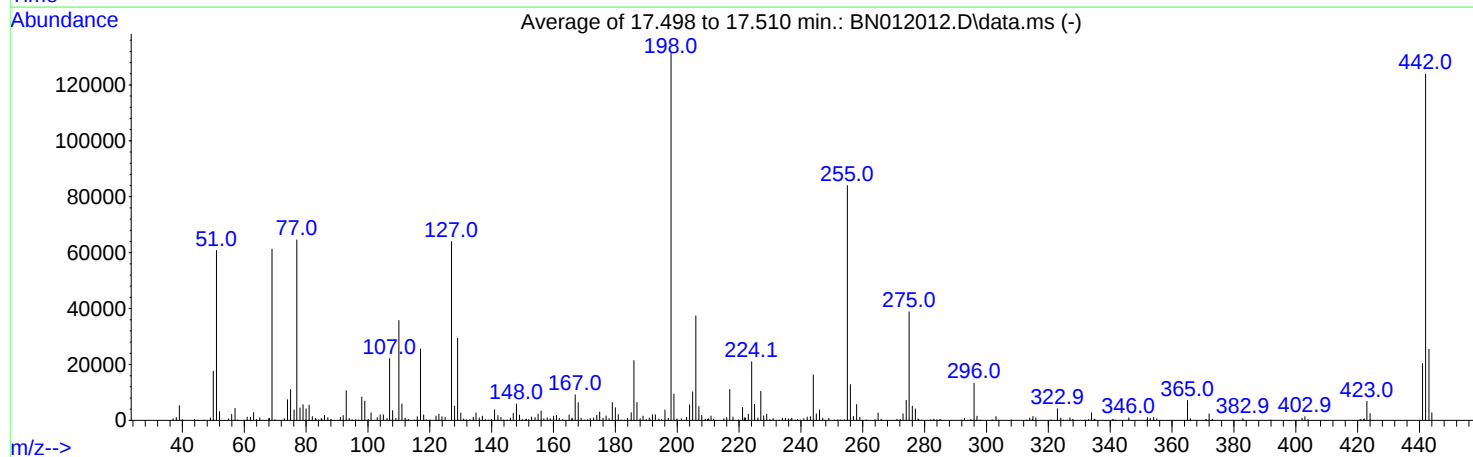


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092920\
 Data File : BN012012.D
 Acq On : 29 Sep 2020 09:22
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN092320.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 29 10:58:58 2020

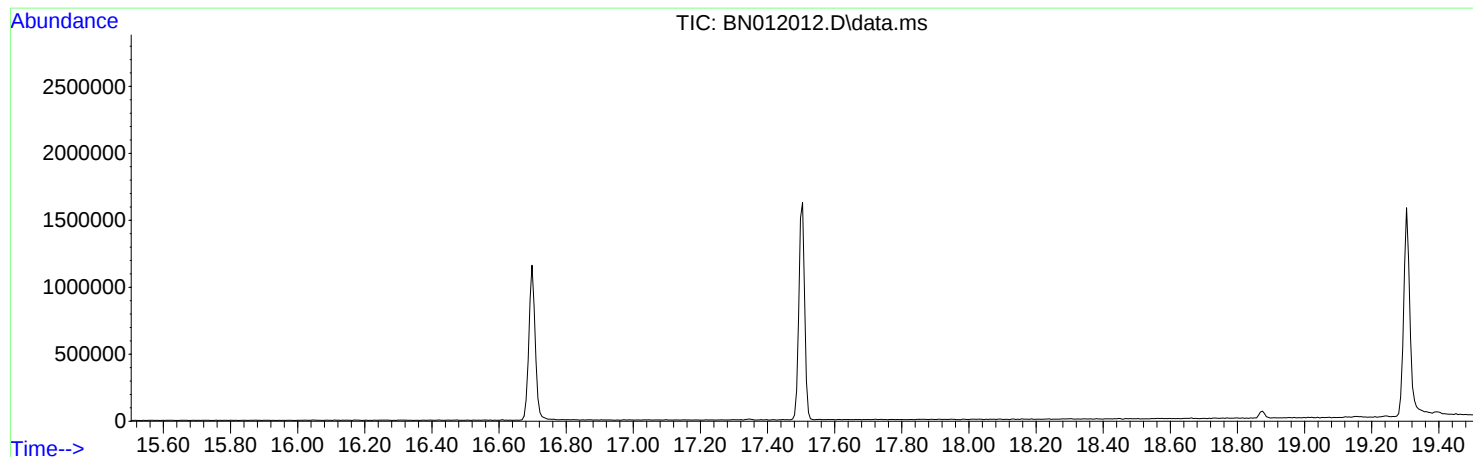

AutoFind: Scans 2467, 2468, 2469; Background Corrected with Scan 2460

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.2	60773	PASS
68	69	0.00	2	1.2	759	PASS
69	198	0.00	100	46.5	61240	PASS
70	69	0.00	2	0.4	232	PASS
127	198	10	80	48.6	63912	PASS
197	198	0.00	2	0.6	740	PASS
198	198	100	100	100.0	131597	PASS
199	198	5	9	7.1	9378	PASS
275	198	10	60	29.5	38821	PASS
365	198	1	100	5.4	7110	PASS
441	198	0.01	100	15.5	20384	PASS
442	198	50	100	94.1	123867	PASS
443	442	15	24	20.5	25416	PASS