

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092921\
 Data File : BN016573.D
 Acq On : 29 Sep 2021 11:18
 Operator : CG/JU
 Sample : M3945-01 2X
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Sep 29 12:25:43 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN092821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 29 10:56:17 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.652	152	30554	0.400	ng	0.00
7) Naphthalene-d8	10.419	136	141367	0.400	ng	# 0.00
13) Acenaphthene-d10	14.281	164	77717	0.400	ng	# 0.00
19) Phenanthrene-d10	17.030	188	166355	0.400	ng	# 0.00
29) Chrysene-d12	21.259	240	218496	0.400	ng	# 0.01
35) Perylene-d12	23.529	264	196615	0.400	ng	# 0.02
System Monitoring Compounds						
4) 2-Fluorophenol	5.291	112	14697	0.193	ng	0.00
5) Phenol-d6	6.840	99	14137	0.185	ng	0.00
8) Nitrobenzene-d5	8.797	82	11912	0.159	ng	0.00
11) 2-Methylnaphthalene-d10	12.016	152	38580	0.192	ng	0.00
14) 2,4,6-Tribromophenol	15.779	330	6713	0.198	ng	0.00
15) 2-Fluorobiphenyl	12.898	172	49948	0.156	ng	0.00
27) Fluoranthene-d10	19.083	212	77368	0.172	ng	0.00
31) Terphenyl-d14	19.693	244	65896	0.140	ng	0.00
Target Compounds						
						Qvalue
9) Naphthalene	10.470	128	48252	0.127	ng	99
12) 2-Methylnaphthalene	12.092	142	24064	0.101	ng	99
16) Acenaphthylene	14.002	152	153944	0.447	ng	99
17) Acenaphthene	14.345	154	149310	0.638	ng	# 93
18) Fluorene	15.334	166	182663	0.640	ng	98
20) 4,6-Dinitro-2-methylph...	15.436	198	292	0.223	ng	# 1
23) Atrazine	16.458	200	113	0.108	ng	# 1
24) Pentachlorophenol	16.689	266	16942	0.500	ng	99
25) Phenanthrene	17.078	178	3521366	7.036	ng	99
26) Anthracene	17.164	178	1134762	2.610	ng	# 96
28) Fluoranthene	19.113	202	7162639	13.093	ng	# 95
30) Pyrene	19.475	202	6261694	8.405	ng	# 92
32) Benzo(a)anthracene	21.238	228	4586260	6.772	ng	# 86
33) Chrysene	21.291	228	6834047	9.894	ng	# 91
34) Bis(2-ethylhexyl)phtha...	21.185	149	1068031	5.296	ng	100
36) Indeno(1,2,3-cd)pyrene	25.826	276	1640929	2.617	ng	99
37) Benzo(b)fluoranthene	22.851	252	6310582	9.613	ng	# 95
39) Benzo(a)pyrene	23.433	252	3533430	5.868	ng	# 93
40) Dibenzo(a,h)anthracene	25.829	278	596131	1.368	ng	# 71
41) Benzo(g,h,i)perylene	26.531	276	1610679	2.825	ng	# 94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092921\
Data File : BN016573.D
Acq On : 29 Sep 2021 11:18
Operator : CG/JU
Sample : M3945-01 2X
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :


Quant Time: Sep 29 12:25:43 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN092821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 29 10:56:17 2021
Response via : Initial Calibration

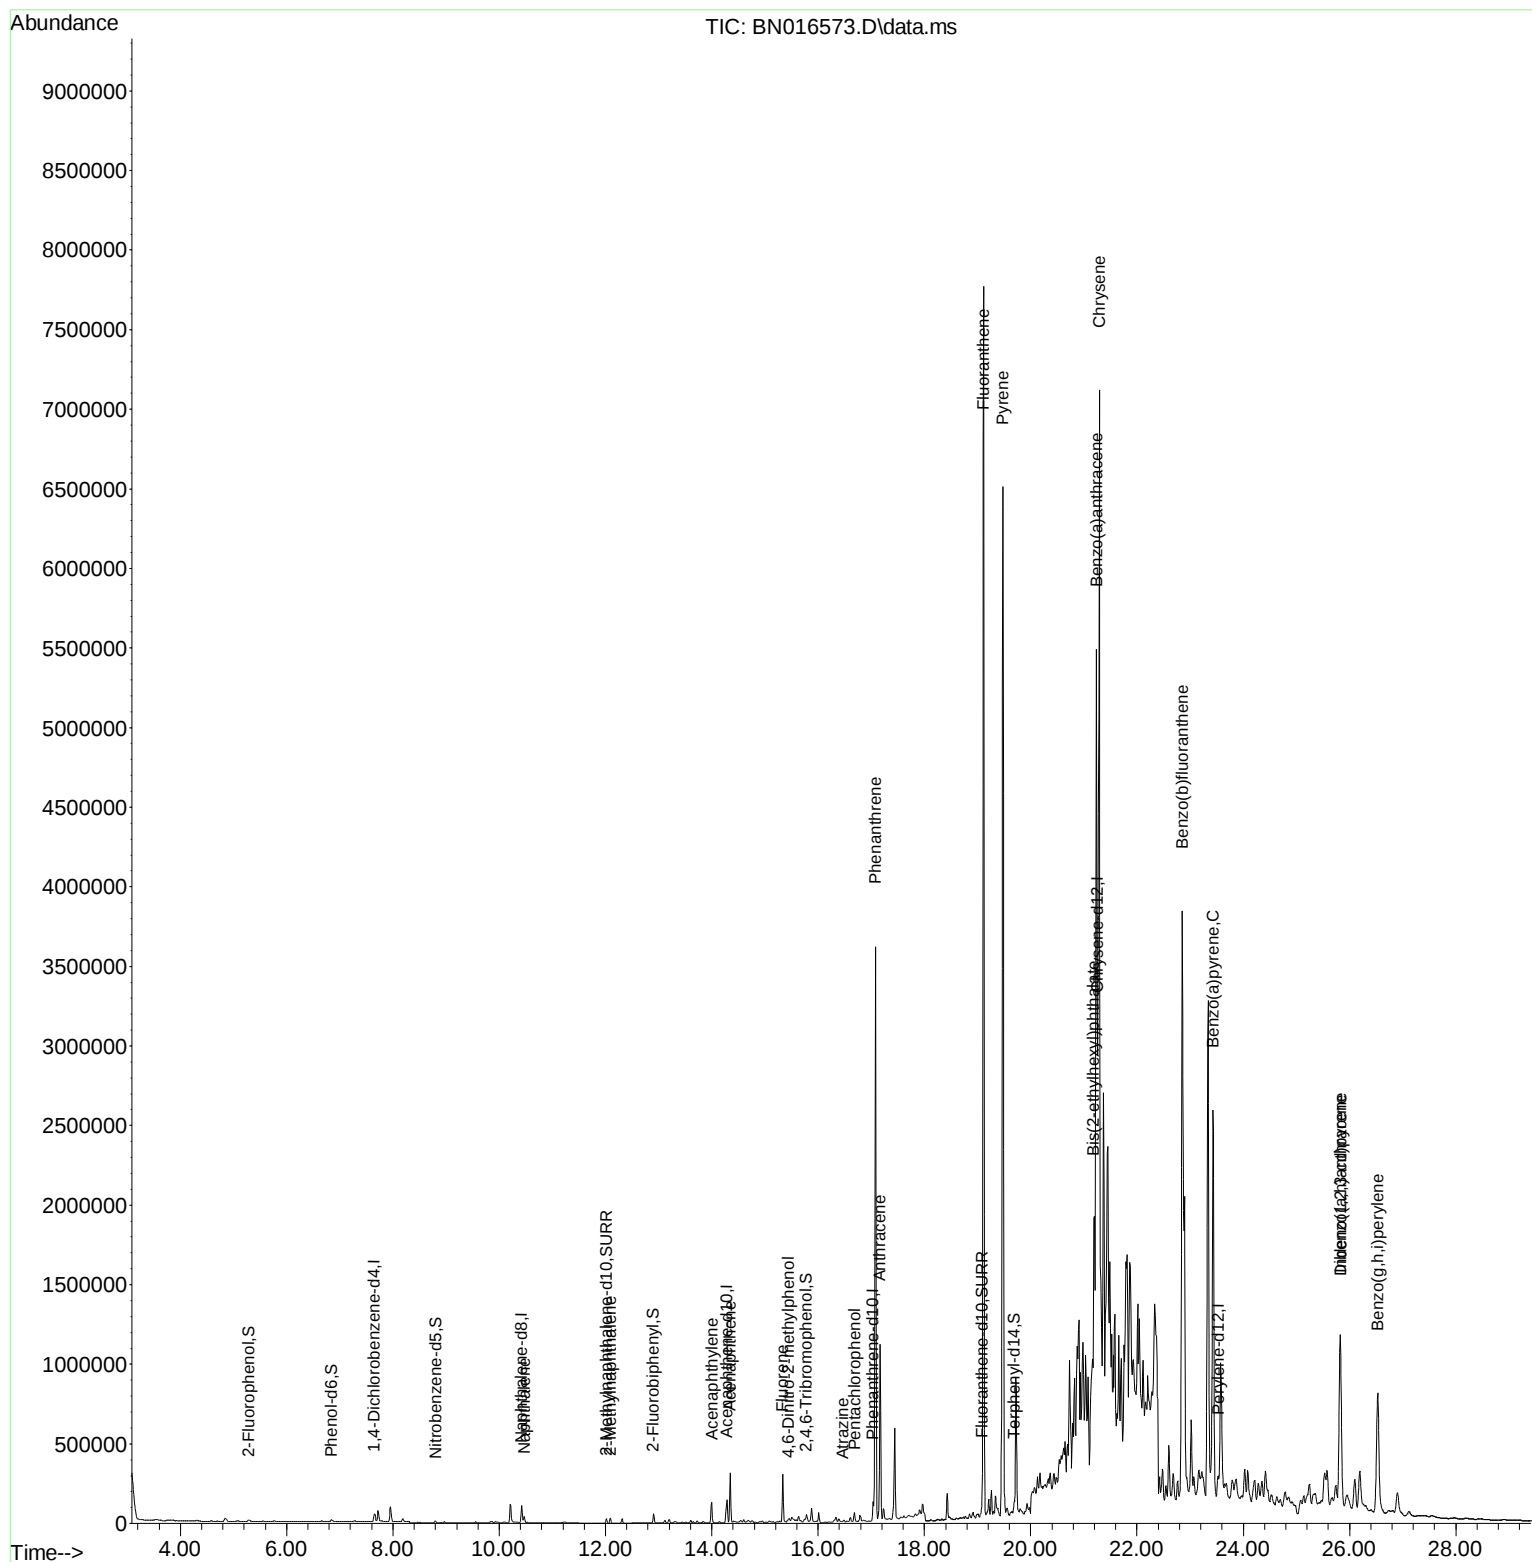



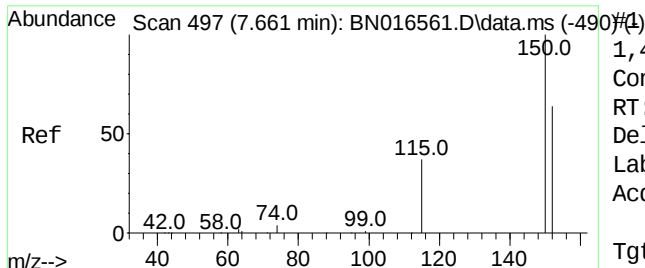


1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.652 min Scan# 496
 Delta R.T. -0.000 min
 Lab File: BN016573.D
 Acq: 29 Sep 2021 11:18

Instrument :
 BNA_N
 ClientSampleId :



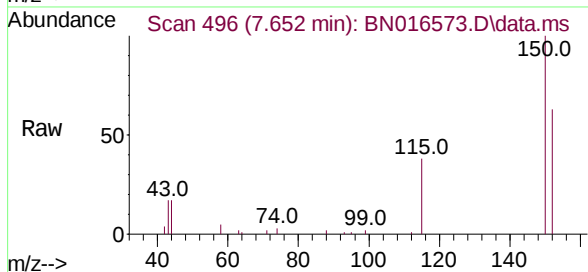



Tgt Ion:	152	Resp:	30554
Ion	Ratio	Lower	Upper
152	100		
150	158.7	125.1	187.7
115	59.9	45.8	68.8

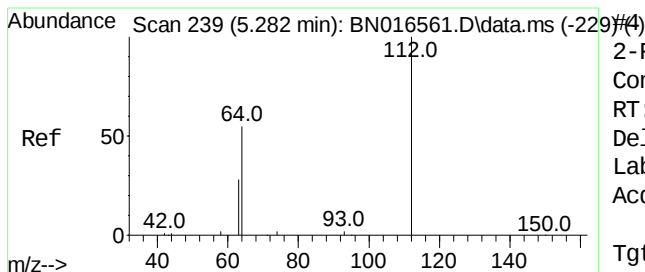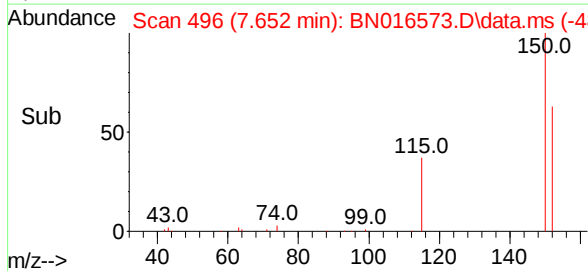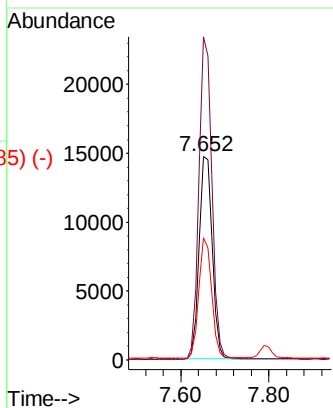

2-Fluorophenol
 Concen: 0.193 ng
 RT: 5.291 min Scan# 240
 Delta R.T. 0.009 min
 Lab File: BN016573.D
 Acq: 29 Sep 2021 11:18

Tgt Ion:	112	Resp:	14697
Ion	Ratio	Lower	Upper
112	100		
64	55.1	48.4	72.6
63	27.6	25.4	38.2


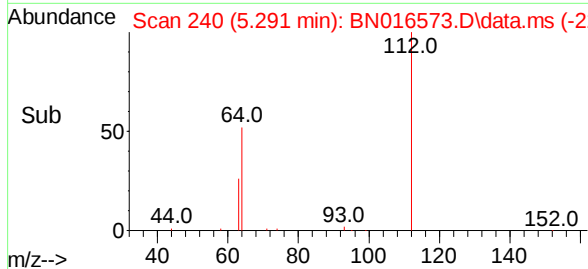

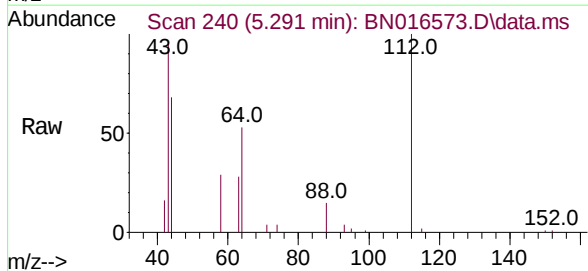


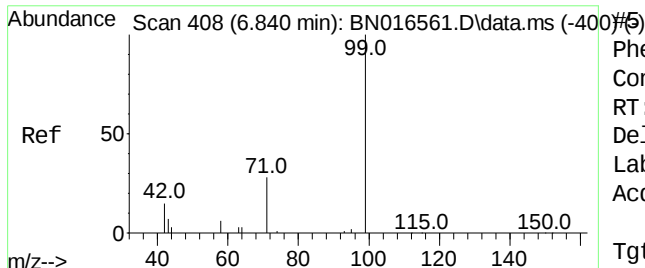

Phenol-d6
 Concen: 0.185 ng
 RT: 6.840 min Scan# 408
 Delta R.T. 0.009 min
 Lab File: BN016573.D
 Acq: 29 Sep 2021 11:18




Instrument :
 BNA_N
 ClientSampleId :


Tgt Ion:	99	Resp:	14137
Ion	Ratio	Lower	Upper
99	100		
42	18.3	19.6	29.4#
71	33.3	24.2	36.2

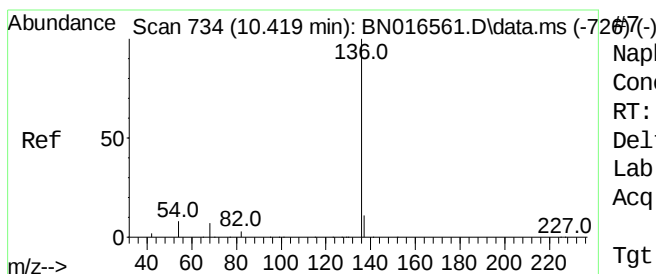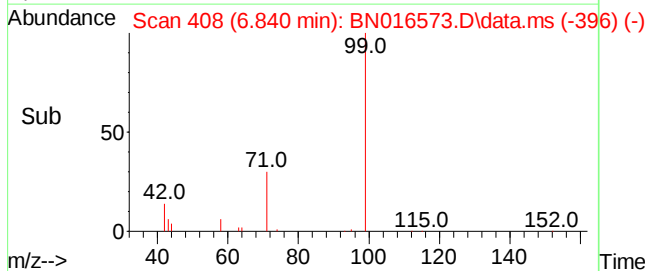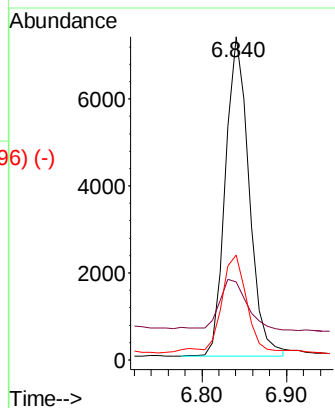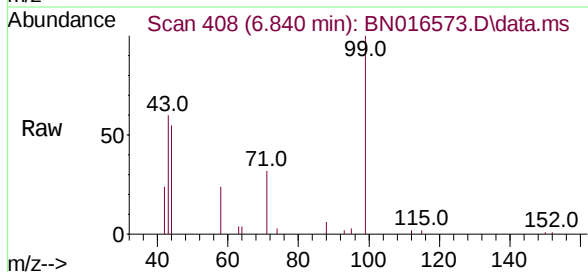

Naphthalene-d8
 Concen: 0.400 ng
 RT: 10.419 min Scan# 734
 Delta R.T. -0.000 min
 Lab File: BN016573.D
 Acq: 29 Sep 2021 11:18

Tgt Ion:	136	Resp:	141367
Ion	Ratio	Lower	Upper
136	100		
137	11.0	8.8	13.2
54	7.2	5.8	8.6
68	5.9	3.6	5.4#


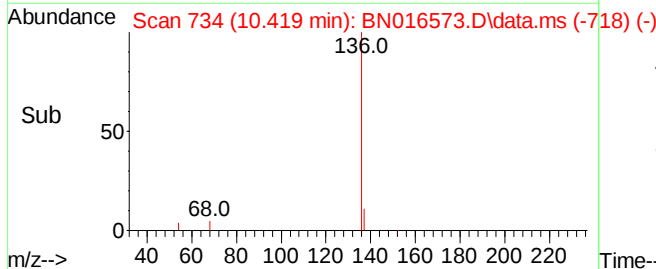
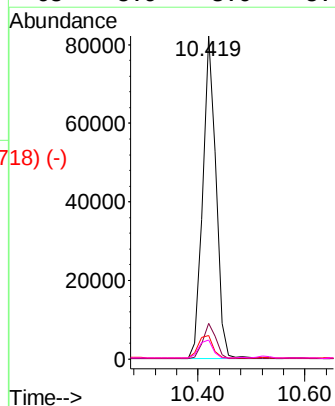
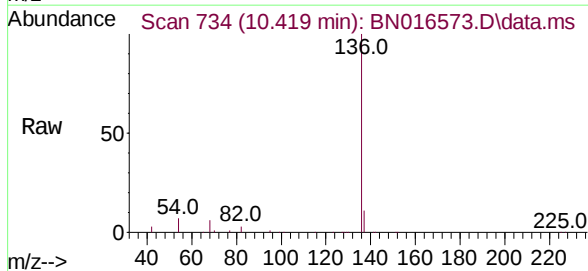


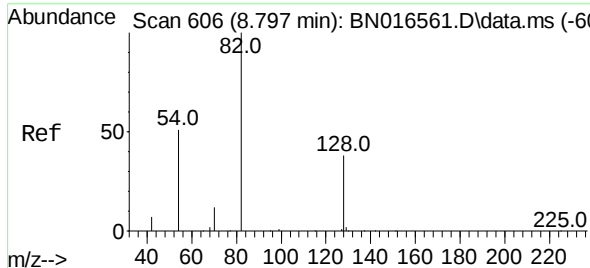

Nitrobenzene-d5
 Concen: 0.159 ng
 RT: 8.797 min Scan# 606
 Delta R.T. -0.000 min
 Lab File: BN016573.D
 Acq: 29 Sep 2021 11:18




Instrument :
 BNA_N
 ClientSampleId :

Tgt Ion:	82	Resp:	11912
Ion	Ratio	Lower	Upper
82	100		
128	42.0	27.4	41.2#
54	49.4	58.5	87.7#

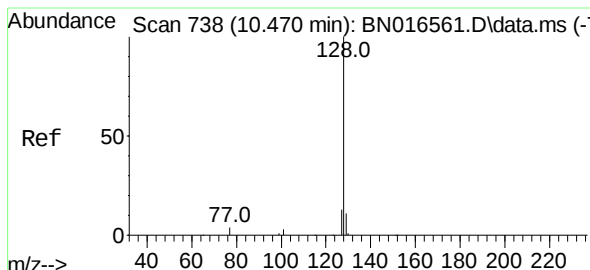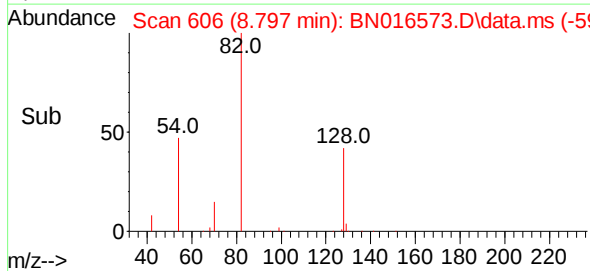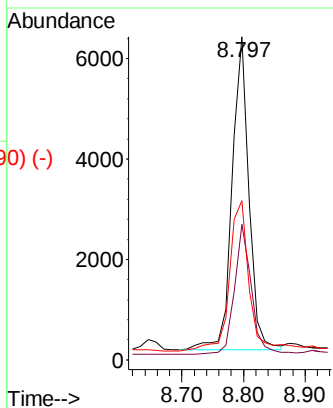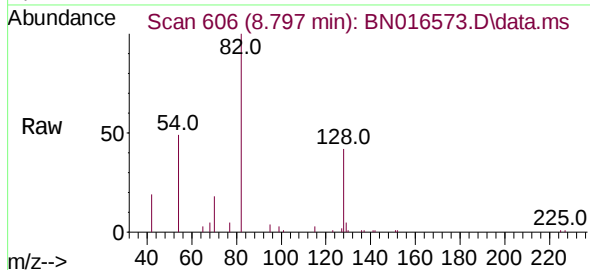


Naphthalene
 Concen: 0.127 ng
 RT: 10.470 min Scan# 738
 Delta R.T. -0.000 min
 Lab File: BN016573.D
 Acq: 29 Sep 2021 11:18

Tgt Ion:	128	Resp:	48252
Ion	Ratio	Lower	Upper
128	100		
129	11.6	8.9	13.3
127	13.0	10.1	15.1

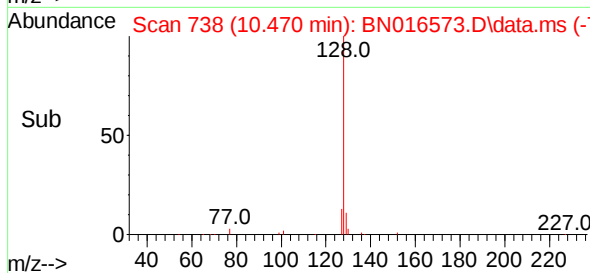

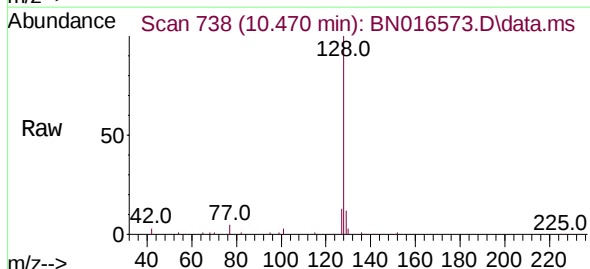


Abundance Scan 935 (12.021 min): BN016561.D\data.ms (-922) (-)

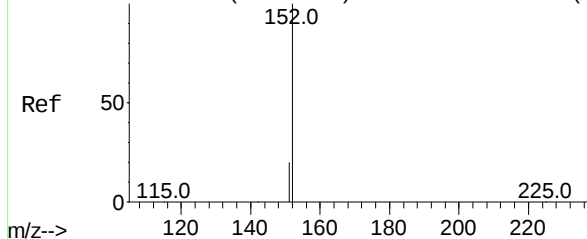


2-Methylnaphthalene-d10
Concen: 0.192 ng
RT: 12.016 min Scan# 934
Delta R.T. -0.000 min
Lab File: BN016573.D
Acq: 29 Sep 2021 11:18

Tgt Ion:152 Resp: 38580
Ion Ratio Lower Upper
152 100
151 20.6 16.6 25.0

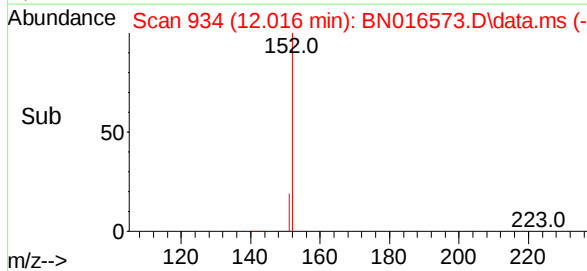
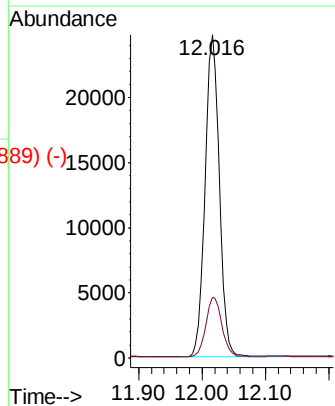
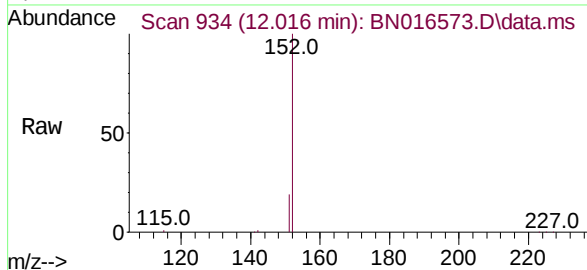


Abundance Scan 951 (12.092 min): BN016561.D\data.ms (-941) (-)

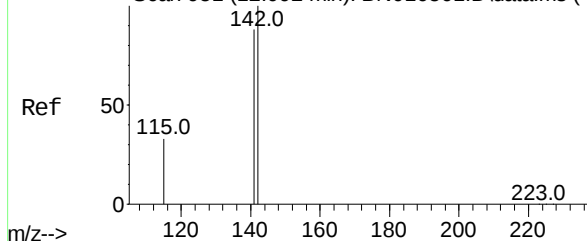

2-Methylnaphthalene
Concen: 0.101 ng
RT: 12.092 min Scan# 951
Delta R.T. -0.000 min
Lab File: BN016573.D
Acq: 29 Sep 2021 11:18


Tgt Ion:142 Resp: 24064
Ion Ratio Lower Upper
142 100
141 86.4 69.9 104.9
115 34.5 27.0 40.4

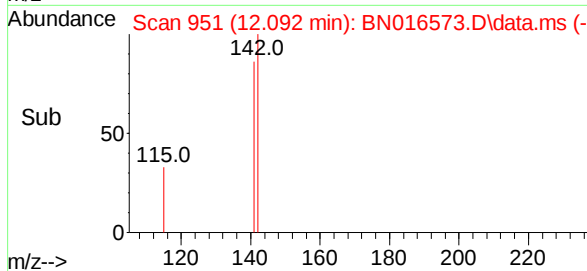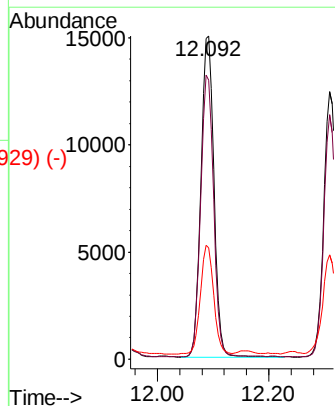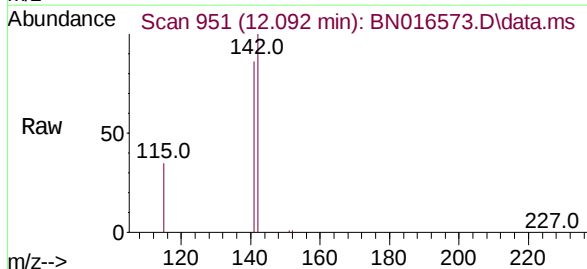



Abundance Scan 1184 (14.282 min): BN016561.D\data.ms (-1168) (-)

Acenaphthene-d10
Concen: 0.400 ng
RT: 14.281 min Scan# 1184
Delta R.T. -0.000 min
Lab File: BN016573.D
Acq: 29 Sep 2021 11:18


Instrument :
BNA_N
ClientSampleId :

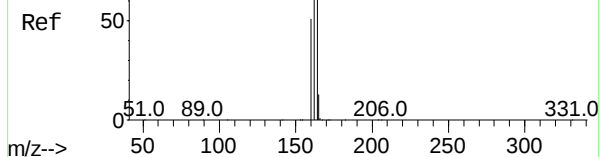

Tgt Ion:	164	Resp:	77717
Ion Ratio	Lower	Upper	
164	100		
162	100.2	79.4	119.0
160	45.6	46.6	70.0#

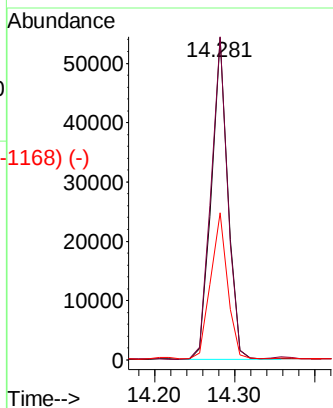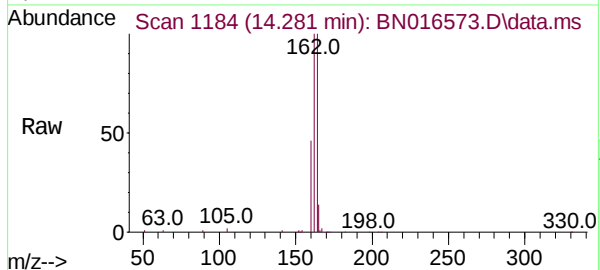



Abundance Scan 1184 (14.281 min): BN016573.D\data.ms (-1168) (-)

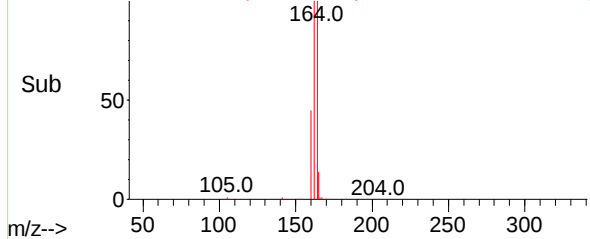


Abundance Scan 1302 (15.779 min): BN016561.D\data.ms (-1294) (-)


2,4,6-Tribromophenol
Concen: 0.198 ng
RT: 15.779 min Scan# 1302
Delta R.T. -0.000 min
Lab File: BN016573.D
Acq: 29 Sep 2021 11:18

Tgt Ion:	330	Resp:	6713
Ion Ratio	Lower	Upper	
330	100		
332	0.0	0.0	0.0
141	35.2	34.4	51.6

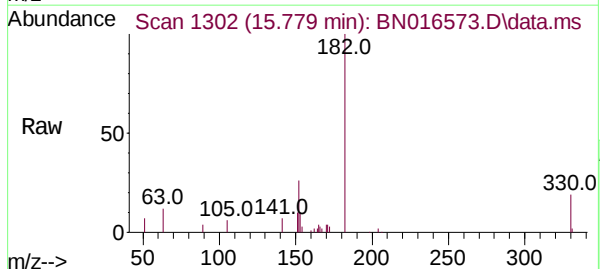

Abundance Scan 1302 (15.779 min): BN016573.D\data.ms (-1294) (-)




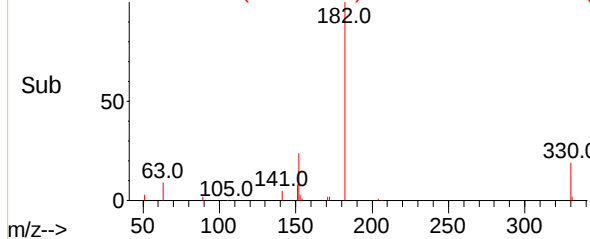


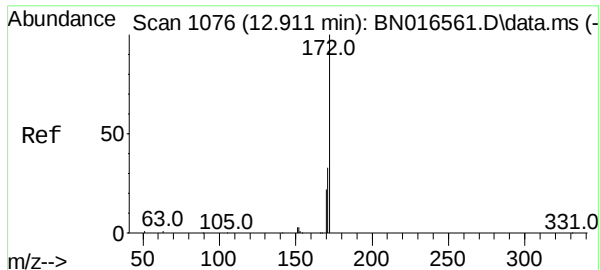

2-Fluorobiphenyl
Concen: 0.156 ng
RT: 12.898 min Scan# 1075
Delta R.T. -0.000 min
Lab File: BN016573.D
Acq: 29 Sep 2021 11:18




Instrument :
BNA_N
ClientSampleId :

Tgt Ion:	172	Resp:	49948
Ion	Ratio	Lower	Upper
172	100		
171	35.5	27.4	41.2
170	24.7	18.9	28.3

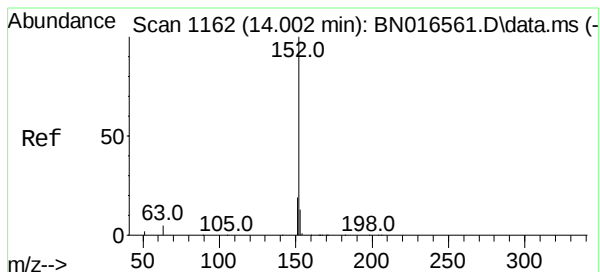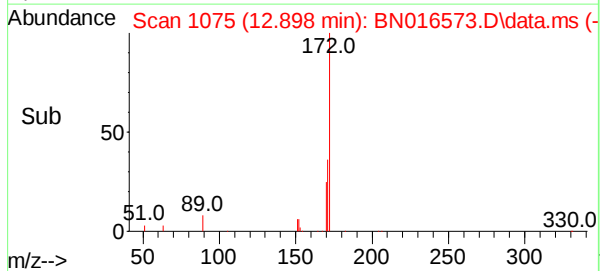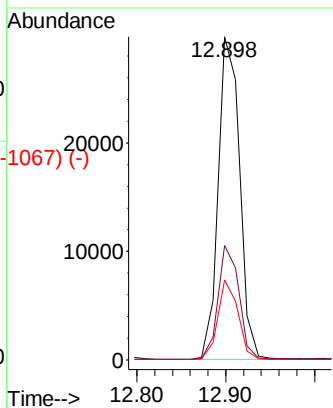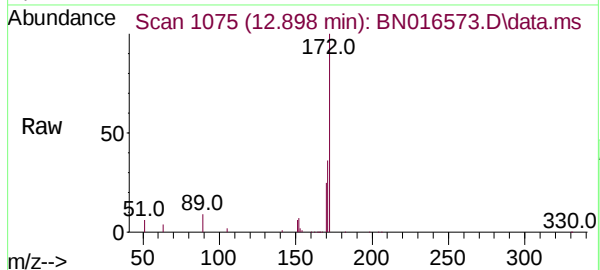


Acenaphthylene
Concen: 0.447 ng
RT: 14.002 min Scan# 1162
Delta R.T. -0.000 min
Lab File: BN016573.D
Acq: 29 Sep 2021 11:18

Tgt Ion:	152	Resp:	153944
Ion	Ratio	Lower	Upper
152	100		
151	19.6	15.4	23.0
153	13.6	10.4	15.6

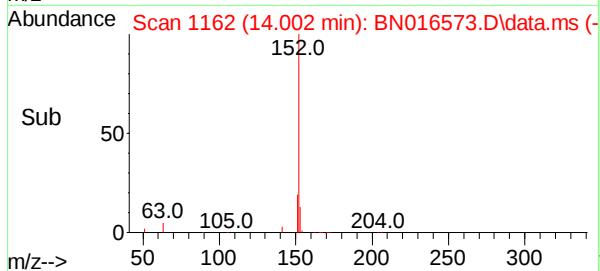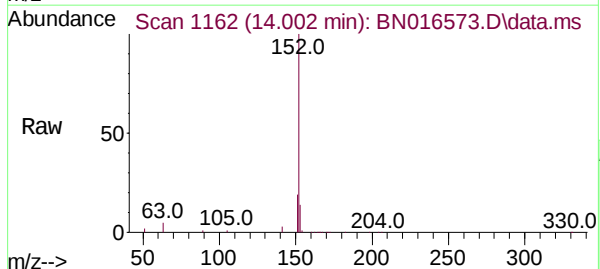



Abundance Scan 1189 (14.345 min): BN016561.D\data.ms (-1189) (-)

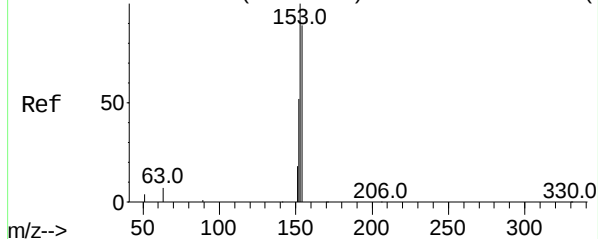


Acenaphthene
Concen: 0.638 ng
RT: 14.345 min Scan# 1189
Delta R.T. -0.000 min
Lab File: BN016573.D
Acq: 29 Sep 2021 11:18

Instrument :
BNA_N
ClientSampleId :


Tgt Ion:	154	Resp:	149310
Ion	Ratio	Lower	Upper
154	100		
153	112.6	91.0	136.4
152	55.3	55.8	83.6#

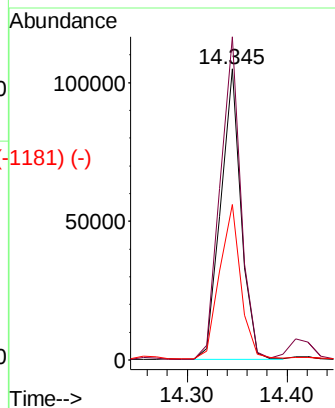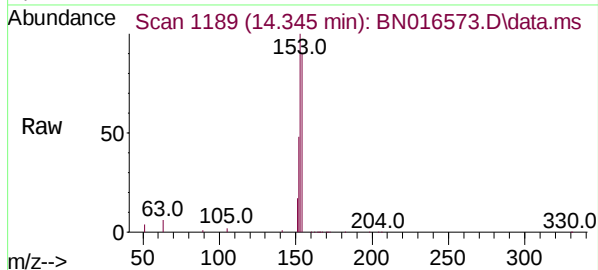

Abundance Scan 1189 (14.345 min): BN016573.D\data.ms (-1181) (-)


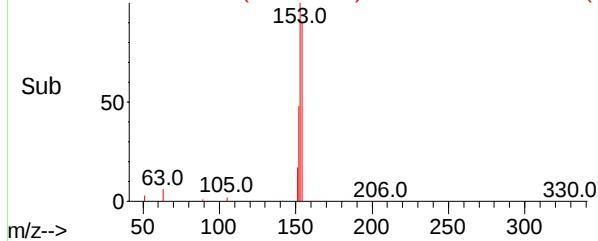


Abundance Scan 1267 (15.335 min): BN016561.D\data.ms (-1267) (-)

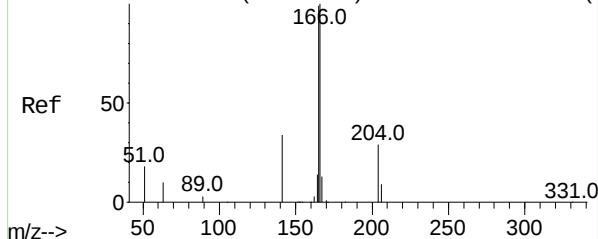


Fluorene
Concen: 0.640 ng
RT: 15.334 min Scan# 1267
Delta R.T. -0.000 min
Lab File: BN016573.D
Acq: 29 Sep 2021 11:18

Tgt Ion:	166	Resp:	182663
Ion	Ratio	Lower	Upper
166	100		
165	98.8	77.6	116.4
167	14.5	10.7	16.1

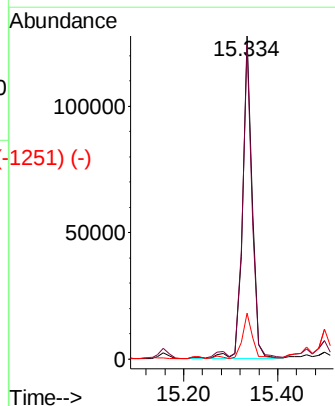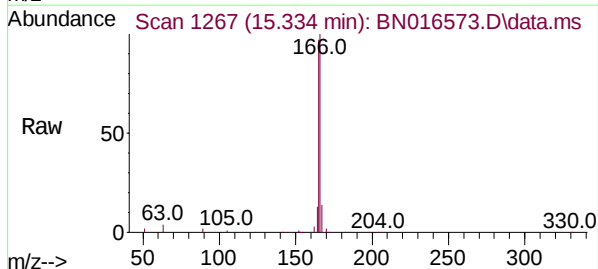


Abundance Scan 1267 (15.334 min): BN016573.D\data.ms (-1251) (-)

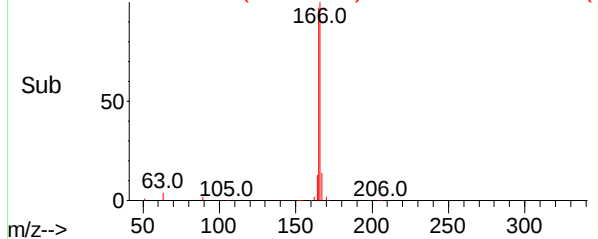




Abundance Scan 1405 (17.042 min): BN016561.D\data.ms (-1388) (-)

Phenanthrene-d10
Concen: 0.400 ng
RT: 17.030 min Scan# 1404
Delta R.T. -0.000 min
Lab File: BN016573.D
Acq: 29 Sep 2021 11:18

Instrument :
BNA_N
ClientSampleId :

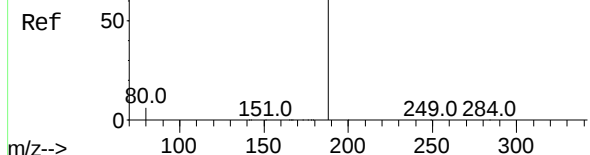





Tgt Ion	Ratio	Lower	Upper
188	100		
94	0.0	0.0	0.0
80	12.7	6.9	10.3#

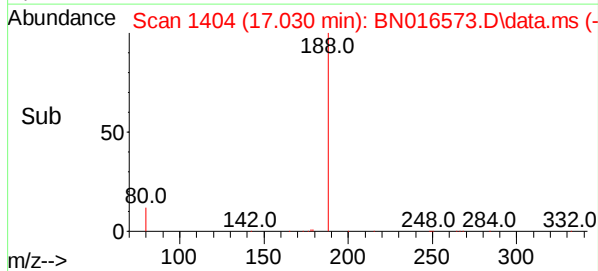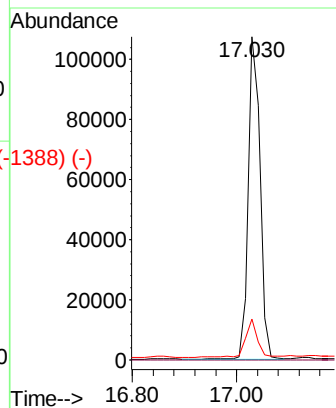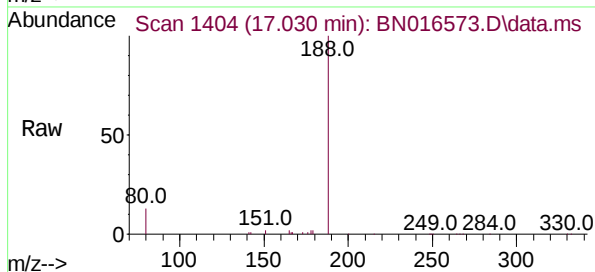


Abundance Scan 1275 (15.436 min): BN016561.D\data.ms (-1266) (-)

4,6-Dinitro-2-methylphenol
Concen: 0.223 ng
RT: 15.436 min Scan# 1275
Delta R.T. 0.013 min
Lab File: BN016573.D
Acq: 29 Sep 2021 11:18

Tgt Ion	Ratio	Lower	Upper
198	100		
182	83.5	17.5	26.3#
77	0.0	0.0	0.0

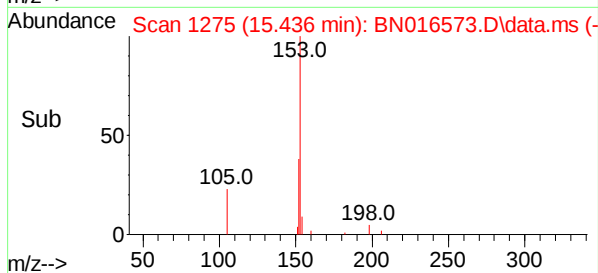
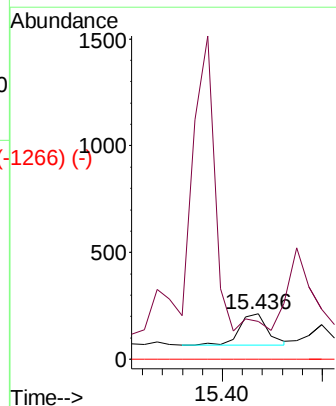
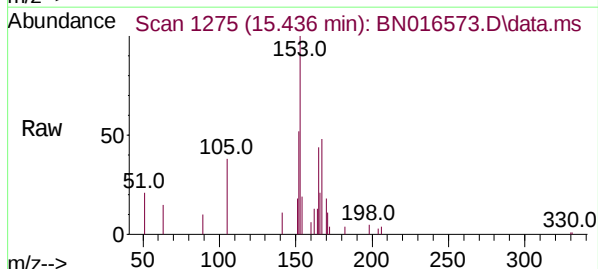
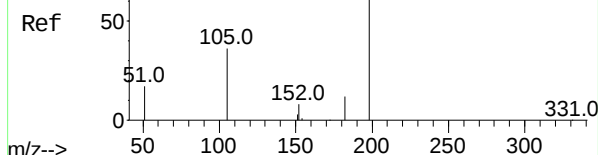


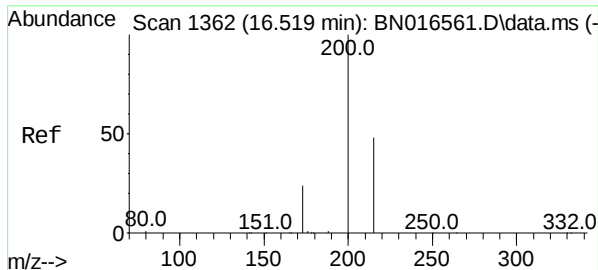

Atrazine
Concen: 0.108 ng
RT: 16.458 min Scan# 1357
Delta R.T. -0.061 min
Lab File: BN016573.D
Acq: 29 Sep 2021 11:18




Instrument :
BNA_N
ClientSampleId :

Tgt Ion:	200	Resp:	113
Ion Ratio	Lower	Upper	
200	100		
173	192.8	22.6	34.0#
215	94.7	38.2	57.4#

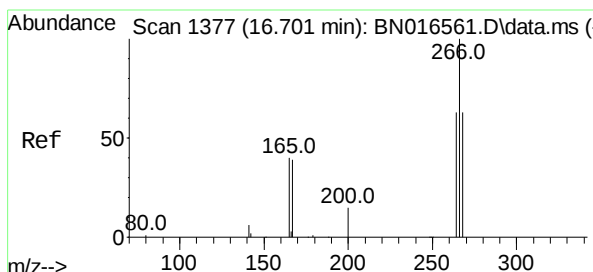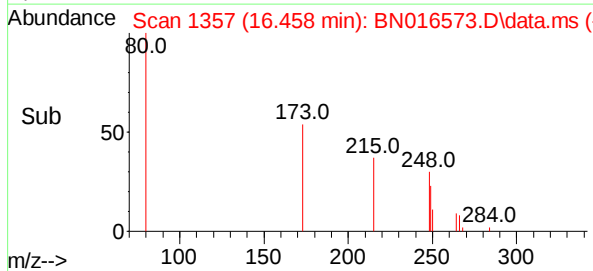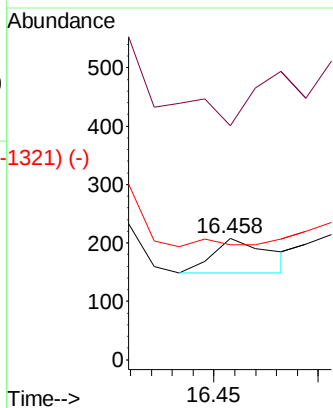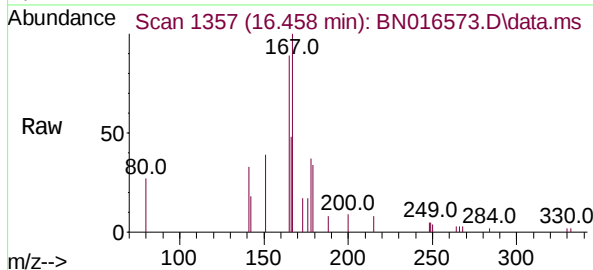

Pentachlorophenol
Concen: 0.500 ng
RT: 16.689 min Scan# 1376
Delta R.T. -0.000 min
Lab File: BN016573.D
Acq: 29 Sep 2021 11:18


Tgt Ion:	266	Resp:	16942
Ion Ratio	Lower	Upper	
266	100		
264	64.0	50.2	75.2
268	64.3	51.8	77.8

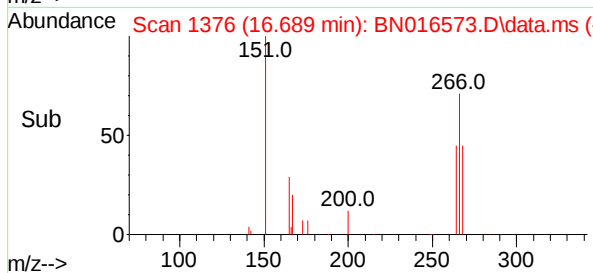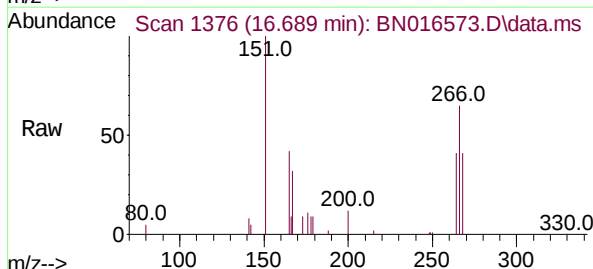

Abundance Scan 1408 (17.079 min): BN016561.D\data.ms (-1425) (-)




Phenanthrene
Concen: 7.036 ng
RT: 17.078 min Scan# 1408
Delta R.T. -0.000 min
Lab File: BN016573.D
Acq: 29 Sep 2021 11:18

Instrument :
BNA_N
ClientSampled :

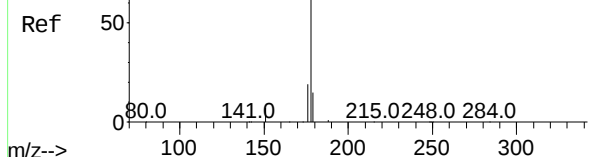

Tgt Ion:178 Resp: 3521366

Ion	Ratio	Lower	Upper
178	100		
176	19.0	15.0	22.6
179	16.0	12.3	18.5


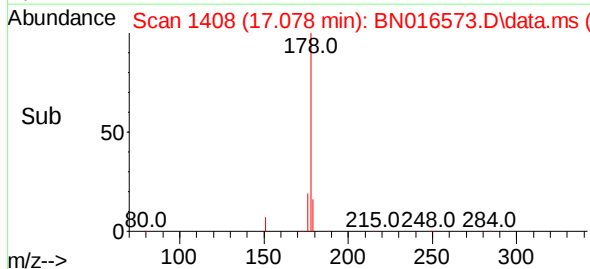
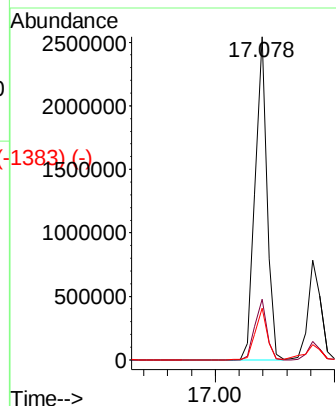
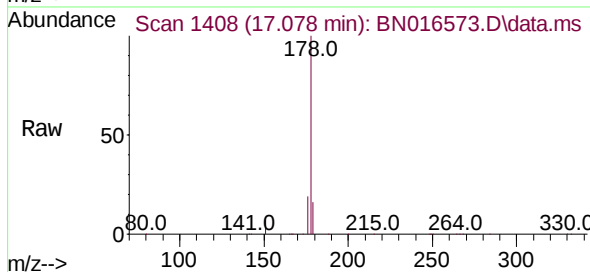


Abundance Scan 1415 (17.164 min): BN016561.D\data.ms (-1425) (-)


Anthracene
Concen: 2.610 ng
RT: 17.164 min Scan# 1415
Delta R.T. -0.000 min
Lab File: BN016573.D
Acq: 29 Sep 2021 11:18

Tgt Ion:178 Resp: 1134762

Ion	Ratio	Lower	Upper
178	100		
176	18.2	14.6	21.8
179	18.5	12.2	18.4#

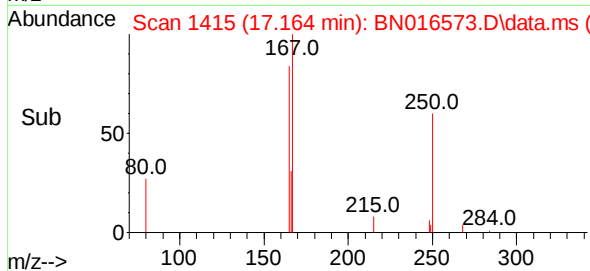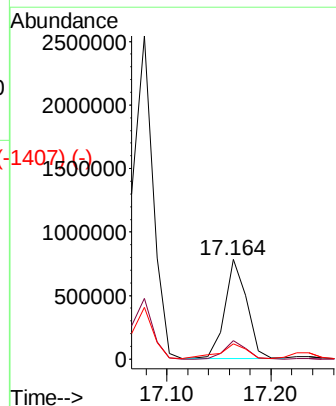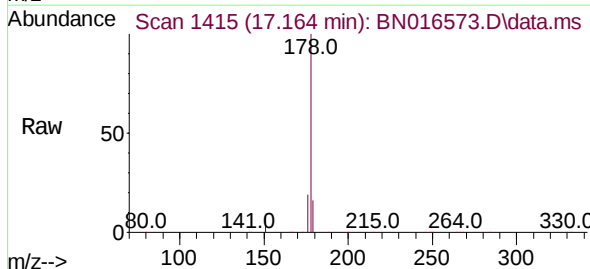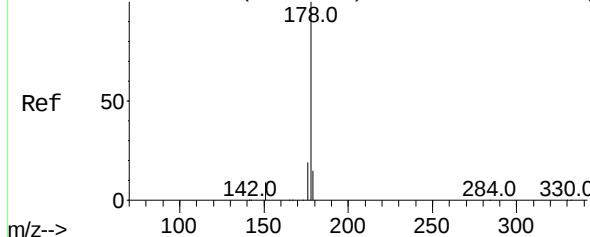




Abundance Scan 1699 (19.078 min): BN016561.D\data.ms (-1627) (-)

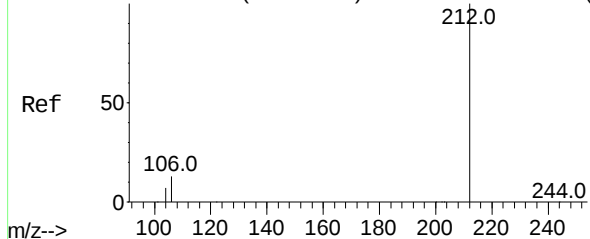


Fluoranthene-d10
Concen: 0.172 ng
RT: 19.083 min Scan# 1700
Delta R.T. 0.005 min
Lab File: BN016573.D
Acq: 29 Sep 2021 11:18

Instrument :
BNA_N
ClientSampleId :

Tgt Ion:	212	Resp:	77368
Ion Ratio	Lower	Upper	
212	100		
106	15.9	8.8	13.2#
104	10.4	5.0	7.4#

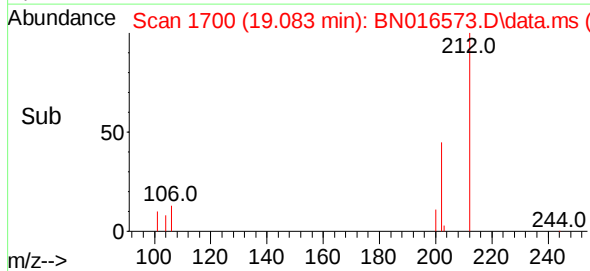
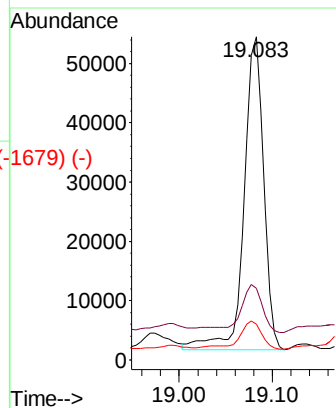
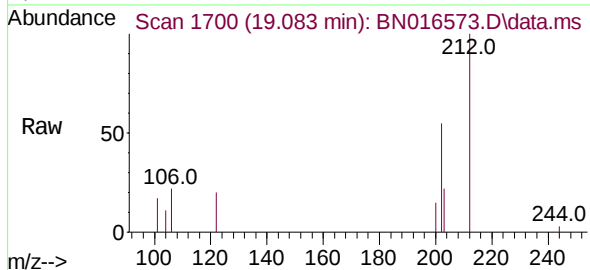


Abundance Scan 1705 (19.108 min): BN016561.D\data.ms (-1628) (-)

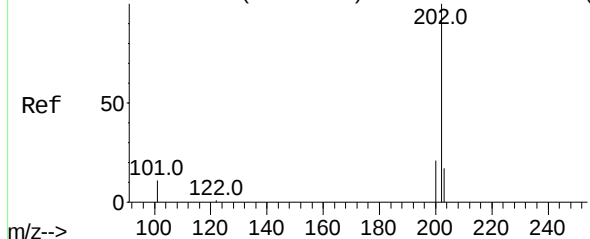

Fluoranthene
Concen: 13.093 ng
RT: 19.113 min Scan# 1706
Delta R.T. 0.005 min
Lab File: BN016573.D
Acq: 29 Sep 2021 11:18


Tgt Ion:	202	Resp:	7162639
Ion Ratio	Lower	Upper	
202	100		
101	12.7	7.5	11.3#
203	18.4	13.9	20.9

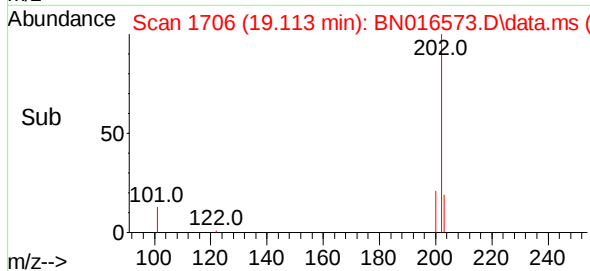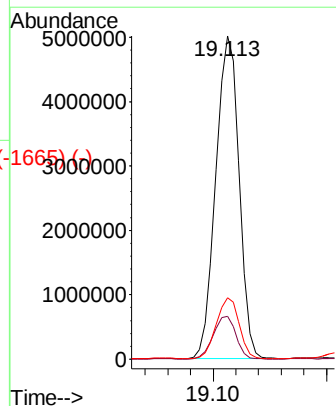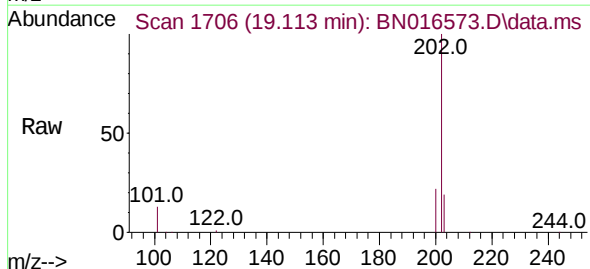




Abundance Scan 2003 (21.249 min): BN016561.D\data.ms (-1929) (-)

Chrysene-d12
Concen: 0.400 ng
RT: 21.259 min Scan# 2004
Delta R.T. 0.011 min
Lab File: BN016573.D
Acq: 29 Sep 2021 11:18

Instrument :
BNA_N
ClientSampled :

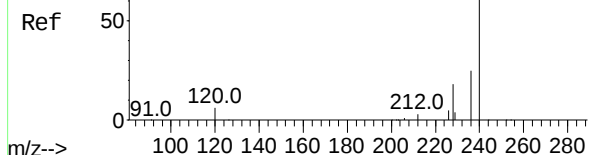





Tgt Ion:	240	Resp:	218496
Ion	Ratio	Lower	Upper
240	100		
120	17.6	9.0	13.4#
236	31.4	21.7	32.5

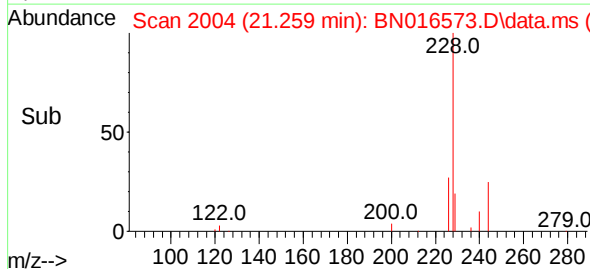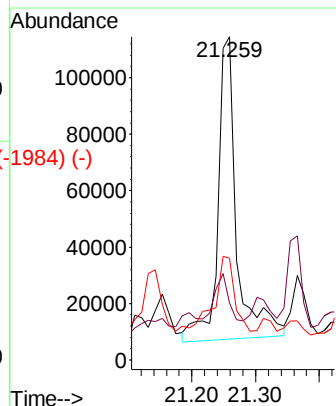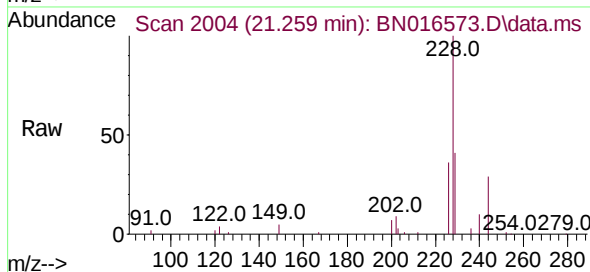

Abundance Scan 1779 (19.475 min): BN016561.D\data.ms (-1739) (-)

Pyrene
Concen: 8.405 ng
RT: 19.475 min Scan# 1779
Delta R.T. -0.000 min
Lab File: BN016573.D
Acq: 29 Sep 2021 11:18


Tgt Ion:	202	Resp:	6261694
Ion	Ratio	Lower	Upper
202	100		
200	21.3	16.3	24.5
203	23.7	13.9	20.9#

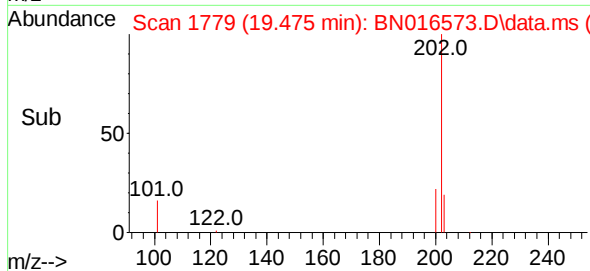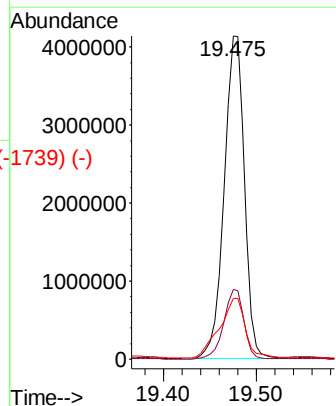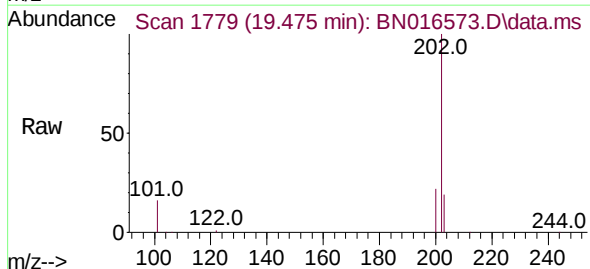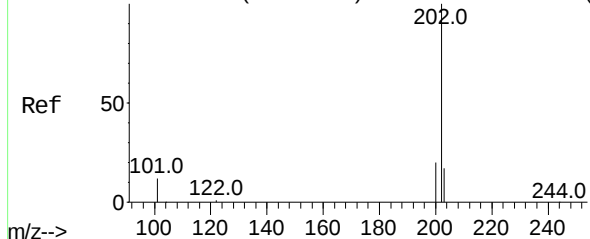




Abundance Scan 1823 (19.694 min): BN016561.D\data.ms (-1824) (-)

Terphenyl-d14
Concen: 0.140 ng
RT: 19.693 min Scan# 1823
Delta R.T. -0.000 min
Lab File: BN016573.D
Acq: 29 Sep 2021 11:18

Instrument :
BNA_N
ClientSampled :

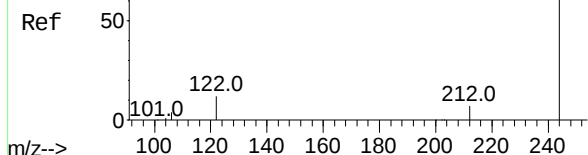


Tgt Ion	Ratio	Lower	Upper
244	100		
212	10.7	6.1	9.1#
122	38.2	8.4	12.6#

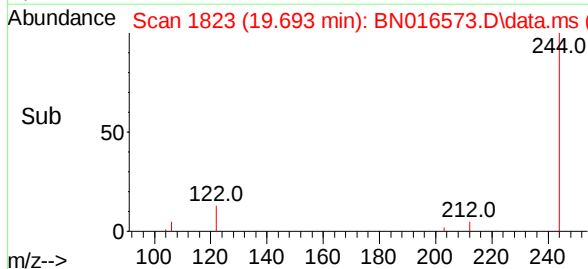
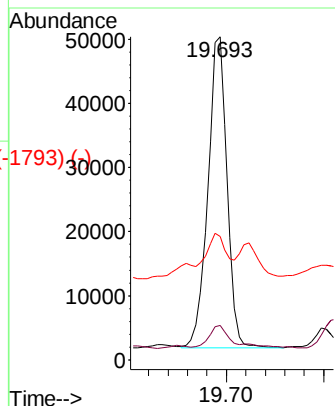
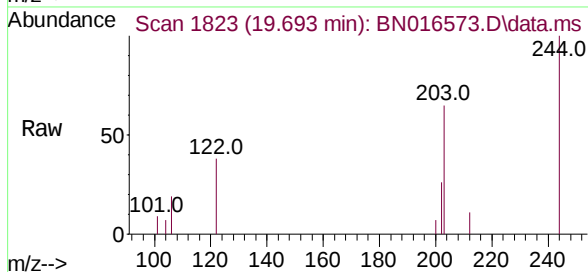



Abundance Scan 2001 (21.228 min): BN016561.D\data.ms (-1932) (-)

Benzo(a)anthracene
Concen: 6.772 ng
RT: 21.238 min Scan# 2002
Delta R.T. 0.011 min
Lab File: BN016573.D
Acq: 29 Sep 2021 11:18

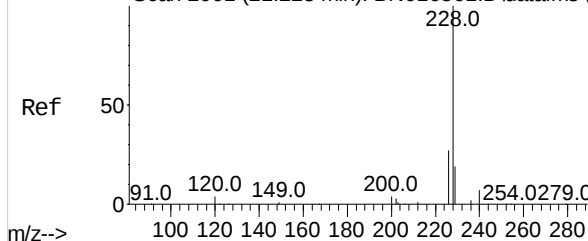

Tgt Ion	Ratio	Lower	Upper
228	100		
226	30.3	21.2	31.8
229	29.7	15.6	23.4#


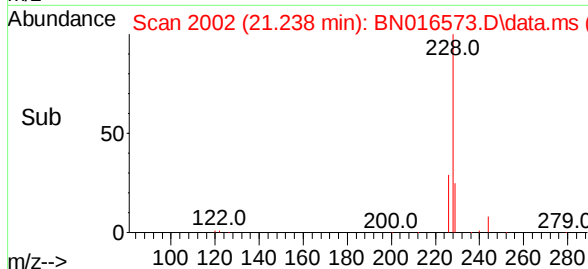
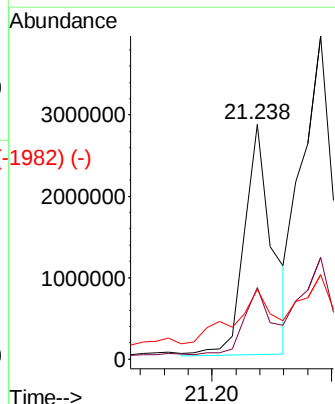
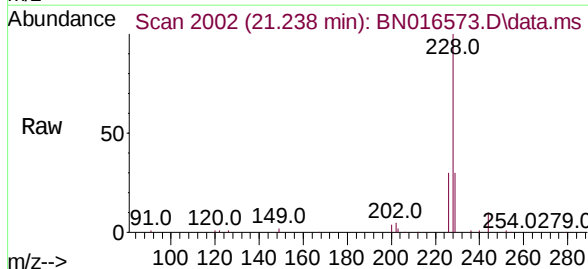


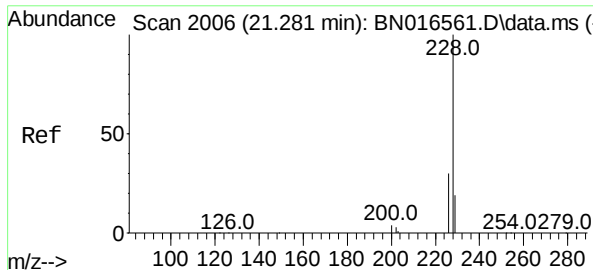

Chrysene
 Concen: 9.894 ng
 RT: 21.291 min Scan# 2007
 Delta R.T. 0.011 min
 Lab File: BN016573.D
 Acq: 29 Sep 2021 11:18




Instrument :
 BNA_N
 ClientSampled :

Tgt Ion:	228	Resp:	6834047
Ion	Ratio	Lower	Upper
228	100		
226	31.5	23.1	34.7
229	26.2	15.8	23.8#

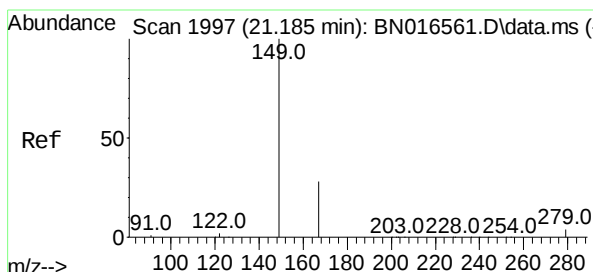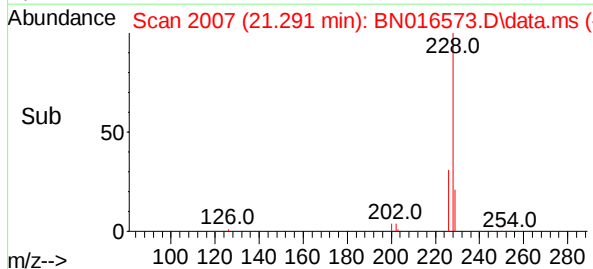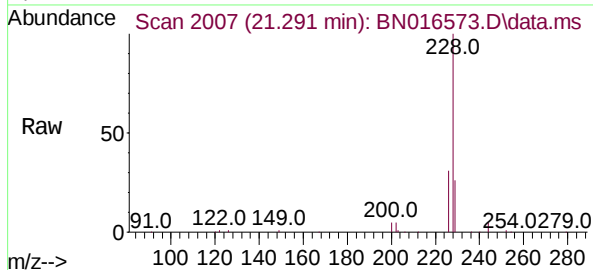

Bis(2-ethylhexyl)phthalate
 Concen: 5.296 ng
 RT: 21.185 min Scan# 1997
 Delta R.T. -0.000 min
 Lab File: BN016573.D
 Acq: 29 Sep 2021 11:18


Tgt Ion:	149	Resp:	1068031
Ion	Ratio	Lower	Upper
149	100		
167	26.6	21.4	32.2
279	3.8	3.1	4.7

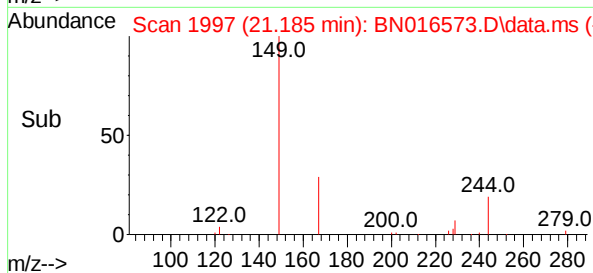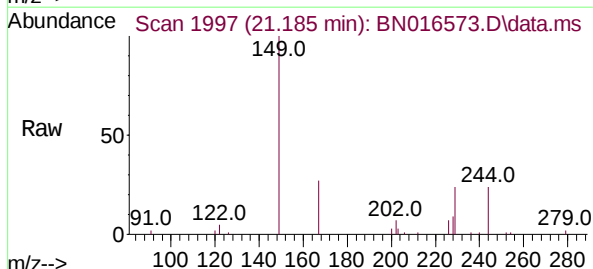


Abundance Scan 2434 (23.509 min): BN016561.D\data.ms (-2434) (-)

Perylene-d12
Concen: 0.400 ng
RT: 23.529 min Scan# 2440
Delta R.T. 0.020 min
Lab File: BN016573.D
Acq: 29 Sep 2021 11:18


Instrument :
BNA_N
ClientSampleId :

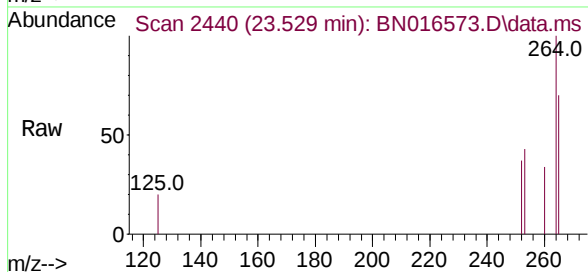

Tgt Ion	Ratio	Lower	Upper
264	100		
260	33.9	19.9	29.9#
265	69.7	20.7	31.1#


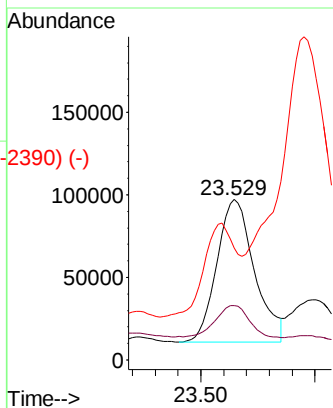


Abundance Scan 2440 (23.529 min): BN016573.D\data.ms (-2390) (-)

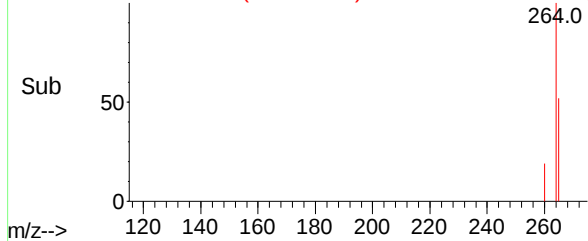


Abundance Scan 3102 (25.795 min): BN016561.D\data.ms (-3102) (-)


Indeno(1,2,3-cd)pyrene
Concen: 2.617 ng
RT: 25.826 min Scan# 3111
Delta R.T. 0.024 min
Lab File: BN016573.D
Acq: 29 Sep 2021 11:18

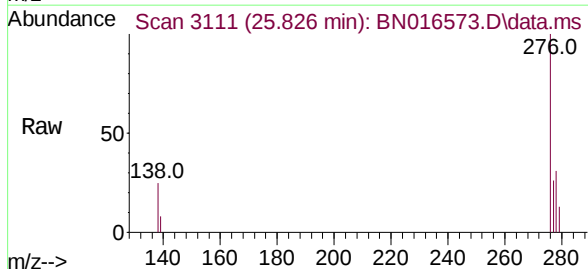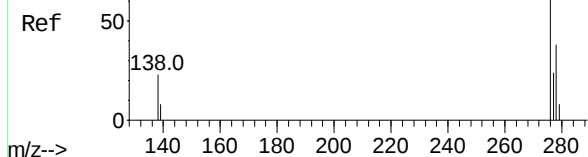


Tgt Ion	Ratio	Lower	Upper
276	100		
138	23.5	18.2	27.2
277	25.0	19.8	29.8



Abundance Scan 3111 (25.826 min): BN016573.D\data.ms (-3075) (-)

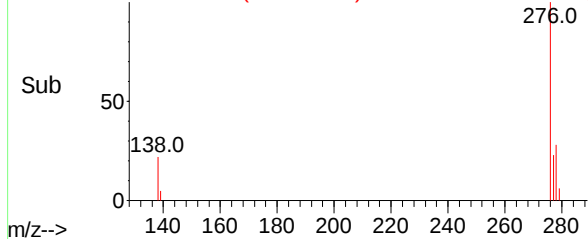



Abundance Scan 2234 (22.824 min): BN016561.D\data.ms (-2177) (-)

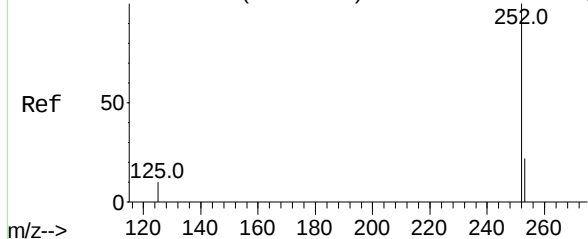


Benzo(b)fluoranthene
Concen: 9.613 ng
RT: 22.851 min Scan# 2242
Delta R.T. 0.024 min
Lab File: BN016573.D
Acq: 29 Sep 2021 11:18

Instrument :
BNA_N
ClientSampleId :


Tgt Ion:252 Resp: 6310582
Ion Ratio Lower Upper
252 100
253 24.2 17.8 26.6
125 11.9 7.3 10.9#

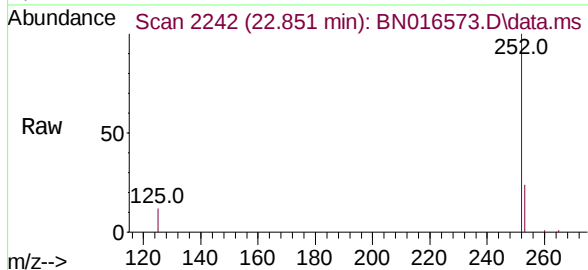

Abundance Scan 2242 (22.851 min): BN016573.D\data.ms (-2177) (-)


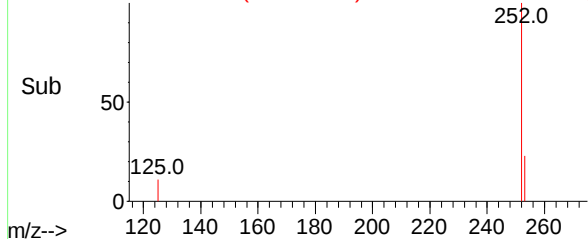


Abundance Scan 2404 (23.406 min): BN016561.D\data.ms (-2347) (-)

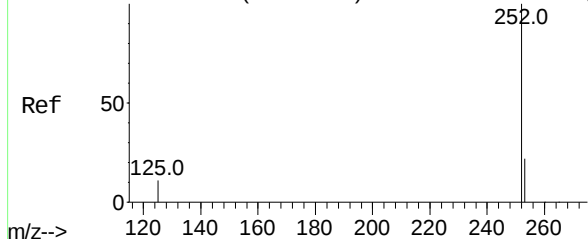


Benzo(a)pyrene
Concen: 5.868 ng
RT: 23.433 min Scan# 2412
Delta R.T. 0.024 min
Lab File: BN016573.D
Acq: 29 Sep 2021 11:18

Tgt Ion:252 Resp: 3533430
Ion Ratio Lower Upper
252 100
253 25.7 17.9 26.9
125 12.6 8.2 12.4#

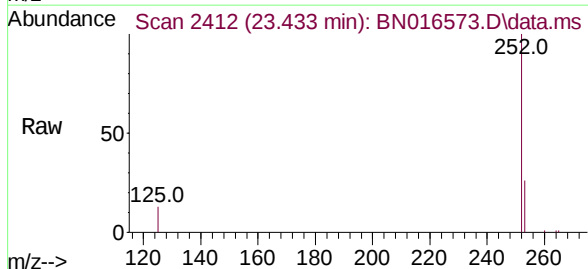


Abundance Scan 2412 (23.433 min): BN016573.D\data.ms (-2347) (-)

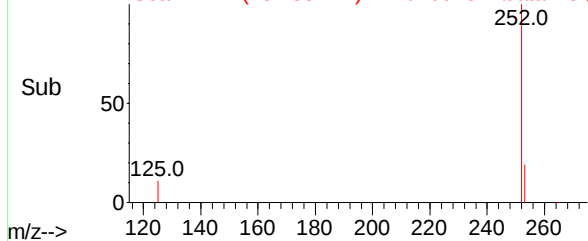




Abundance Scan 3109 (25.819 min): BN016561.D\data.ms (-3049) (-)

Dibenzo(a,h)anthracene
Concen: 1.368 ng
RT: 25.829 min Scan# 3112
Delta R.T. 0.007 min
Lab File: BN016573.D
Acq: 29 Sep 2021 11:18

Instrument :
BNA_N
ClientSampleId :

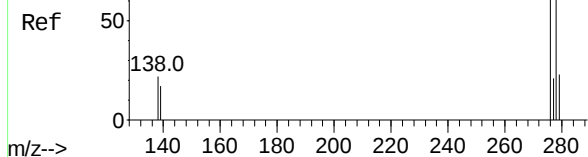


Tgt Ion	Ratio	Lower	Upper
278	100		
139	24.3	12.1	18.1#
279	40.6	19.2	28.8#

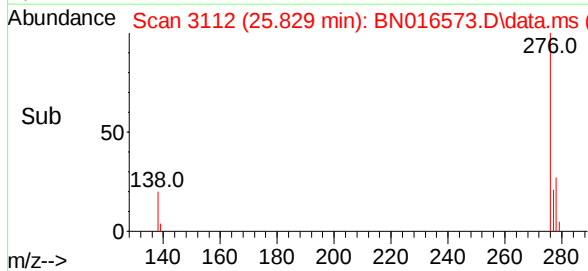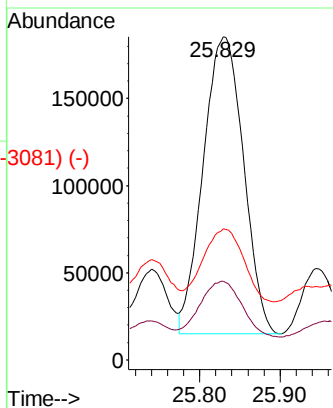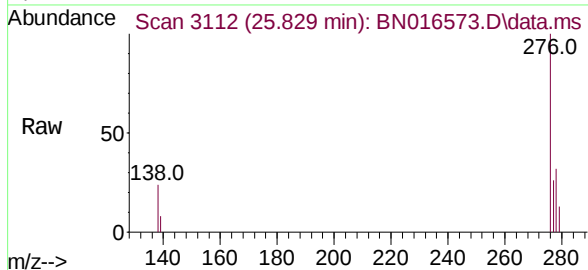

Abundance Scan 3306 (26.493 min): BN016561.D\data.ms (-3249) (-)

Benzo(g,h,i)perylene
Concen: 2.825 ng
RT: 26.531 min Scan# 3317
Delta R.T. 0.034 min
Lab File: BN016573.D
Acq: 29 Sep 2021 11:18

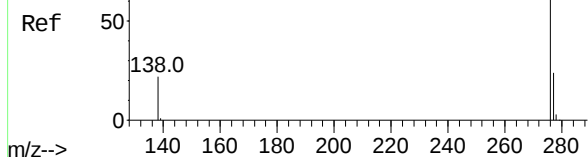

Tgt Ion	Ratio	Lower	Upper
276	100		
277	25.4	18.9	28.3
138	23.8	15.7	23.5#

