
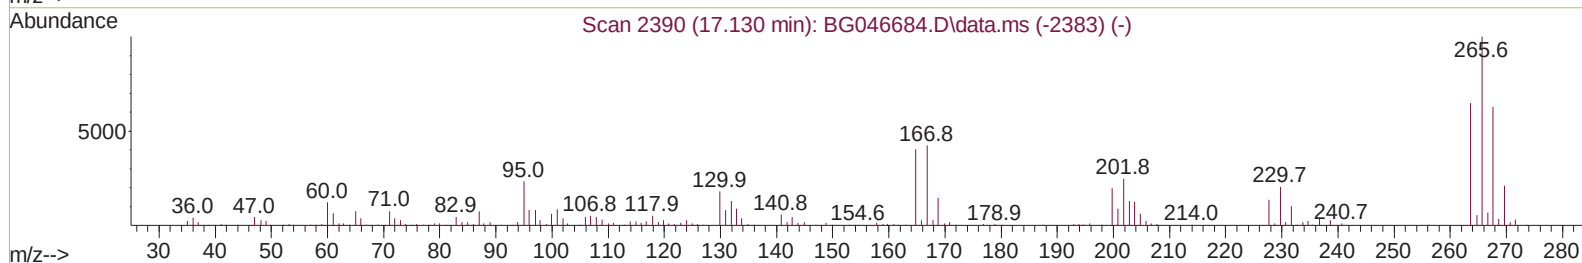
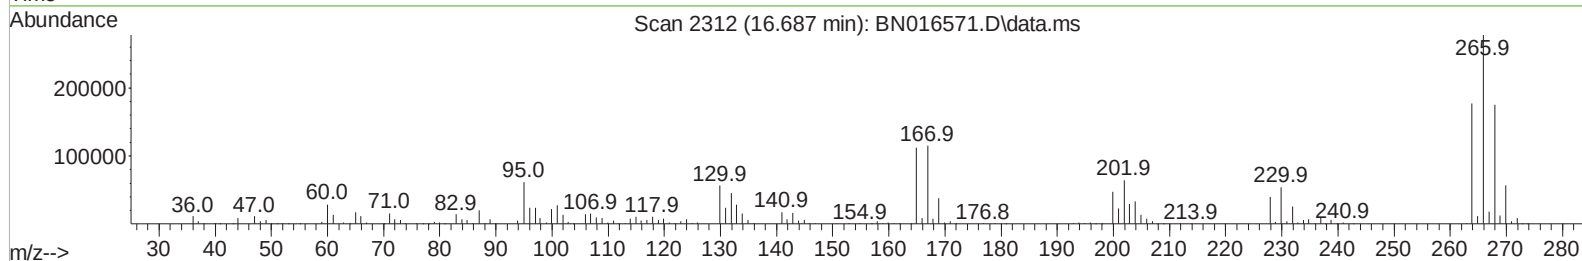


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092921\
Data File : BN016570.D
Acq On : 29 Sep 2021 09:14
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 29 10:50:14 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 28 17:48:03 2021
Response via : Initial Calibration

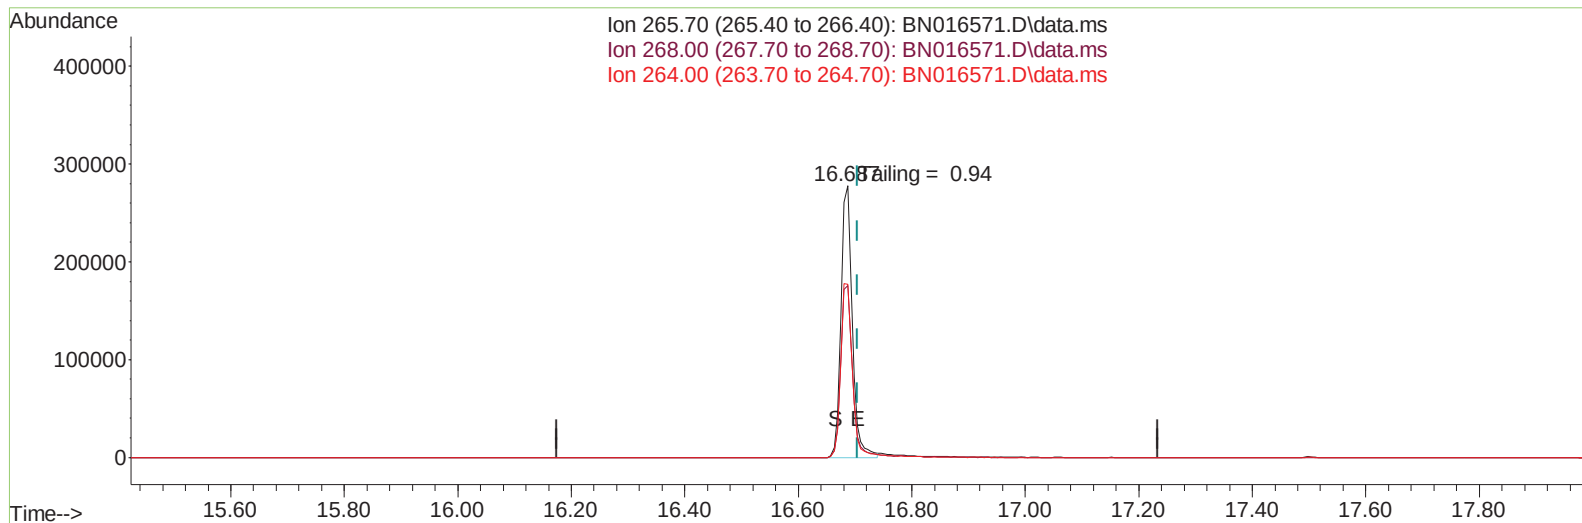

TIC: BN016571.D\data.ms

(70) Pentachlorophenol (C)




16.687min (-0.017) 24924.62 ng

response 395312

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.25
264.00	61.60	63.85
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092921\
 Data File : BN016570.D
 Acq On : 29 Sep 2021 09:14
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 29 10:50:14 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 28 17:48:03 2021
 Response via : Initial Calibration

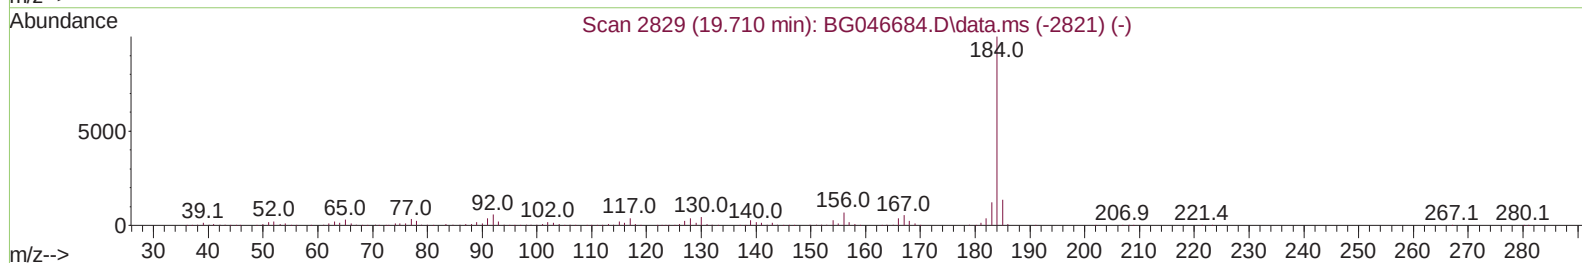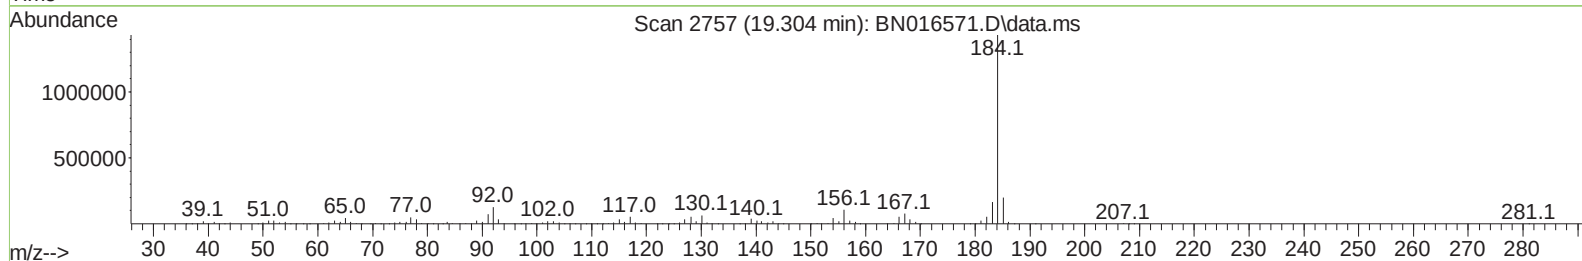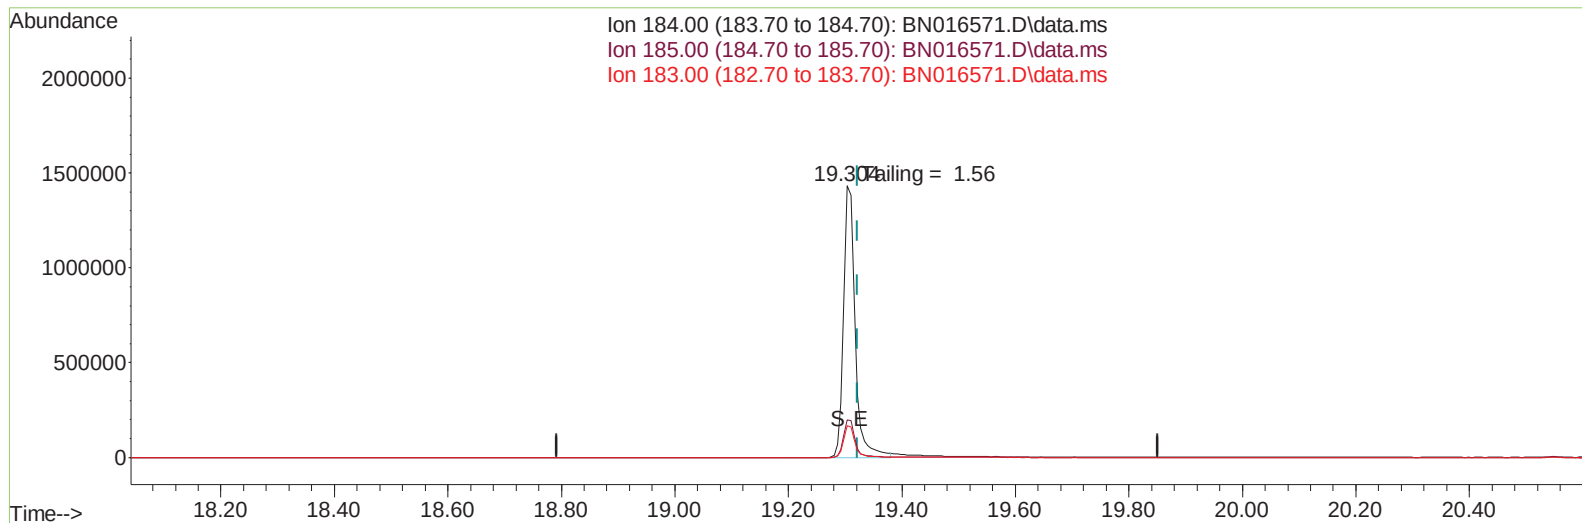

TIC: BN016571.D\data.ms

(77) Benzidine**19.304min (-0.017) 0.00 ng****response 2114271**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.79
183.00	13.20	11.62
0.00	0.00	0.00