
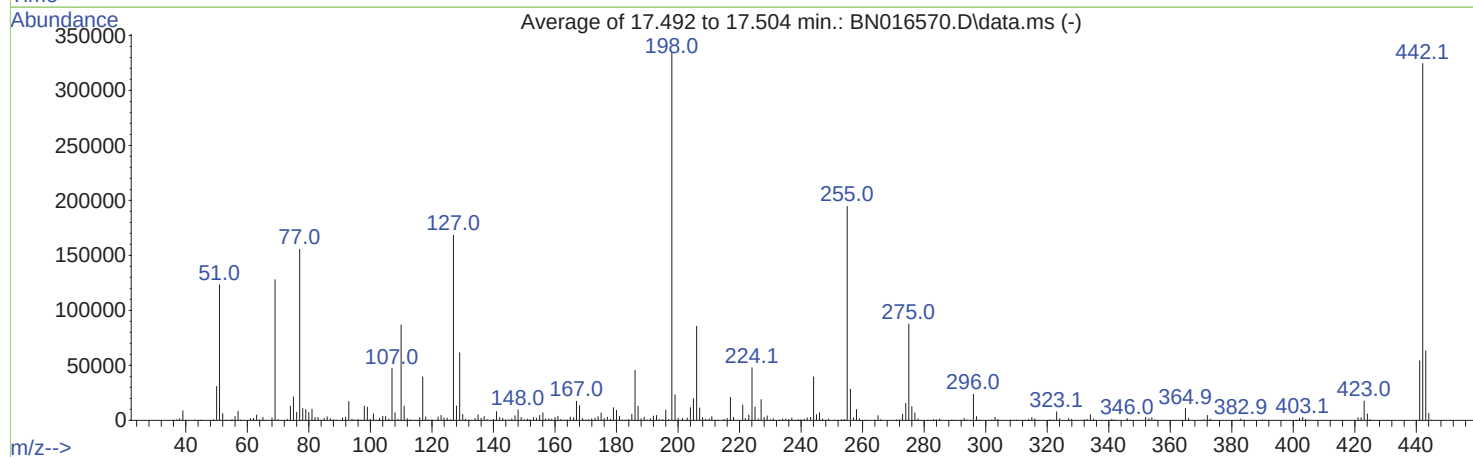


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092921\
 Data File : BN016570.D
 Acq On : 29 Sep 2021 09:14
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN092821.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Sep 29 10:56:17 2021

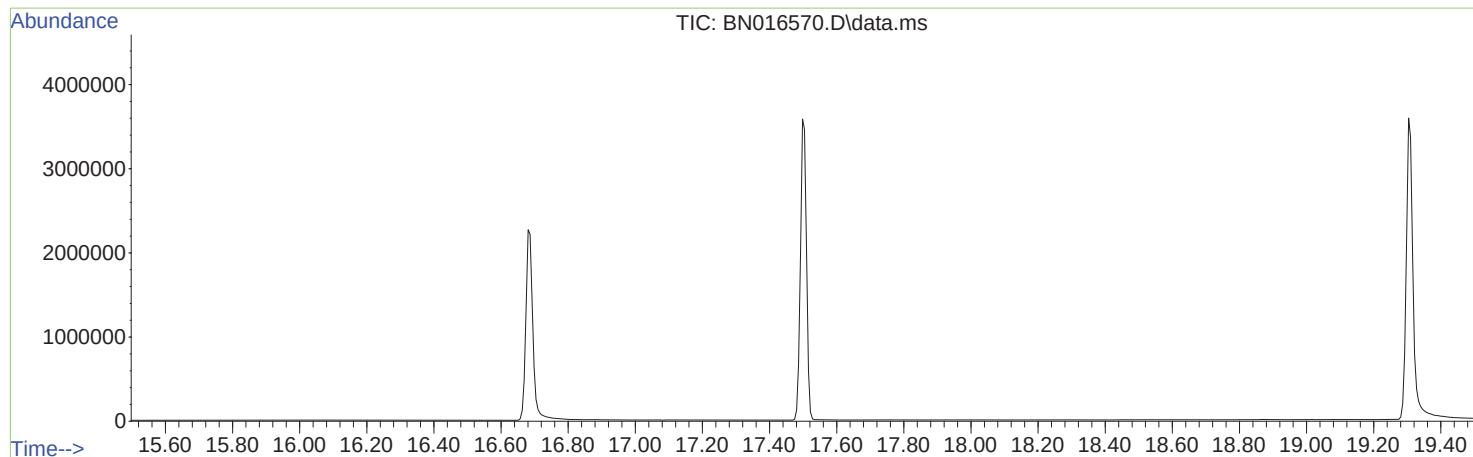




AutoFind: Scans 2449, 2450, 2451; Background Corrected with Scan 2443

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	36.8	123221	PASS
68	69	0.00	2	1.8	2267	PASS
69	198	0.00	100	38.2	127816	PASS
70	69	0.00	2	0.6	806	PASS
127	198	10	80	50.4	168525	PASS
197	198	0.00	2	0.3	918	PASS
198	198	100	100	100.0	334464	PASS
199	198	5	9	7.0	23339	PASS
275	198	10	60	26.2	87603	PASS
365	198	1	100	3.3	10879	PASS
441	198	0.01	100	16.2	54229	PASS
442	442	50	100	100.0	324437	PASS
443	442	15	24	19.5	63203	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092921\
Data File : BN016570.D
Acq On : 29 Sep 2021 09:14
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 29 10:50:14 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 28 17:48:03 2021
Response via : Initial Calibration

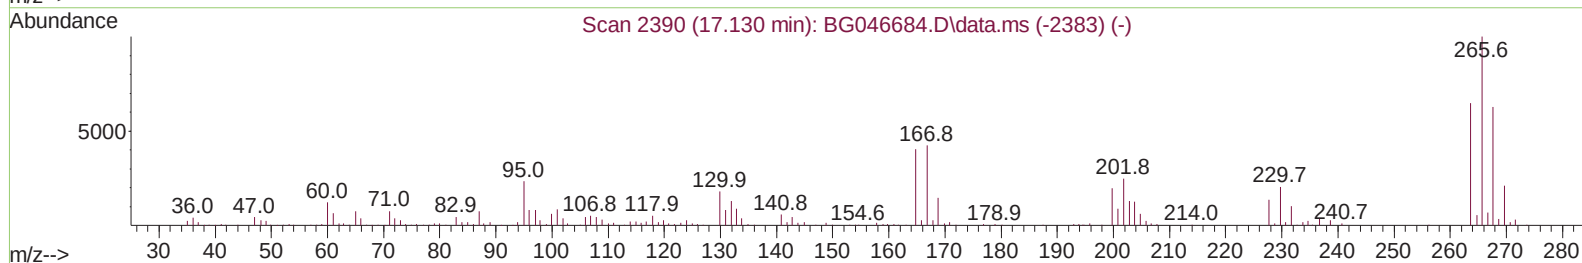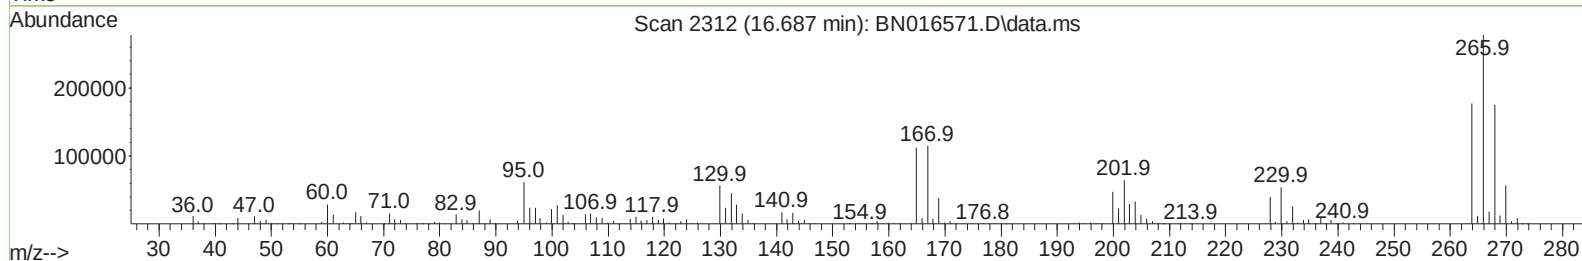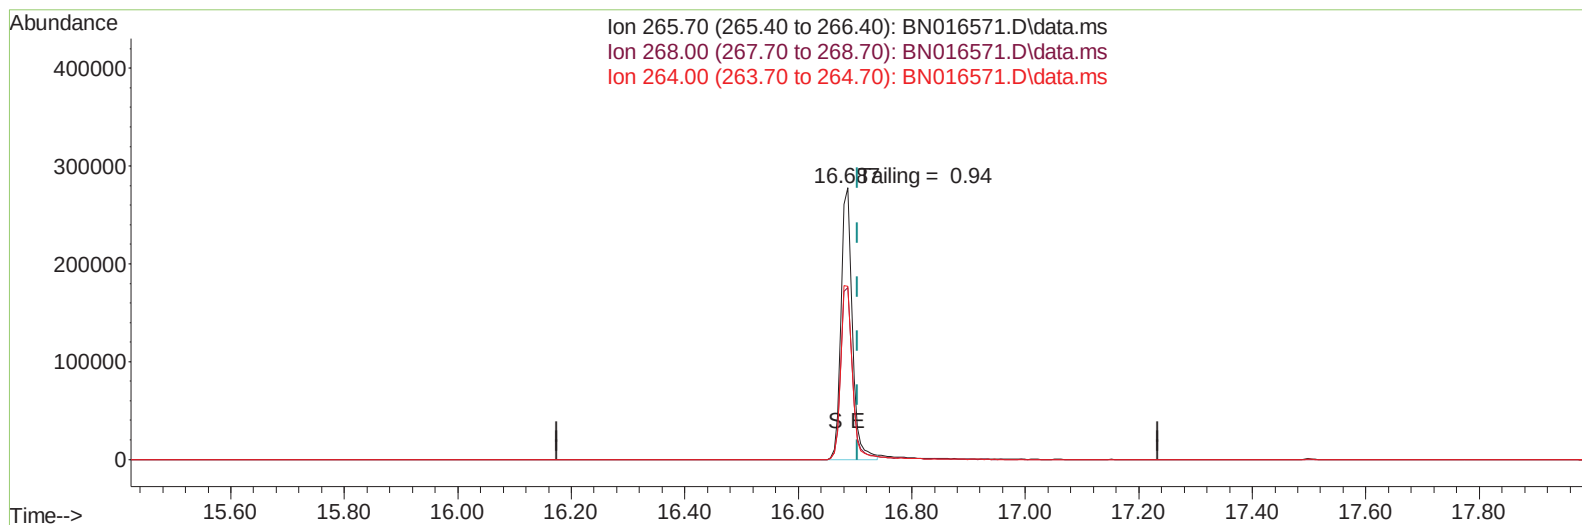

TIC: BN016571.D\data.ms

(70) Pentachlorophenol (C)

16.687min (-0.017) 24924.62 ng




response 395312

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.25
264.00	61.60	63.85
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092921\
Data File : BN016570.D
Acq On : 29 Sep 2021 09:14
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 29 10:50:14 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 28 17:48:03 2021
Response via : Initial Calibration

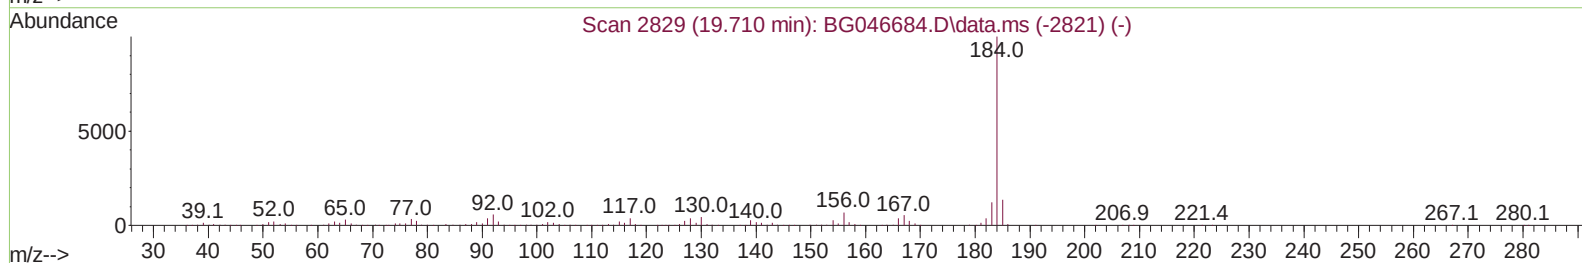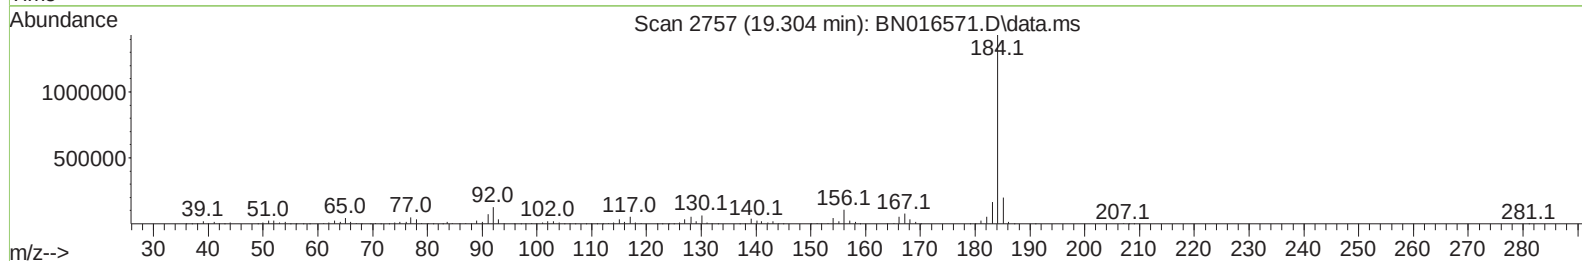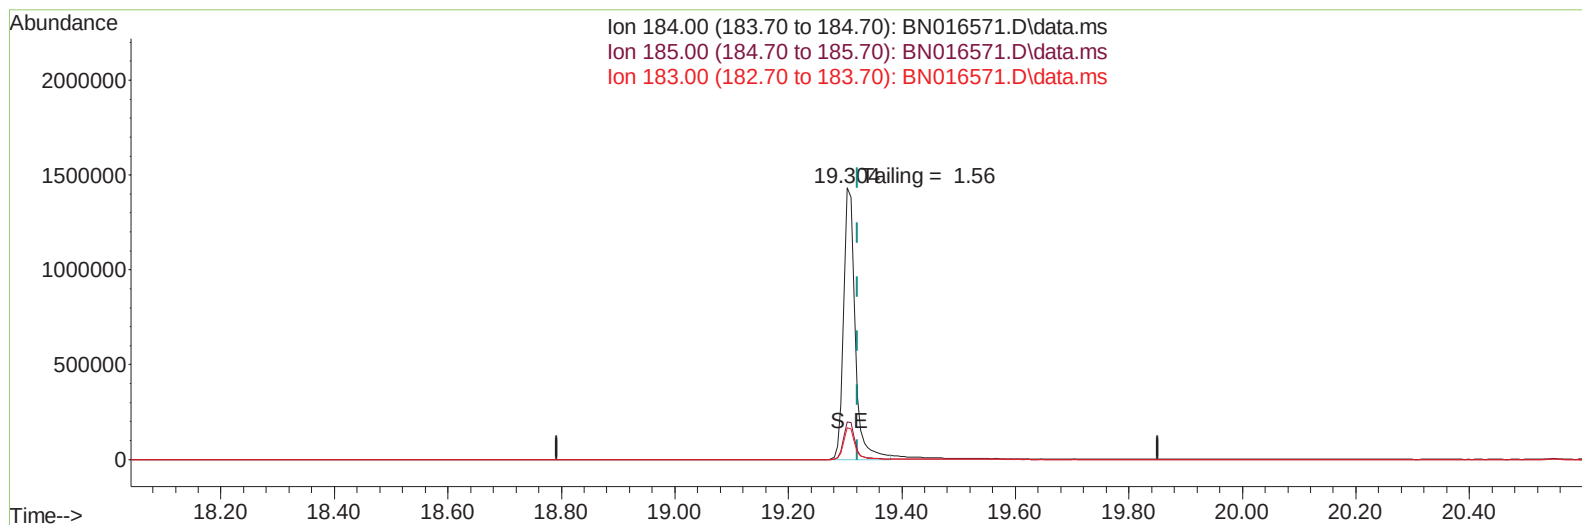

TIC: BN016571.D\data.ms

(77) Benzidine

19.304min (-0.017) 0.00 ng

response 2114271

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.79
183.00	13.20	11.62
0.00	0.00	0.00

DDT Breakdown

Instrument :
BNA_N
ClientSampleId :
DFTPP

Date	Instrument Name	DFTPP Data File
9/29/2021	BNA_N	BN016570.D
Compound Name	Response	Retention Time
DDT	946005	20.551
DDD	3554	20.1
DDE	190	19.592
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3744	949749	0.39