

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092922\
 Data File : BN021948.D
 Acq On : 28 Sep 2022 19:36
 Operator : CG/JU
 Sample : SSTDICV0.4
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 ICVBN092922

Quant Time: Sep 30 02:28:18 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN092922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 30 02:27:15 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.033	152	4101	0.400	ng	0.00
7) Naphthalene-d8	10.856	136	12266	0.400	ng	0.00
13) Acenaphthene-d10	14.686	164	6359	0.400	ng	0.00
19) Phenanthrene-d10	17.437	188	12764	0.400	ng	0.00
29) Chrysene-d12	21.628	240	9934	0.400	ng	# 0.00
35) Perylene-d12	24.129	264	8320	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.563	112	4224	0.387	ng	0.00
5) Phenol-d6	7.188	99	5259	0.381	ng	0.00
8) Nitrobenzene-d5	9.211	82	3880	0.379	ng	0.00
11) 2-Methylnaphthalene-d10	12.448	152	10092	0.381	ng	0.00
14) 2,4,6-Tribromophenol	16.184	330	938	0.344	ng	0.00
15) 2-Fluorobiphenyl	13.317	172	11412	0.406	ng	0.00
27) Fluoranthene-d10	19.471	212	13107	0.379	ng	0.00
31) Terphenyl-d14	20.060	244	9269	0.422	ng	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.382	88	2166	0.373	ng	99
3) n-Nitrosodimethylamine	3.721	42	2278	0.388	ng	97
6) bis(2-Chloroethyl)ether	7.448	93	5269	0.392	ng	100
9) Naphthalene	10.909	128	14760	0.400	ng	100
10) Hexachlorobutadiene	11.187	225	2608	0.406	ng	# 100
12) 2-Methylnaphthalene	12.157	142	2490	0.343	ng	99
16) Acenaphthylene	14.408	152	10925	0.370	ng	99
17) Acenaphthene	14.750	154	8364	0.396	ng	99
18) Fluorene	15.737	166	10047	0.379	ng	96
20) 4,6-Dinitro-2-methylph...	15.824	198	453	0.274	ng	# 34
21) 4-Bromophenyl-phenylether	16.618	248	3150	0.391	ng	99
22) Hexachlorobenzene	16.742	284	3787	0.405	ng	100
23) Atrazine	16.891	200	2372	0.359	ng	99
24) Pentachlorophenol	17.090	266	1048	0.323	ng	98
25) Phenanthrene	17.475	178	17241	0.395	ng	100
26) Anthracene	17.574	178	13250	0.371	ng	99
28) Fluoranthene	19.501	202	17765	0.379	ng	100
30) Pyrene	19.863	202	17981	0.392	ng	98
32) Benzo(a)anthracene	21.610	228	14894	0.387	ng	98
33) Chrysene	21.663	228	16101	0.400	ng	99
34) Bis(2-ethylhexyl)phtha...	21.520	149	8230	0.356	ng	100
36) Indeno(1,2,3-cd)pyrene	26.754	276	17211	0.391	ng	99
37) Benzo(b)fluoranthene	23.357	252	15122	0.391	ng	99
38) Benzo(k)fluoranthene	23.407	252	14781	0.391	ng	99
39) Benzo(a)pyrene	24.015	252	11499	0.389	ng	99
40) Dibenzo(a,h)anthracene	26.775	278	13944	0.397	ng	99
41) Benzo(g,h,i)perylene	27.567	276	14467	0.377	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092922\
 Data File : BN021948.D
 Acq On : 28 Sep 2022 19:36
 Operator : CG/JU
 Sample : SSTDICV0.4
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 ICVBN092922

Quant Time: Sep 30 02:28:18 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN092922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 30 02:27:15 2022
 Response via : Initial Calibration




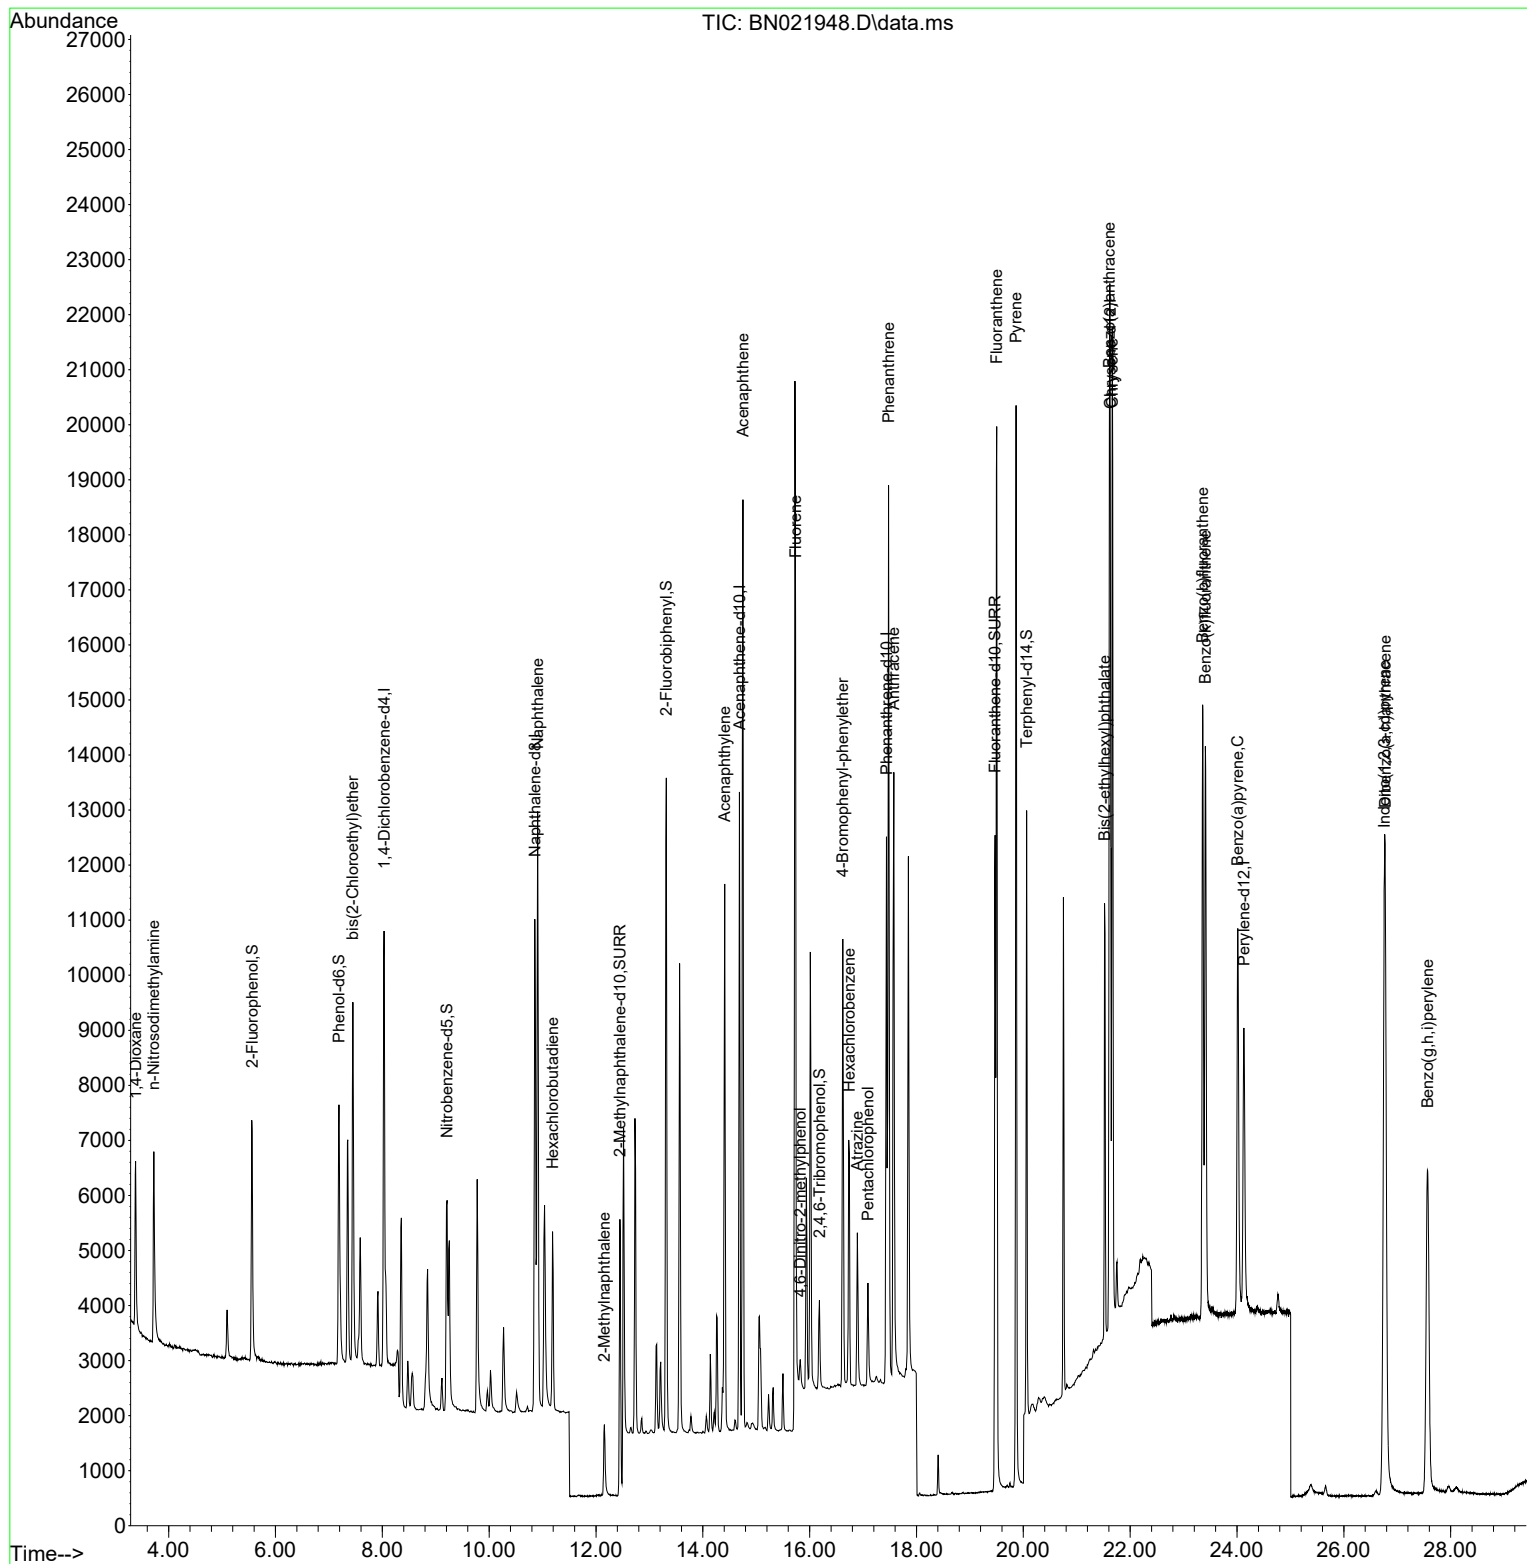




#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 8.033 min Scan# 61
 Delta R.T. -0.000 min
 Lab File: BN021948.D
 Acq: 28 Sep 2022 19:36




Instrument :
 BNA_N
 ClientSampleId :
 ICVBN092922


Tgt Ion:152 Resp: 4101
 Ion Ratio Lower Upper
 152 100
 150 152.2 120.2 180.4
 115 62.4 49.4 74.2

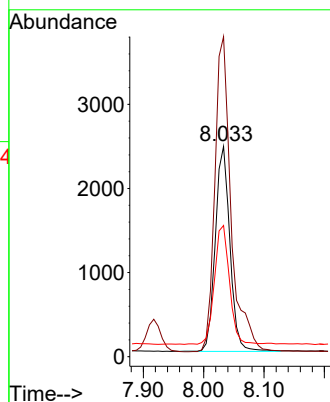

#2
 1,4-Dioxane
 Concen: 0.373 ng
 RT: 3.382 min Scan# 14
 Delta R.T. 0.000 min
 Lab File: BN021948.D
 Acq: 28 Sep 2022 19:36

Tgt Ion: 88 Resp: 2166
 Ion Ratio Lower Upper
 88 100
 43 28.4 23.8 35.6
 58 74.9 59.8 89.8


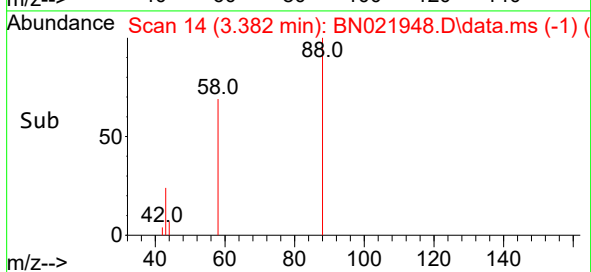
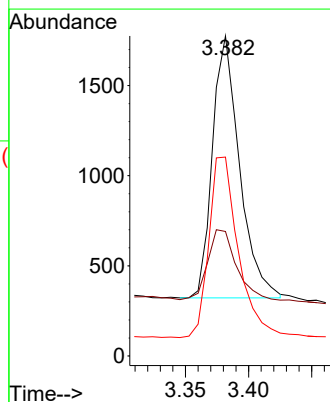





#3
n-Nitrosodimethylamine
Concen: 0.388 ng
RT: 3.721 min Scan# 61
Delta R.T. 0.000 min
Lab File: BN021948.D
Acq: 28 Sep 2022 19:36




Instrument :
BNA_N
ClientSampleId :
ICVBN092922


Tgt Ion: 42 Resp: 2278
Ion Ratio Lower Upper
42 100
74 134.6 105.0 157.4
44 9.3 9.0 13.4

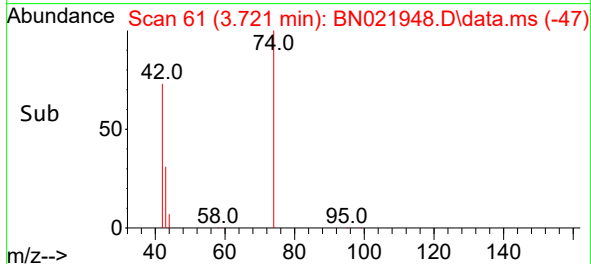

#4
2-Fluorophenol
Concen: 0.387 ng
RT: 5.563 min Scan# 316
Delta R.T. 0.007 min
Lab File: BN021948.D
Acq: 28 Sep 2022 19:36

Tgt Ion: 112 Resp: 4224
Ion Ratio Lower Upper
112 100
64 57.5 45.9 68.9
63 30.4 24.0 36.0


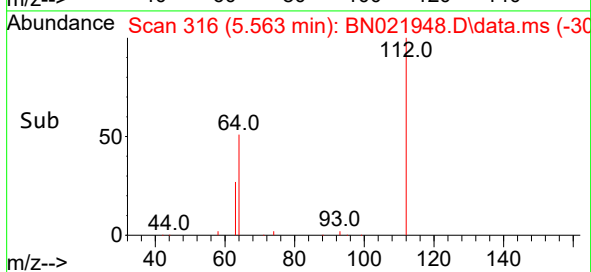






#5
Phenol-d6
Concen: 0.381 ng
RT: 7.188 min Scan# 541
Delta R.T. 0.000 min
Lab File: BN021948.D
Acq: 28 Sep 2022 19:36




Instrument :
BNA_N
ClientSampleId :
ICVBN092922


Tgt Ion:	99	Resp:	5259
Ion	Ratio	Lower	Upper
99	100		
42	19.5	15.9	23.9
71	32.1	25.9	38.9

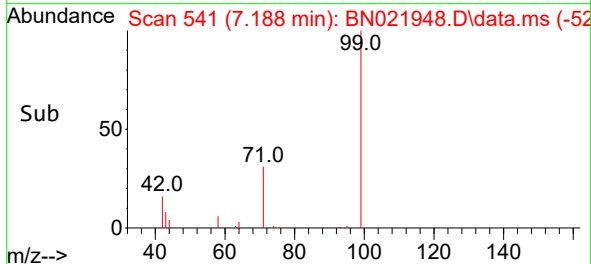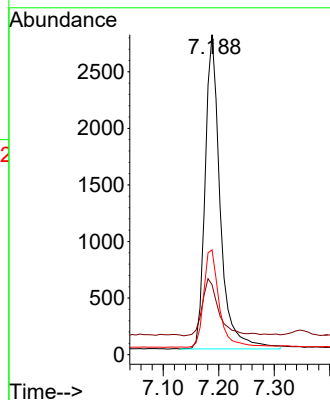

#6
bis(2-Chloroethyl)ether
Concen: 0.392 ng
RT: 7.448 min Scan# 577
Delta R.T. 0.000 min
Lab File: BN021948.D
Acq: 28 Sep 2022 19:36

Tgt Ion:	93	Resp:	5269
Ion	Ratio	Lower	Upper
93	100		
63	77.3	61.6	92.4
95	33.0	26.6	40.0



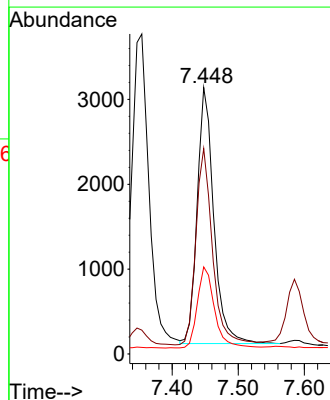





#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.856 min Scan# 91
Delta R.T. 0.000 min
Lab File: BN021948.D
Acq: 28 Sep 2022 19:36




Instrument :
BNA_N
ClientSampleId :
ICVBN092922


Tgt Ion:	136	Resp:	12266
Ion	Ratio	Lower	Upper
136	100		
137	11.5	9.4	14.2
54	9.6	7.8	11.8
68	8.1	6.9	10.3

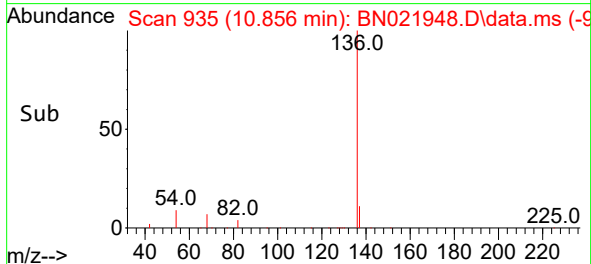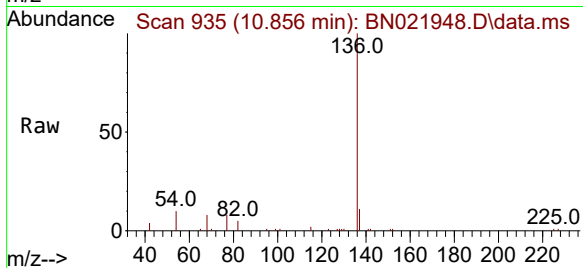

#8
Nitrobenzene-d5
Concen: 0.379 ng
RT: 9.211 min Scan# 781
Delta R.T. 0.000 min
Lab File: BN021948.D
Acq: 28 Sep 2022 19:36

Tgt Ion:	82	Resp:	3880
Ion	Ratio	Lower	Upper
82	100		
128	45.4	37.7	56.5
54	47.2	37.1	55.7

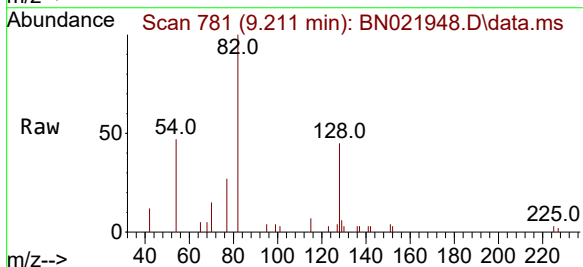



#9

Naphthalene

Concen: 0.400 ng

RT: 10.909 min Scan# 940

Delta R.T. 0.000 min

Lab File: BN021948.D

Acq: 28 Sep 2022 19:36

Instrument :

BNA_N

ClientSampleId :

ICVBN092922





Tgt Ion:128 Resp: 14760

Ion Ratio Lower Upper

128 100

129 11.6 9.4 14.0

127 13.3 10.6 16.0

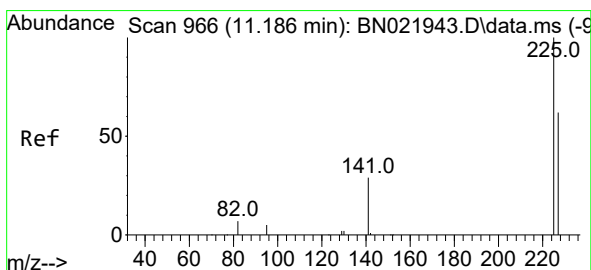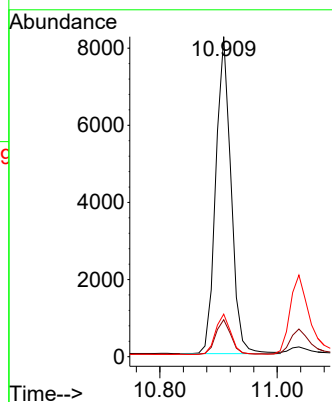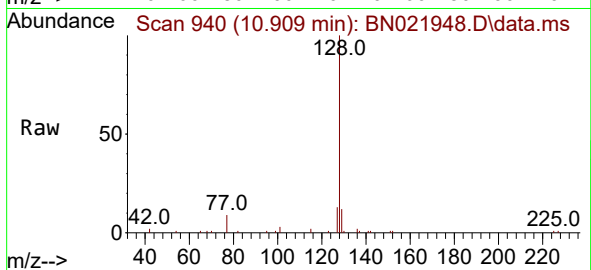

#10

Hexachlorobutadiene

Concen: 0.406 ng

RT: 11.187 min Scan# 966

Delta R.T. 0.000 min

Lab File: BN021948.D

Acq: 28 Sep 2022 19:36




Tgt Ion:225 Resp: 2608


Ion Ratio Lower Upper

225 100

223 0.0 0.0 0.0

227 63.3 50.5 75.7


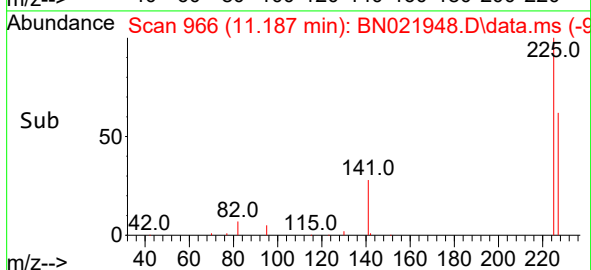

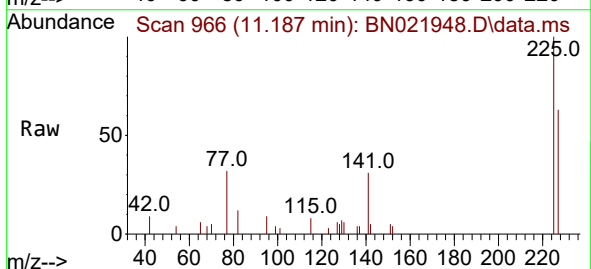




#11
2-Methylnaphthalene-d10
Concen: 0.381 ng
RT: 12.448 min Scan# 11
Delta R.T. 0.000 min
Lab File: BN021948.D
Acq: 28 Sep 2022 19:36




Instrument :
BNA_N
ClientSampleId :
ICVBN092922


Tgt Ion:152 Resp: 10092
Ion Ratio Lower Upper
152 100
151 21.6 15.7 23.5

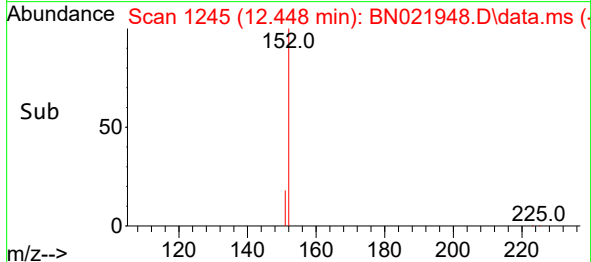

#12
2-Methylnaphthalene
Concen: 0.343 ng
RT: 12.157 min Scan# 1168
Delta R.T. 0.000 min
Lab File: BN021948.D
Acq: 28 Sep 2022 19:36

Tgt Ion:142 Resp: 2490
Ion Ratio Lower Upper
142 100
141 15.5 12.7 19.1
115 11.9 9.6 14.4


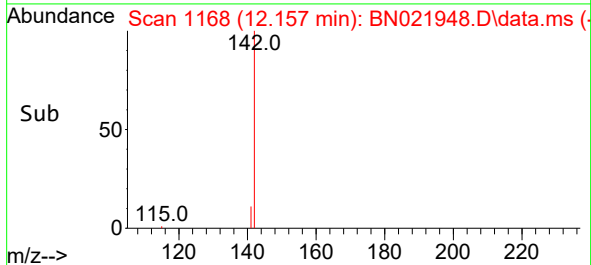






#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.686 min Scan# 1464
Delta R.T. 0.000 min
Lab File: BN021948.D
Acq: 28 Sep 2022 19:36




Instrument :
BNA_N
ClientSampleId :
ICVBN092922


Tgt Ion:164 Resp: 6359
Ion Ratio Lower Upper
164 100
162 104.4 82.8 124.2
160 50.3 39.5 59.3

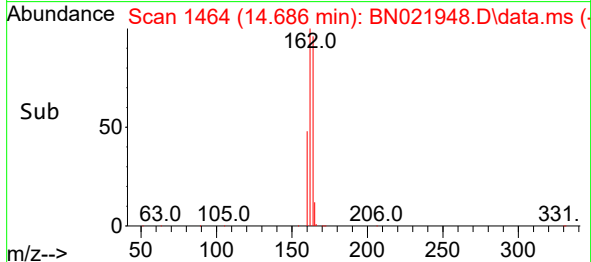

#14
2,4,6-Tribromophenol
Concen: 0.344 ng
RT: 16.184 min Scan# 1598
Delta R.T. 0.000 min
Lab File: BN021948.D
Acq: 28 Sep 2022 19:36

Tgt Ion:330 Resp: 938
Ion Ratio Lower Upper
330 100
332 96.1 78.7 118.1
141 45.0 35.0 52.4




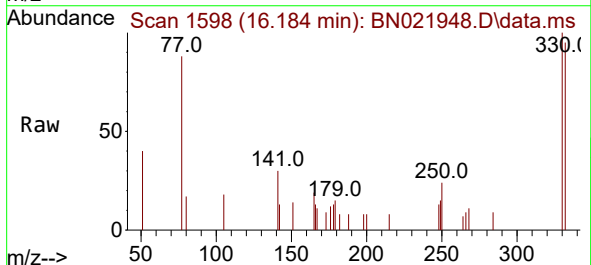




#15
2-Fluorobiphenyl
Concen: 0.406 ng
RT: 13.317 min Scan# 11
Delta R.T. 0.000 min
Lab File: BN021948.D
Acq: 28 Sep 2022 19:36




Instrument :
BNA_N
ClientSampleId :
ICVBN092922


Tgt Ion:172 Resp: 11412
Ion Ratio Lower Upper
172 100
171 34.1 27.4 41.2
170 23.0 18.6 28.0

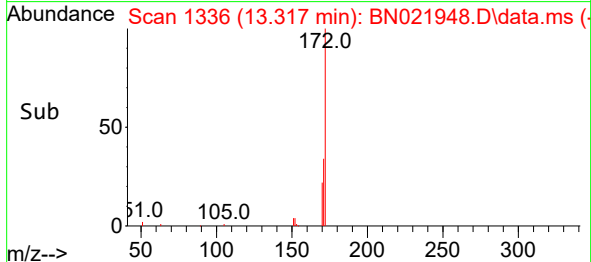

#16
Acenaphthylene
Concen: 0.370 ng
RT: 14.408 min Scan# 1438
Delta R.T. 0.000 min
Lab File: BN021948.D
Acq: 28 Sep 2022 19:36

Tgt Ion:152 Resp: 10925
Ion Ratio Lower Upper
152 100
151 19.1 15.5 23.3
153 13.1 10.6 15.8




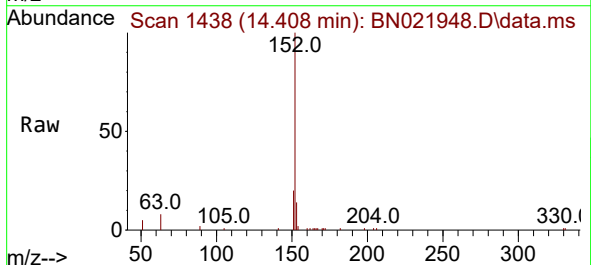




#17
Acenaphthene
Concen: 0.396 ng
RT: 14.750 min Scan# 1470
Delta R.T. 0.000 min
Lab File: BN021948.D
Acq: 28 Sep 2022 19:36




Instrument :
BNA_N
ClientSampleId :
ICVBN092922


Tgt Ion:154 Resp: 8364
Ion Ratio Lower Upper
154 100
153 115.3 91.5 137.3
152 58.2 45.9 68.9

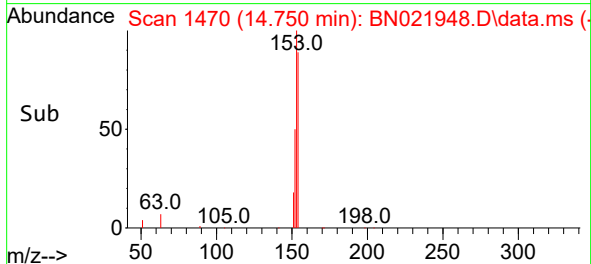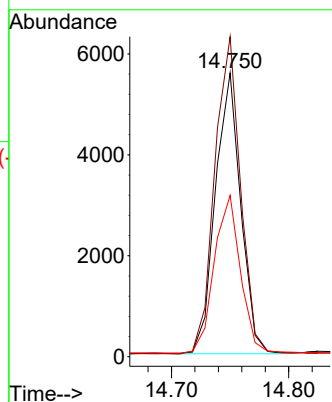

#18
Fluorene
Concen: 0.379 ng
RT: 15.737 min Scan# 1562
Delta R.T. 0.012 min
Lab File: BN021948.D
Acq: 28 Sep 2022 19:36

Tgt Ion:166 Resp: 10047
Ion Ratio Lower Upper
166 100
165 102.2 78.9 118.3
167 14.1 10.3 15.5



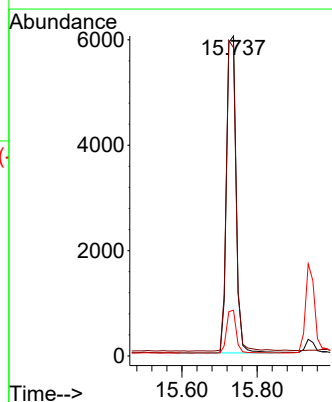





#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.437 min Scan# 1699
Delta R.T. 0.000 min
Lab File: BN021948.D
Acq: 28 Sep 2022 19:36




Instrument :
BNA_N
ClientSampleId :
ICVBN092922


Tgt Ion:188 Resp: 12764
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 12.1 9.4 14.2

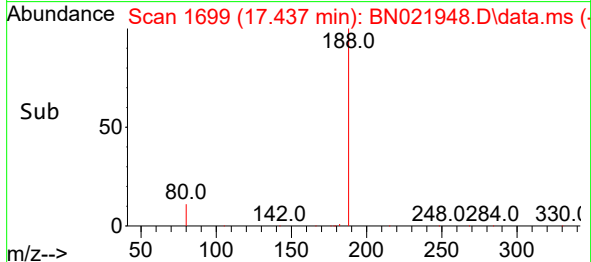

#20
4,6-Dinitro-2-methylphenol
Concen: 0.274 ng
RT: 15.824 min Scan# 1569
Delta R.T. 0.000 min
Lab File: BN021948.D
Acq: 28 Sep 2022 19:36

Tgt Ion:198 Resp: 453
Ion Ratio Lower Upper
198 100
51 137.9 235.8 353.6#
105 82.4 61.2 91.8




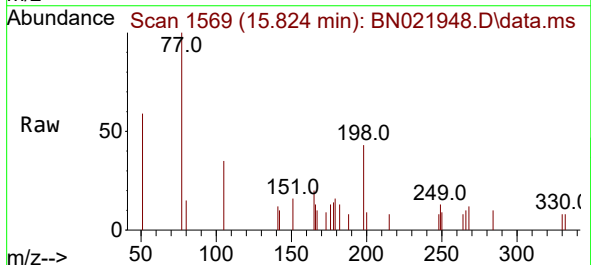




#21
4-Bromophenyl-phenylether
Concen: 0.391 ng
RT: 16.618 min Scan# 1633
Delta R.T. 0.000 min
Lab File: BN021948.D
Acq: 28 Sep 2022 19:36




Instrument :
BNA_N
ClientSampleId :
ICVBN092922


Tgt Ion:248 Resp: 3150
Ion Ratio Lower Upper
248 100
250 91.6 72.9 109.3
141 100.4 79.0 118.6

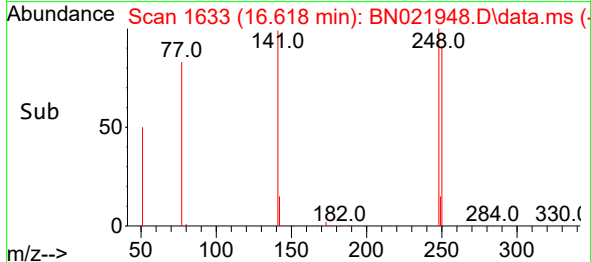

#22
Hexachlorobenzene
Concen: 0.405 ng
RT: 16.742 min Scan# 1643
Delta R.T. 0.000 min
Lab File: BN021948.D
Acq: 28 Sep 2022 19:36

Tgt Ion:284 Resp: 3787
Ion Ratio Lower Upper
284 100
142 40.4 32.6 49.0
249 32.1 25.6 38.4

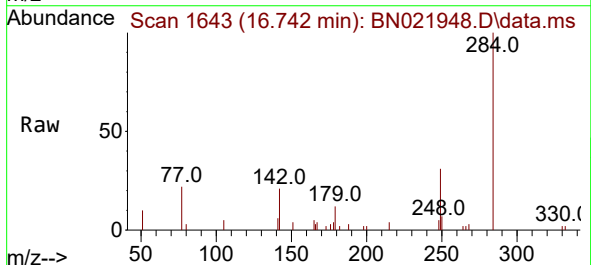

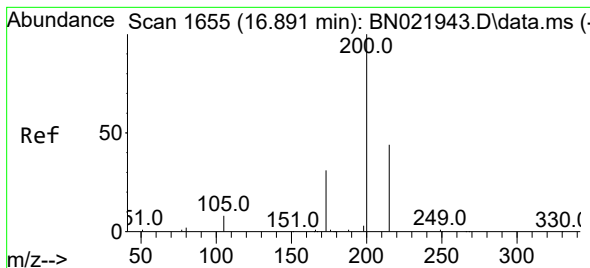

#23

Atrazine

Concen: 0.359 ng

RT: 16.891 min Scan# 1655

Delta R.T. 0.000 min

Lab File: BN021948.D

Acq: 28 Sep 2022 19:36

Instrument :

BNA_N

ClientSampleId :

ICVBN092922





Tgt Ion:200 Resp: 2372

Ion Ratio Lower Upper

200 100

173 33.2 27.0 40.6

215 46.5 36.8 55.2

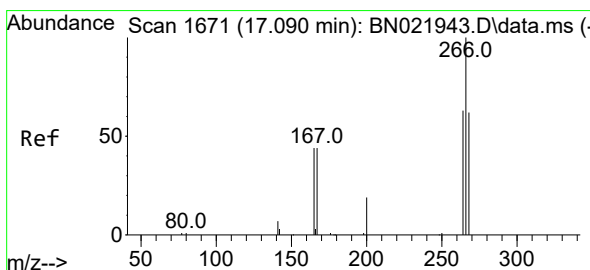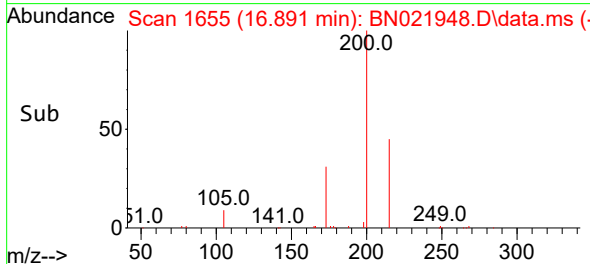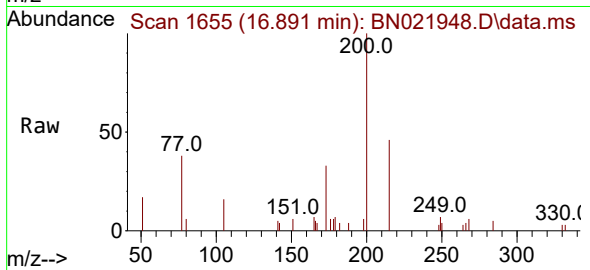

#24

Pentachlorophenol

Concen: 0.323 ng

RT: 17.090 min Scan# 1671

Delta R.T. 0.000 min

Lab File: BN021948.D

Acq: 28 Sep 2022 19:36




Tgt Ion:266 Resp: 1048


Ion Ratio Lower Upper

266 100

264 62.3 49.1 73.7

268 62.5 48.5 72.7

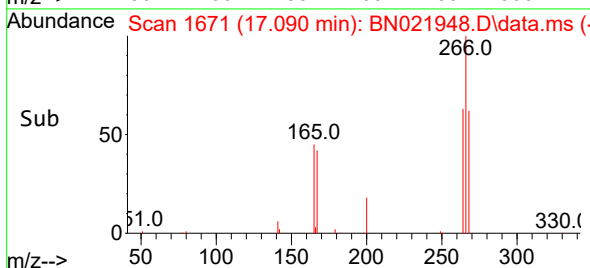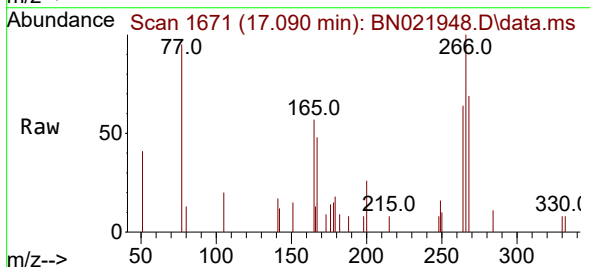



#25

Phenanthrene

Concen: 0.395 ng

RT: 17.475 min Scan# 1702

Delta R.T. 0.000 min

Lab File: BN021948.D

Acq: 28 Sep 2022 19:36

Instrument :

BNA_N

ClientSampleId :

ICVBN092922





Tgt Ion:178 Resp: 17241

Ion Ratio Lower Upper

178 100

176 19.4 15.6 23.4

179 15.4 12.2 18.4

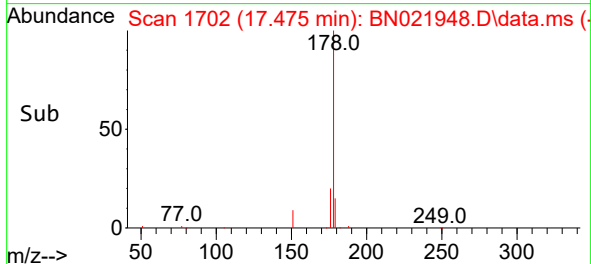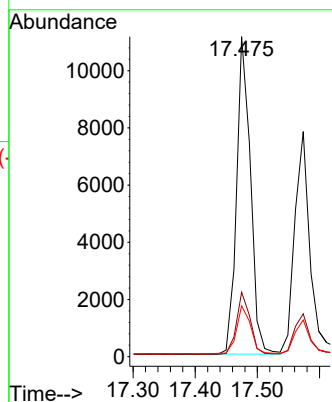

#26

Anthracene

Concen: 0.371 ng

RT: 17.574 min Scan# 1710

Delta R.T. 0.000 min

Lab File: BN021948.D

Acq: 28 Sep 2022 19:36




Tgt Ion:178 Resp: 13250


Ion Ratio Lower Upper

178 100

176 18.6 15.1 22.7

179 15.1 12.2 18.4


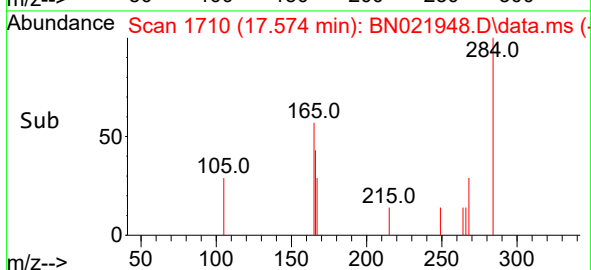






#27
Fluoranthene-d10
Concen: 0.379 ng
RT: 19.471 min Scan# 2092
Delta R.T. 0.000 min
Lab File: BN021948.D
Acq: 28 Sep 2022 19:36




Instrument :
BNA_N
ClientSampleId :
ICVBN092922


Tgt Ion:212 Resp: 13107
Ion Ratio Lower Upper
212 100
106 18.3 14.8 22.2
104 10.4 8.4 12.6

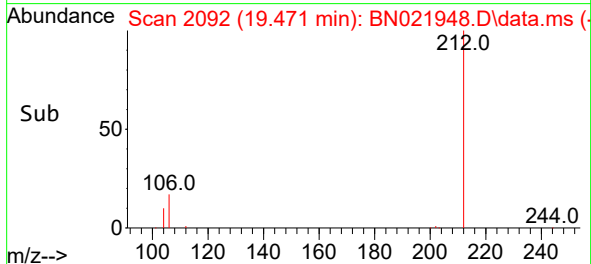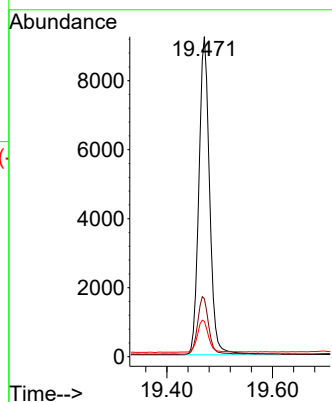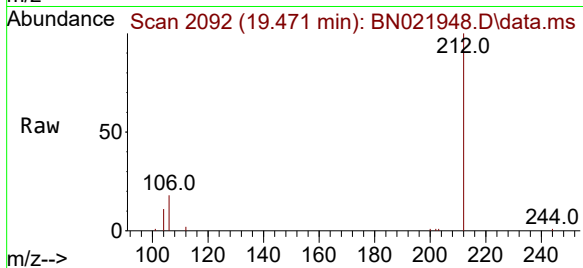

#28
Fluoranthene
Concen: 0.379 ng
RT: 19.501 min Scan# 2099
Delta R.T. 0.000 min
Lab File: BN021948.D
Acq: 28 Sep 2022 19:36

Tgt Ion:202 Resp: 17765
Ion Ratio Lower Upper
202 100
101 14.0 11.2 16.8
203 17.1 13.5 20.3

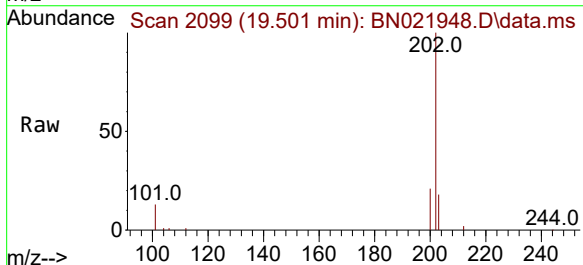

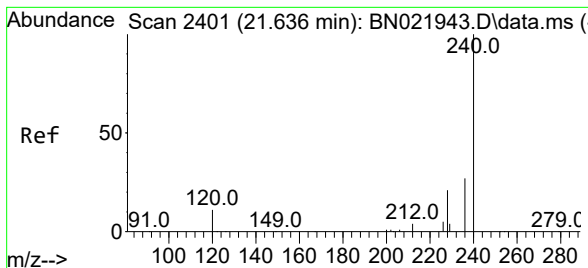

#29

Chrysene-d12

Concen: 0.400 ng

RT: 21.628 min Scan# 2400

Delta R.T. -0.009 min

Lab File: BN021948.D

Acq: 28 Sep 2022 19:36

Instrument :

BNA_N

ClientSampleId :

ICVBN092922





Tgt Ion:240 Resp: 9934

Ion Ratio Lower Upper

240 100

120 19.5 12.2 18.2#

236 29.1 22.6 34.0

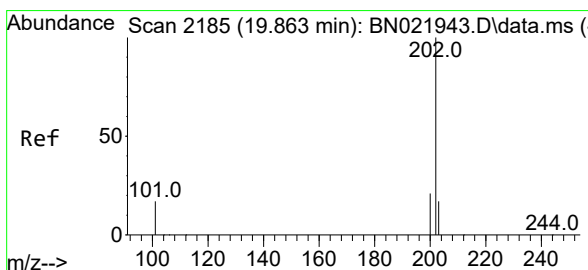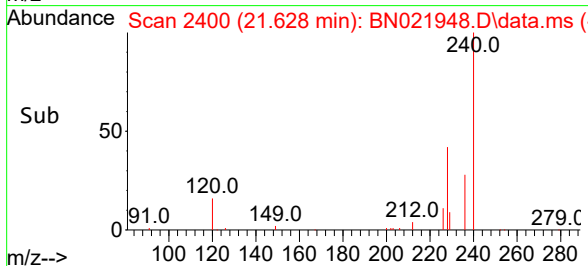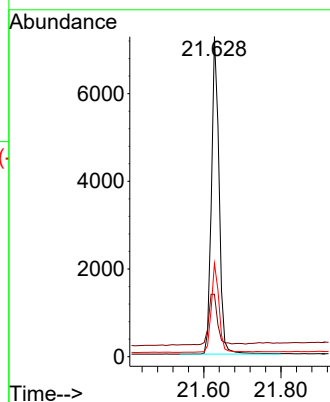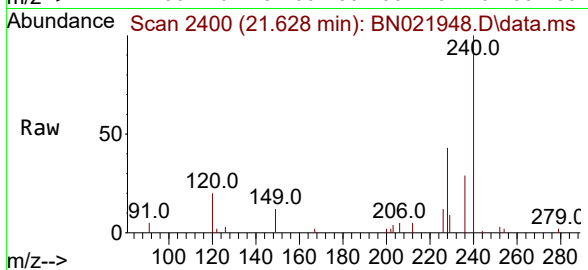

#30

Pyrene

Concen: 0.392 ng

RT: 19.863 min Scan# 2185

Delta R.T. 0.000 min

Lab File: BN021948.D

Acq: 28 Sep 2022 19:36




Tgt Ion:202 Resp: 17981


Ion Ratio Lower Upper

202 100

200 21.1 16.1 24.1

203 17.9 13.8 20.6


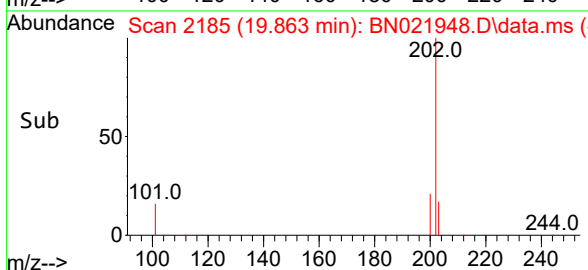
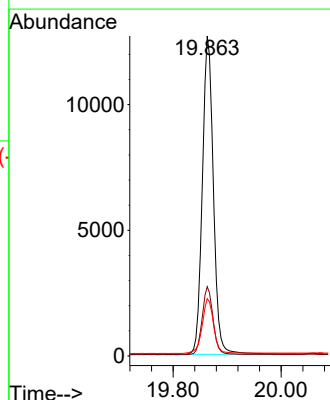
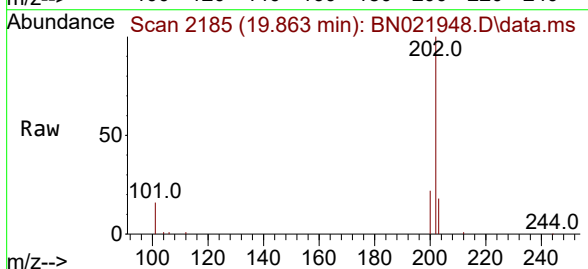




#31
 Terphenyl-d14
 Concen: 0.422 ng
 RT: 20.060 min Scan# 21
 Delta R.T. 0.000 min
 Lab File: BN021948.D
 Acq: 28 Sep 2022 19:36




Instrument :
 BNA_N
 ClientSampleId :
 ICVBN092922


Tgt Ion:244 Resp: 9269
 Ion Ratio Lower Upper
 244 100
 212 9.6 7.9 11.9
 122 17.2 15.3 22.9

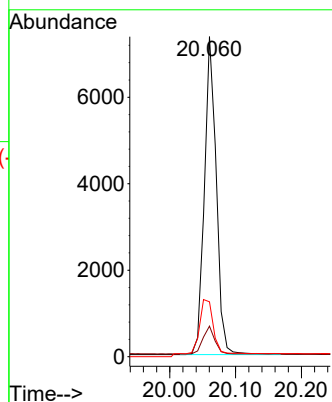

#32
 Benzo(a)anthracene
 Concen: 0.387 ng
 RT: 21.610 min Scan# 2398
 Delta R.T. -0.009 min
 Lab File: BN021948.D
 Acq: 28 Sep 2022 19:36

Tgt Ion:228 Resp: 14894
 Ion Ratio Lower Upper
 228 100
 226 29.0 21.9 32.9
 229 19.7 15.8 23.8

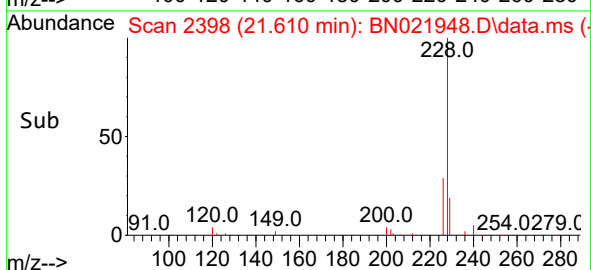

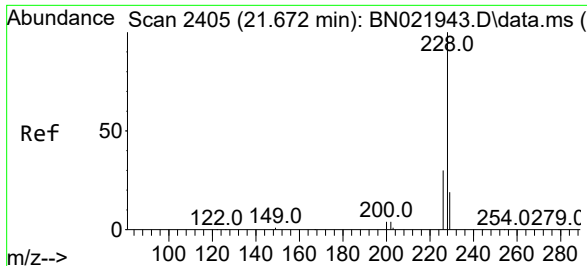

#33

Chrysene

Concen: 0.400 ng

RT: 21.663 min Scan# 2404

Delta R.T. -0.009 min

Lab File: BN021948.D

Acq: 28 Sep 2022 19:36

Instrument :

BNA_N

ClientSampleId :

ICVBN092922





Tgt Ion:228 Resp: 16101

Ion Ratio Lower Upper

228 100

226 31.2 24.6 36.8

229 19.6 15.8 23.8

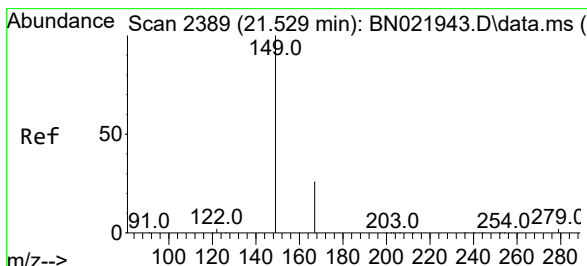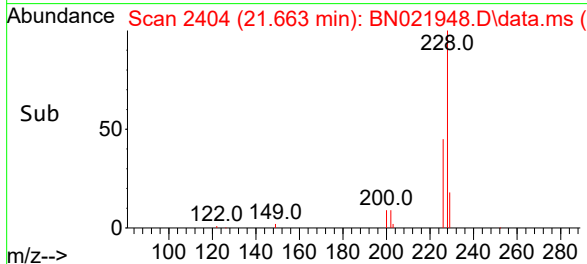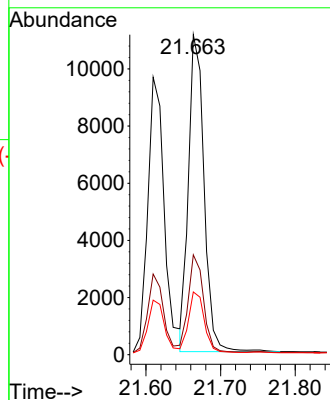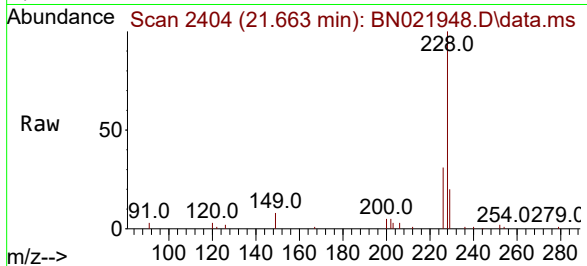

#34

Bis(2-ethylhexyl)phthalate

Concen: 0.356 ng

RT: 21.520 min Scan# 2388

Delta R.T. -0.009 min

Lab File: BN021948.D

Acq: 28 Sep 2022 19:36




Tgt Ion:149 Resp: 8230


Ion Ratio Lower Upper

149 100

167 25.8 20.6 30.8

279 2.7 2.0 3.0

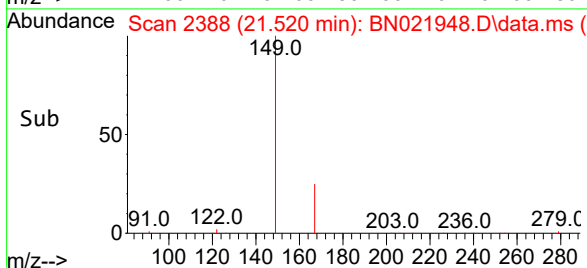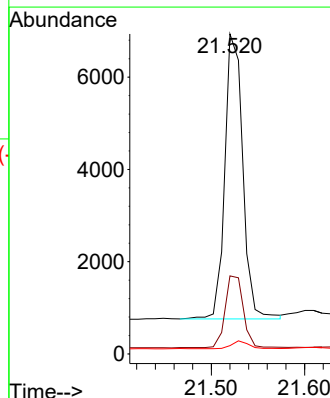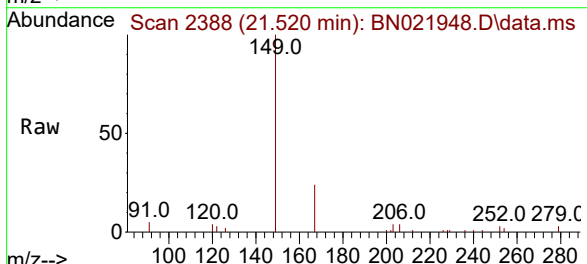



#35

Perylene-d12

Concen: 0.400 ng

RT: 24.129 min Scan# 3078

Delta R.T. -0.006 min

Lab File: BN021948.D

Acq: 28 Sep 2022 19:36

Instrument :

BNA_N

ClientSampleId :

ICVBN092922





Tgt Ion:264 Resp: 8320

Ion Ratio Lower Upper

264 100

260 27.4 21.0 31.4

265 85.1 67.8 101.8

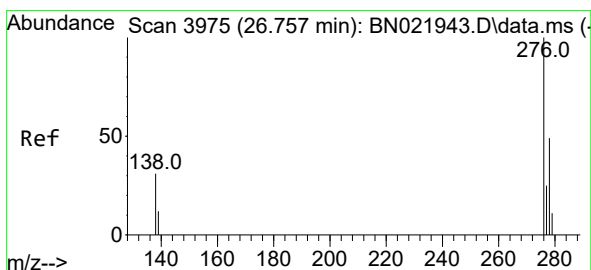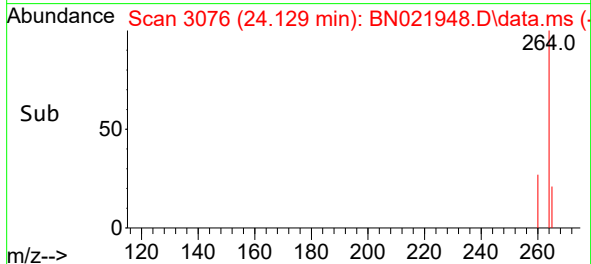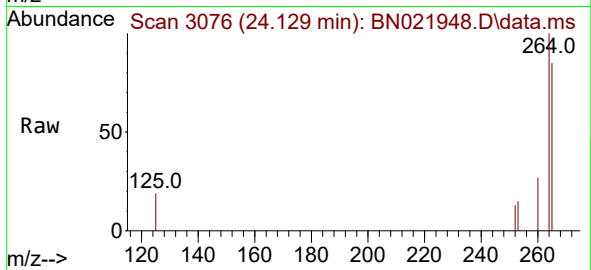

#36

Indeno(1,2,3-cd)pyrene

Concen: 0.391 ng

RT: 26.754 min Scan# 3974

Delta R.T. -0.003 min

Lab File: BN021948.D

Acq: 28 Sep 2022 19:36




Tgt Ion:276 Resp: 17211


Ion Ratio Lower Upper

276 100

138 34.3 27.3 40.9

277 25.2 19.8 29.6

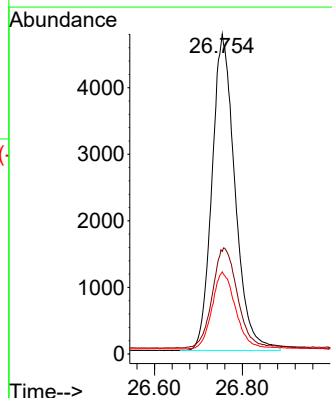



#37

Benzo(b)fluoranthene

Concen: 0.391 ng

RT: 23.357 min Scan# 2812

Delta R.T. -0.006 min

Lab File: BN021948.D


Acq: 28 Sep 2022 19:36

Instrument :

BNA_N

ClientSampleId :

ICVBN092922






Tgt Ion:252 Resp: 15122

Ion Ratio Lower Upper

252 100

253 27.2 21.4 32.0

125 20.0 16.2 24.4

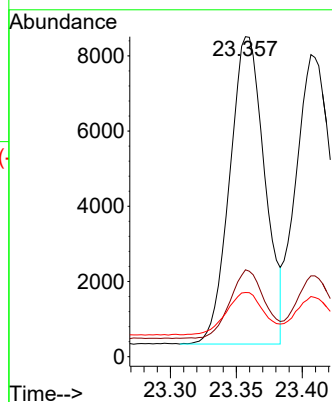

#38

Benzo(k)fluoranthene

Concen: 0.391 ng

RT: 23.407 min Scan# 2829

Delta R.T. -0.009 min

Lab File: BN021948.D

Acq: 28 Sep 2022 19:36




Tgt Ion:252 Resp: 14781


Ion Ratio Lower Upper

252 100

253 26.8 21.8 32.6

125 19.9 15.8 23.8

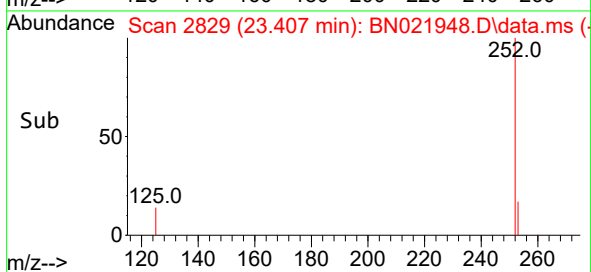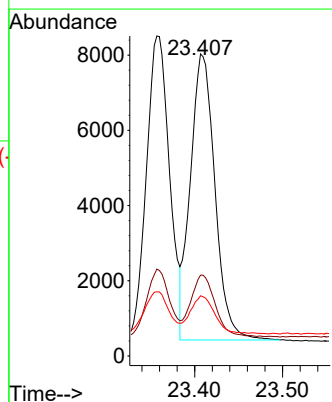



#39

Benzo(a)pyrene

Concen: 0.389 ng

RT: 24.015 min Scan# 3039

Delta R.T. -0.006 min

Lab File: BN021948.D

Acq: 28 Sep 2022 19:36

Instrument :

BNA_N

ClientSampleId :

ICVBN092922





Tgt Ion:252 Resp: 11499

Ion Ratio Lower Upper

252 100

253 29.3 23.9 35.9

125 26.9 20.9 31.3

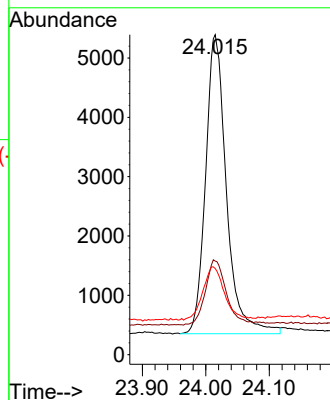

#40

Dibenzo(a,h)anthracene

Concen: 0.397 ng

RT: 26.775 min Scan# 3981

Delta R.T. -0.009 min

Lab File: BN021948.D

Acq: 28 Sep 2022 19:36




Tgt Ion:278 Resp: 13944


Ion Ratio Lower Upper

278 100

139 25.2 20.1 30.1

279 26.8 21.8 32.8

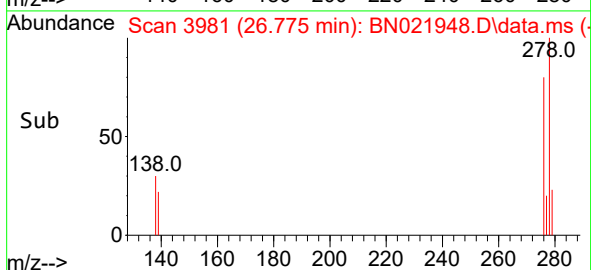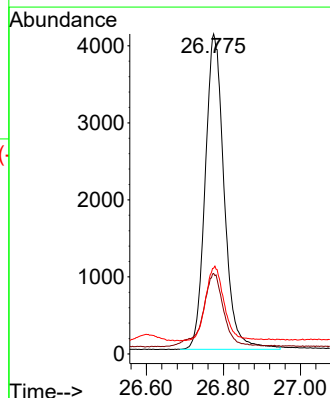

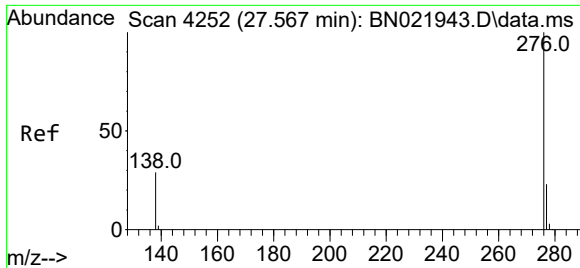

#41

Benzo(g,h,i)perylene

Concen: 0.377 ng

RT: 27.567 min Scan# 41

Delta R.T. 0.000 min

Lab File: BN021948.D


Acq: 28 Sep 2022 19:36

Instrument :

BNA_N

ClientSampleId :

ICVBN092922

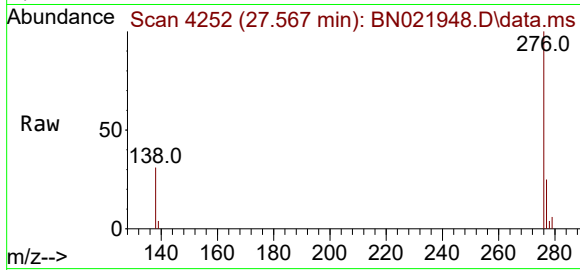

Tgt Ion:276 Resp: 14467

Ion Ratio Lower Upper

276 100

277 25.1 20.0 30.0

138 31.3 24.6 37.0

