
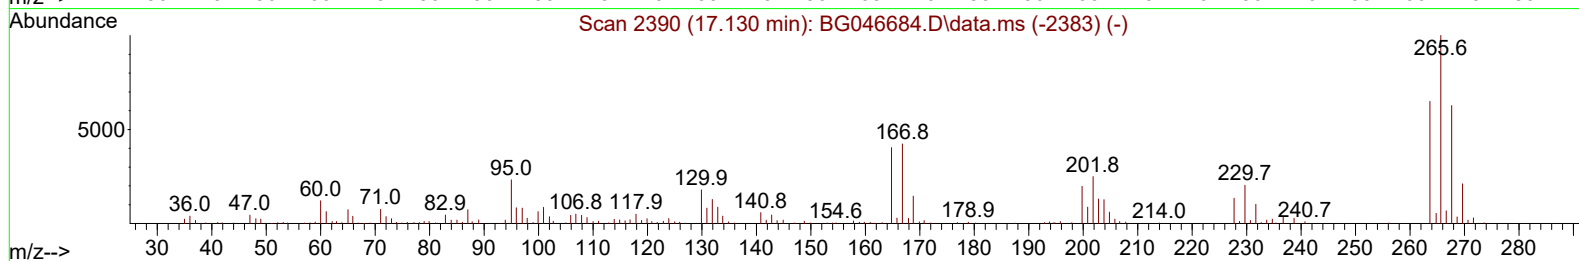
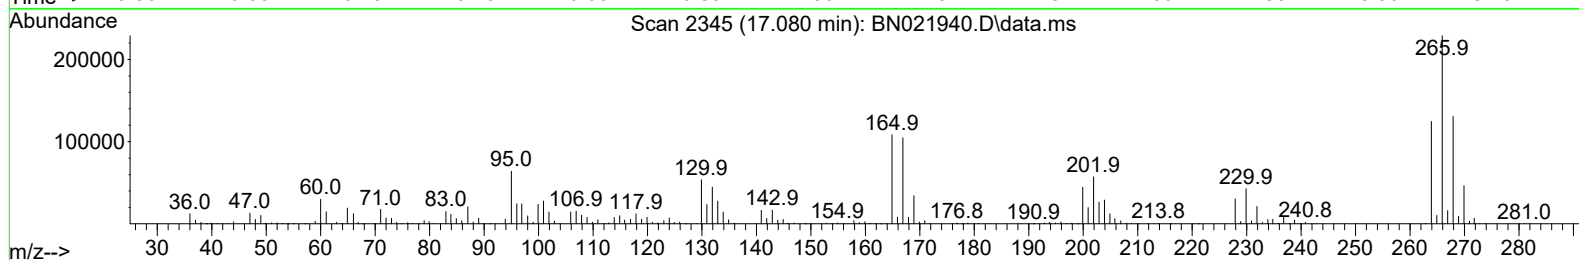


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092922\
Data File : BN021940.D
Acq On : 28 Sep 2022 14:22
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 29 05:19:21 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 29 05:19:16 2022
Response via : Initial Calibration

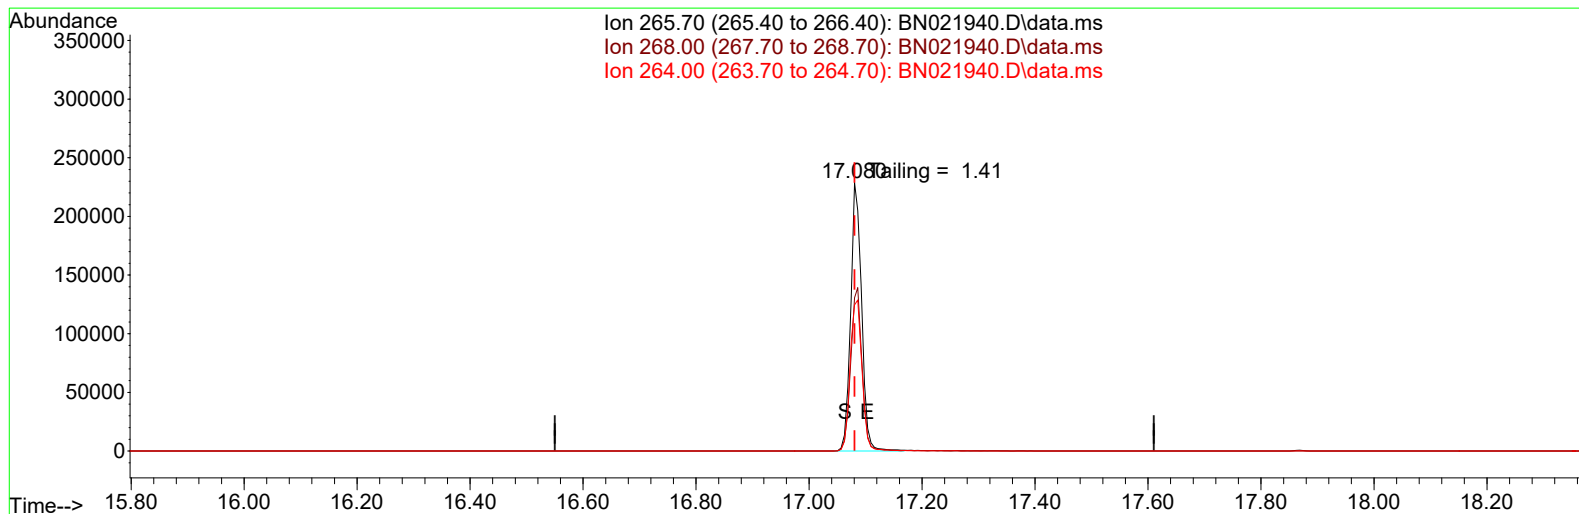

TIC: BN021940.D\data.ms

(70) Pentachlorophenol (C)




17.080min (0.000) 22489.55 ng

response 309744

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	57.10
264.00	61.60	54.45
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092922\
 Data File : BN021940.D
 Acq On : 28 Sep 2022 14:22
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 29 05:19:21 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 29 05:19:16 2022
 Response via : Initial Calibration

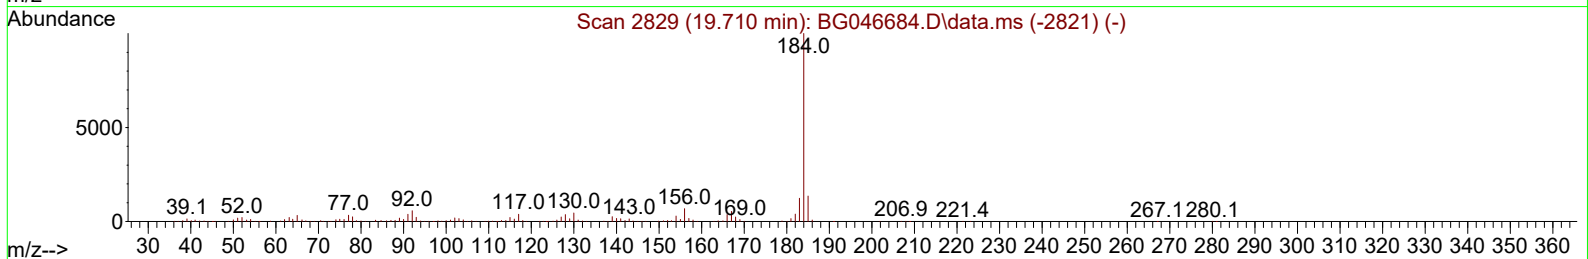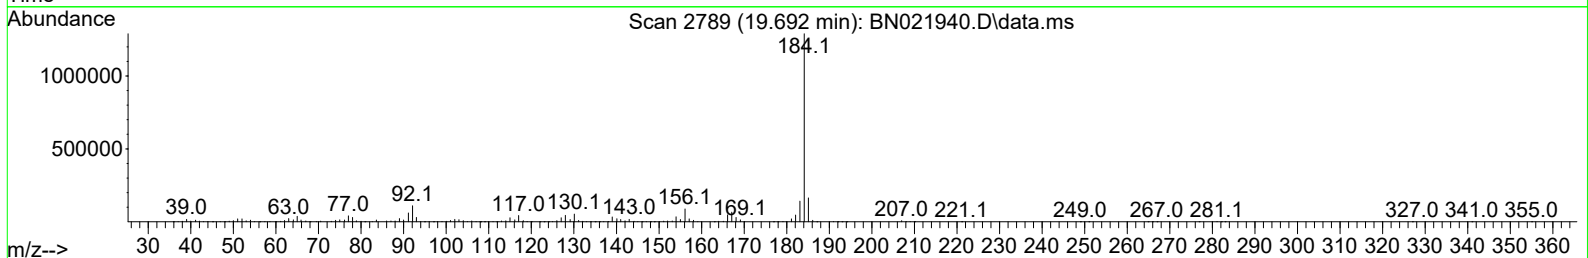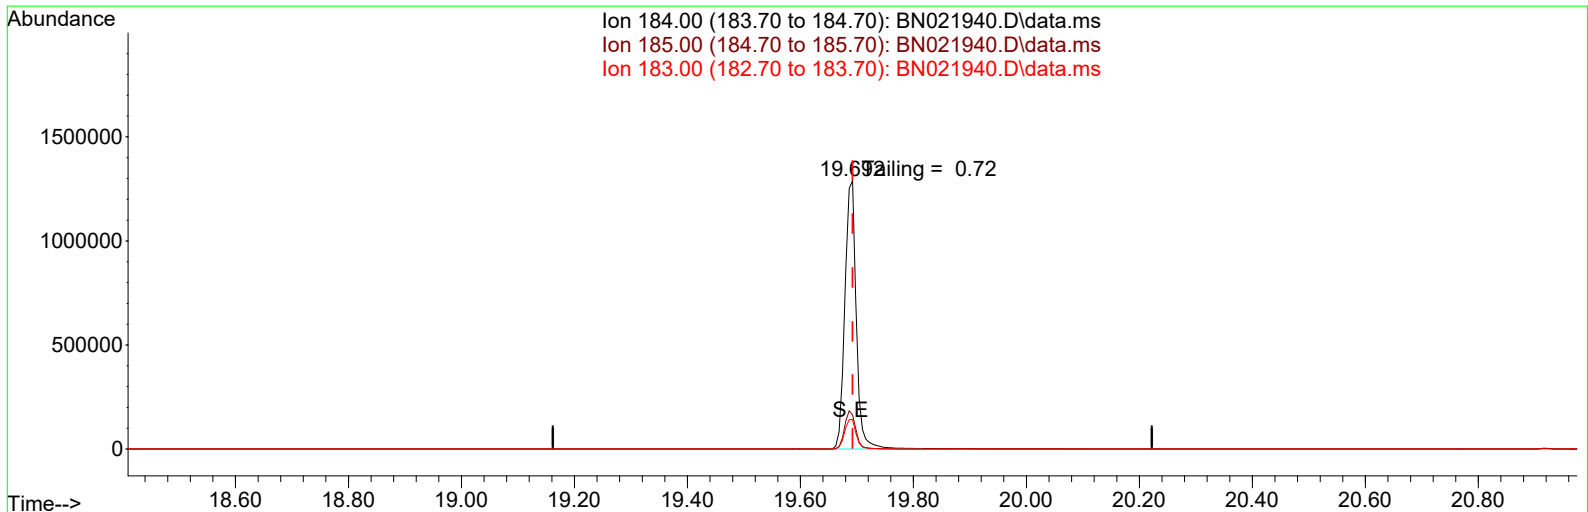

TIC: BN021940.D\data.ms

(77) Benzidine

19.692min (0.000) 0.00 ng

response 1805500

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	12.70
183.00	13.20	11.00
0.00	0.00	0.00