
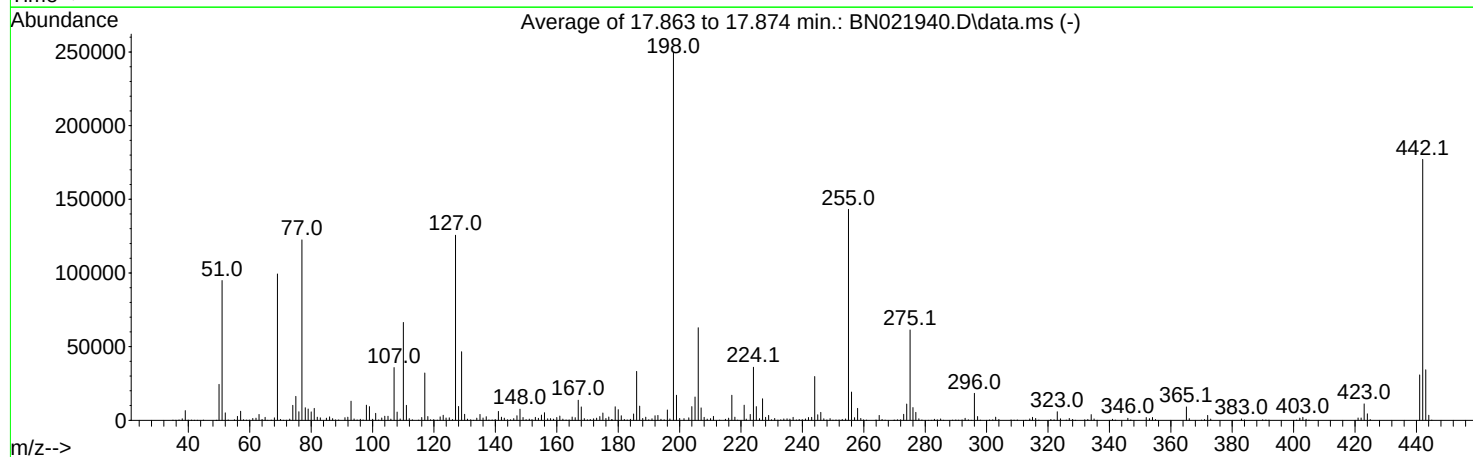


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092922\
 Data File : BN021940.D
 Acq On : 28 Sep 2022 14:22
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Sep 28 02:59:31 2022

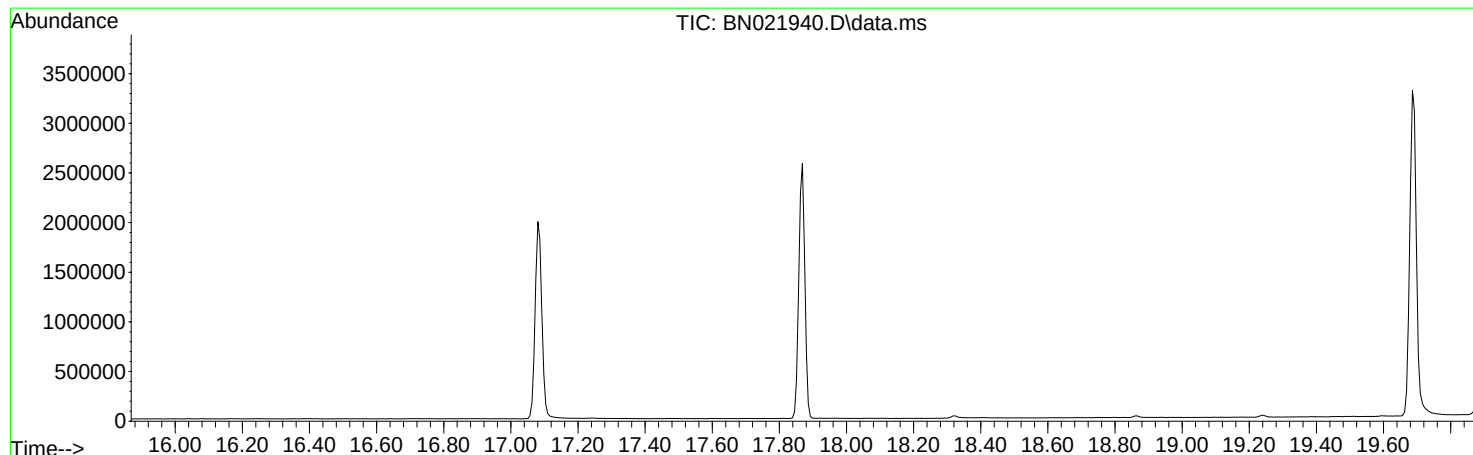




AutoFind: Scans 2478, 2479, 2480; Background Corrected with Scan 2471

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.0	94843	PASS
68	69	0.00	2	1.7	1658	PASS
69	198	0.00	100	39.8	99296	PASS
70	69	0.00	2	0.6	640	PASS
127	198	10	80	50.3	125605	PASS
197	198	0.00	2	0.4	891	PASS
198	198	100	100	100.0	249685	PASS
199	198	5	9	6.8	17023	PASS
275	198	10	60	24.5	61269	PASS
365	198	1	100	3.6	9053	PASS
441	198	0.01	100	12.4	30845	PASS
442	442	50	100	100.0	177024	PASS
443	442	15	24	19.4	34293	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092922\
 Data File : BN021940.D
 Acq On : 28 Sep 2022 14:22
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Sep 29 05:19:21 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 29 05:19:16 2022
 Response via : Initial Calibration

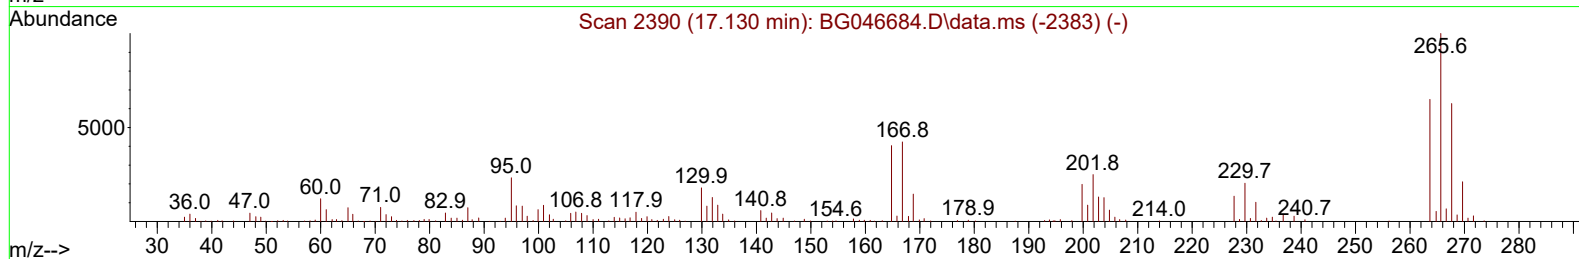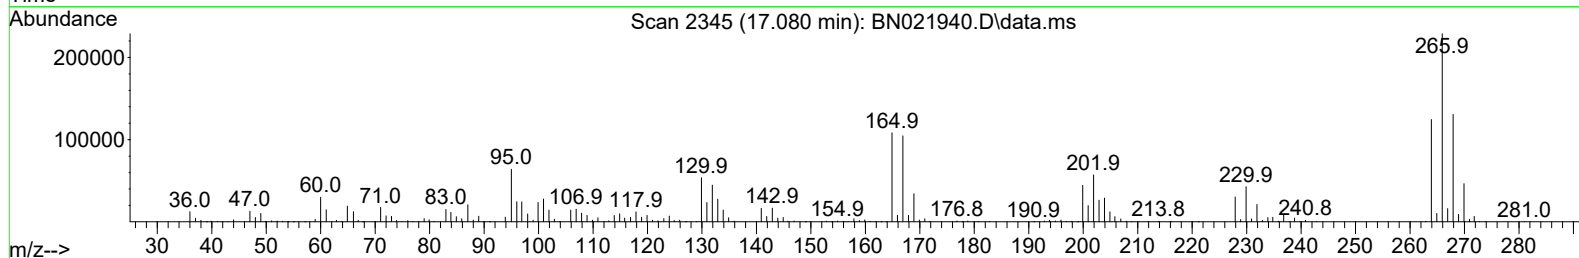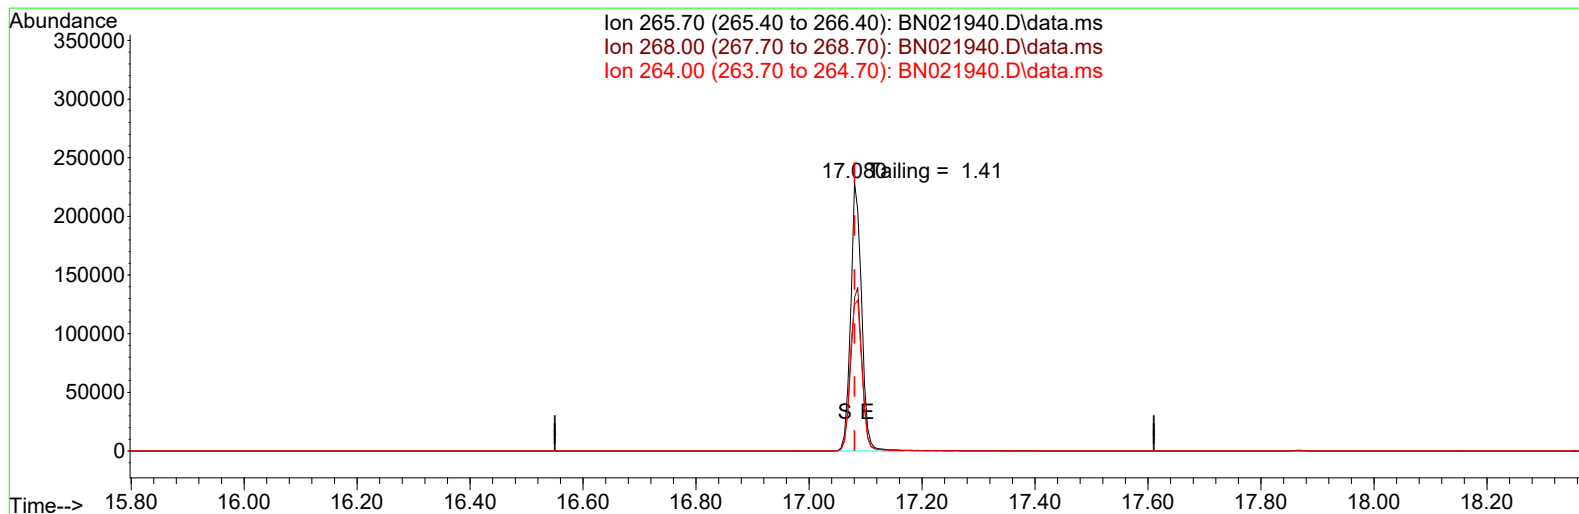

TIC: BN021940.D\data.ms

(70) Pentachlorophenol (C)

17.080min (0.000) 22489.55 ng




response 309744

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	57.10
264.00	61.60	54.45
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092922\
Data File : BN021940.D
Acq On : 28 Sep 2022 14:22
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 29 05:19:21 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 29 05:19:16 2022
Response via : Initial Calibration

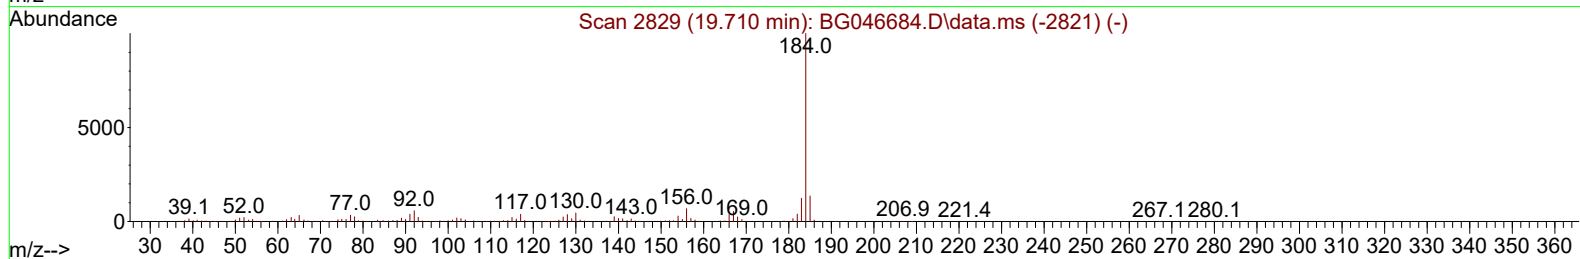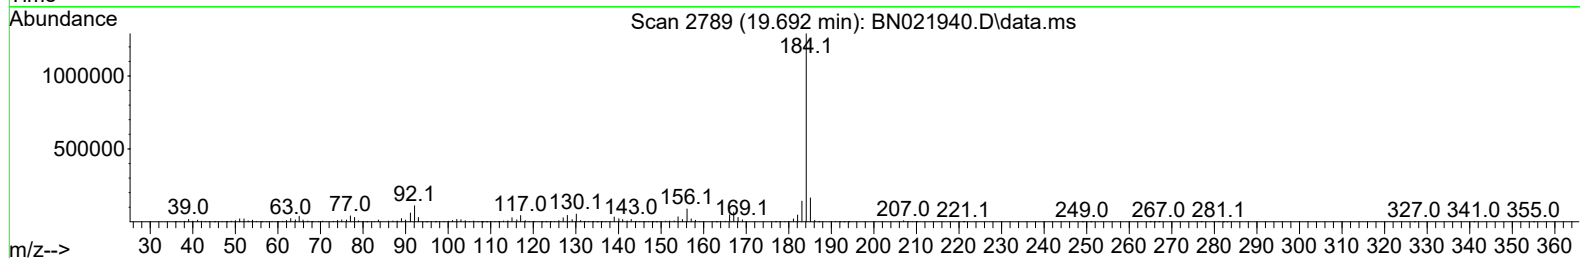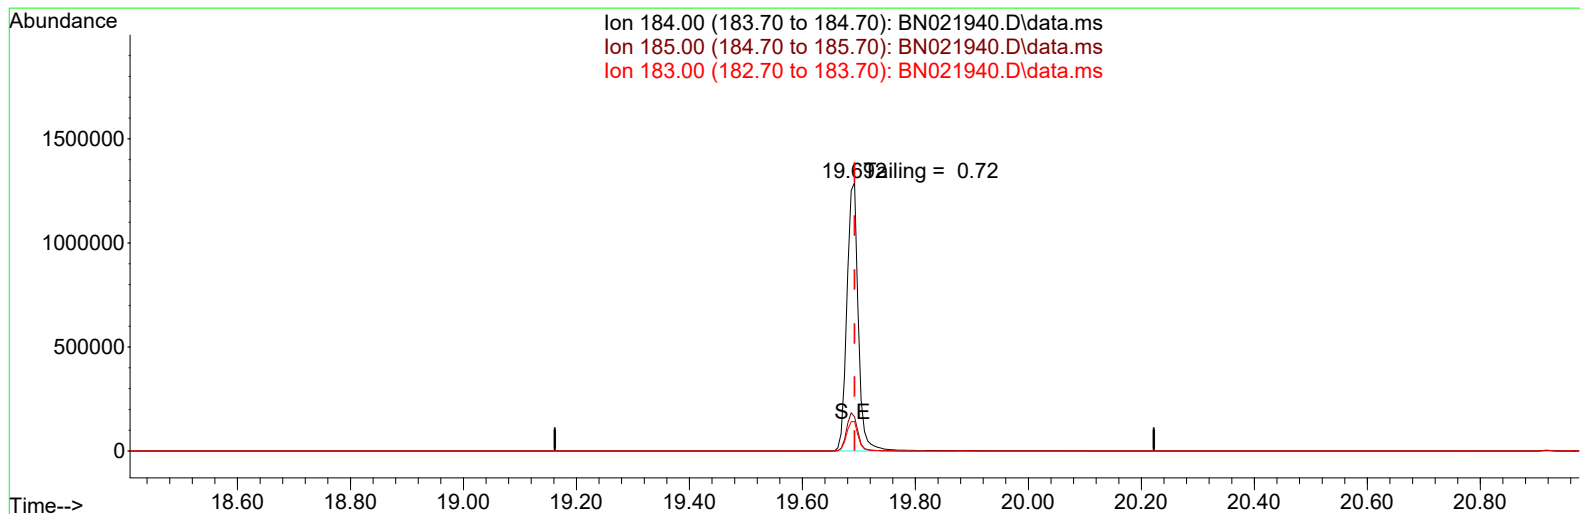

TIC: BN021940.D\data.ms

(77) Benzidine

19.692min (0.000) 0.00 ng

response 1805500

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	12.70
183.00	13.20	11.00
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/29/2022	BNA_N	<u>BN021940.D</u>
Compound Name	Response	Retention Time
DDT	846144	20.921
DDD	8650	20.48
DDE	65	19.968
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8715	854859	1.02

Instrument :
BNA_N
ClientSampleId :
DFTPP