


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092922\
 Data File : BN021951.D
 Acq On : 29 Sep 2022 09:42
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN092922.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Sep 30 02:27:15 2022

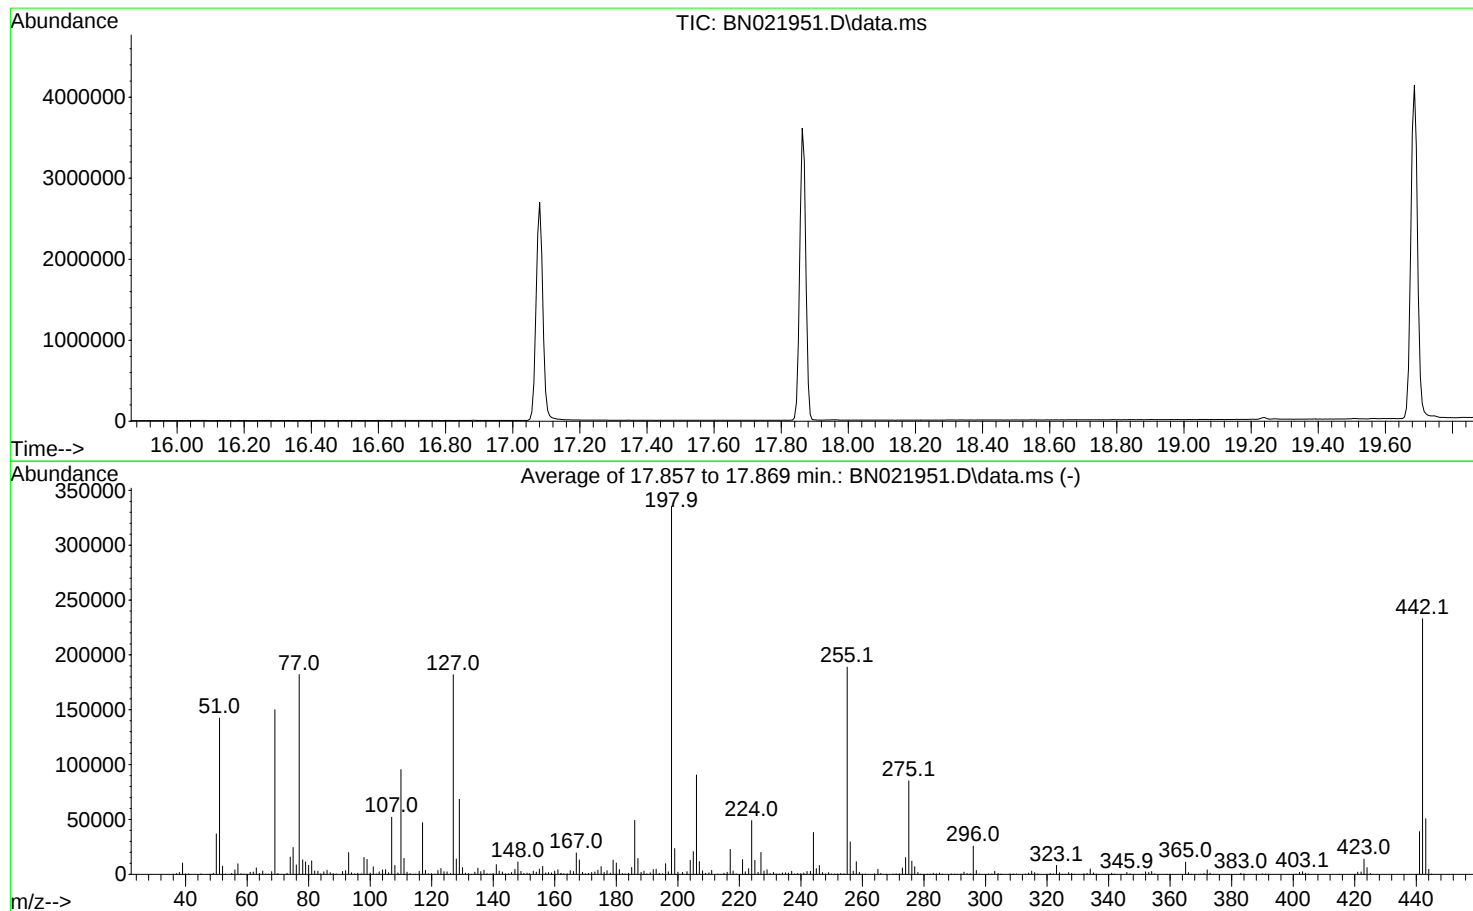




AutoFind: Scans 2477, 2478, 2479; Background Corrected with Scan 2470

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.5	142421	PASS
68	69	0.00	2	1.6	2473	PASS
69	198	0.00	100	44.7	149995	PASS
70	69	0.00	2	0.5	812	PASS
127	198	10	80	54.3	181995	PASS
197	198	0.00	2	0.7	2309	PASS
198	198	100	100	100.0	335360	PASS
199	198	5	9	7.0	23376	PASS
275	198	10	60	25.4	85144	PASS
365	198	1	100	3.3	10971	PASS
441	198	0.01	100	11.6	38947	PASS
442	442	50	100	100.0	233003	PASS
443	442	15	24	21.8	50715	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092922\
 Data File : BN021951.D
 Acq On : 29 Sep 2022 09:42
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Sep 30 05:17:19 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 30 05:17:14 2022
 Response via : Initial Calibration

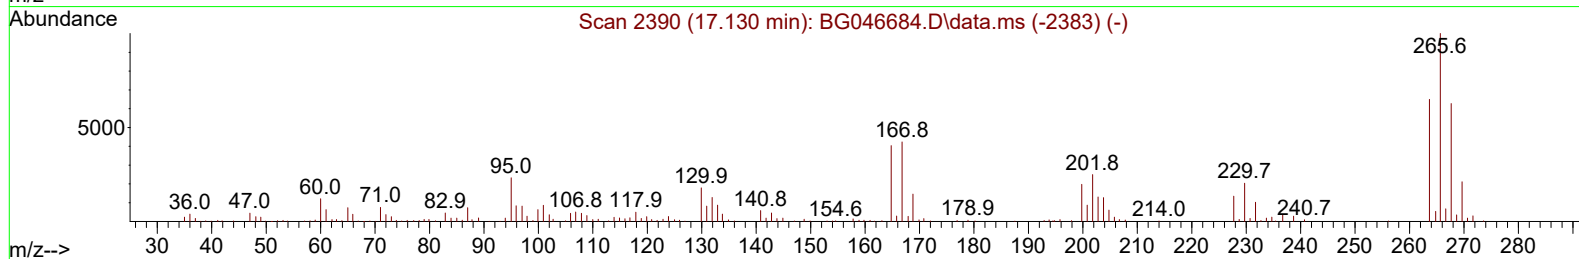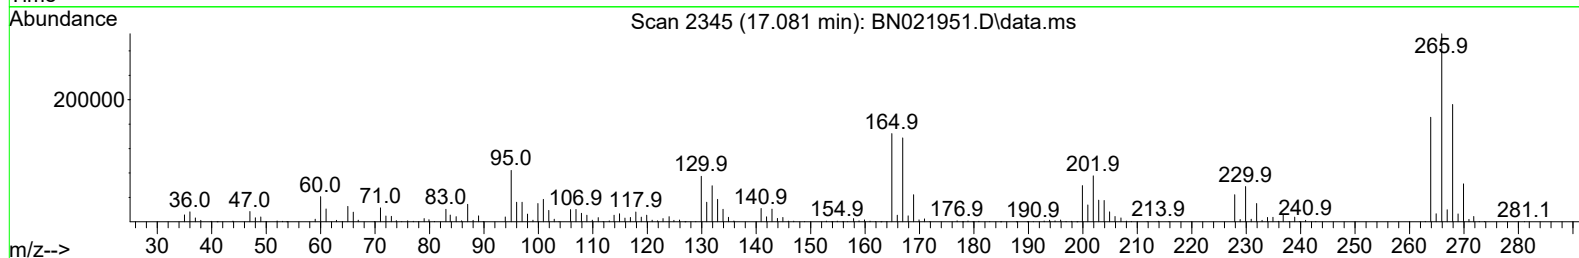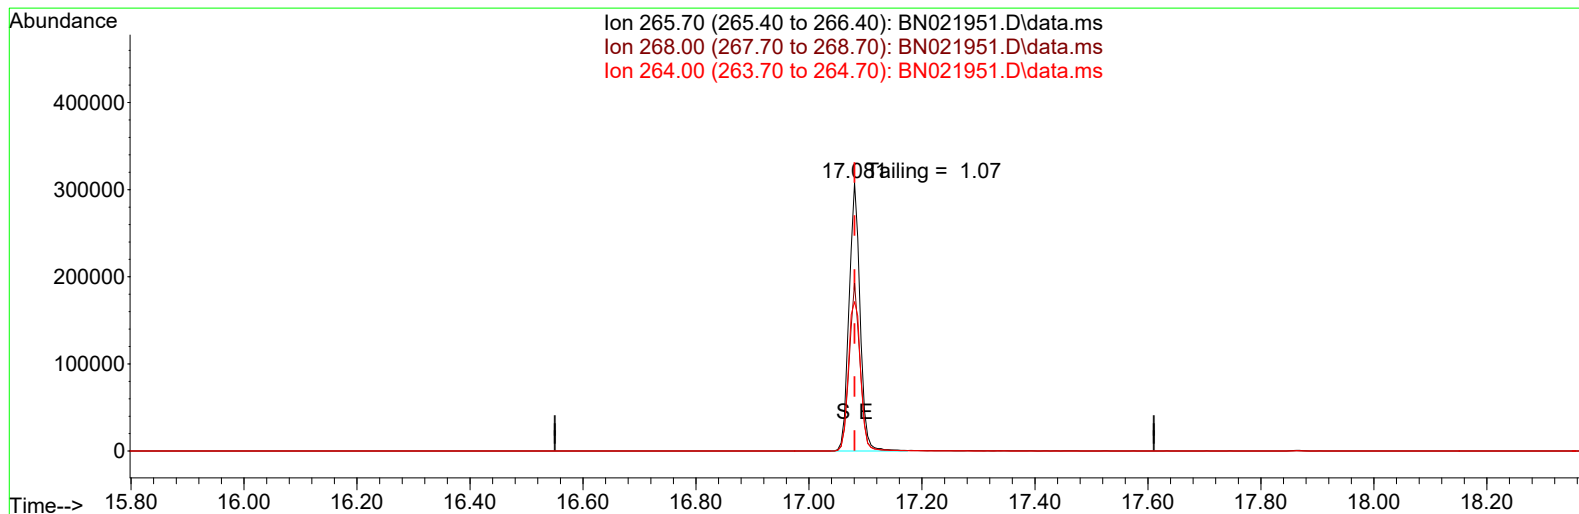

TIC: BN021951.D\data.ms

(70) Pentachlorophenol (C)

17.081min (0.000) 20228.59 ng




response 419097

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.40
264.00	61.60	55.63
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092922\
Data File : BN021951.D
Acq On : 29 Sep 2022 09:42
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 30 05:17:19 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 30 05:17:14 2022
Response via : Initial Calibration

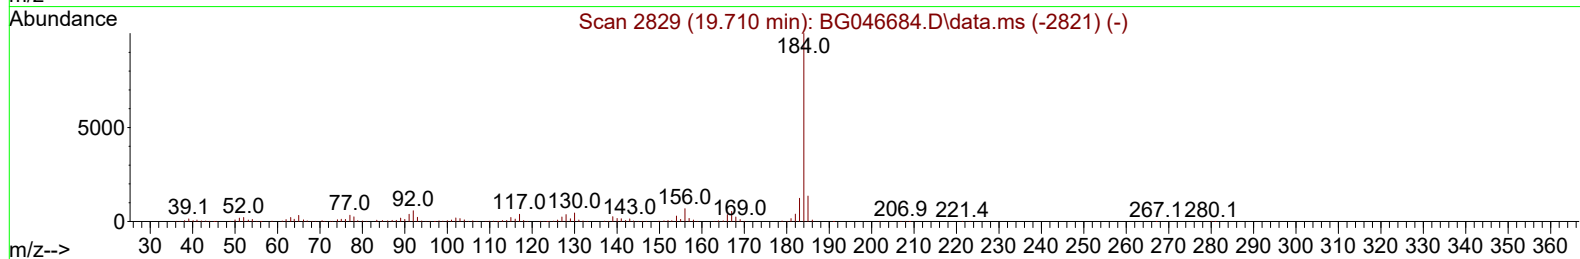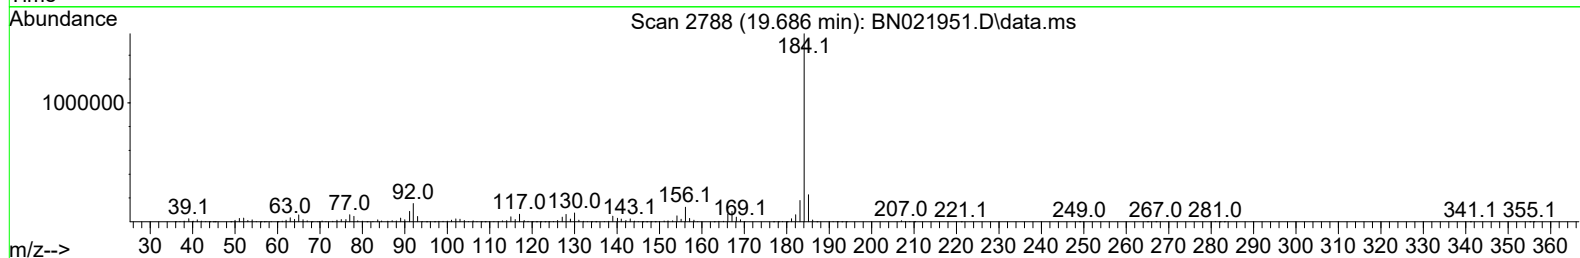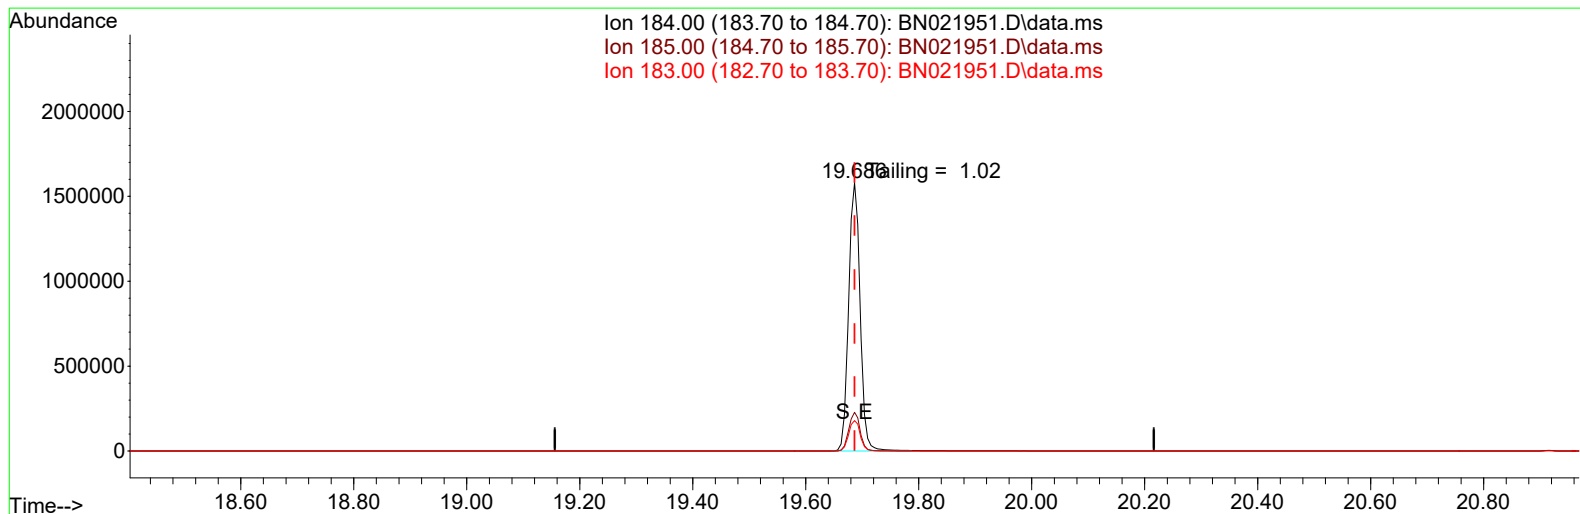

TIC: BN021951.D\data.ms

(77) Benzidine

19.686min (0.000) 0.00 ng

response 2245238

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.42
183.00	13.20	11.32
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/29/2022	BNA_N	<u>BN021951.D</u>
Compound Name	Response	Retention Time
DDT	966934	20.916
DDD	85092	20.474
DDE	3146	19.963
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
88238	1055172	8.36

Instrument :
BNA_N
ClientSampleId :
DFTPP