
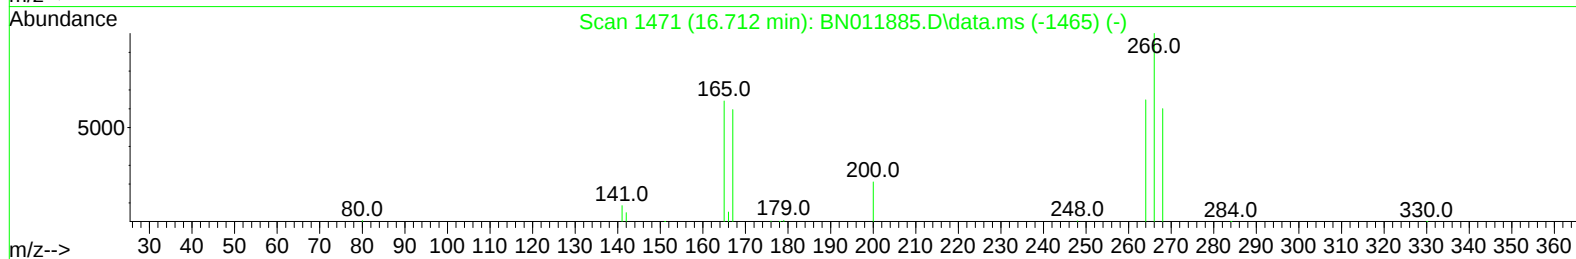
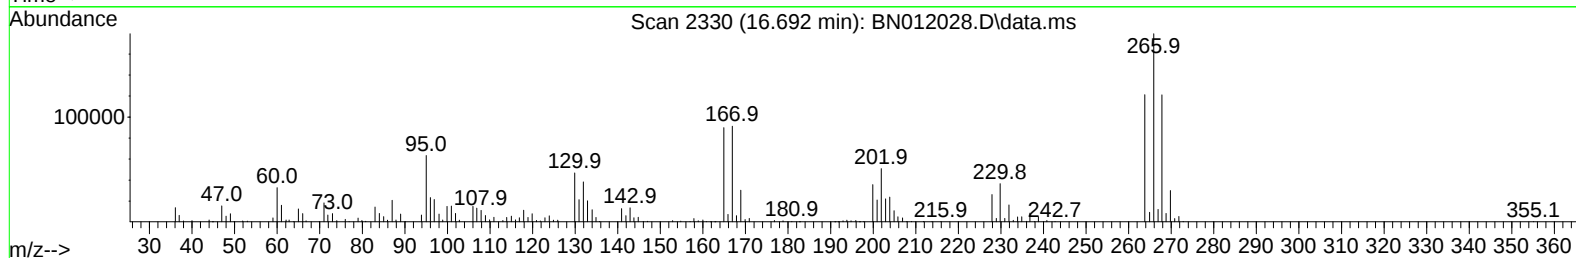


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN093020\
 Data File : BN012028.D
 Acq On : 30 Sep 2020 07:56
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 01 00:26:13 2020
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN092320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 30 16:28:17 2020
 Response via : Initial Calibration

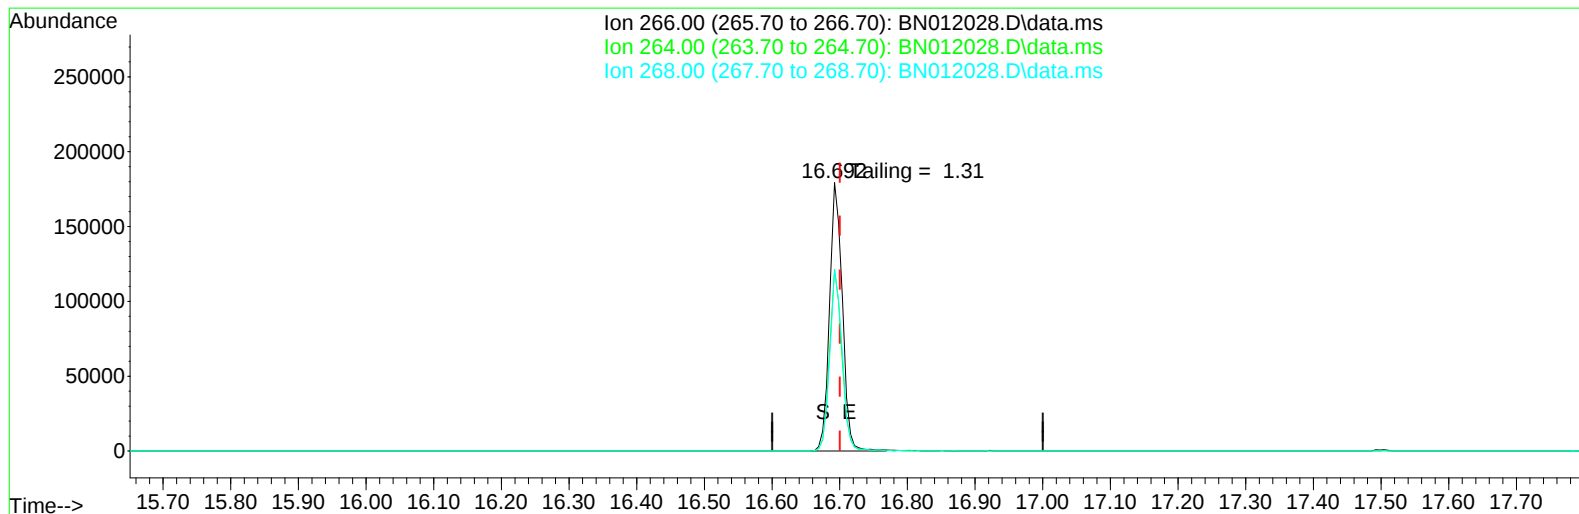

TIC: BN012028.D\data.ms

(24) Pentachlorophenol

16.692min (-0.008) 0.00 ng

response 236583

Ion	Exp%	Act%
266.00	100.00	100.00
264.00	64.00	64.99
268.00	65.50	65.18
0.00	0.00	0.00