
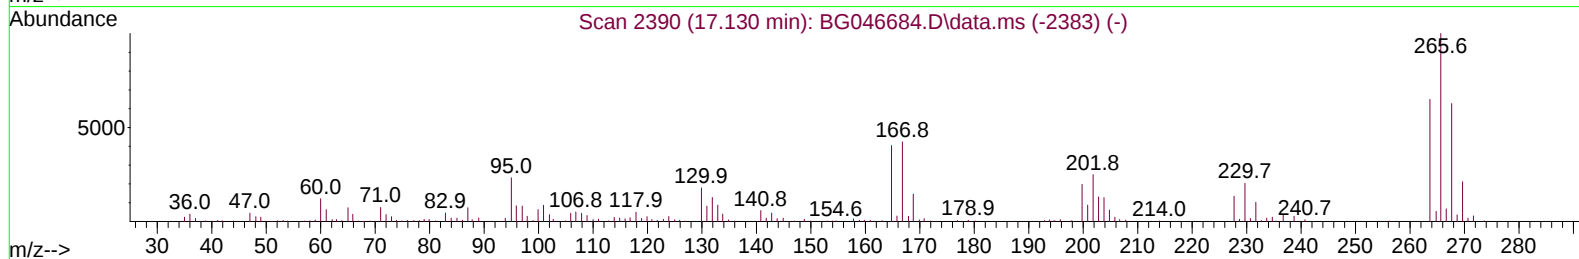
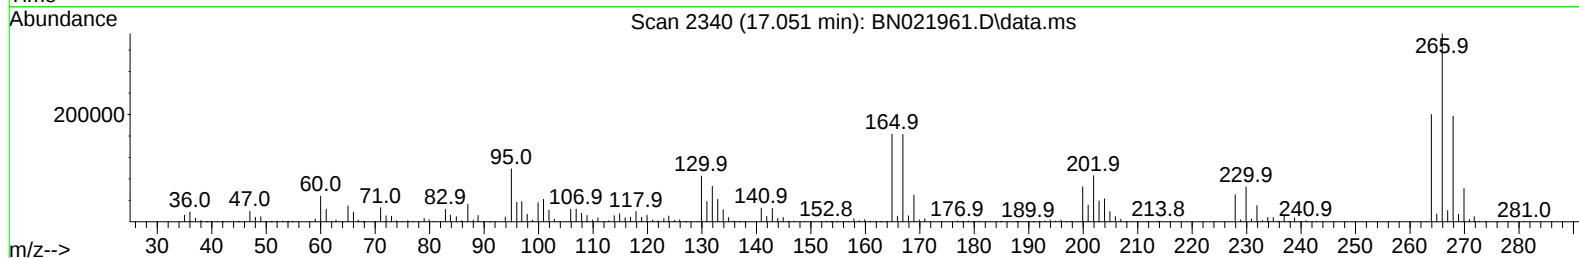


Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN093022\  
Data File : BN021961.D  
Acq On : 30 Sep 2022 11:00  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 30 18:40:08 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Sep 30 18:40:02 2022  
Response via : Initial Calibration

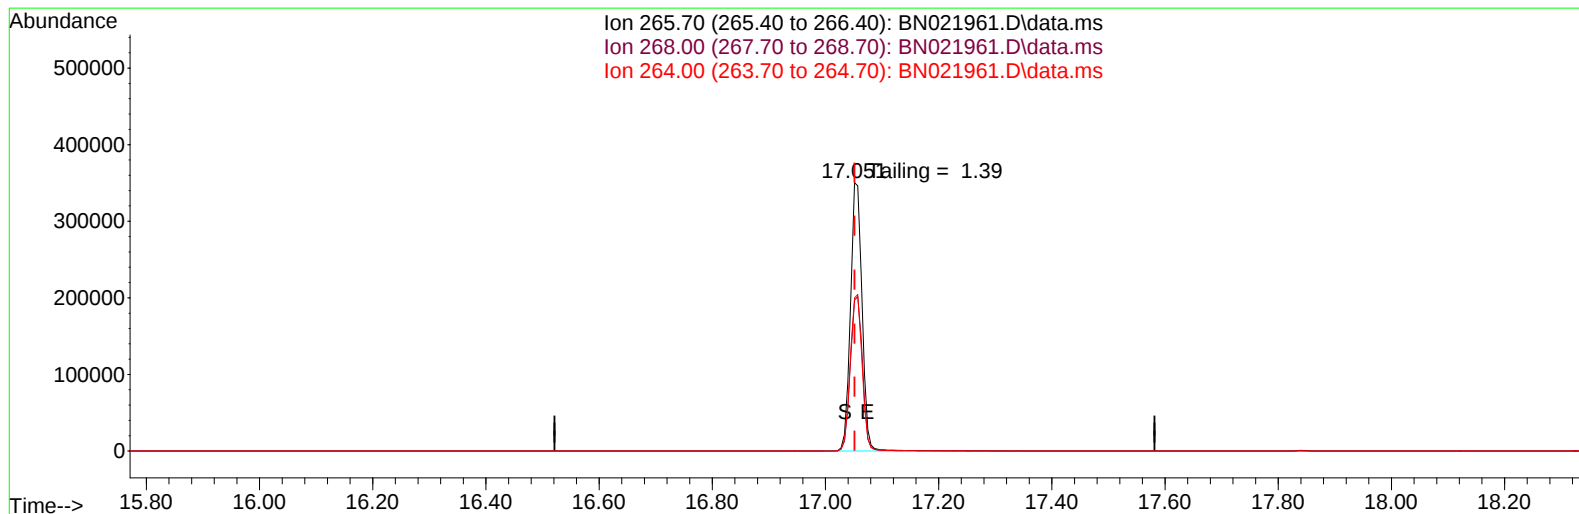

TIC: BN021961.D\data.ms

**(70) Pentachlorophenol (C)**




17.051min ( 0.000) 27153.20 ng

response 498421

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 62.20  | 56.21  |
| 264.00 | 61.60  | 57.05  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN093022\  
Data File : BN021961.D  
Acq On : 30 Sep 2022 11:00  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 30 18:40:08 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Sep 30 18:40:02 2022  
Response via : Initial Calibration

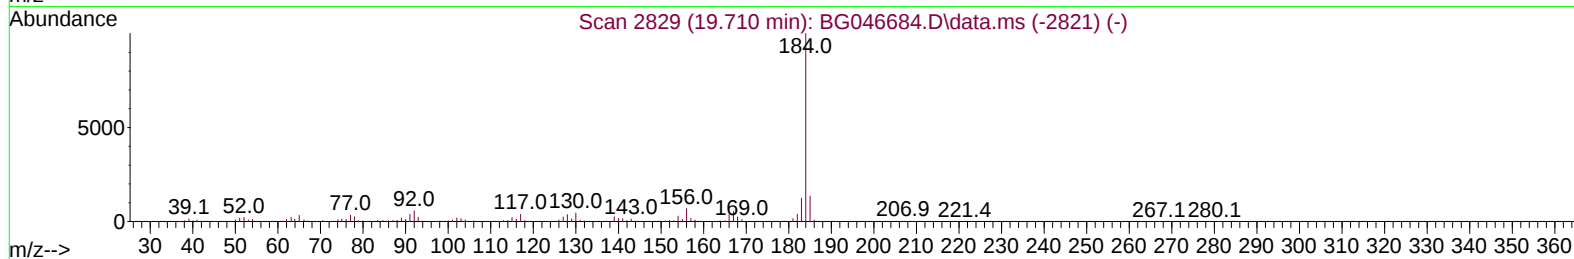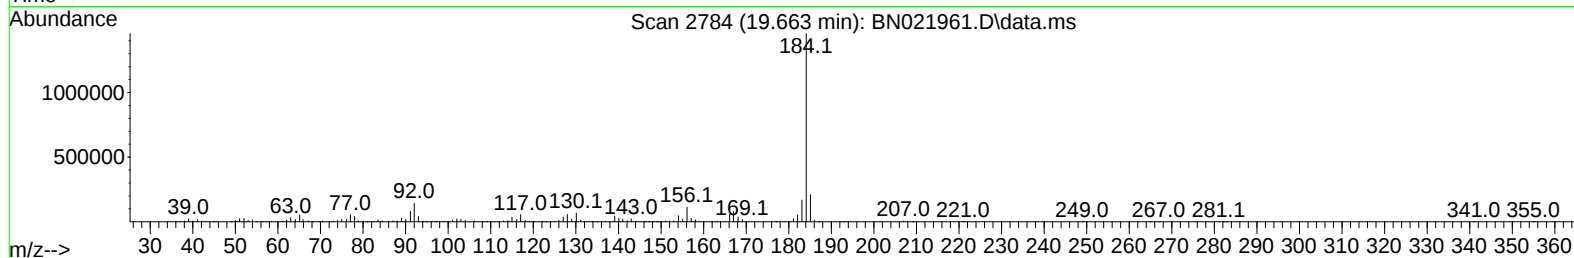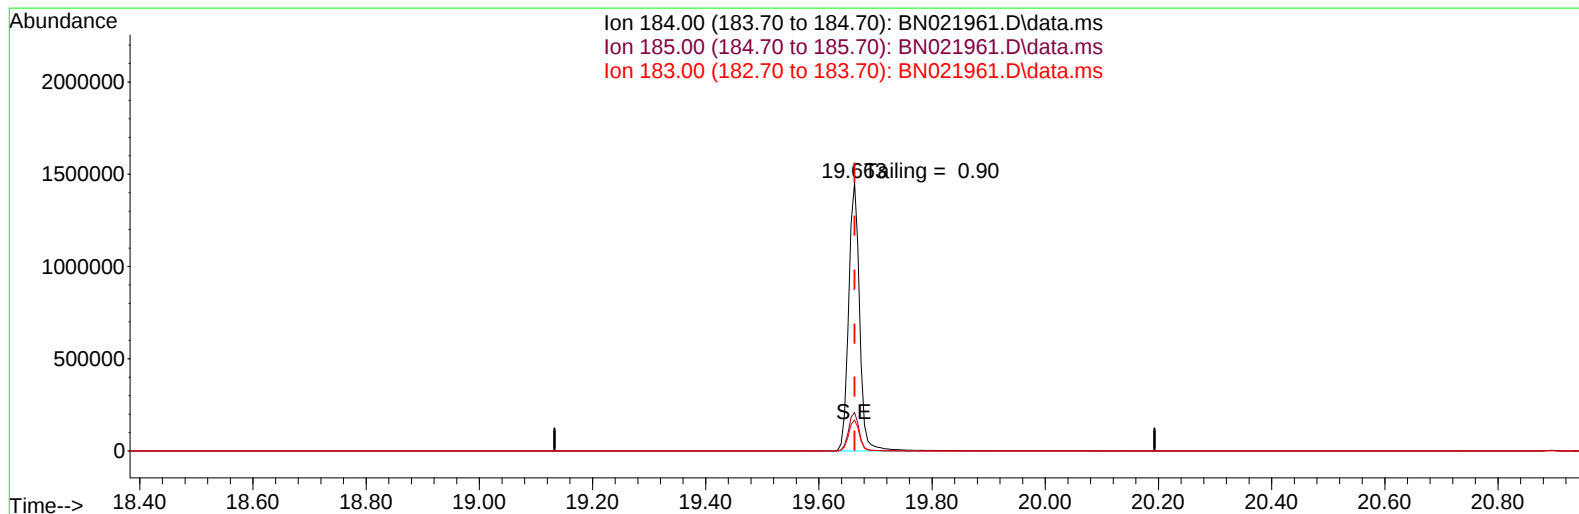

TIC: BN021961.D\data.ms

**(77) Benzidine**

19.663min ( 0.000) 0.00 ng

response 1959891

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.50  | 14.38  |
| 183.00 | 13.20  | 11.58  |
| 0.00   | 0.00   | 0.00   |