
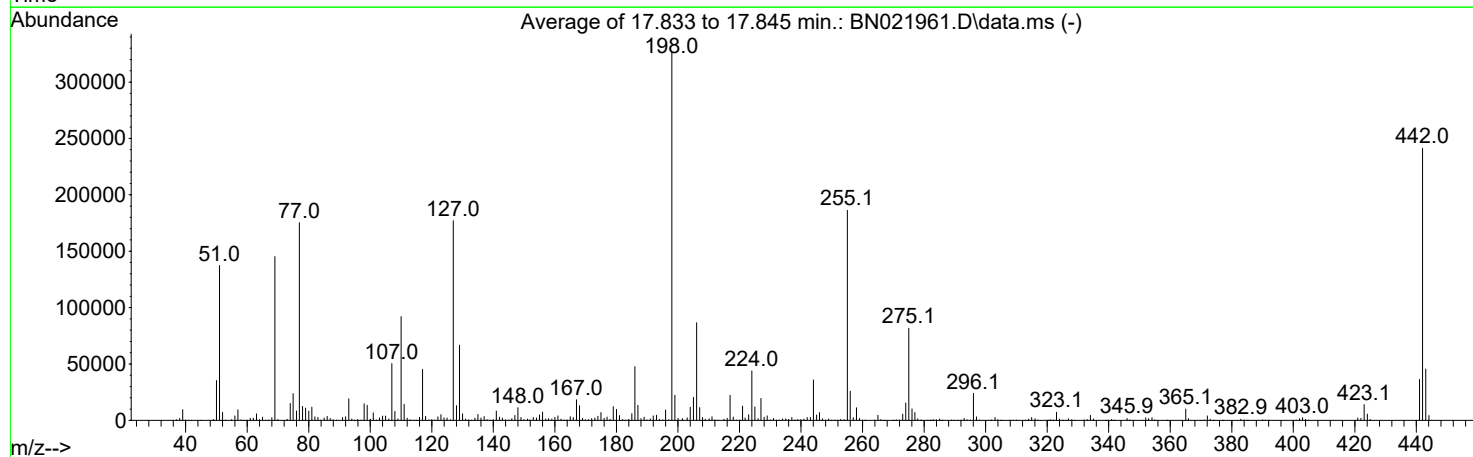


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN093022\
 Data File : BN021961.D
 Acq On : 30 Sep 2022 11:00
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN093022.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Sep 30 16:20:22 2022

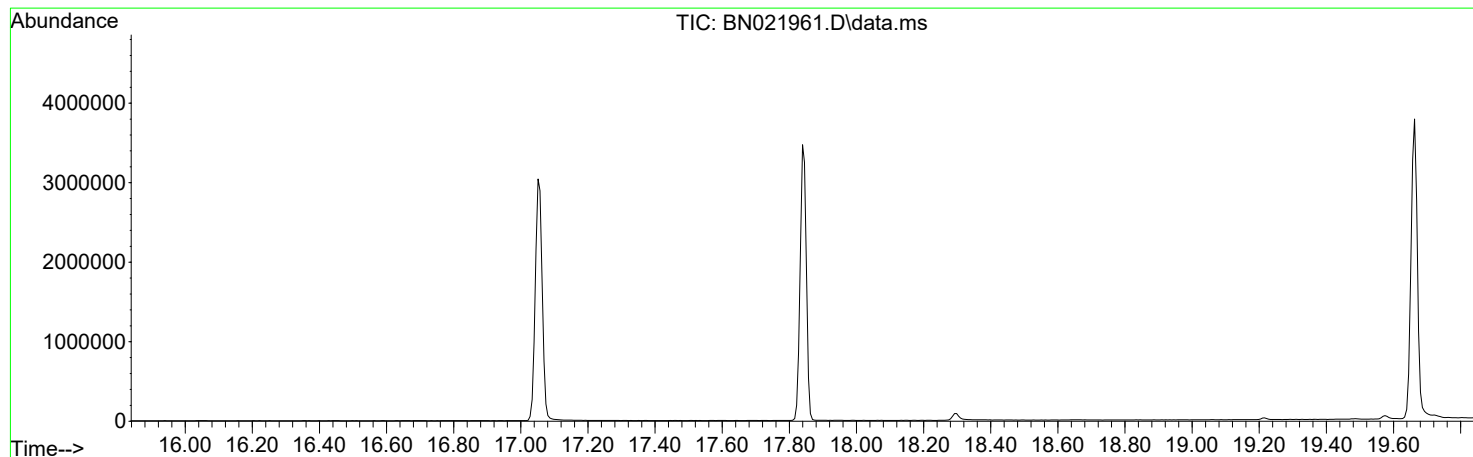

AutoFind: Scans 2473, 2474, 2475; Background Corrected with Scan 2466

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.1	137348	PASS
68	69	0.00	2	1.6	2387	PASS
69	198	0.00	100	44.5	145269	PASS
70	69	0.00	2	0.5	719	PASS
127	198	10	80	54.3	177045	PASS
197	198	0.00	2	0.2	596	PASS
198	198	100	100	100.0	326187	PASS
199	198	5	9	6.8	22341	PASS
275	198	10	60	25.0	81704	PASS
365	198	1	100	3.1	10070	PASS
441	198	0.01	100	11.1	36328	PASS
442	442	50	100	100.0	241280	PASS
443	442	15	24	18.9	45515	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
9/30/2022	BNA_N	<u>BN021961.D</u>
Compound Name	Response	Retention Time
DDT	1053993	20.89
DDD	2902	20.45
DDE	55	19.93
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2957	1056950	0.28

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN093022\
 Data File : BN021961.D
 Acq On : 30 Sep 2022 11:00
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Sep 30 18:40:08 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 30 18:40:02 2022
 Response via : Initial Calibration

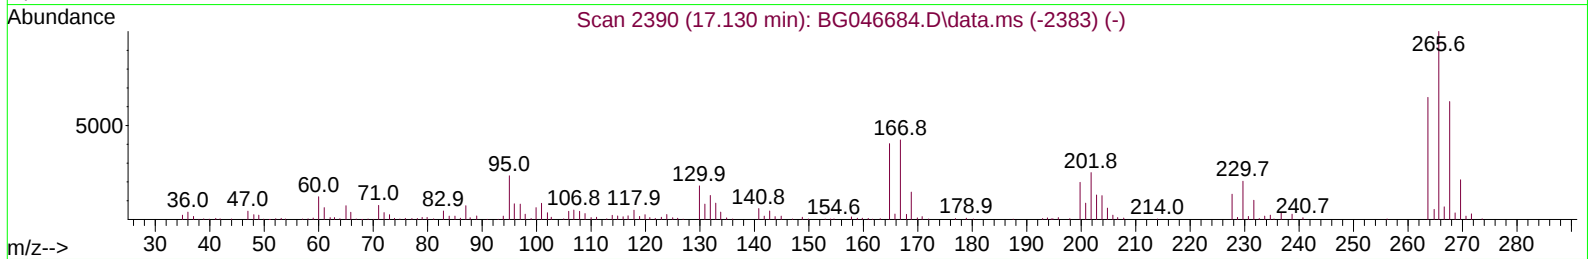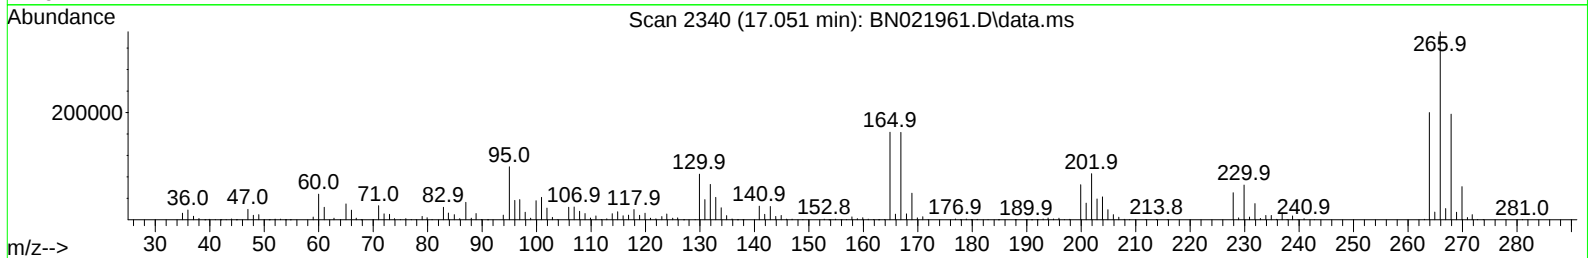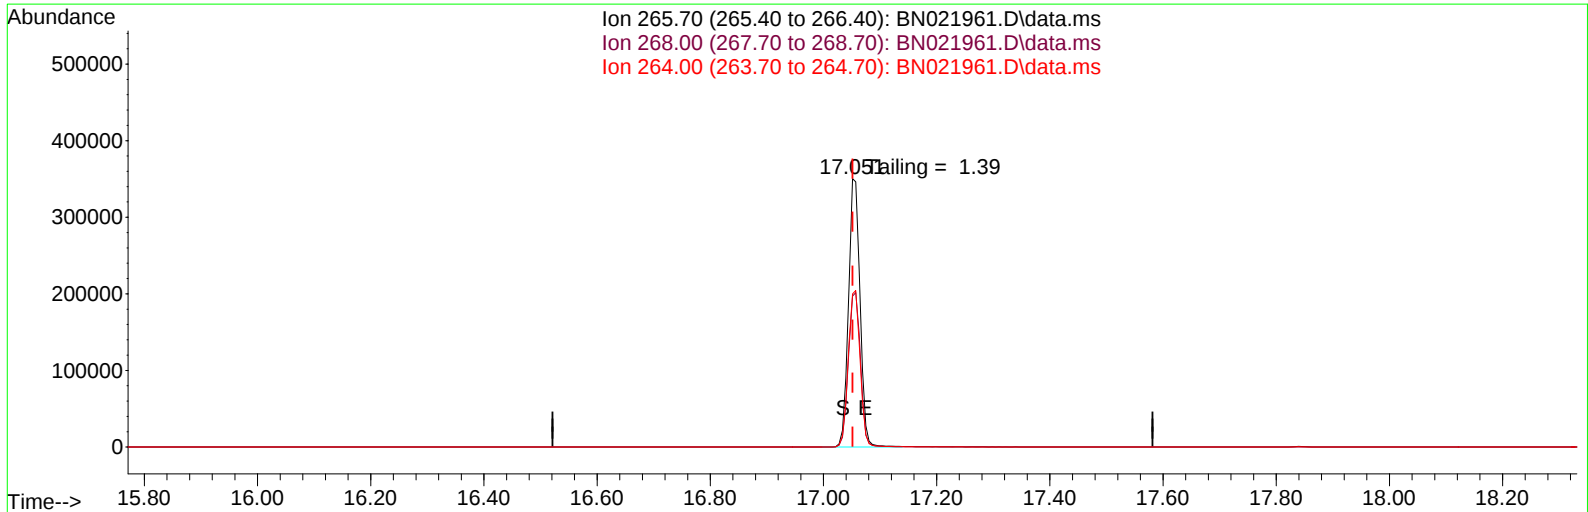

TIC: BN021961.D\data.ms

(70) Pentachlorophenol (C)

17.051min (0.000) 27153.20 ng

response 498421

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	56.21
264.00	61.60	57.05
0.00	0.00	0.00

