

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN093024\
 Data File : BN034281.D
 Acq On : 30 Sep 2024 17:29
 Operator : RC/JU
 Sample : PB163394BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK394

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN034281.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.999	16	19	33	rVB	99240	126566	1.89%	0.193%
2	3.387	81	85	109	rBV	976409	1391090	20.80%	2.124%
3	3.693	132	137	149	rVB	383224	494182	7.39%	0.755%
4	6.587	622	629	648	rBV	1175741	1930990	28.87%	2.949%
5	6.746	650	656	667	rVB	1084631	1639242	24.51%	2.503%
6	6.928	680	687	703	rBV	1305648	2064153	30.87%	3.152%
7	7.387	758	765	775	rBV	768502	1177936	17.61%	1.799%
8	8.105	877	887	906	rBV	1457739	2425500	36.27%	3.704%
9	8.534	949	960	979	rBV	1181183	1960514	29.32%	2.994%
10	9.246	1072	1081	1093	rBV	918100	1516364	22.67%	2.316%
11	9.669	1148	1153	1160	rVB8	4940	12322	0.18%	0.019%
12	9.775	1164	1171	1185	rBV	1422179	2415623	36.12%	3.689%
13	10.063	1215	1220	1226	rBV4	8270	21034	0.31%	0.032%
14	10.146	1226	1234	1246	rVB	1013395	1647985	24.64%	2.517%
15	10.293	1251	1259	1280	rBV	1261366	2264858	33.87%	3.459%
16	11.746	1500	1506	1514	rBV	20208	40200	0.60%	0.061%
17	13.469	1792	1799	1810	rBV	2297804	3455363	51.67%	5.277%
18	13.728	1836	1843	1856	rBV	2924742	4284137	64.06%	6.542%
19	14.040	1889	1896	1908	rBV	1423682	2086883	31.21%	3.187%
20	14.269	1927	1935	1961	rBV	817471	1488056	22.25%	2.272%
21	15.045	2060	2067	2083	rBV	3579612	5192329	77.64%	7.929%
22	15.175	2083	2089	2103	rVV	916029	1341899	20.07%	2.049%
23	15.287	2105	2108	2113	rVB	17960	26145	0.39%	0.040%
24	15.839	2197	2202	2206	rBV3	10129	13883	0.21%	0.021%
25	16.581	2324	2328	2334	rBV5	4349	8002	0.12%	0.012%
26	16.798	2359	2365	2375	rBV	1634413	2314452	34.61%	3.534%
27	16.898	2375	2382	2404	rVB2	3851778	5563533	83.19%	8.496%
28	17.492	2479	2483	2489	rBV7	5003	8933	0.13%	0.014%
29	18.769	2695	2700	2705	rBV2	47612	66521	0.99%	0.102%
30	18.839	2708	2712	2719	rBV2	41179	61276	0.92%	0.094%
31	19.204	2768	2774	2791	rBV	4498477	6361143	95.12%	9.714%
32	20.239	2948	2950	2956	rBV6	12881	15584	0.23%	0.024%
33	21.027	3078	3084	3094	rBV	1722069	2447733	36.60%	3.738%
34	23.557	3505	3514	3533	rBV2	2962838	6687460	100.00%	10.213%
35	23.733	3536	3544	3552	rBV	1225703	2710633	40.53%	4.140%
36	24.721	3707	3712	3719	rVB3	96806	219315	3.28%	0.335%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN093024\
Data File : BN034281.D
Acq On : 30 Sep 2024 17:29
Operator : RC/JU
Sample : PB163394BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK394

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 65481839

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN093024\
Data File : BN034281.D
Acq On : 30 Sep 2024 17:29
Operator : RC/JU
Sample : PB163394BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK394

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

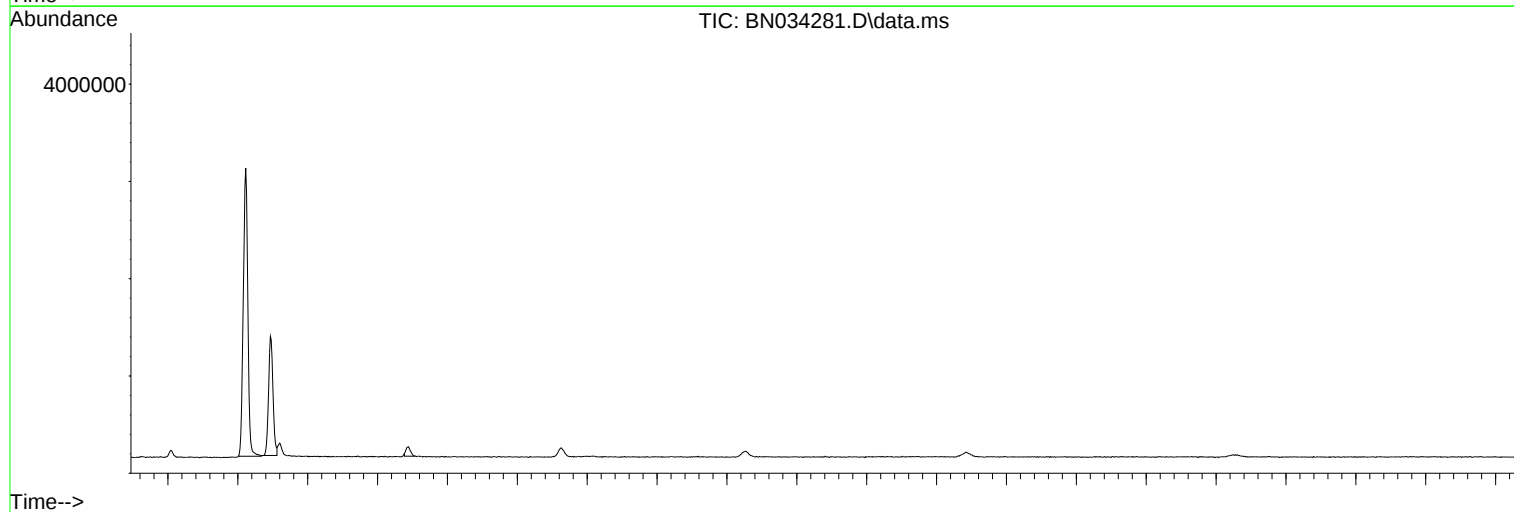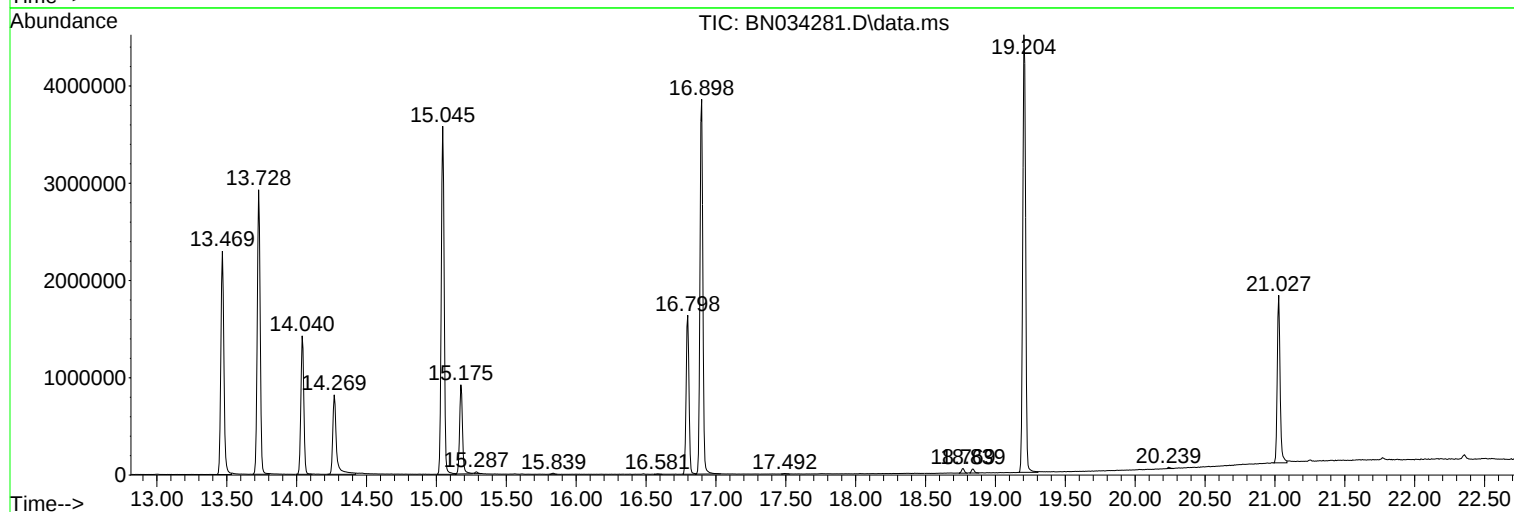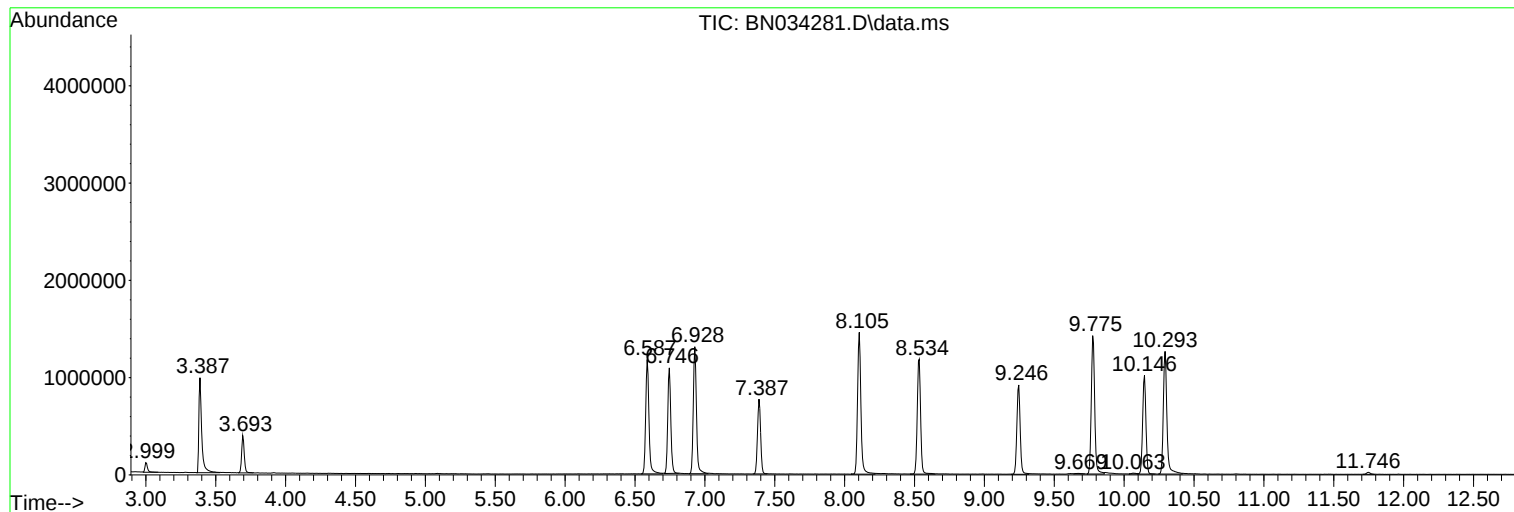

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN093024\
Data File : BN034281.D
Acq On : 30 Sep 2024 17:29
Operator : RC/JU
Sample : PB163394BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK394










Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Toluene Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.693	8.39 ng/ul	494182	1,4-Dichlorobenzene-d4	7.387

Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	Toluene	92	C7H8	000108-88-3	94
2	Toluene	92	C7H8	000108-88-3	93
3	Toluene	92	C7H8	000108-88-3	91
4	Toluene	92	C7H8	000108-88-3	91
5	Toluene	92	C7H8	000108-88-3	91

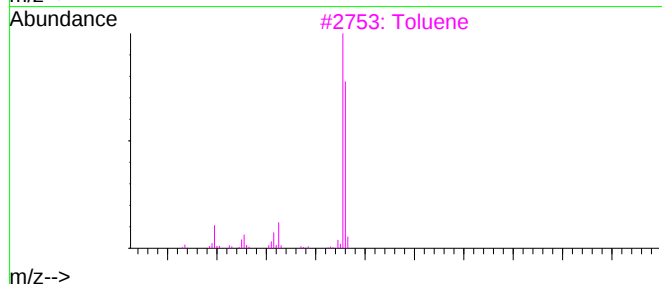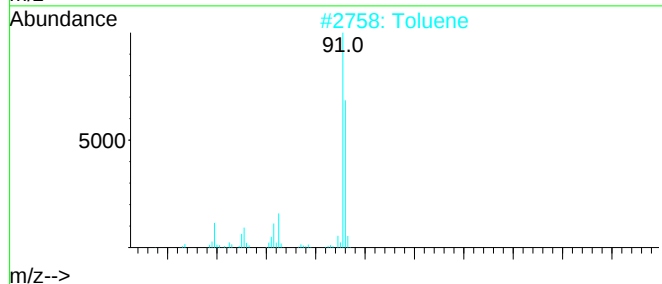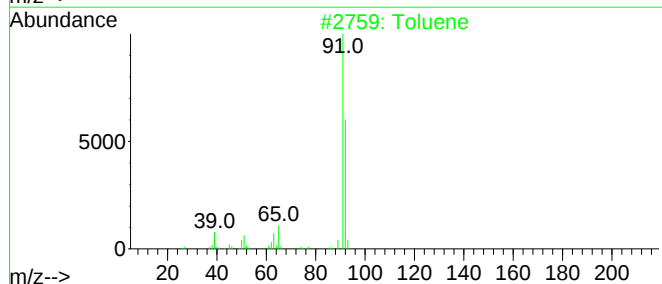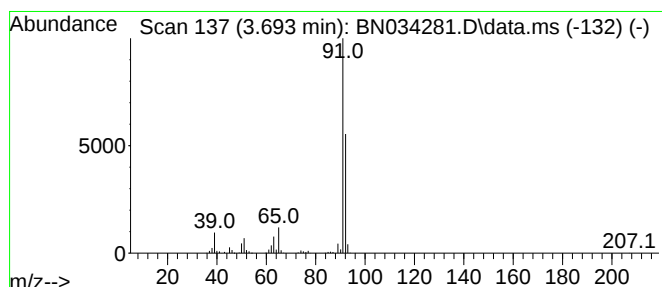

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN093024\
Data File : BN034281.D
Acq On : 30 Sep 2024 17:29
Operator : RC/JU
Sample : PB163394BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK394

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Toluene	3.693	8.4	ng/u1	494182	1	7.387	1177940	20.0