

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100124\
 Data File : BN034311.D
 Acq On : 01 Oct 2024 21:08
 Operator : RC/JU
 Sample : P4019-02
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DDC38

Quant Time: Oct 01 23:35:39 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Sep 30 14:14:38 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.393	152	214860	20.000	ng/ul	0.00
20) Naphthalene-d8	10.151	136	805875	20.000	ng/ul	# 0.01
38) Acenaphthene-d10	14.045	164	533271	20.000	ng/ul	0.00
64) Phenanthrene-d10	16.822	188	1056204	20.000	ng/ul	0.02
79) Chrysene-d12	21.033	240	1048248	20.000	ng/ul	0.00
88) Perylene-d12	23.745	264	1212373	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.017	96	3853	0.732	ng/uL	0.02
4) Pyridine-d5	3.387	84	988	0.063	ng/ul	0.00
7) Phenol-d5	6.605	99	83486	4.378	ng/ul	0.02
9) Bis-(2-Chloroethyl)eth...	6.746	67	78937	6.672	ng/ul	0.00
11) 2-Chlorophenol-d4	6.940	132	51011	3.398	ng/ul	0.01
15) 4-Methylphenol-d8	8.122	113	6778	0.432	ng/ul	0.02
21) Nitrobenzene-d5	8.540	128	28289	4.404	ng/ul	0.01
24) 2-Nitrophenol-d4	9.246	143	30873	4.674	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.793	165	44015	3.538	ng/ul	0.02
31) 4-Chloroaniline-d4	10.340	131	557	0.030	ng/ul	0.05
46) Dimethylphthalate-d6	13.469	166	190532	4.781	ng/ul	0.00
49) Acenaphthylene-d8	13.734	160	204251	4.556	ng/ul	0.00
54) 4-Nitrophenol-d4	14.287	143	85573	10.463	ng/ul	0.01
60) Fluorene-d10	15.051	176	170513	5.048	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.186	200	23460	3.725	ng/ul	0.01
73) Anthracene-d10	16.822	188	1056204	21.270	ng/ul	-0.08
81) Pyrene-d10	19.210	212	243746	4.173	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.557	264	170005	2.730	ng/ul	0.00
Target Compounds						
					Qvalue	
6) Benzaldehyde	6.563	77	247962	24.634	ng/ul#	1
16) Acetophenone	8.346	105	327006	13.156	ng/ul	90
17) N-Nitroso-di-n-propyla...	8.210	70	39834	3.236	ng/ul#	63
19) Hexachloroethane	8.493	117	339963	52.399	ng/ul#	11
22) Nitrobenzene	8.575	77	50047	3.113	ng/ul#	38
23) Isophorone	9.099	82	259093	8.739	ng/ul#	48
25) 2-Nitrophenol	9.299	139	9911	1.341	ng/ul#	1
26) 2,4-Dimethylphenol	9.369	107	54409	3.578	ng/ul#	63
29) 2,4-Dichlorophenol	9.822	162	29646	2.354	ng/ul#	74
30) Naphthalene	10.198	128	1452169	32.944	ng/ul	97
34) Caprolactam	11.093	113	28171	5.618	ng/ul#	1
35) 4-Chloro-3-methylphenol	11.481	107	21027	1.418	ng/ul#	30
36) 2-Methylnaphthalene	11.828	142	2123602	69.939	ng/ul	99
37) 1-Methylnaphthalene	12.051	142	1270027	41.322	ng/ul	98
41) 2,4,6-Trichlorophenol	12.469	196	25279	2.477	ng/ul	98
42) 2,4,5-Trichlorophenol	12.545	196	40969	3.654	ng/ul	97
43) 1,1'-Biphenyl	12.869	154	257616	6.408	ng/ul#	88
45) 2-Nitroaniline	13.098	65	22934	2.266	ng/ul#	1
48) 2,6-Dinitrotoluene	13.610	165	41191	5.150	ng/ul#	77
52) Acenaphthene	14.110	153	67706	1.933	ng/ul	90
53) 2,4-Dinitrophenol	14.157	184	7974	1.695	ng/ul#	1
55) 4-Nitrophenol	14.275	109	39514	5.689	ng/ul#	41
56) Dibenzofuran	14.451	168	119444	2.494	ng/ul#	58
57) 2,4-Dinitrotoluene	14.428	165	13679	1.134	ng/ul#	70

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100124\
 Data File : BN034311.D
 Acq On : 01 Oct 2024 21:08
 Operator : RC/JU
 Sample : P4019-02
 Misc :
 ALS Vial : 19 Sample Multiplier: 1


Instrument :
 BNA_N
 ClientSampleId :
 DDC38


Quant Time: Oct 01 23:35:39 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Sep 30 14:14:38 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
58) 2,3,4,6-Tetrachlorophenol	14.698	232	2723562	292.772	ng/ul	94
61) Fluorene	15.104	166	198383	5.063	ng/ul#	93
66) 4,6-Dinitro-2-methylph...	15.222	198	65549	9.373	ng/ul#	35
67) N-Nitrosodiphenylamine	15.334	169	244882	7.737	ng/ul#	38
69) Hexachlorobenzene	16.110	284	12534	1.007	ng/ul#	1
71) Pentachlorophenol	16.486	266	6601957	796.273	ng/ul	96
72) Phenanthrene	16.863	178	841482	14.449	ng/ul#	96
74) Anthracene	16.863	178	841482	14.150	ng/ul	96
86) Bis(2-ethylhexyl)phtha...	20.980	149	111483	2.314	ng/ul#	85

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Oct 01 23:35:39 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Sep 30 14:14:38 2024
Response via : Initial Calibration









#6
Benzaldehyde
Concen: 24.634 ng/ul
RT: 6.563 min Scan# 61
Delta R.T. 0.018 min
Lab File: BN034311.D
Acq: 01 Oct 2024 21:08




Instrument :
BNA_N
ClientSampleId :
DDC38


Tgt Ion: 77 Resp: 247962
Ion Ratio Lower Upper
77 100
105 846.1 76.4 114.6#
106 75.8 69.8 104.6

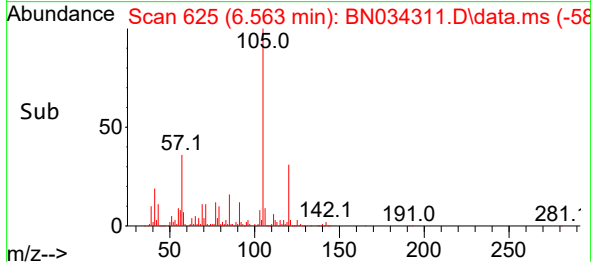

#16
Acetophenone
Concen: 13.156 ng/ul
RT: 8.346 min Scan# 928
Delta R.T. 0.141 min
Lab File: BN034311.D
Acq: 01 Oct 2024 21:08

Tgt Ion: 105 Resp: 327006
Ion Ratio Lower Upper
105 100
77 67.0 61.1 91.7
51 32.0 22.6 33.8


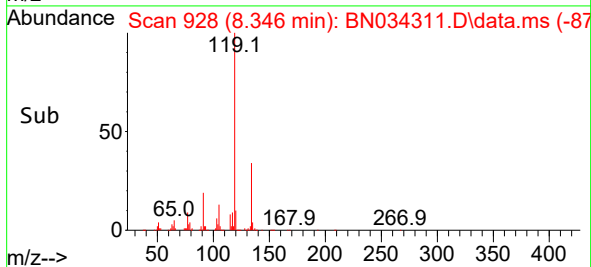

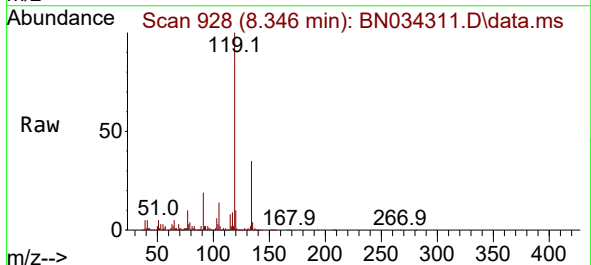




#17
N-Nitroso-di-n-propylamine
Concen: 3.236 ng/ul
RT: 8.210 min Scan# 902
Delta R.T. 0.012 min
Lab File: BN034311.D
Acq: 01 Oct 2024 21:08




Instrument :
BNA_N
ClientSampleId :
DDC38


Tgt Ion: 70 Resp: 39834
Ion Ratio Lower Upper
70 100
42 89.4 47.9 71.9#
101 3.8 7.5 11.3#
130 0.8 16.2 24.2#

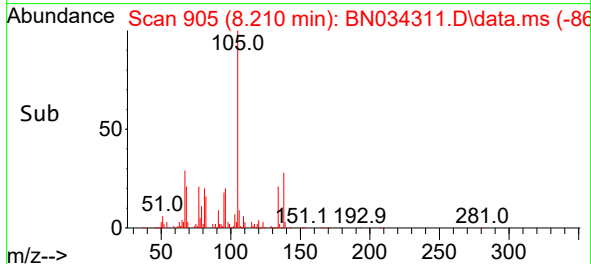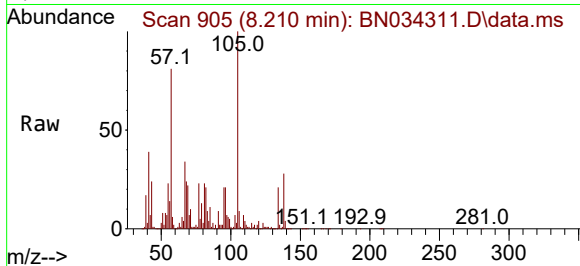

#19
Hexachloroethane
Concen: 52.399 ng/ul
RT: 8.493 min Scan# 953
Delta R.T. 0.053 min
Lab File: BN034311.D
Acq: 01 Oct 2024 21:08

Tgt Ion: 117 Resp: 339963
Ion Ratio Lower Upper
117 100
201 0.0 73.9 110.9#
199 0.0 44.0 66.0#


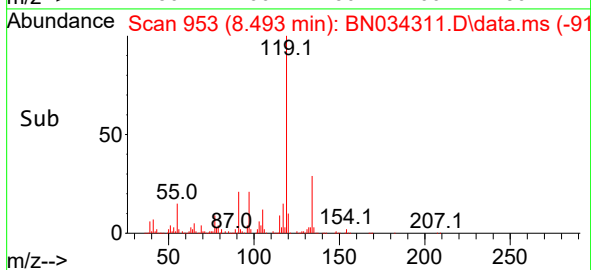

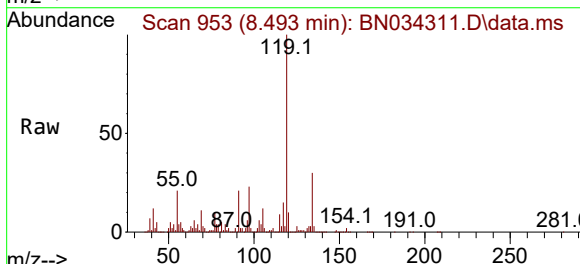




#22
Nitrobenzene
Concen: 3.113 ng/ul
RT: 8.575 min Scan# 90
Delta R.T. 0.006 min
Lab File: BN034311.D
Acq: 01 Oct 2024 21:08




Instrument :
BNA_N
ClientSampleId :
DDC38


Tgt Ion: 77 Resp: 50047
Ion Ratio Lower Upper
77 100
123 22.5 34.5 51.7#
65 76.5 11.0 16.6#

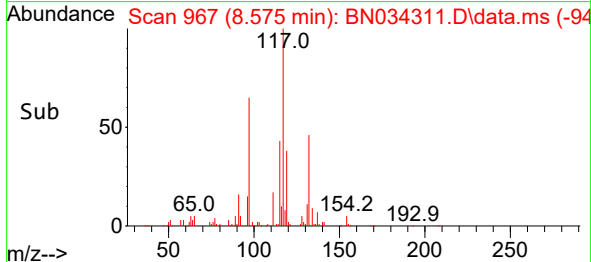

#23
Isophorone
Concen: 8.739 ng/ul
RT: 9.099 min Scan# 1056
Delta R.T. -0.000 min
Lab File: BN034311.D
Acq: 01 Oct 2024 21:08

Tgt Ion: 82 Resp: 259093
Ion Ratio Lower Upper
82 100
95 65.3 6.1 9.1#
138 17.2 13.4 20.0


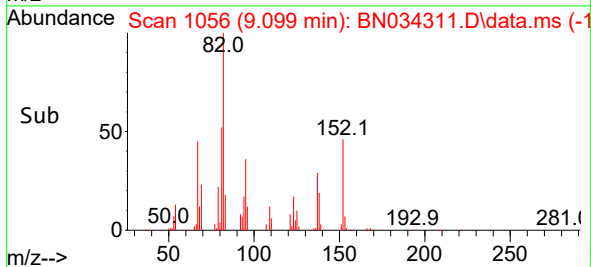

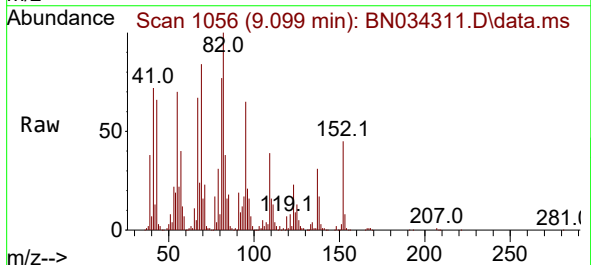




#25
2-Nitrophenol
Concen: 1.341 ng/ul
RT: 9.299 min Scan# 1100
Delta R.T. 0.023 min
Lab File: BN034311.D
Acq: 01 Oct 2024 21:08




Instrument :
BNA_N
ClientSampleId :
DDC38


Tgt Ion:139 Resp: 9911
Ion Ratio Lower Upper
139 100
65 224.0 42.0 63.0#
109 474.3 26.5 39.7#

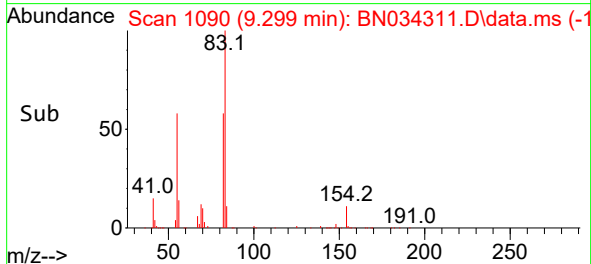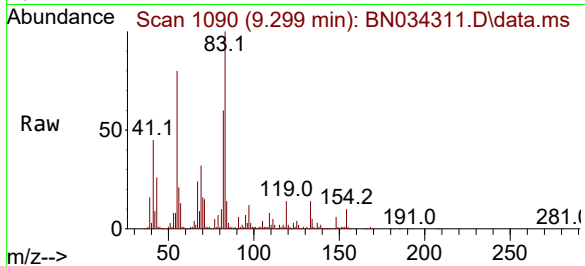

#26
2,4-Dimethylphenol
Concen: 3.578 ng/ul
RT: 9.369 min Scan# 1102
Delta R.T. 0.018 min
Lab File: BN034311.D
Acq: 01 Oct 2024 21:08

Tgt Ion:107 Resp: 54409
Ion Ratio Lower Upper
107 100
121 36.3 38.4 57.6#
122 35.6 62.9 94.3#

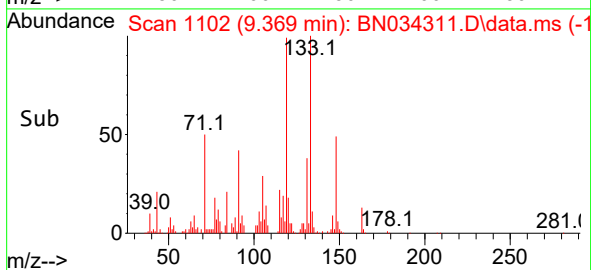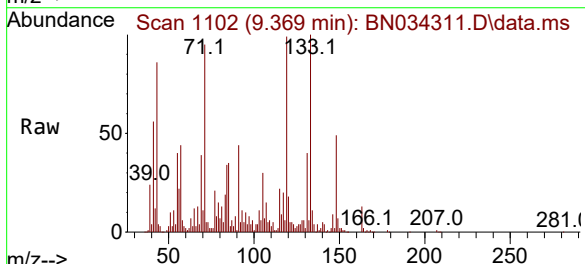



#29

2,4-Dichlorophenol

Concen: 2.354 ng/ul

RT: 9.822 min Scan# 1179

Delta R.T. 0.018 min

Lab File: BN034311.D

Acq: 01 Oct 2024 21:08

Instrument :

BNA_N

ClientSampleId :

DDC38





Tgt Ion:162 Resp: 29646

Ion Ratio Lower Upper

162 100

164 40.3 53.0 79.6#

98 46.8 30.6 46.0#

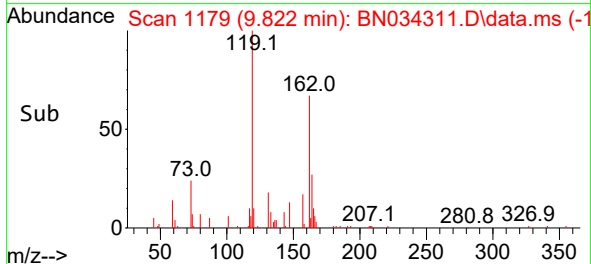

#30

Naphthalene

Concen: 32.944 ng/ul

RT: 10.198 min Scan# 1243

Delta R.T. 0.006 min

Lab File: BN034311.D

Acq: 01 Oct 2024 21:08




Tgt Ion:128 Resp: 1452169


Ion Ratio Lower Upper

128 100

129 12.1 8.7 13.1

127 14.3 10.6 16.0



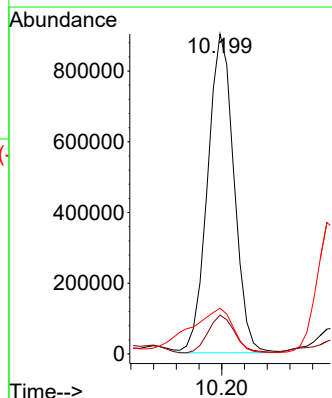
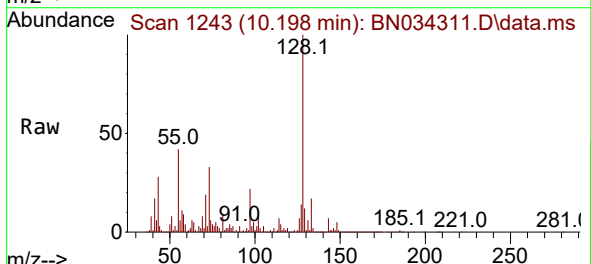




#34
Caprolactam
Concen: 5.618 ng/ul
RT: 11.093 min Scan# 11
Delta R.T. 0.006 min
Lab File: BN034311.D
Acq: 01 Oct 2024 21:08




Instrument :
BNA_N
ClientSampleId :
DDC38


Tgt Ion:113 Resp: 28171
Ion Ratio Lower Upper
113 100
55 893.6 137.0 205.6#
56 486.8 99.7 149.5#

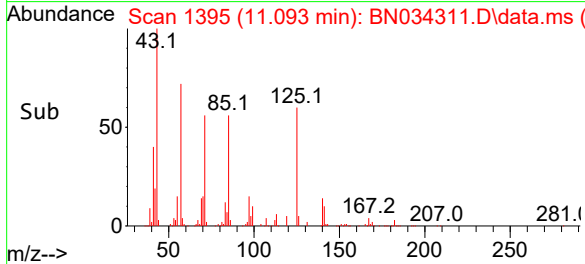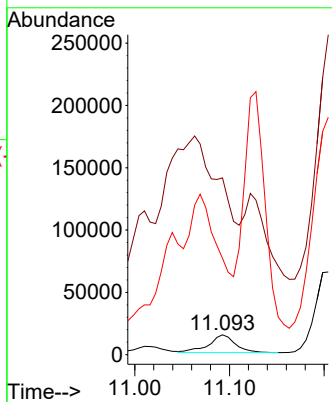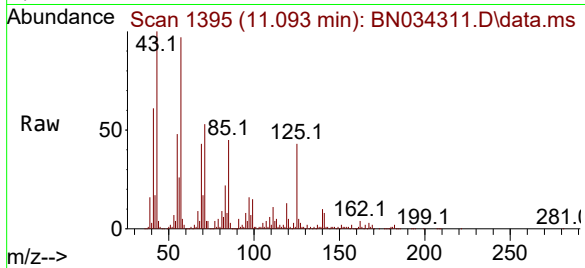

#35
4-Chloro-3-methylphenol
Concen: 1.418 ng/ul
RT: 11.481 min Scan# 1461
Delta R.T. 0.029 min
Lab File: BN034311.D
Acq: 01 Oct 2024 21:08

Tgt Ion:107 Resp: 21027
Ion Ratio Lower Upper
107 100
144 8.5 19.1 28.7#
142 5.6 61.4 92.0#


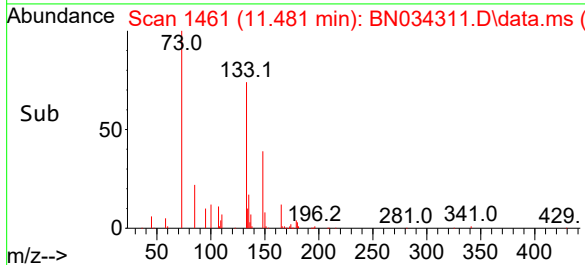

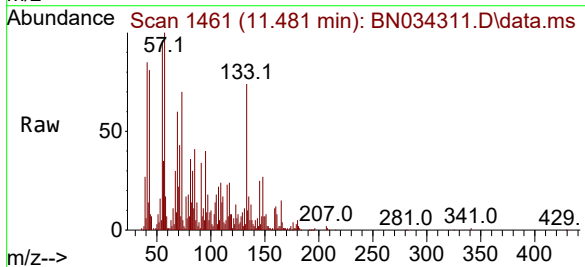




#36
2-Methylnaphthalene
Concen: 69.939 ng/ul
RT: 11.828 min Scan# 1520
Delta R.T. 0.012 min
Lab File: BN034311.D
Acq: 01 Oct 2024 21:08




Instrument :
BNA_N
ClientSampleId :
DDC38


Tgt Ion:142 Resp: 2123602
Ion Ratio Lower Upper
142 100
141 89.1 72.2 108.2

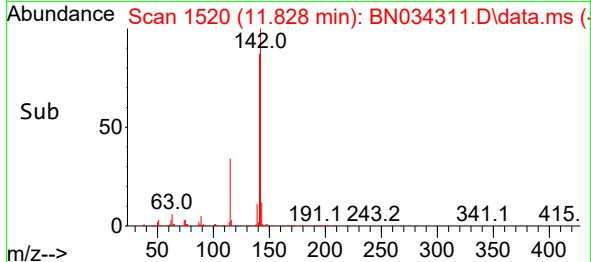

#37
1-Methylnaphthalene
Concen: 41.322 ng/ul
RT: 12.051 min Scan# 1558
Delta R.T. 0.012 min
Lab File: BN034311.D
Acq: 01 Oct 2024 21:08

Tgt Ion:142 Resp: 1270027
Ion Ratio Lower Upper
142 100
141 92.5 72.5 108.7
116 3.9 3.2 4.8

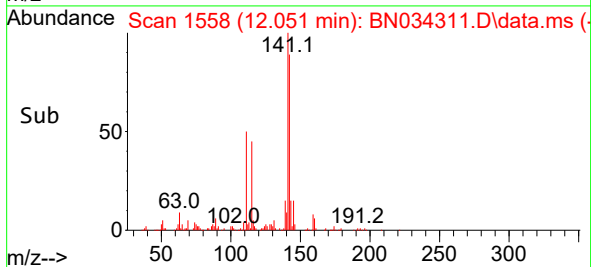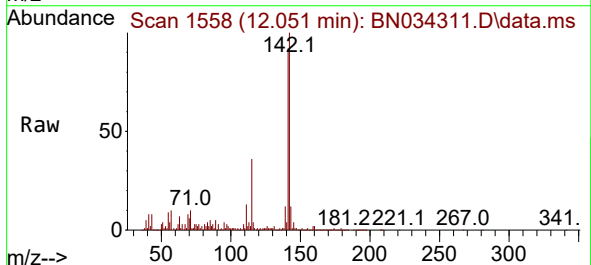



#41

2,4,6-Trichlorophenol

Concen: 2.477 ng/ul

RT: 12.469 min Scan# 1626

Delta R.T. 0.018 min

Lab File: BN034311.D

Acq: 01 Oct 2024 21:08

Instrument :

BNA_N

ClientSampleId :

DDC38





Tgt Ion:196 Resp: 25279

Ion Ratio Lower Upper

196 100

198 90.9 75.0 112.4

200 31.1 24.7 37.1

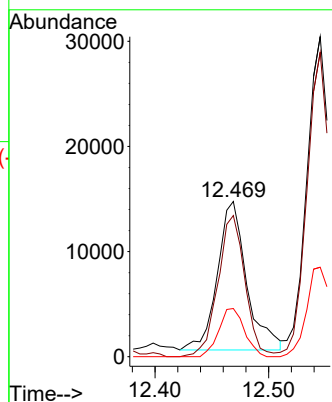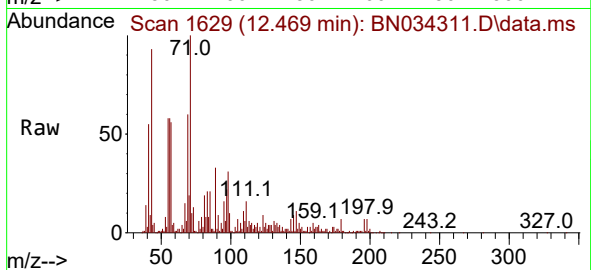

#42

2,4,5-Trichlorophenol

Concen: 3.654 ng/ul

RT: 12.545 min Scan# 1642

Delta R.T. 0.023 min

Lab File: BN034311.D

Acq: 01 Oct 2024 21:08




Tgt Ion:196 Resp: 40969


Ion Ratio Lower Upper

196 100

198 95.1 77.1 115.7

200 28.0 25.2 37.8


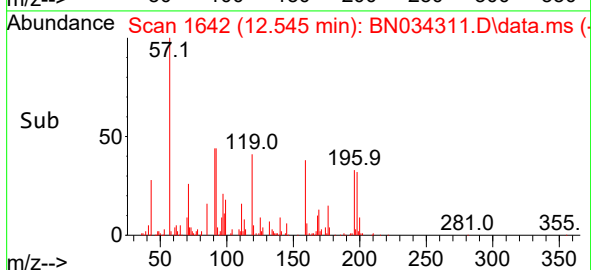

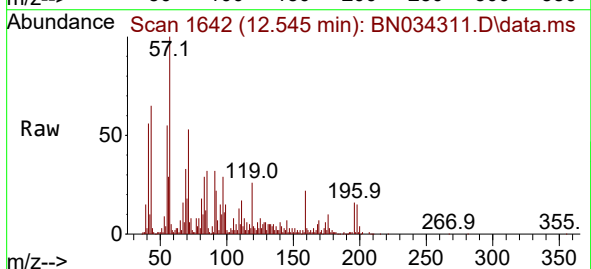




#43
1,1'-Biphenyl
Concen: 6.408 ng/ul
RT: 12.869 min Scan# 1696
Delta R.T. 0.006 min
Lab File: BN034311.D
Acq: 01 Oct 2024 21:08




Instrument :
BNA_N
ClientSampleId :
DDC38


Tgt Ion:154 Resp: 257616
Ion Ratio Lower Upper
154 100
153 51.3 33.3 49.9#
76 12.3 10.2 15.4

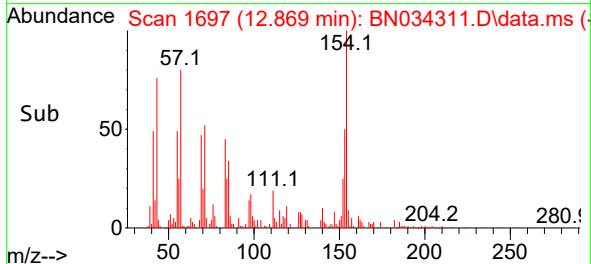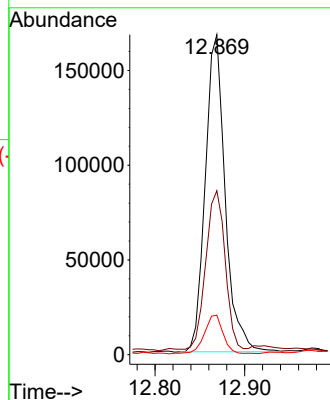

#45
2-Nitroaniline
Concen: 2.266 ng/ul
RT: 13.098 min Scan# 1736
Delta R.T. -0.018 min
Lab File: BN034311.D
Acq: 01 Oct 2024 21:08

Tgt Ion: 65 Resp: 22934
Ion Ratio Lower Upper
65 100
92 27.8 53.2 79.8#
138 239.7 80.9 121.3#

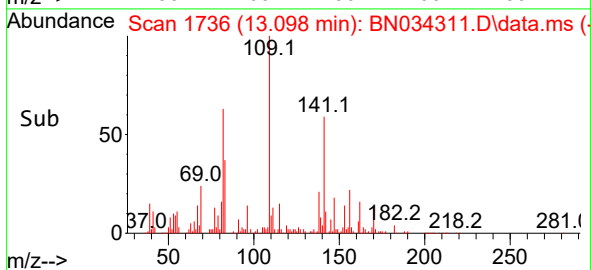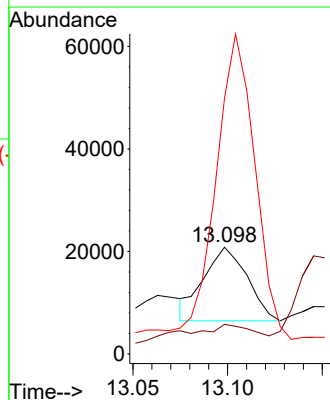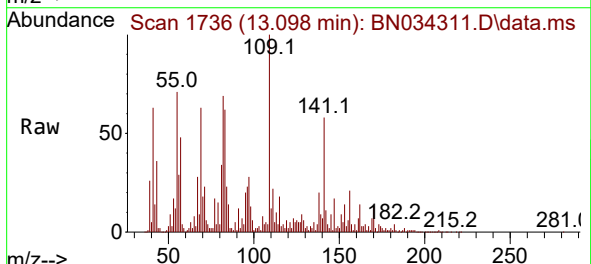



#48

2,6-Dinitrotoluene

Concen: 5.150 ng/ul

RT: 13.610 min Scan# 1823

Delta R.T. -0.024 min

Lab File: BN034311.D

Acq: 01 Oct 2024 21:08

Instrument :

BNA_N

ClientSampleId :

DDC38





Tgt Ion:165 Resp: 41191

Ion Ratio Lower Upper

165 100

89 62.9 48.6 72.8

121 59.8 19.0 28.6#

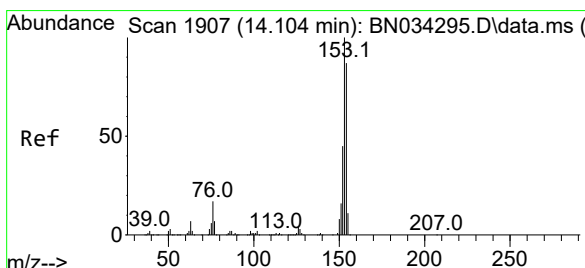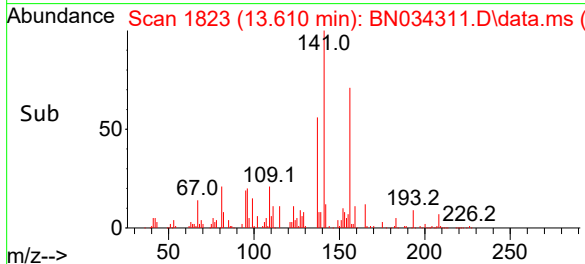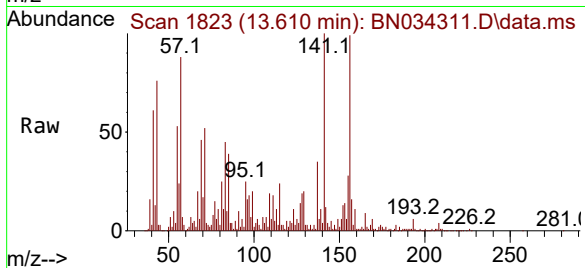

#52

Acenaphthene

Concen: 1.933 ng/ul

RT: 14.110 min Scan# 1908

Delta R.T. 0.006 min

Lab File: BN034311.D

Acq: 01 Oct 2024 21:08




Tgt Ion:153 Resp: 67706


Ion Ratio Lower Upper

153 100

152 55.8 37.8 56.8

154 80.6 71.2 106.8


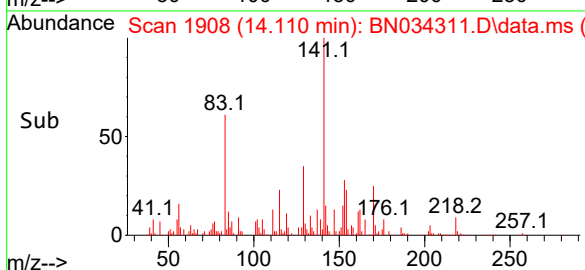

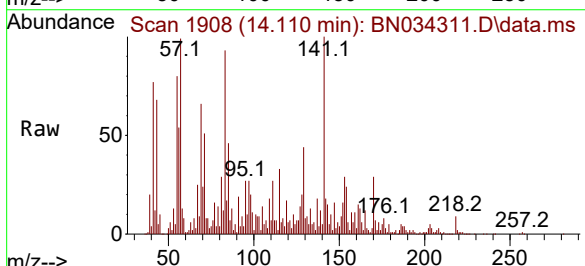


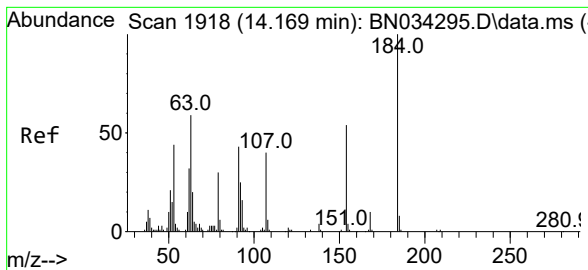

#53
2,4-Dinitrophenol
Concen: 1.695 ng/ul
RT: 14.157 min Scan# 1916
Delta R.T. -0.012 min
Lab File: BN034311.D
Acq: 01 Oct 2024 21:08




Instrument :
BNA_N
ClientSampleId :
DDC38


Tgt Ion:184 Resp: 7974
Ion Ratio Lower Upper
184 100
63 162.1 61.1 91.7#
154 162.4 58.5 87.7#

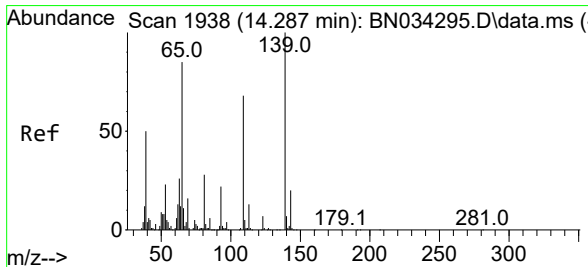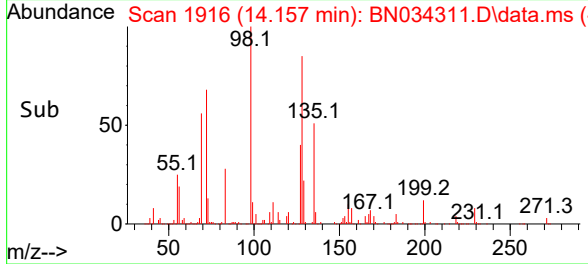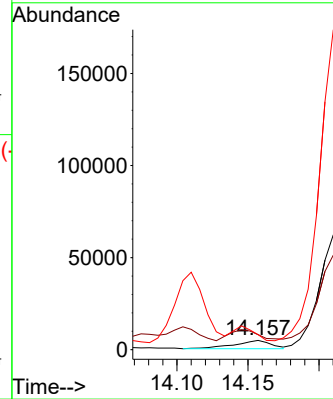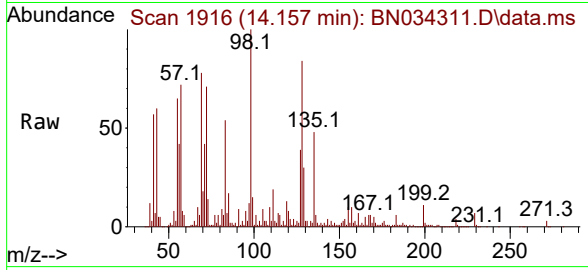

#55
4-Nitrophenol
Concen: 5.689 ng/ul
RT: 14.275 min Scan# 1936
Delta R.T. -0.012 min
Lab File: BN034311.D
Acq: 01 Oct 2024 21:08

Tgt Ion:109 Resp: 39514
Ion Ratio Lower Upper
109 100
139 66.0 102.8 154.2#
65 49.4 97.7 146.5#


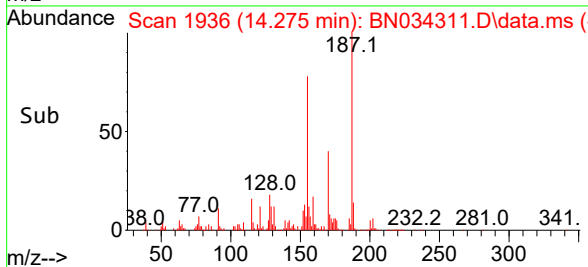
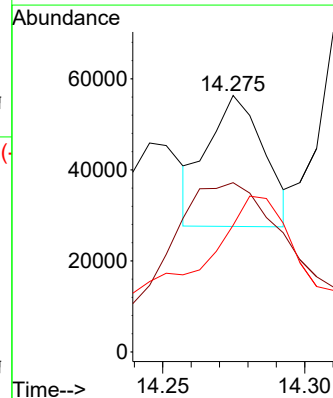
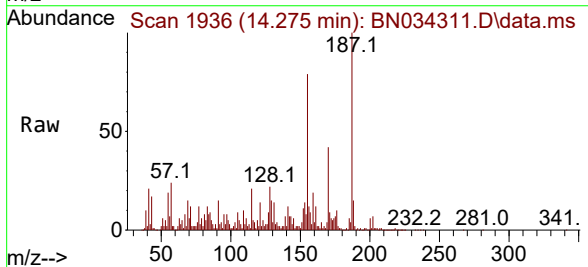




#56
Dibenzenofuran
Concen: 2.494 ng/ul
RT: 14.451 min Scan# 1966
Delta R.T. 0.006 min
Lab File: BN034311.D
Acq: 01 Oct 2024 21:08




Instrument :
BNA_N
ClientSampleId :
DDC38


Tgt Ion:168 Resp: 119444
Ion Ratio Lower Upper
168 100
139 65.2 31.7 47.5#

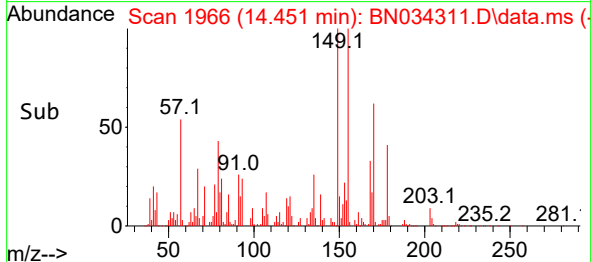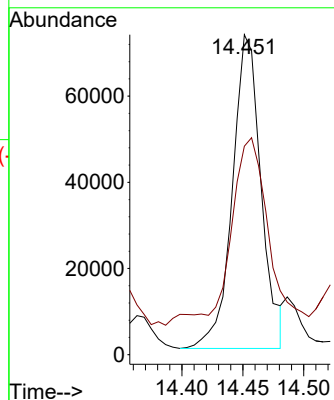

#57
2,4-Dinitrotoluene
Concen: 1.134 ng/ul
RT: 14.428 min Scan# 1962
Delta R.T. -0.000 min
Lab File: BN034311.D
Acq: 01 Oct 2024 21:08


Tgt Ion:165 Resp: 13679
Ion Ratio Lower Upper
165 100
63 57.6 37.8 56.8#
182 90.8 2.3 3.5#

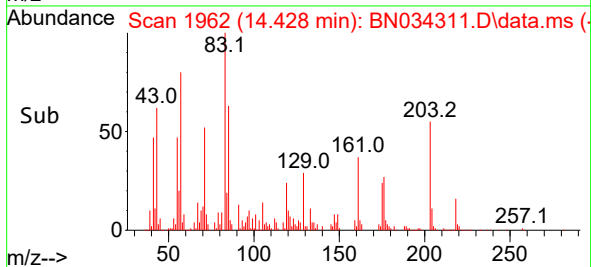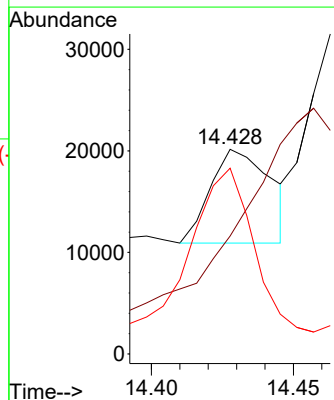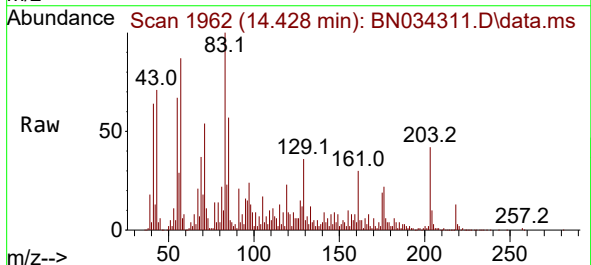






#58
2,3,4,6-Tetrachlorophenol
Concen: 292.772 ng/ul
RT: 14.698 min Scan# 2008
Delta R.T. 0.018 min
Lab File: BN034311.D
Acq: 01 Oct 2024 21:08


Instrument :
BNA_N
ClientSampleId :
DDC38





Tgt Ion:232 Resp: 2723562
Ion Ratio Lower Upper
232 100
131 45.3 41.0 61.6
130 3.1 2.2 3.2
166 31.9 27.1 40.7

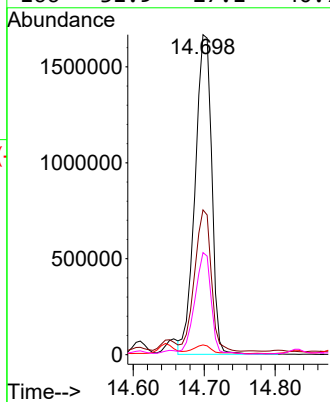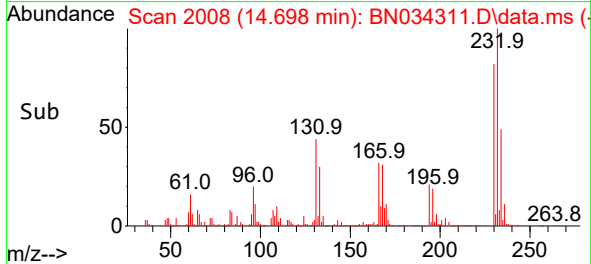


#61
Fluorene
Concen: 5.063 ng/ul
RT: 15.104 min Scan# 2077
Delta R.T. 0.006 min
Lab File: BN034311.D
Acq: 01 Oct 2024 21:08

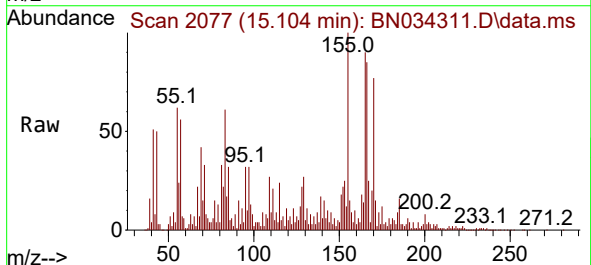

Tgt Ion:166 Resp: 198383
Ion Ratio Lower Upper
166 100
165 105.3 81.9 122.9
167 29.4 10.9 16.3#



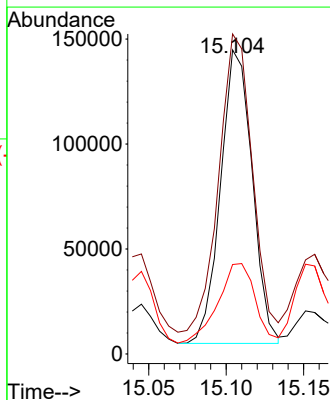
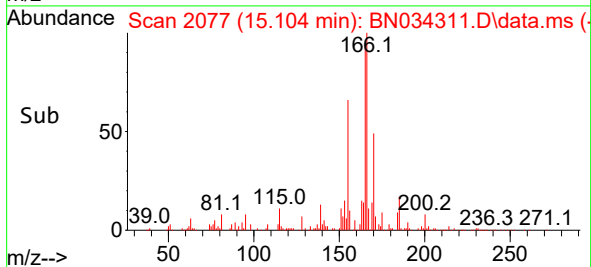




#66
4,6-Dinitro-2-methylphenol
Concen: 9.373 ng/ul
RT: 15.222 min Scan# 2097
Delta R.T. 0.029 min
Lab File: BN034311.D
Acq: 01 Oct 2024 21:08




Instrument :
BNA_N
ClientSampleId :
DDC38


Tgt Ion:198 Resp: 65549
Ion Ratio Lower Upper
198 100
182 7.2 3.2 4.8#
77 63.8 21.1 31.7#

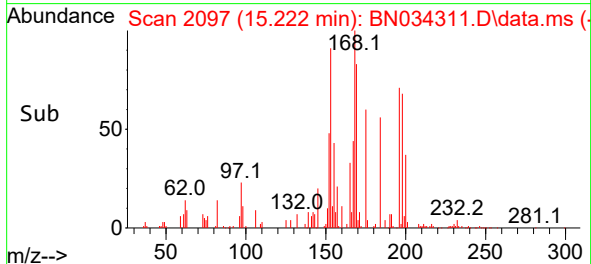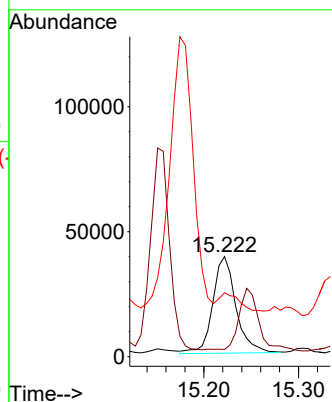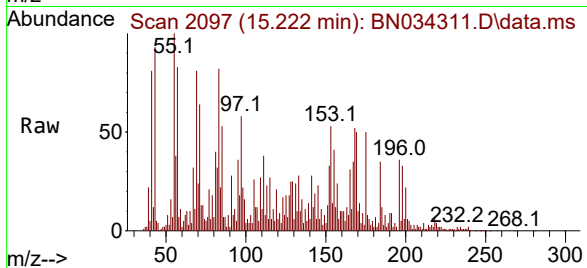

#67
N-Nitrosodiphenylamine
Concen: 7.737 ng/ul
RT: 15.334 min Scan# 2116
Delta R.T. 0.012 min
Lab File: BN034311.D
Acq: 01 Oct 2024 21:08

Tgt Ion:169 Resp: 244882
Ion Ratio Lower Upper
169 100
168 8.9 52.8 79.2#
167 9.3 28.6 43.0#


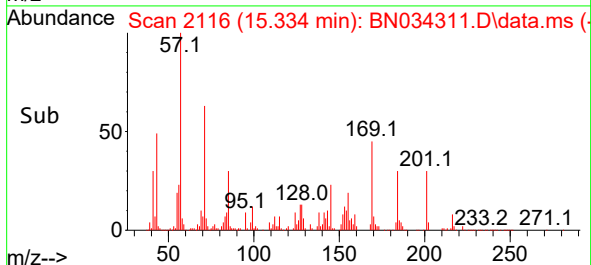

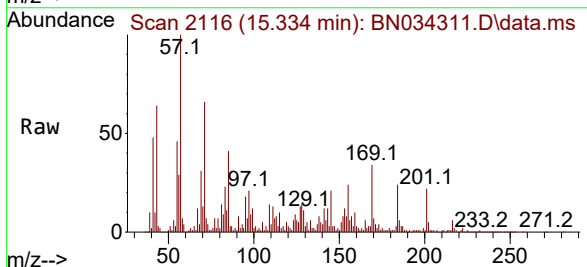




#69
Hexachlorobenzene
Concen: 1.007 ng/ul
RT: 16.110 min Scan# 2112
Delta R.T. 0.006 min
Lab File: BN034311.D
Acq: 01 Oct 2024 21:08




Instrument :
BNA_N
ClientSampleId :
DDC38


Tgt Ion:284 Resp: 12534
Ion Ratio Lower Upper
284 100
142 177.9 31.3 46.9#
249 35.6 25.1 37.7

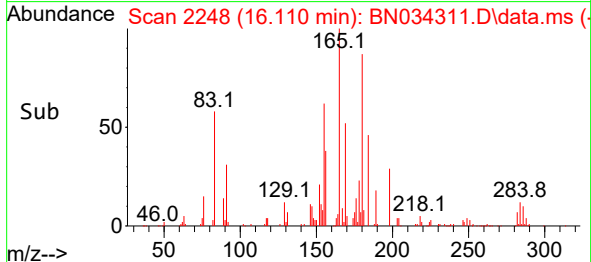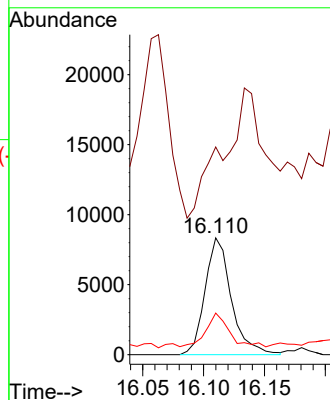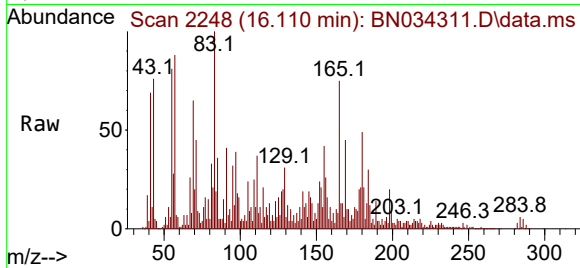

#71
Pentachlorophenol
Concen: 796.273 ng/ul
RT: 16.486 min Scan# 2312
Delta R.T. 0.029 min
Lab File: BN034311.D
Acq: 01 Oct 2024 21:08

Tgt Ion:266 Resp: 6601957
Ion Ratio Lower Upper
266 100
264 61.9 51.1 76.7
268 62.5 52.8 79.2


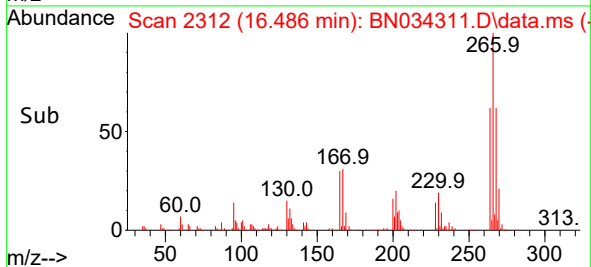
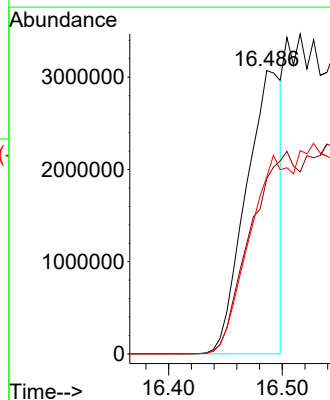
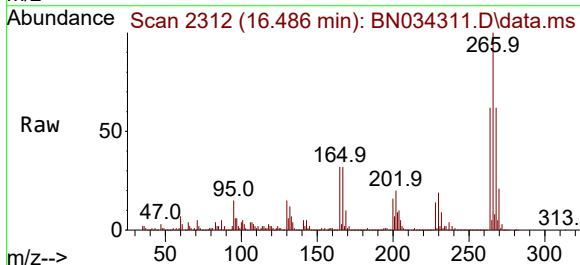




#72
Phenanthrene
Concen: 14.449 ng/ul
RT: 16.863 min Scan# 21
Delta R.T. 0.023 min
Lab File: BN034311.D
Acq: 01 Oct 2024 21:08




Instrument :
BNA_N
ClientSampleId :
DDC38


Tgt Ion:178 Resp: 841482
Ion Ratio Lower Upper
178 100
179 18.1 11.9 17.9#
176 19.3 15.2 22.8

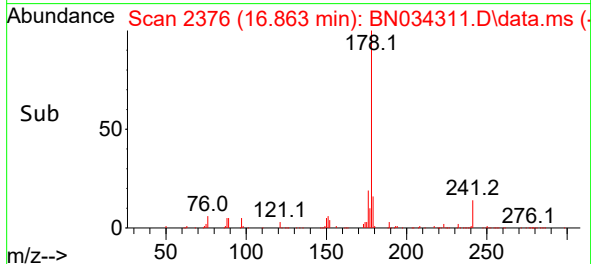

#74
Anthracene
Concen: 14.150 ng/ul
RT: 16.863 min Scan# 2376
Delta R.T. -0.071 min
Lab File: BN034311.D
Acq: 01 Oct 2024 21:08

Tgt Ion:178 Resp: 841482
Ion Ratio Lower Upper
178 100
179 18.1 12.2 18.2
176 19.3 15.0 22.6

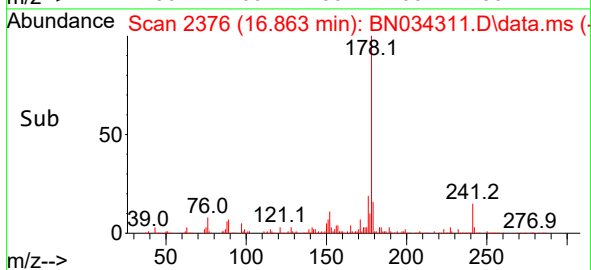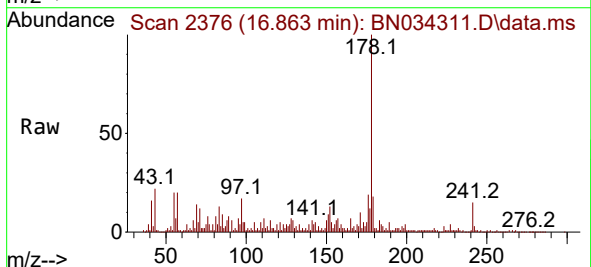



#86
 Bis(2-ethylhexyl)phthalate
 Concen: 2.314 ng/ul
 RT: 20.980 min Scan# 3076
 Delta R.T. -0.000 min
 Lab File: BN034311.D
 Acq: 01 Oct 2024 21:08

Instrument :
 BNA_N
 ClientSampleId :
 DDC38

Tgt Ion:149 Resp: 111483
 Ion Ratio Lower Upper
 149 100
 167 33.9 20.6 31.0#
 279 7.3 3.0 4.6#

