




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100124\
Data File : BN034303.D
Acq On : 01 Oct 2024 15:14
Operator : RC/JU
Sample : P4019-18
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DDCF2

Manual IntegrationsAPPROVED

Quant Time: Oct 01 23:33:49 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Sep 30 14:14:38 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/02/2024
Supervised By :mohammad ahmed 10/04/2024

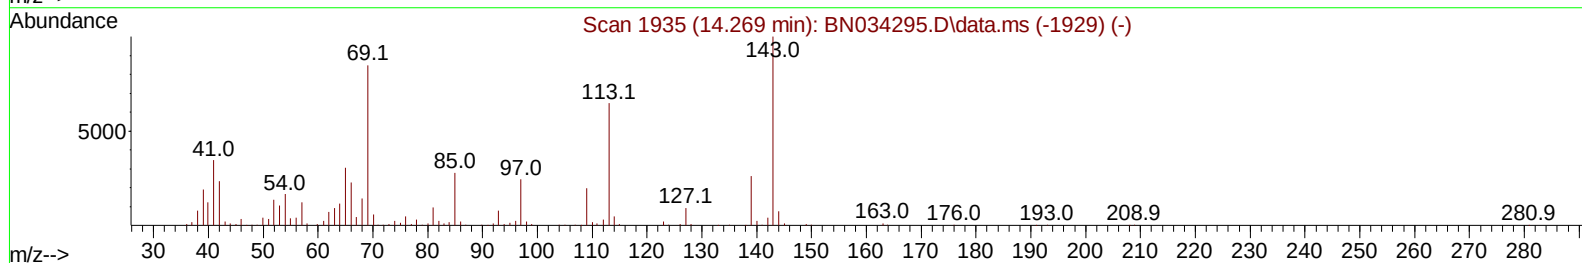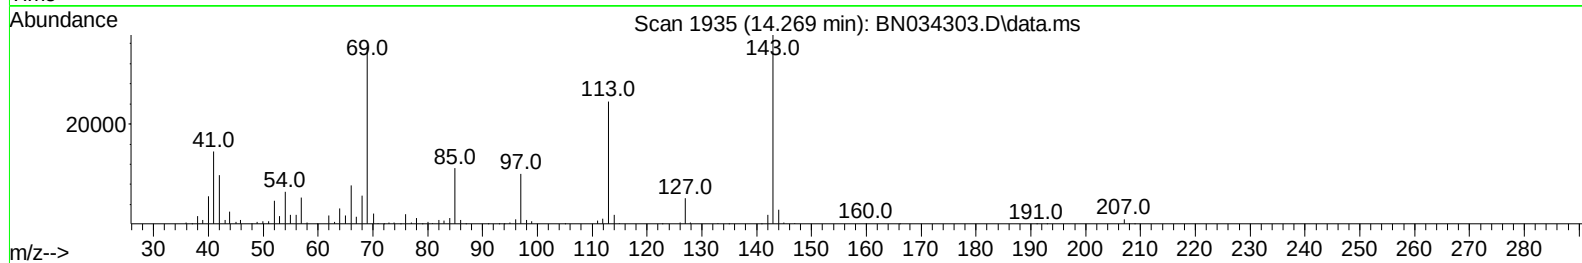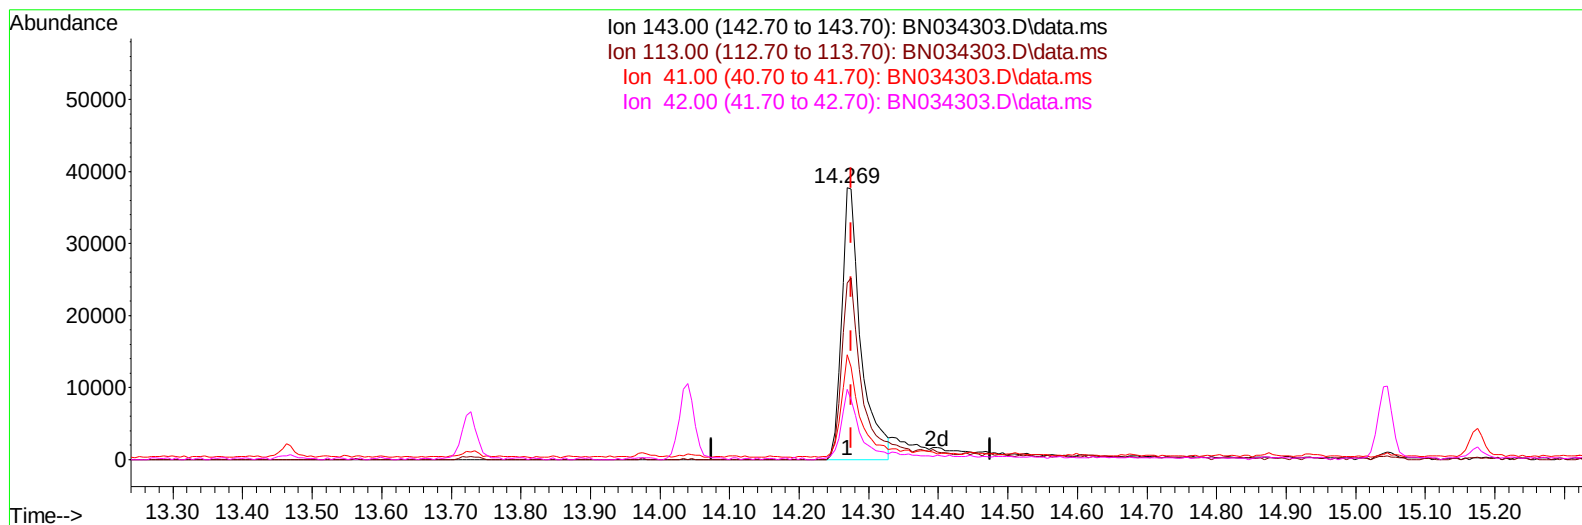

TIC: BN034303.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.269min (-0.006) 7.35 ng/u1

response 71754

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	76.90	64.98
41.00	41.70	38.47
42.00	28.50	25.93




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100124\
Data File : BN034303.D
Acq On : 01 Oct 2024 15:14
Operator : RC/JU
Sample : P4019-18
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DDCF2

Manual IntegrationsAPPROVED

Quant Time: Oct 01 23:33:49 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Sep 30 14:14:38 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/02/2024
Supervised By :mohammad ahmed 10/04/2024

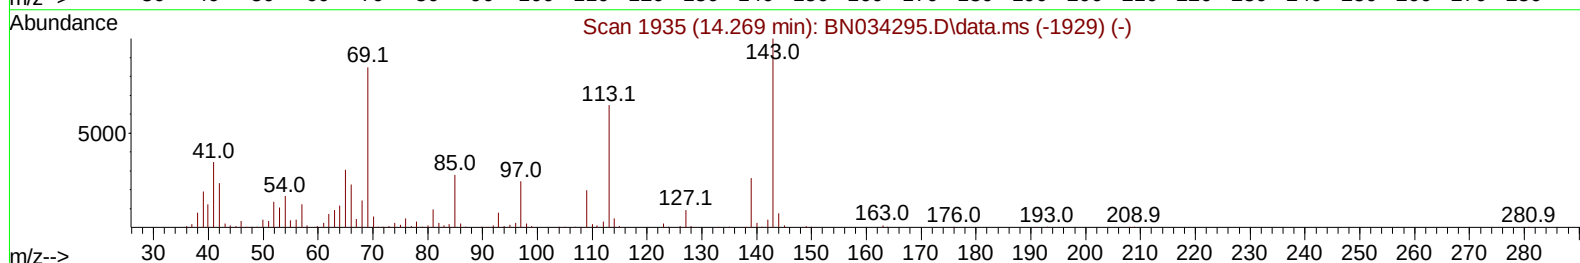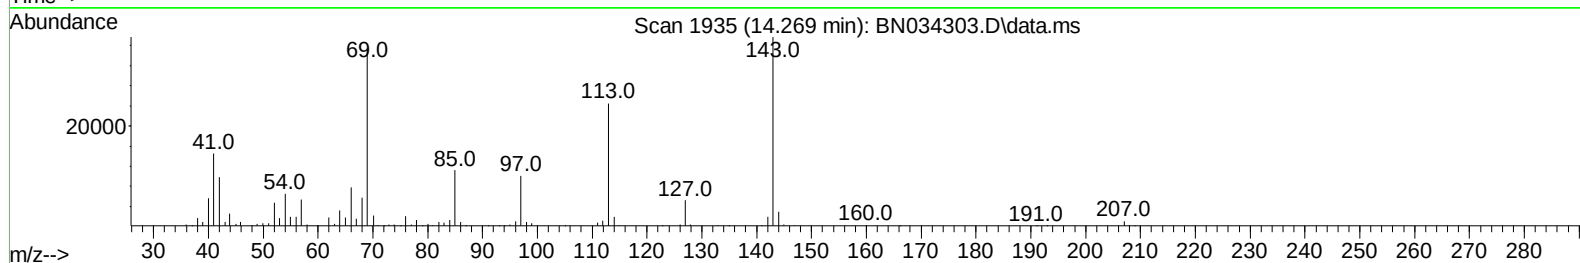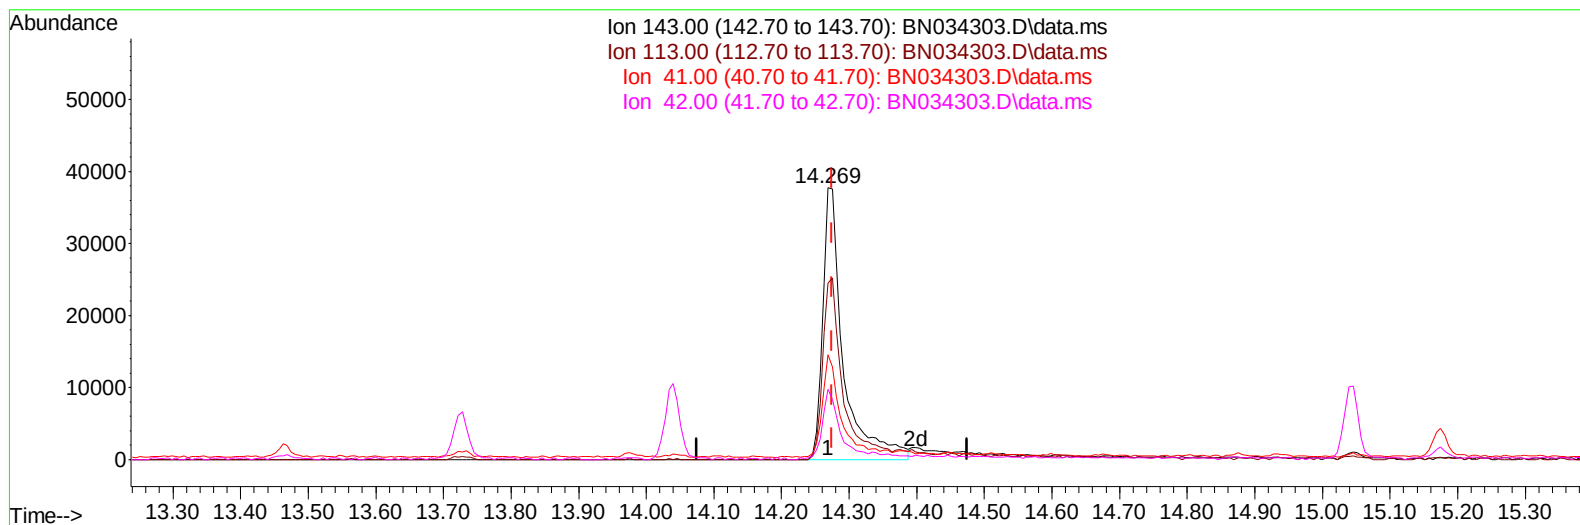

TIC: BN034303.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.269min (-0.006) 8.15 ng/ul m

response 79535

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	76.90	64.98
41.00	41.70	38.47
42.00	28.50	25.93

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100124\
 Data File : BN034303.D
 Acq On : 01 Oct 2024 15:14
 Operator : RC/JU
 Sample : P4019-18
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DDCF2

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 10/02/2024
 Supervised By :mohammad ahmed 10/04/2024

Quant Time: Oct 02 00:00:34 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Sep 30 14:14:38 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.387	152	258892	20.000	ng/ul	0.00
20) Naphthalene-d8	10.146	136	1036290	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.040	164	636322	20.000	ng/ul	0.00
64) Phenanthrene-d10	16.798	188	1274903	20.000	ng/ul	0.00
79) Chrysene-d12	21.027	240	1186391	20.000	ng/ul	0.00
88) Perylene-d12	23.739	264	1393001	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.005	96	17306	2.728	ng/uL	0.00
4) Pyridine-d5	3.393	84	91499	4.852	ng/ul	0.00
7) Phenol-d5	6.587	99	303356	13.203	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.740	67	192514	13.504	ng/ul	0.00
11) 2-Chlorophenol-d4	6.928	132	283945	15.700	ng/ul	0.00
15) 4-Methylphenol-d8	8.105	113	258080	13.651	ng/ul	0.00
21) Nitrobenzene-d5	8.528	128	133114	16.116	ng/ul	0.00
24) 2-Nitrophenol-d4	9.240	143	141159	16.619	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.775	165	254960	15.939	ng/ul	0.00
31) 4-Chloroaniline-d4	10.293	131	359535	14.846	ng/ul	0.00
46) Dimethylphthalate-d6	13.469	166	806286	16.955	ng/ul	0.00
49) Acenaphthylene-d8	13.728	160	943679	17.640	ng/ul	0.00
54) 4-Nitrophenol-d4	14.269	143	79535m	8.150	ng/ul	0.00
60) Fluorene-d10	15.045	176	705764	17.512	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.175	200	70442	9.267	ng/ul	0.00
73) Anthracene-d10	16.892	188	1076592	17.961	ng/ul	0.00
81) Pyrene-d10	19.204	212	1234447	18.675	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.557	264	1292306	18.060	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100124\
Data File : BN034303.D
Acq On : 01 Oct 2024 15:14
Operator : RC/JU
Sample : P4019-18
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DDCF2

Manual IntegrationsAPPROVED

Quant Time: Oct 02 00:00:34 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Sep 30 14:14:38 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/02/2024
Supervised By :mohammad ahmed 10/04/2024

