




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100124\
Data File : BN034304.D
Acq On : 01 Oct 2024 15:53
Operator : RC/JU
Sample : P4019-19
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DDCF3

Manual IntegrationsAPPROVED

Quant Time: Oct 01 23:33:57 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Sep 30 14:14:38 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/02/2024
Supervised By :mohammad ahmed 10/04/2024

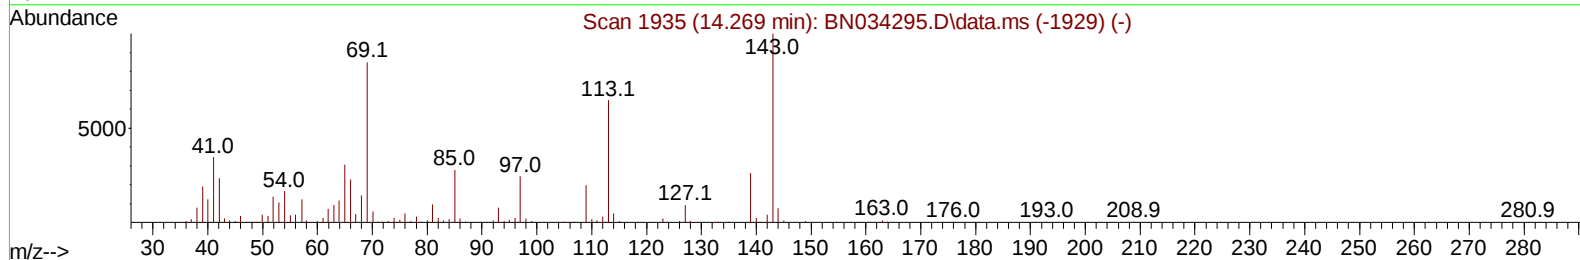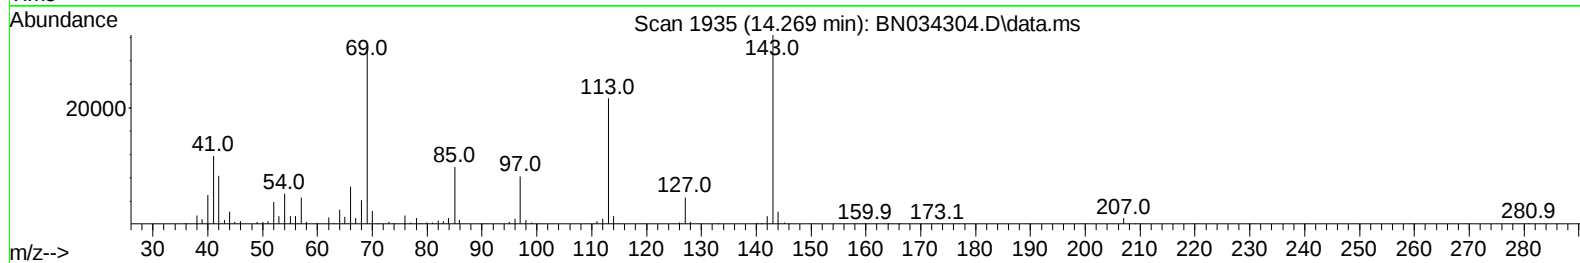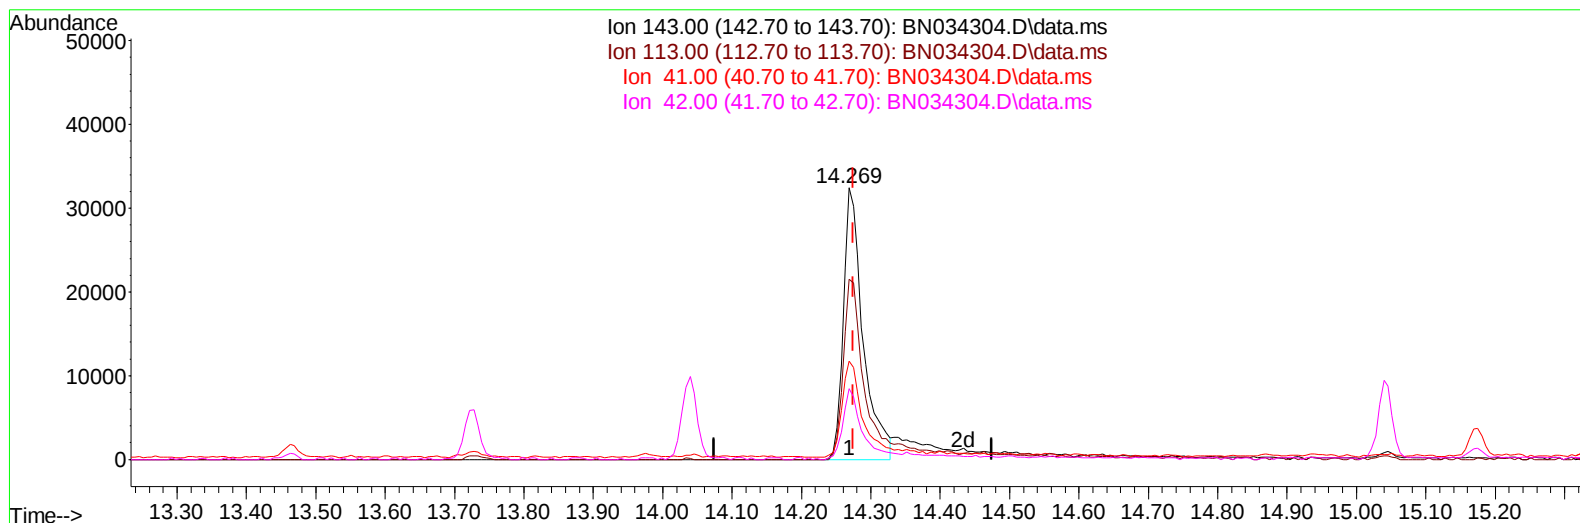

TIC: BN034304.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.269min (-0.006) 6.96 ng/u1

response 63898

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	76.90	66.46
41.00	41.70	36.17
42.00	28.50	25.96




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100124\
Data File : BN034304.D
Acq On : 01 Oct 2024 15:53
Operator : RC/JU
Sample : P4019-19
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DDCF3

Manual IntegrationsAPPROVED

Quant Time: Oct 01 23:33:57 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Sep 30 14:14:38 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/02/2024
Supervised By :mohammad ahmed 10/04/2024

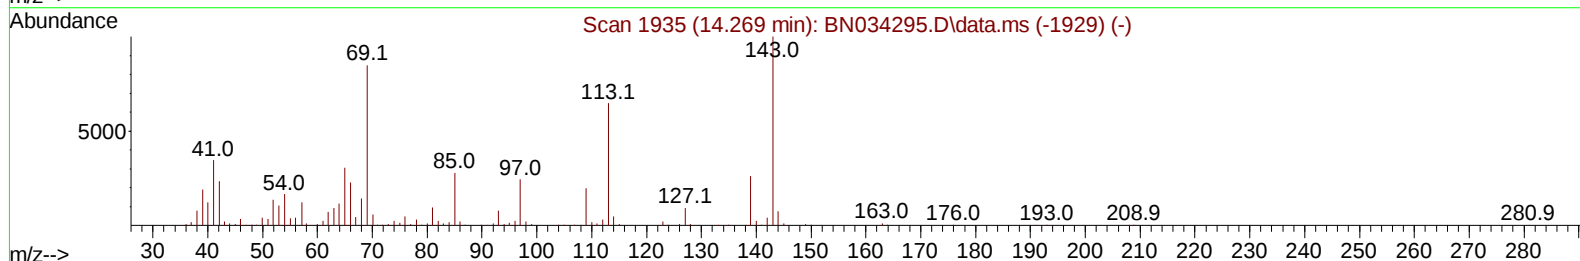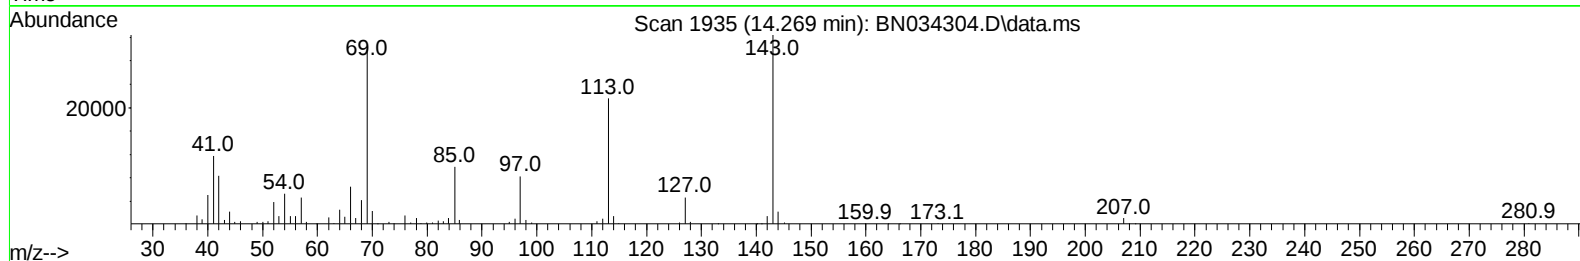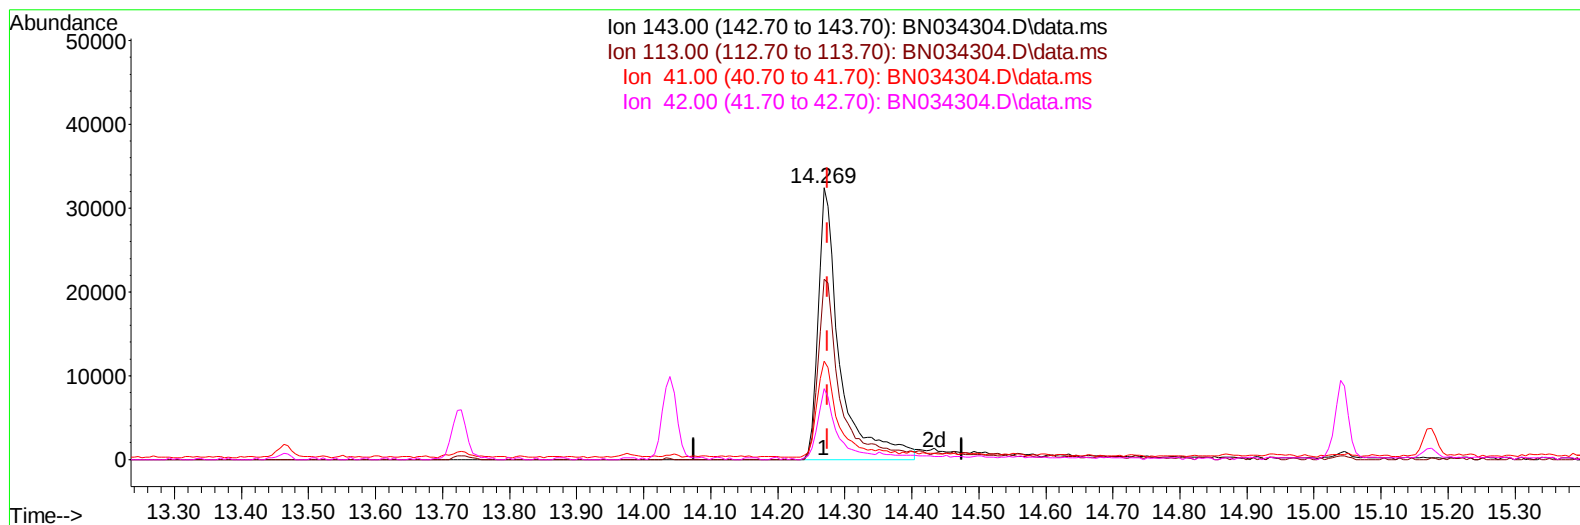

TIC: BN034304.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.269min (-0.006) 7.94 ng/ul m

response 72853

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	76.90	66.46
41.00	41.70	36.17
42.00	28.50	25.96

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100124\
 Data File : BN034304.D
 Acq On : 01 Oct 2024 15:53
 Operator : RC/JU
 Sample : P4019-19
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DDCF3

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 10/02/2024
 Supervised By :mohammad ahmed 10/04/2024

Quant Time: Oct 02 00:01:43 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Sep 30 14:14:38 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.387	152	243329	20.000	ng/ul	0.00
20) Naphthalene-d8	10.146	136	980111	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.039	164	598213	20.000	ng/ul	0.00
64) Phenanthrene-d10	16.798	188	1192935	20.000	ng/ul	0.00
79) Chrysene-d12	21.033	240	1151972	20.000	ng/ul	0.00
88) Perylene-d12	23.745	264	1344755	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.005	96	16677	2.797	ng/uL	0.00
4) Pyridine-d5	3.393	84	167883	9.472	ng/ul	0.00
7) Phenol-d5	6.587	99	302843	14.023	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.740	67	186411	13.912	ng/ul	0.00
11) 2-Chlorophenol-d4	6.928	132	273349	16.080	ng/ul	0.00
15) 4-Methylphenol-d8	8.104	113	252678	14.220	ng/ul	0.00
21) Nitrobenzene-d5	8.528	128	126198	16.154	ng/ul	0.00
24) 2-Nitrophenol-d4	9.240	143	132293	16.468	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.775	165	241651	15.973	ng/ul	0.00
31) 4-Chloroaniline-d4	10.293	131	335015	14.627	ng/ul	0.00
46) Dimethylphthalate-d6	13.469	166	739355	16.538	ng/ul	0.00
49) Acenaphthylene-d8	13.728	160	870221	17.303	ng/ul	0.00
54) 4-Nitrophenol-d4	14.269	143	72853m	7.940	ng/ul	0.00
60) Fluorene-d10	15.045	176	643728	16.990	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.175	200	60957	8.570	ng/ul	0.00
73) Anthracene-d10	16.892	188	971529	17.322	ng/ul	0.00
81) Pyrene-d10	19.204	212	1107737	17.259	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.557	264	1238285	17.926	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100124\
Data File : BN034304.D
Acq On : 01 Oct 2024 15:53
Operator : RC/JU
Sample : P4019-19
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DDCF3

Manual IntegrationsAPPROVED

Quant Time: Oct 02 00:01:43 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Sep 30 14:14:38 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/02/2024
Supervised By :mohammad ahmed 10/04/2024

