


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN100219\
 Data File : BN007965.D
 Acq On : 02 Oct 2019 14:54
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN091819.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Oct 03 18:39:49 2019

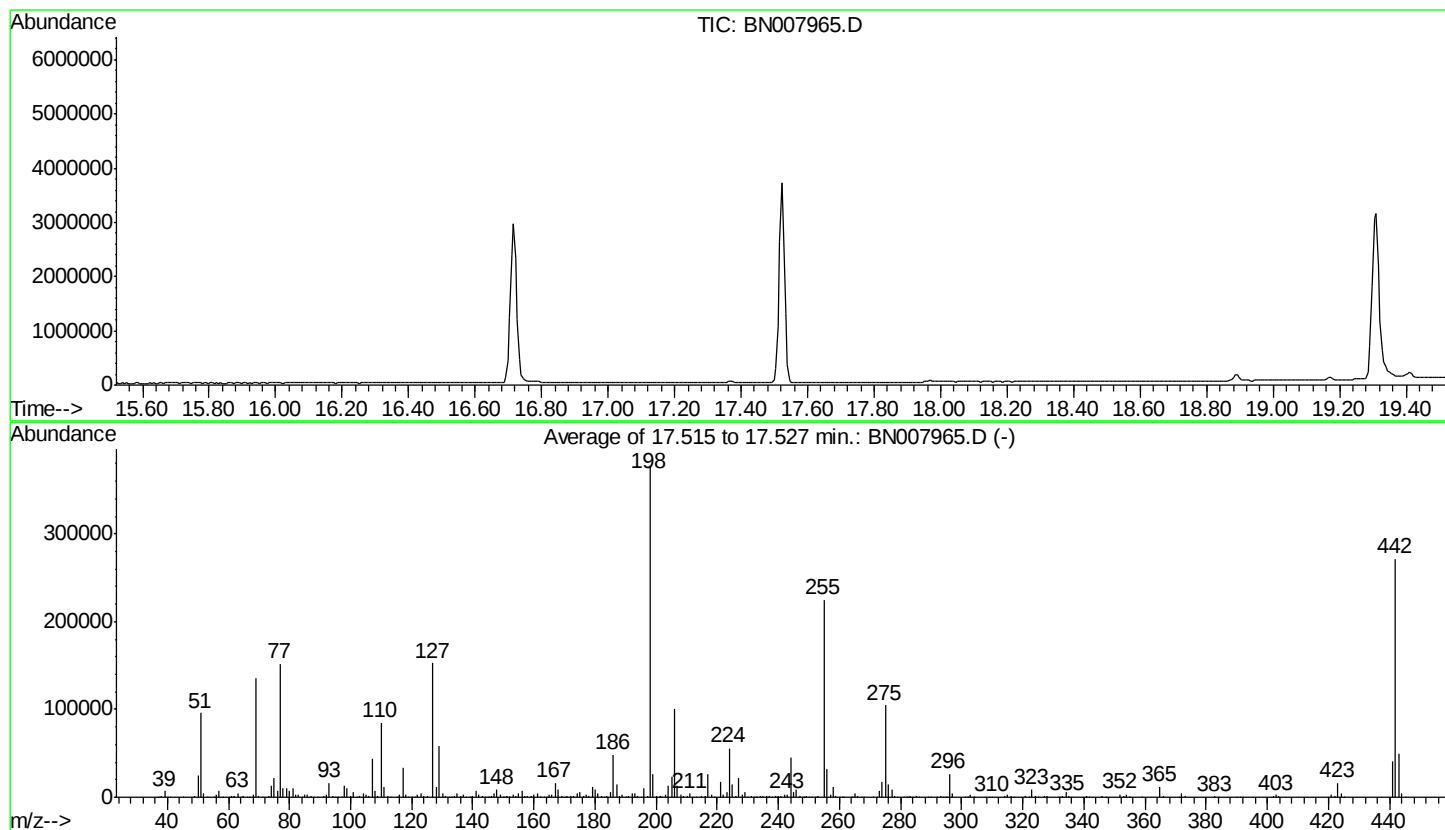

AutoFind: Scans 2470, 2471, 2472; Background Corrected with Scan 2463

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.3	95658	PASS
68	69	0.00	2	1.7	2330	PASS
69	198	0.00	100	35.9	135608	PASS
70	69	0.00	2	0.6	874	PASS
127	198	10	80	40.4	152512	PASS
197	198	0.00	2	0.2	845	PASS
198	198	100	100	100.0	377792	PASS
199	198	5	9	7.0	26288	PASS
275	198	10	60	27.6	104413	PASS
365	198	1	100	3.2	11906	PASS
441	198	0.01	100	10.7	40578	PASS
442	198	50	100	71.9	271466	PASS
443	442	15	24	18.5	50149	PASS