

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN100220\
 Data File : BN012043.D
 Acq On : 02 Oct 2020 19:06
 Operator : CG/JU
 Sample : L4166-04
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AC3

Quant Time: Oct 03 02:14:17 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN100220.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Oct 03 02:12:24 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.66	152	273988	20.00	ng/ul	0.00
18) Naphthalene-d8	10.43	136	1082966	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.30	164	636334	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.05	188	1289589	20.00	ng/ul	0.00
78) Chrysene-d12	21.25	240	1215675	20.00	ng/ul	0.00
86) Perylene-d12	23.45	264	1314136	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.19	96	30310	4.81	ng/uL	0.00
5) Phenol-d5	6.83	99	456521	19.96	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.00	67	336540	23.95	ng/ul	0.00
9) 2-Chlorophenol-d4	7.19	132	397305	21.49	ng/ul	0.00
13) 4-Methylphenol-d8	8.36	113	379267	21.07	ng/ul	0.00
19) Nitrobenzene-d5	8.80	128	196308	22.83	ng/ul	0.00
22) 2-Nitrophenol-d4	9.52	143	208053	22.37	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.06	165	348983	19.57	ng/ul	0.00
29) 4-Chloroaniline-d4	10.57	131	464402	22.09	ng/ul	0.00
44) Dimethylphthalate-d6	13.71	166	1236181	24.77	ng/ul	0.00
47) Acenaphthylene-d8	13.99	160	1266004	21.25	ng/ul	0.00
52) 4-Nitrophenol-d4	14.49	143	109740	11.94	ng/ul	0.00
58) Fluorene-d10	15.29	176	948551	21.77	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.41	200	129851	15.78	ng/ul	0.00
71) Anthracene-d10	17.14	188	1315603	21.04	ng/ul	0.00
79) Pyrene-d10	19.45	212	1307030	20.44	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.31	264	1362182	18.47	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.76	163	269015	5.230	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN100220\
Data File : BN012043.D
Acq On : 02 Oct 2020 19:06
Operator : CG/JU
Sample : L4166-04
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AC3

Quant Time: Oct 03 02:14:17 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN100220.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Oct 03 02:12:24 2020
Response via : Initial Calibration

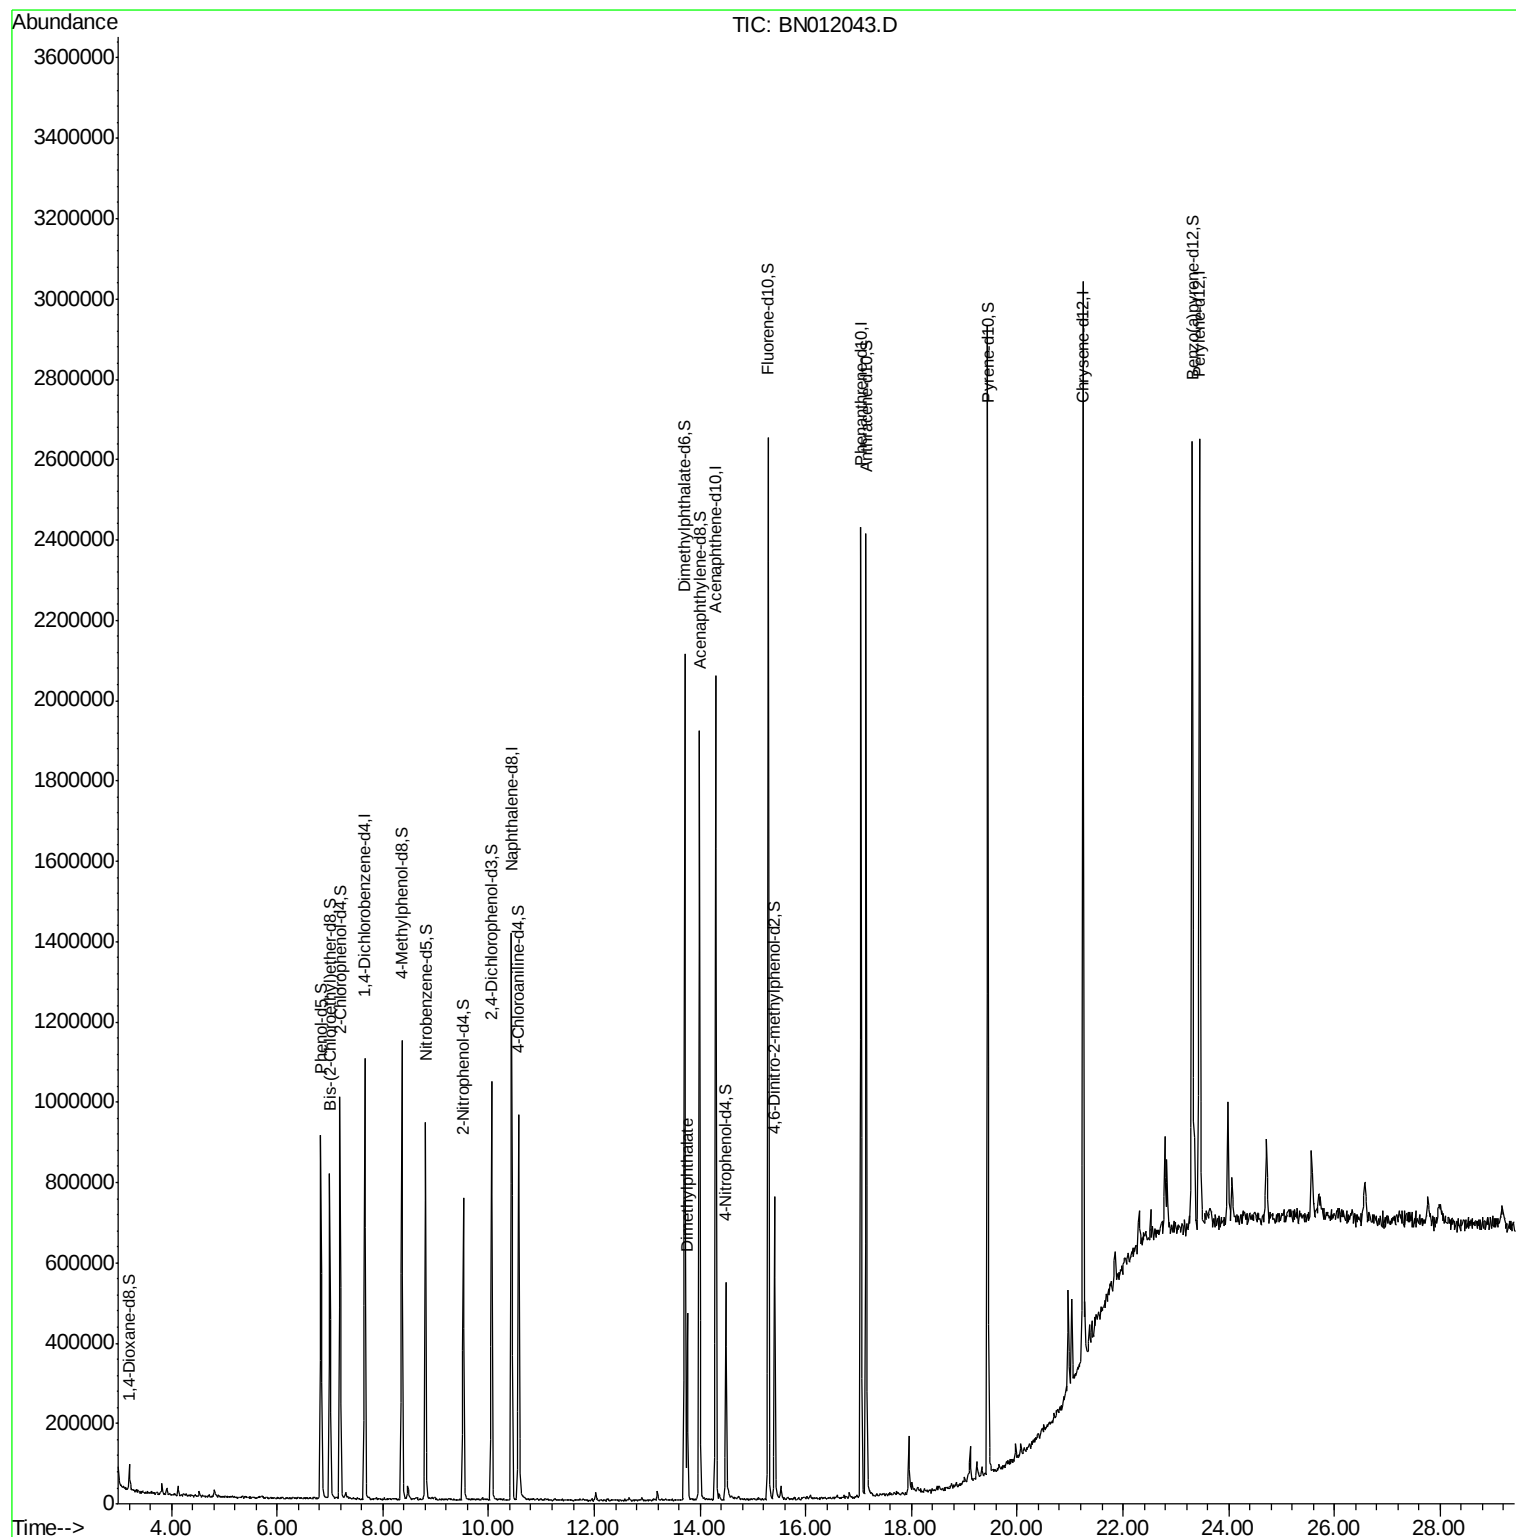

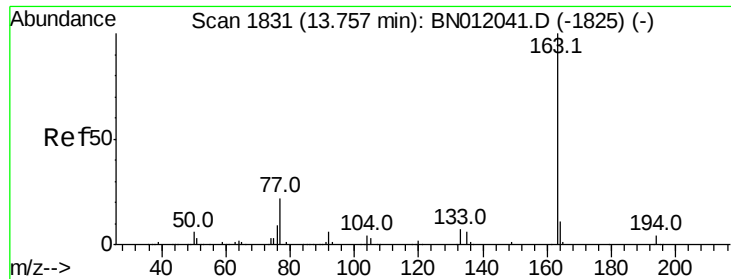

#45

Dimethylphthalate

Concen: 5.230 ng/ul

RT: 13.76 min Scan# 1831

Delta R.T. -0.01 min

Lab File: BN012043.D

Acq: 02 Oct 2020 19:06

Instrument :

BNA_N

ClientSampleId :

C0AC3


Tot Ion:163 Resp: 269015

Ion Ratio Lower Upper

163 100

194 3.4 3.4 5.0

164 9.8 7.8 11.8

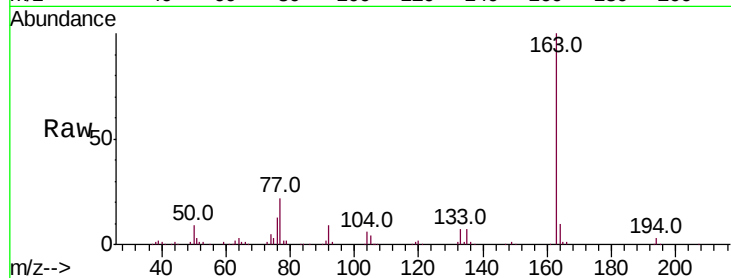

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

