

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN100220\
 Data File : BN012046.D
 Acq On : 02 Oct 2020 20:54
 Operator : CG/JU
 Sample : L4166-09
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AD1

Quant Time: Oct 03 02:14:36 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN100220.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Oct 03 02:12:24 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.66	152	229591	20.00	ng/ul	0.00
18) Naphthalene-d8	10.43	136	854013	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.30	164	507491	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.04	188	1022430	20.00	ng/ul	0.00
78) Chrysene-d12	21.24	240	1013762	20.00	ng/ul	0.00
86) Perylene-d12	23.45	264	1154257	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.20	96	14840	2.81	ng/uL	0.00
5) Phenol-d5	6.83	99	221427	11.55	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.00	67	164067	13.94	ng/ul	0.00
9) 2-Chlorophenol-d4	7.19	132	194012	12.52	ng/ul	0.00
13) 4-Methylphenol-d8	8.36	113	183203	12.15	ng/ul	0.00
19) Nitrobenzene-d5	8.80	128	91738	13.53	ng/ul	0.00
22) 2-Nitrophenol-d4	9.53	143	93367	12.73	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.06	165	164083	11.67	ng/ul	0.00
29) 4-Chloroaniline-d4	10.57	131	228484	13.78	ng/ul	0.00
44) Dimethylphthalate-d6	13.71	166	634491	15.94	ng/ul	0.00
47) Acenaphthylene-d8	13.99	160	612590	12.89	ng/ul	0.00
52) 4-Nitrophenol-d4	14.49	143	46399	6.33	ng/ul	0.00
58) Fluorene-d10	15.29	176	475082	13.67	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.41	200	56344	8.63	ng/ul	0.00
71) Anthracene-d10	17.04	188	1022430	20.62	ng/ul	-0.10
79) Pyrene-d10	19.44	212	738797	13.86	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.31	264	806113	12.44	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.76	163	139037	3.389	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN100220\
Data File : BN012046.D
Acq On : 02 Oct 2020 20:54
Operator : CG/JU
Sample : L4166-09
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AD1

Quant Time: Oct 03 02:14:36 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN100220.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Oct 03 02:12:24 2020
Response via : Initial Calibration

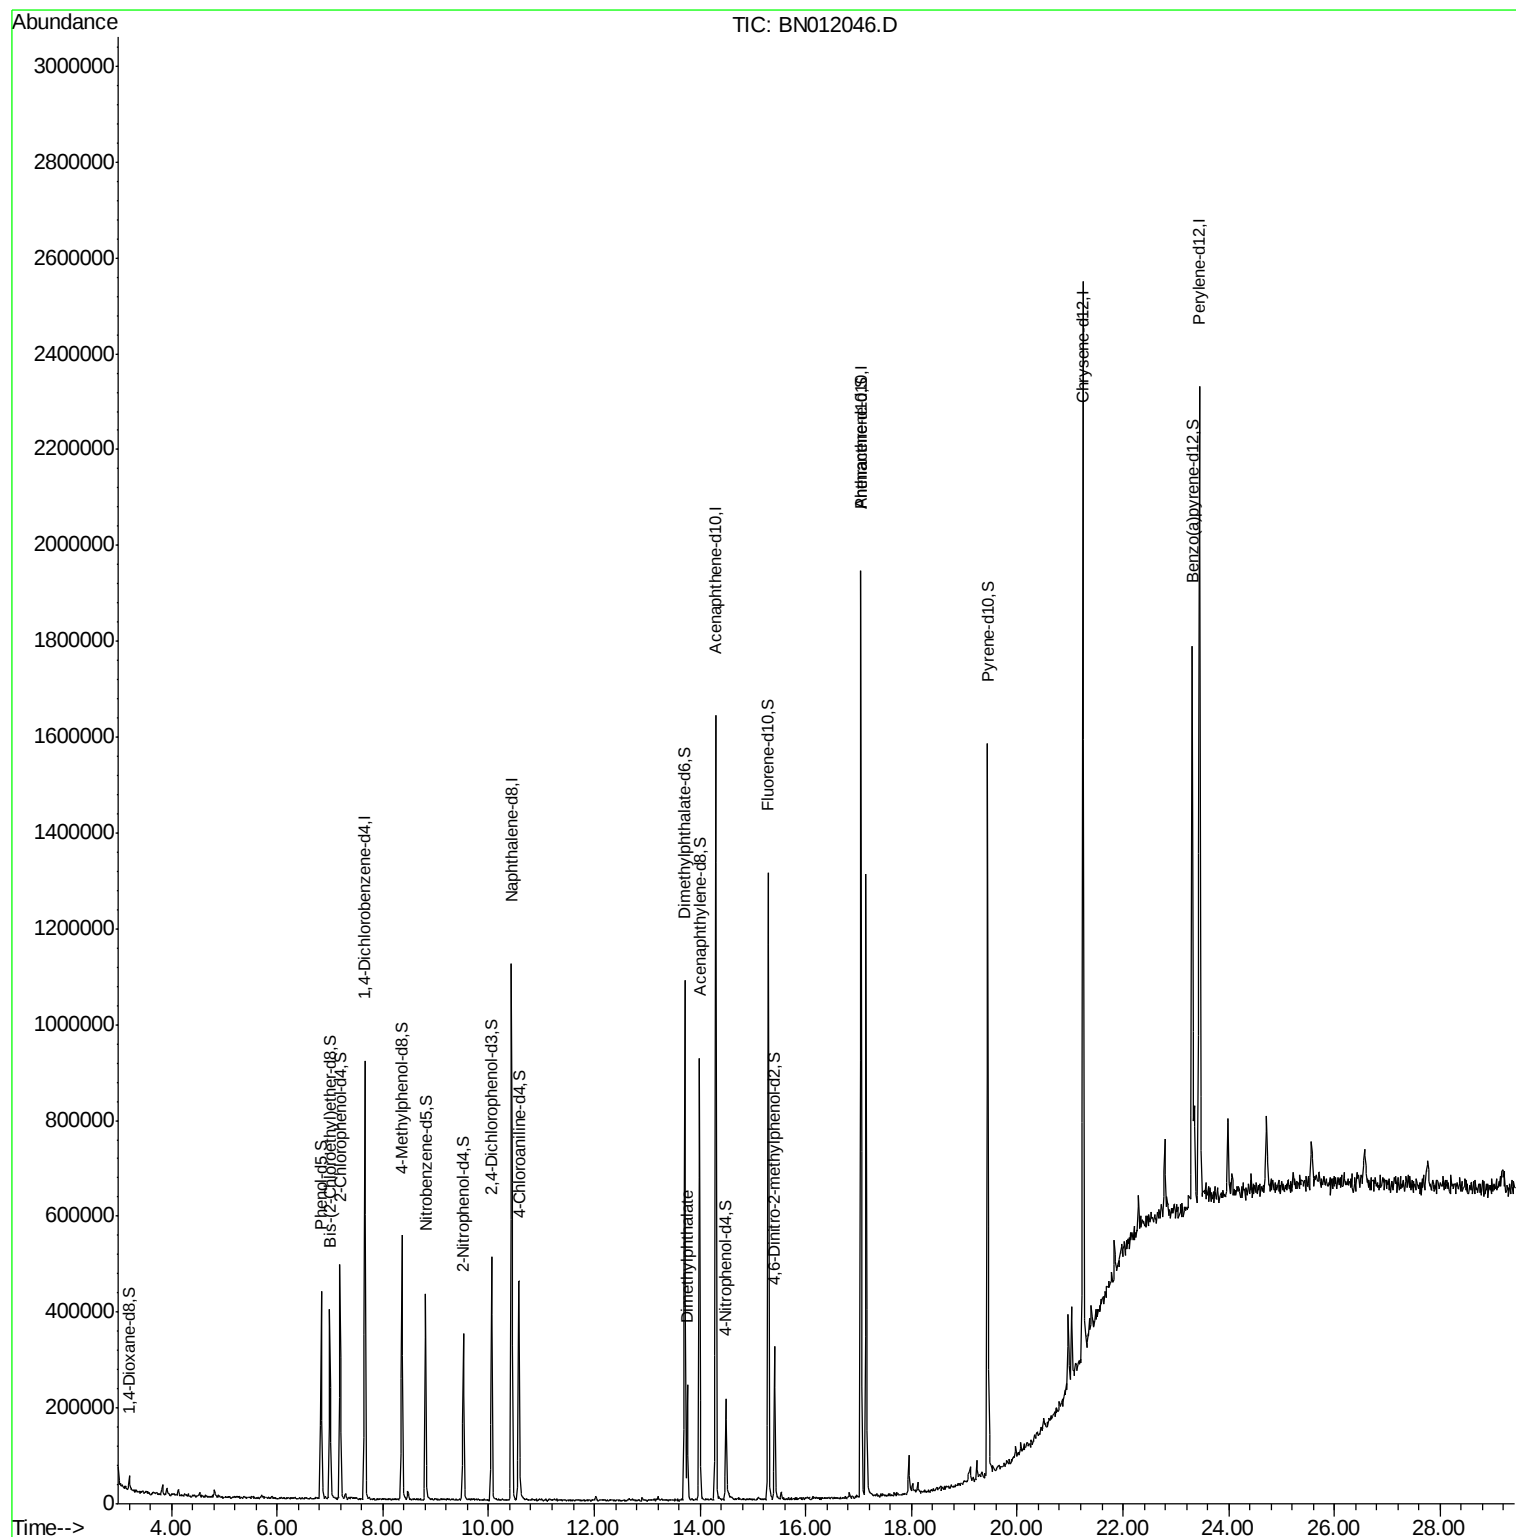

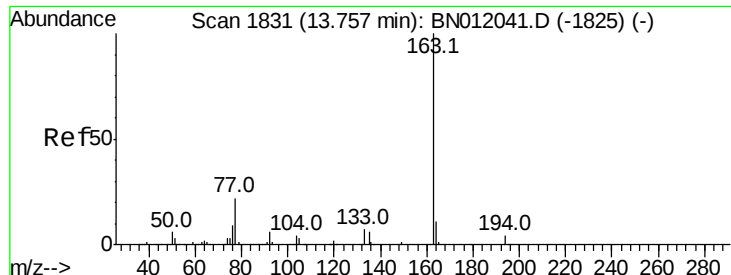

#45

Dimethylphthalate

Concen: 3.389 ng/ul

RT: 13.76 min Scan# 1831

Delta R.T. -0.01 min

Lab File: BN012046.D

Acq: 02 Oct 2020 20:54

Instrument :

BNA_N

ClientSampleId :

C0AD1


Tot Ion:163 Resp: 139037

Ion Ratio Lower Upper

163 100

194 4.6 3.4 5.0

164 9.7 7.8 11.8

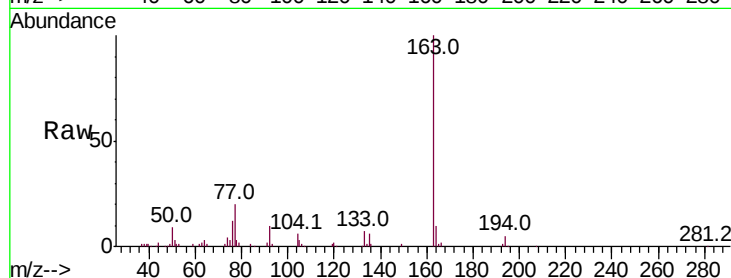

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

