

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN100220\
 Data File : BN012047.D
 Acq On : 02 Oct 2020 21:31
 Operator : CG/JU
 Sample : L4166-03
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AC2

Quant Time: Oct 03 02:14:43 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN100220.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Oct 03 02:12:24 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.66	152	229660	20.00	ng/ul	0.00
18) Naphthalene-d8	10.43	136	870406	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.30	164	514249	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.05	188	1026123	20.00	ng/ul	0.00
78) Chrysene-d12	21.24	240	1040983	20.00	ng/ul	0.00
86) Perylene-d12	23.45	264	1145770	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.20	96	18136	3.44	ng/uL	0.00
5) Phenol-d5	6.83	99	250225	13.05	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.00	67	180699	15.34	ng/ul	0.00
9) 2-Chlorophenol-d4	7.19	132	218693	14.11	ng/ul	0.00
13) 4-Methylphenol-d8	8.36	113	206093	13.66	ng/ul	0.00
19) Nitrobenzene-d5	8.80	128	102150	14.78	ng/ul	0.00
22) 2-Nitrophenol-d4	9.52	143	104771	14.02	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.06	165	183623	12.81	ng/ul	0.00
29) 4-Chloroaniline-d4	10.57	131	244360	14.46	ng/ul	0.00
44) Dimethylphthalate-d6	13.71	166	667093	16.54	ng/ul	0.00
47) Acenaphthylene-d8	13.99	160	675110	14.02	ng/ul	0.00
52) 4-Nitrophenol-d4	14.49	143	53384	7.19	ng/ul	0.00
58) Fluorene-d10	15.29	176	506735	14.39	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.41	200	66326	10.13	ng/ul	0.00
71) Anthracene-d10	17.14	188	728306	14.64	ng/ul	0.00
79) Pyrene-d10	19.44	212	749367	13.69	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.31	264	843077	13.11	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.76	163	130292	3.135	ng/ul#	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN100220\
Data File : BN012047.D
Acq On : 02 Oct 2020 21:31
Operator : CG/JU
Sample : L4166-03
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AC2

Quant Time: Oct 03 02:14:43 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN100220.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Oct 03 02:12:24 2020
Response via : Initial Calibration

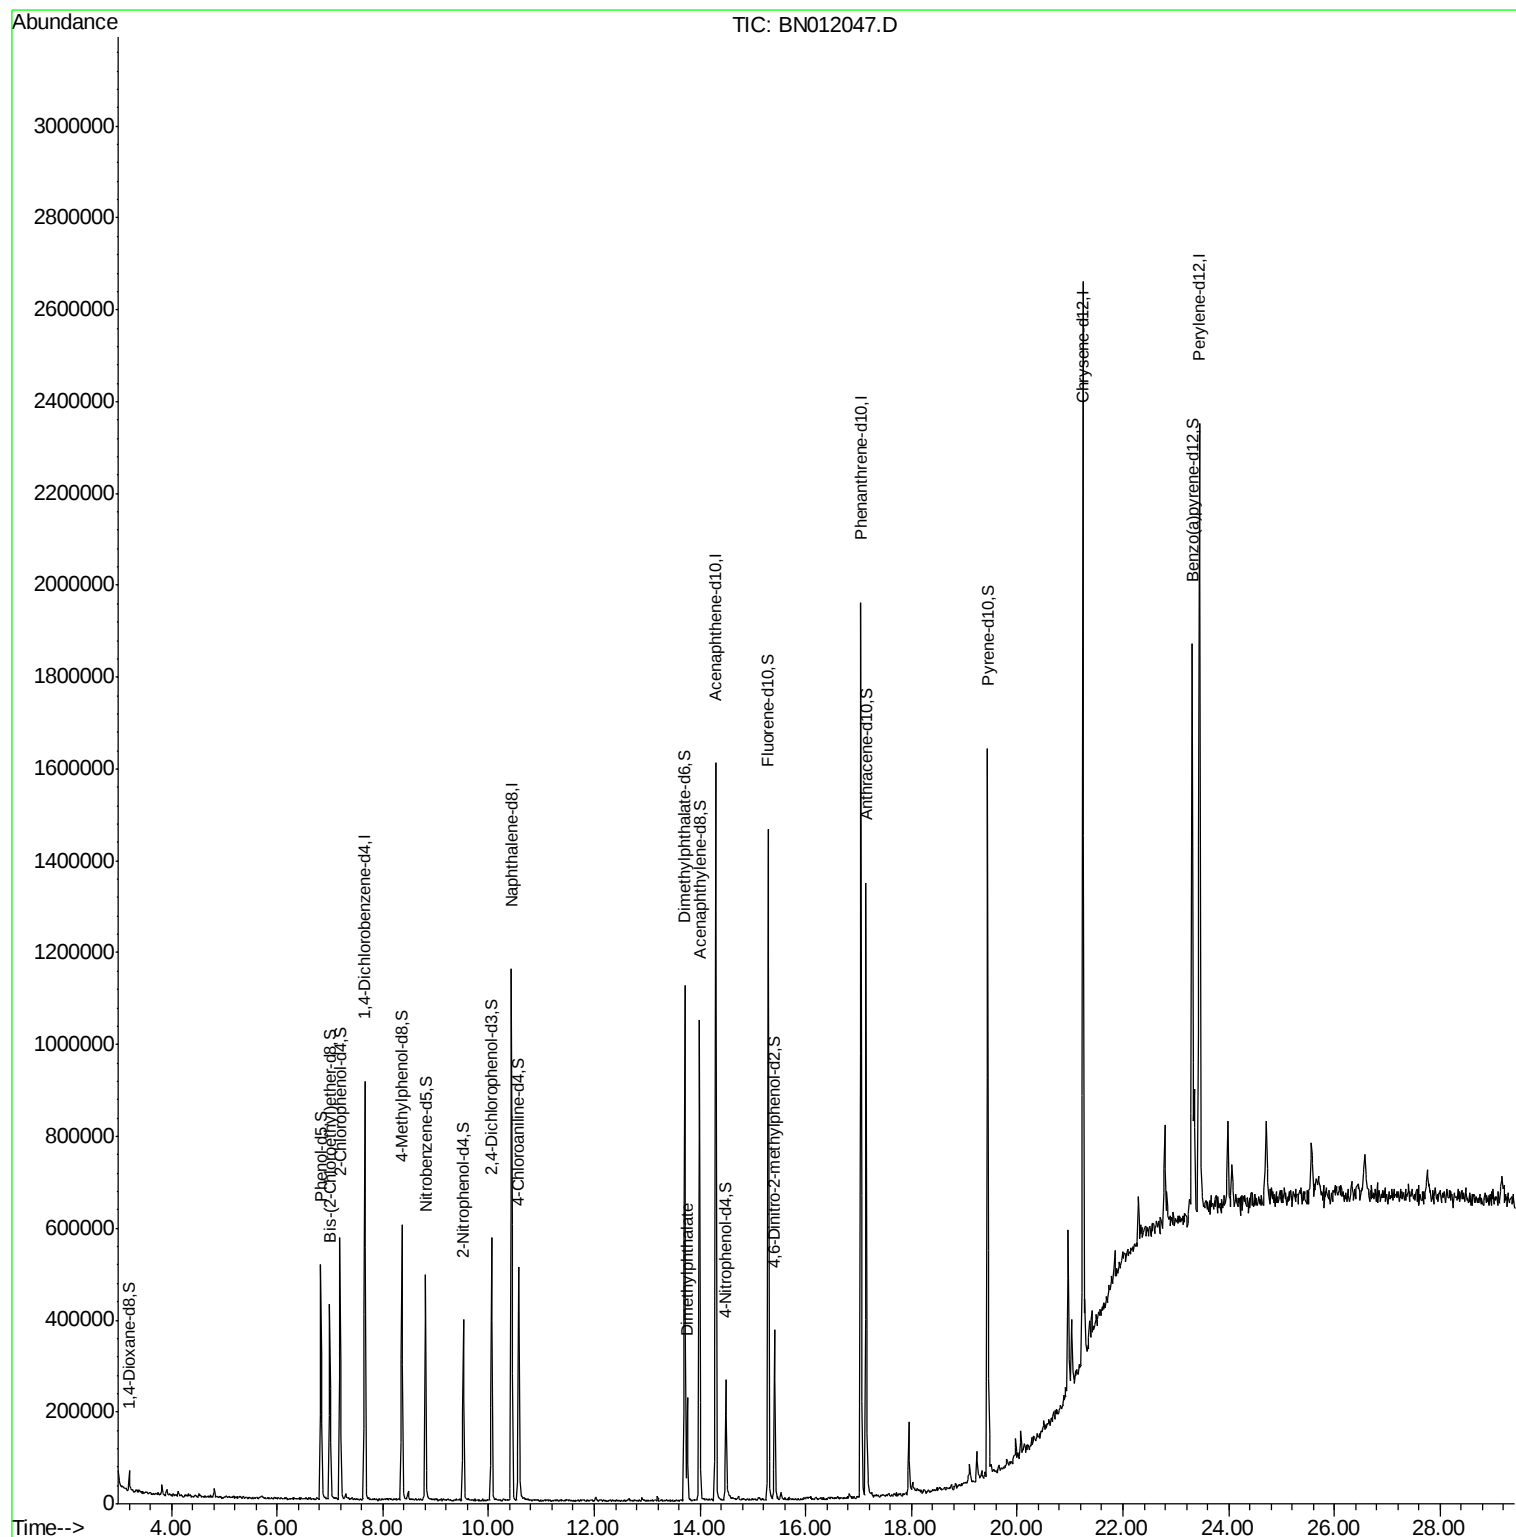

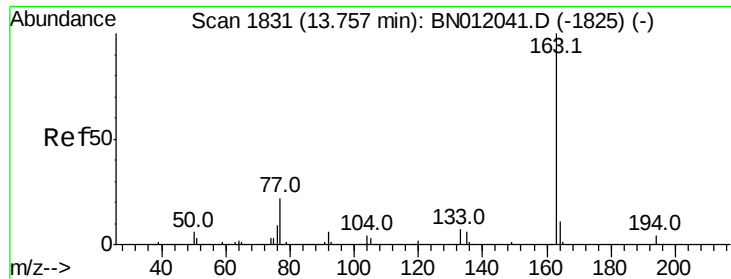

#45

Dimethylphthalate

Concen: 3.135 ng/ul

RT: 13.76 min Scan# 1831

Delta R.T. -0.01 min

Lab File: BN012047.D

Acq: 02 Oct 2020 21:31

Instrument :

BNA_N

ClientSampleId :

C0AC2

Tot Ion:163 Resp: 130292

Ion Ratio Lower Upper

163 100

194 4.2 3.4 5.0

164 11.9 7.8 11.8#

