

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN100220\
 Data File : BN012048.D
 Acq On : 02 Oct 2020 22:07
 Operator : CG/JU
 Sample : L4166-07
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AC7

Quant Time: Oct 03 02:14:51 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN100220.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Oct 03 02:12:24 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.66	152	201961	20.00	ng/ul	0.00
18) Naphthalene-d8	10.43	136	785643	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.30	164	469932	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.05	188	944529	20.00	ng/ul	0.00
78) Chrysene-d12	21.24	240	911389	20.00	ng/ul	0.00
86) Perylene-d12	23.45	264	1032135	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.20	96	15014	3.23	ng/uL	0.00
5) Phenol-d5	6.83	99	220778	13.10	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.00	67	167478	16.17	ng/ul	0.00
9) 2-Chlorophenol-d4	7.19	132	193801	14.22	ng/ul	0.00
13) 4-Methylphenol-d8	8.36	113	184392	13.90	ng/ul	0.00
19) Nitrobenzene-d5	8.80	128	93213	14.94	ng/ul	0.00
22) 2-Nitrophenol-d4	9.52	143	92282	13.68	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.06	165	169214	13.08	ng/ul	0.00
29) 4-Chloroaniline-d4	10.57	131	225978	14.81	ng/ul	0.00
44) Dimethylphthalate-d6	13.71	166	653173	17.72	ng/ul	0.00
47) Acenaphthylene-d8	13.99	160	631227	14.35	ng/ul	0.00
52) 4-Nitrophenol-d4	14.49	143	50072	7.38	ng/ul	0.00
58) Fluorene-d10	15.29	176	485077	15.08	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.41	200	60137	9.98	ng/ul	0.00
71) Anthracene-d10	17.14	188	723367	15.79	ng/ul	0.00
79) Pyrene-d10	19.45	212	752219	15.69	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.31	264	815426	14.08	ng/ul	0.00
Target Compounds						
45) Dimethylphthalate	13.76	163	128473	3.382	ng/ul#	97
80) Pyrene	19.47	202	71764	1.092	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN100220\
Data File : BN012048.D
Acq On : 02 Oct 2020 22:07
Operator : CG/JU
Sample : L4166-07
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AC7

Quant Time: Oct 03 02:14:51 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN100220.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Oct 03 02:12:24 2020
Response via : Initial Calibration

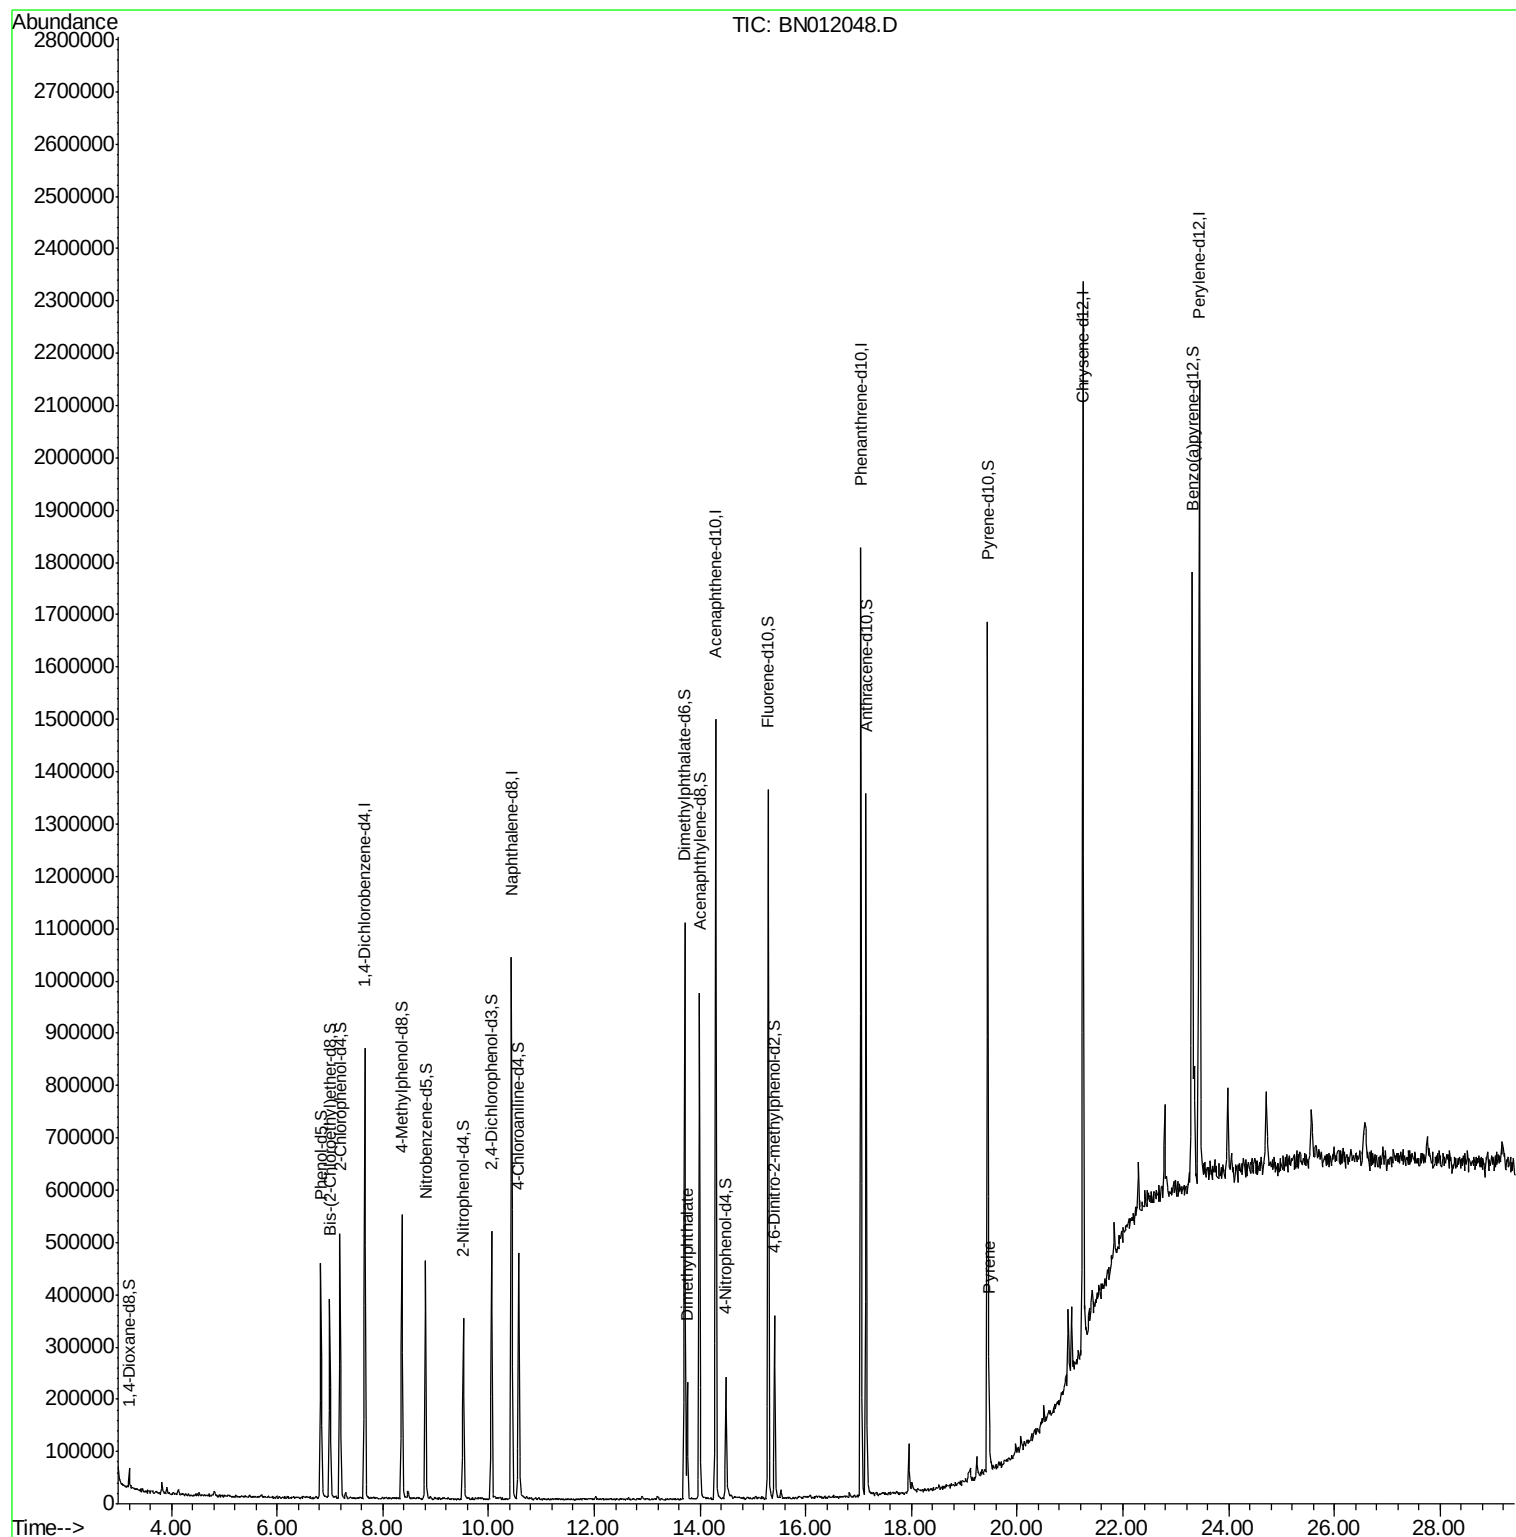


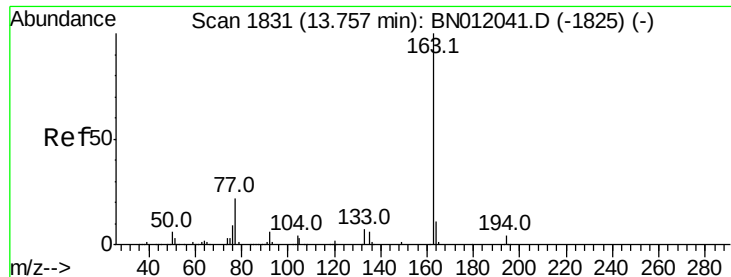




#45
Dimethylphthalate
Concen: 3.382 ng/ul
RT: 13.76 min Scan# 1831
Delta R.T. -0.01 min
Lab File: BN012048.D
Acq: 02 Oct 2020 22:07

Instrument :
BNA_N
ClientSampleId :
C0AC7

Tot Ion:163 Resp: 128473
Ion Ratio Lower Upper
163 100
194 5.3 3.4 5.0#
164 10.7 7.8 11.8

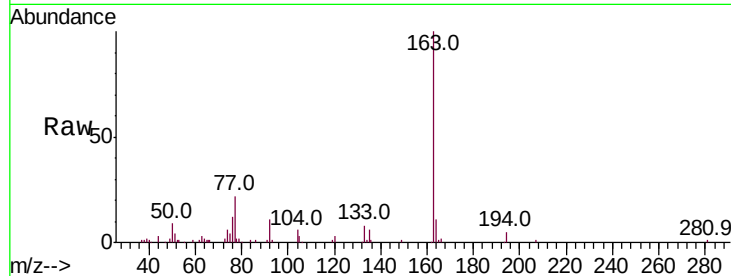


Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

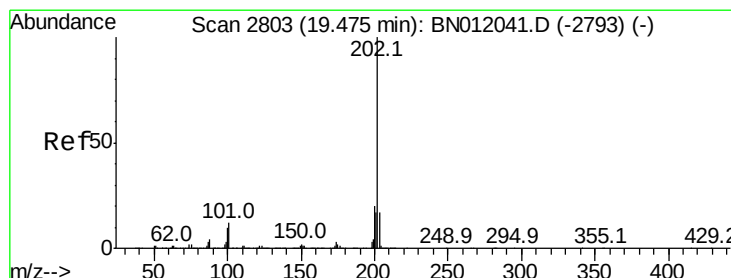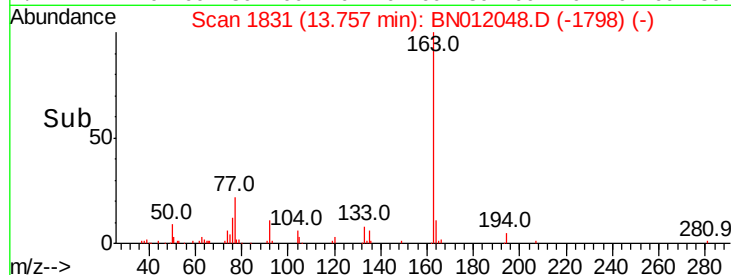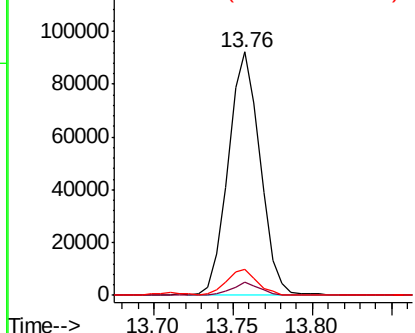

#80
Pyrene
Concen: 1.092 ng/ul
RT: 19.47 min Scan# 2802
Delta R.T. -0.01 min
Lab File: BN012048.D
Acq: 02 Oct 2020 22:07

Tgt Ion:202 Resp: 71764
Ion Ratio Lower Upper
202 100
101 12.9 10.2 15.2
100 10.4 8.8 13.2

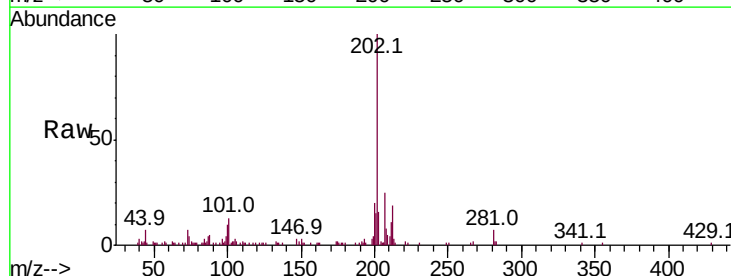

Abundance Ion 202.00 (201.70 to 202.70): E
Ion 101.00 (100.70 to 101.70): E
Ion 100.00 (99.70 to 100.70): B

