

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN100220\
 Data File : BN012052.D
 Acq On : 03 Oct 2020 00:32
 Operator : CG/JU
 Sample : L4166-02
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AB9

Quant Time: Oct 03 02:15:20 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN100220.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Oct 03 02:12:24 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.66	152	266275	20.00	ng/ul	0.00
18) Naphthalene-d8	10.43	136	1033297	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.30	164	620474	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.05	188	1218075	20.00	ng/ul	0.00
78) Chrysene-d12	21.24	240	1195199	20.00	ng/ul	0.00
86) Perylene-d12	23.44	264	1319233	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.19	96	30101	4.92	ng/uL	0.00
5) Phenol-d5	6.83	99	464109	20.88	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.00	67	295274	21.63	ng/ul	0.00
9) 2-Chlorophenol-d4	7.19	132	399403	22.22	ng/ul	0.00
13) 4-Methylphenol-d8	8.36	113	376311	21.51	ng/ul	0.00
19) Nitrobenzene-d5	8.80	128	170986	20.84	ng/ul	0.00
22) 2-Nitrophenol-d4	9.52	143	189381	21.34	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.05	165	342783	20.14	ng/ul	0.00
29) 4-Chloroaniline-d4	10.57	131	475181	23.69	ng/ul	0.00
44) Dimethylphthalate-d6	13.71	166	1055208	21.68	ng/ul	0.00
47) Acenaphthylene-d8	13.99	160	1317143	22.67	ng/ul	0.00
52) 4-Nitrophenol-d4	14.49	143	97377	10.86	ng/ul	0.00
58) Fluorene-d10	15.29	176	901064	21.21	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.41	200	97717	12.57	ng/ul	0.00
71) Anthracene-d10	17.14	188	1358537	23.00	ng/ul	0.00
79) Pyrene-d10	19.44	212	1438341	22.88	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.30	264	1555680	21.01	ng/ul	-0.01


Target Compounds					Ovalue	
45) Dimethylphthalate	13.76	163	233993	4.666	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN100220\
Data File : BN012052.D
Acq On : 03 Oct 2020 00:32
Operator : CG/JU
Sample : L4166-02
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AB9

Quant Time: Oct 03 02:15:20 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN100220.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Oct 03 02:12:24 2020
Response via : Initial Calibration

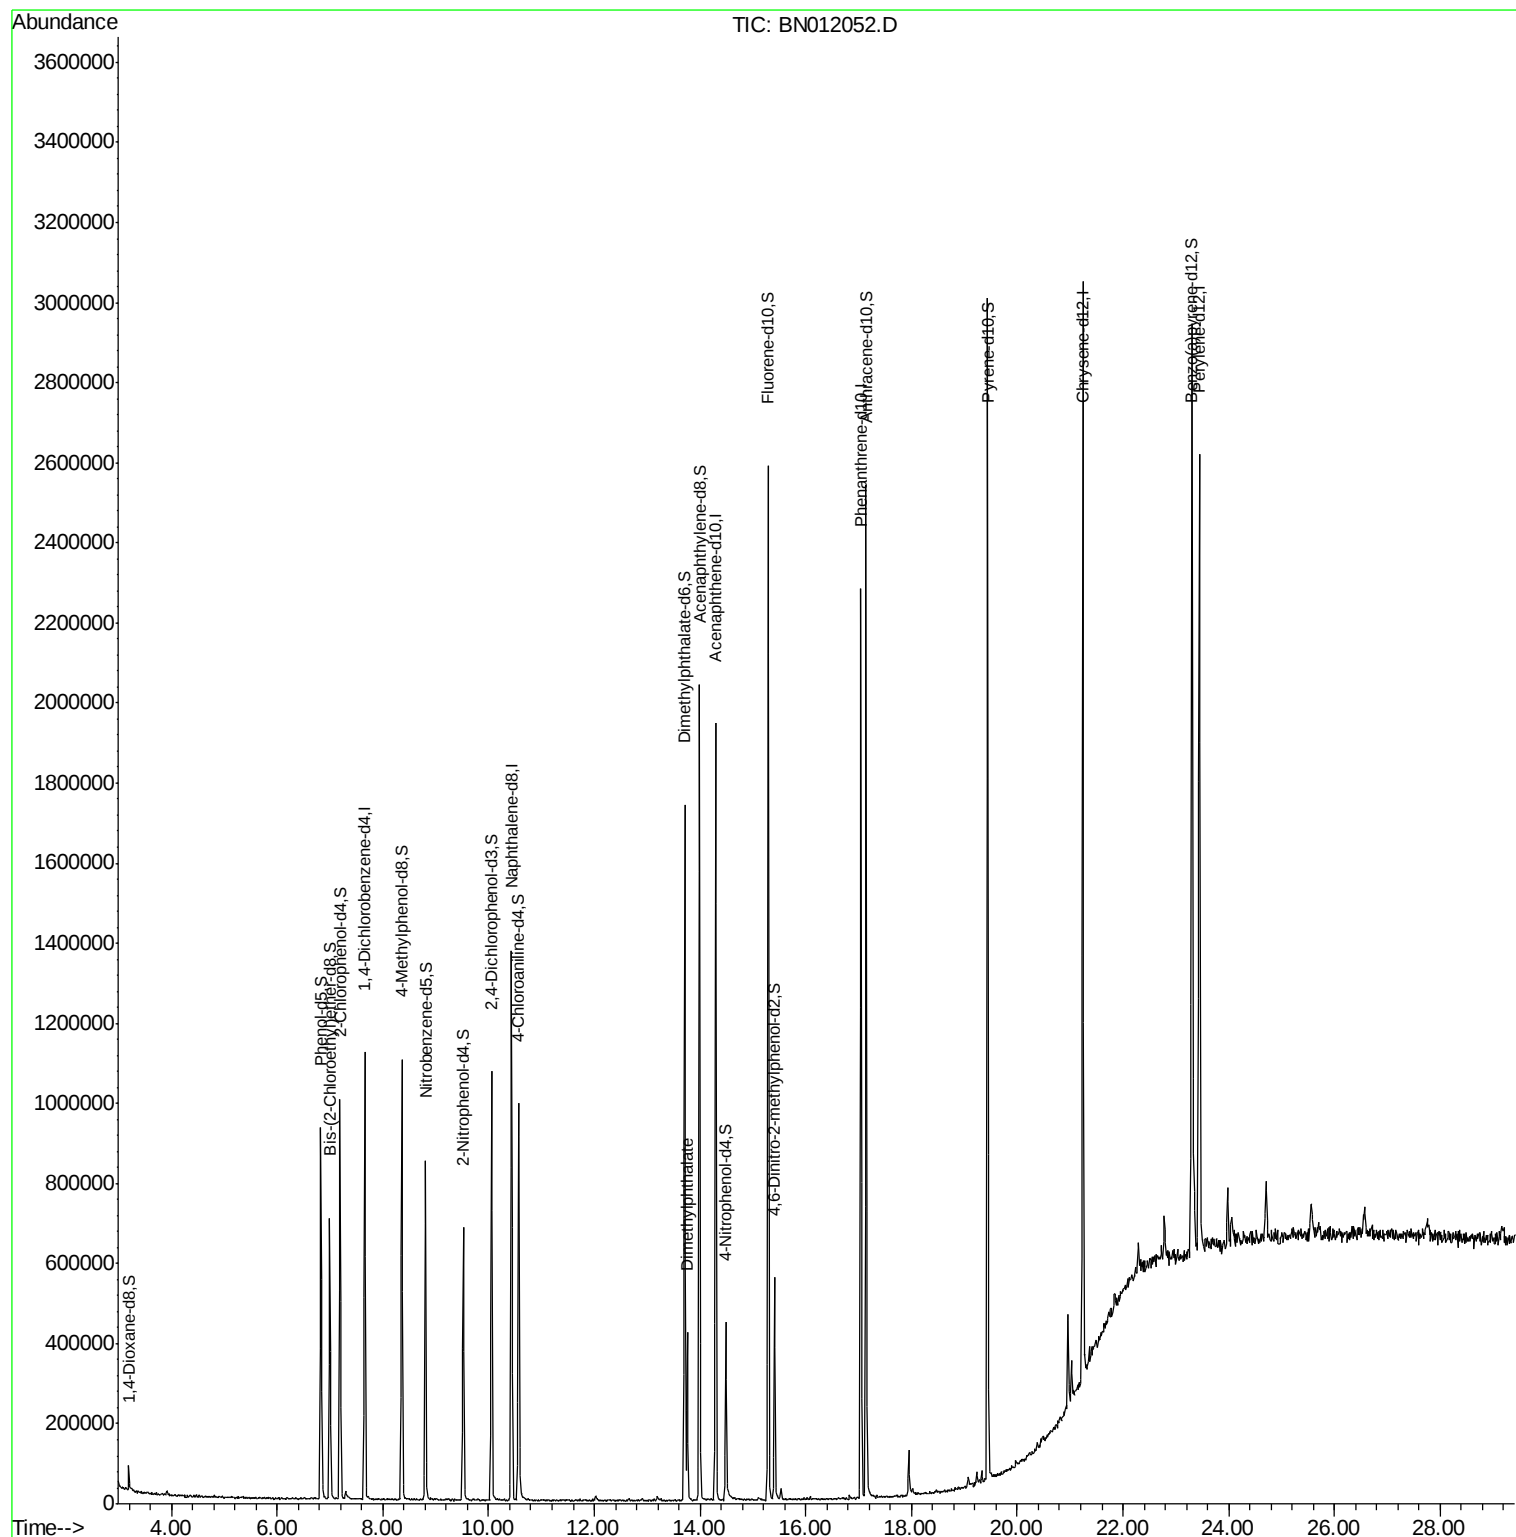


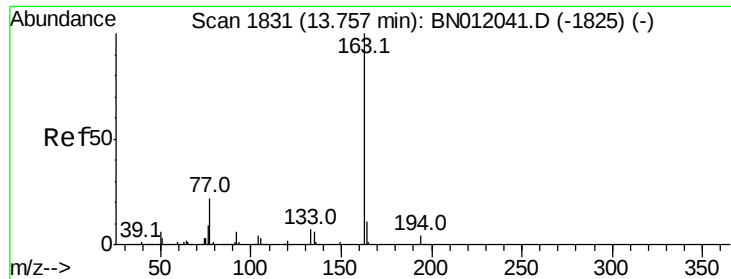

#45
 Dimethylphthalate
 Concen: 4.666 ng/ul
 RT: 13.76 min Scan# 1831
 Delta R.T. -0.01 min
 Lab File: BN012052.D
 Acq: 03 Oct 2020 00:32

Instrument :
 BNA_N
 ClientSampleId :
 C0AB9

Tot Ion	Ratio	Lower	Upper
163	100		
194	4.3	3.4	5.0
164	9.4	7.8	11.8

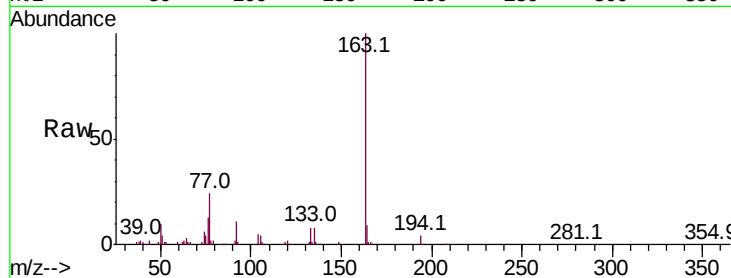

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

