

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100220\
 Data File : BN012043.D
 Acq On : 02 Oct 2020 19:06
 Operator : CG/JU
 Sample : L4166-04
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AC3

Quant Time: Oct 03 02:13:32 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN100220.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Oct 03 02:12:24 2020
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.657	152	273988	20.00	ng/ul	0.00
18) Naphthalene-d8	10.434	136	1082966	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.298	164	636334	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.045	188	1289589	20.00	ng/ul	0.00
78) Chrysene-d12	21.245	240	1215675	20.00	ng/ul	0.00
86) Perylene-d12	23.451	264	1314136	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.193	96	30310	4.81	ng/uL	0.00
5) Phenol-d5	6.828	99	456521	19.96	ng/ul	0.00
7) Bis-(2-Chloroethyl)eth...	6.999	67	336540	23.95	ng/ul	0.00
9) 2-Chlorophenol-d4	7.193	132	397305	21.49	ng/ul	0.00
13) 4-Methylphenol-d8	8.357	113	379267	21.07	ng/ul	0.00
19) Nitrobenzene-d5	8.804	128	196308	22.83	ng/ul	0.00
22) 2-Nitrophenol-d4	9.522	143	208053	22.37	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.057	165	348983	19.57	ng/ul	0.00
29) 4-Chloroaniline-d4	10.569	131	464402	22.09	ng/ul	0.00
44) Dimethylphthalate-d6	13.710	166	1236181	24.77	ng/ul	0.00
47) Acenaphthylene-d8	13.987	160	1266004	21.25	ng/ul	0.00
52) 4-Nitrophenol-d4	14.492	143	109740	11.94	ng/ul	0.00
58) Fluorene-d10	15.292	176	948551	21.77	ng/ul	0.00
63) 4,6-Dinitro-2-methylph...	15.410	200	129851	15.78	ng/ul	0.00
71) Anthracene-d10	17.139	188	1315603	21.04	ng/ul	0.00
79) Pyrene-d10	19.445	212	1307030	20.44	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.310	264	1362182	18.47	ng/ul	0.00
Target Compounds						
45) Dimethylphthalate	13.757	163	269015	5.23	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100220\
Data File : BN012043.D
Acq On : 02 Oct 2020 19:06
Operator : CG/JU
Sample : L4166-04
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AC3


Quant Time: Oct 03 02:13:32 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN100220.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Oct 03 02:12:24 2020
Response via : Initial Calibration

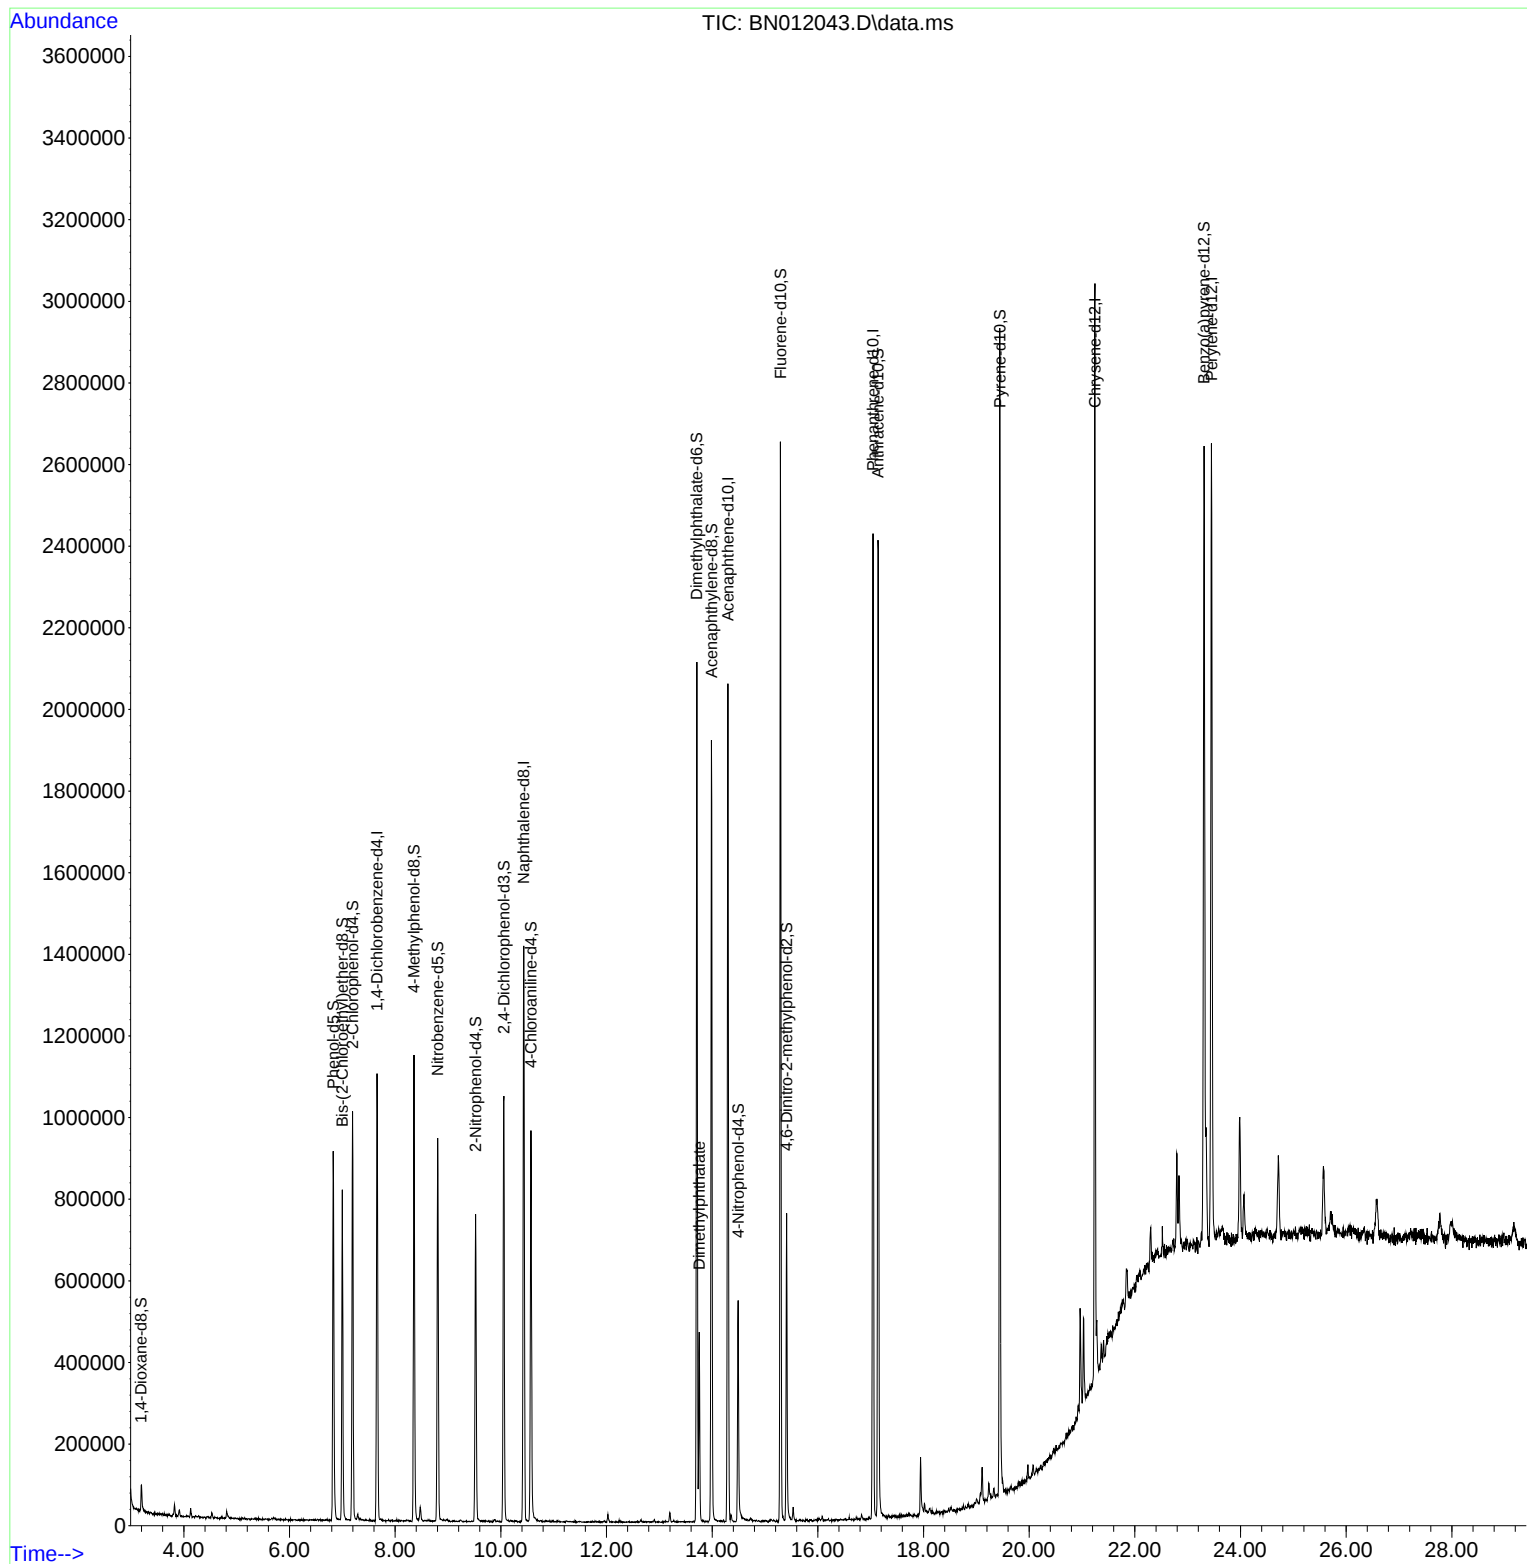

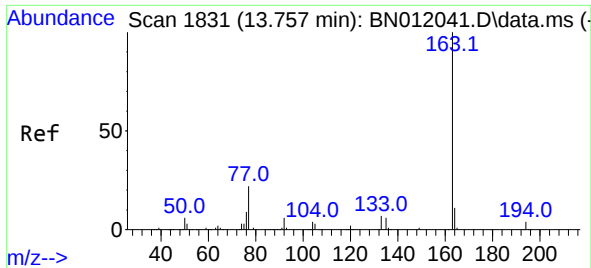

#45
Dimethylphthalate
Concen: 5.23 ng/ul
RT: 13.757 min Scan# 1831
Delta R.T. -0.006 min
Lab File: BN012043.D
Acq: 02 Oct 2020 19:06

Instrument :
BNA_N
ClientSampleId :
C0AC3

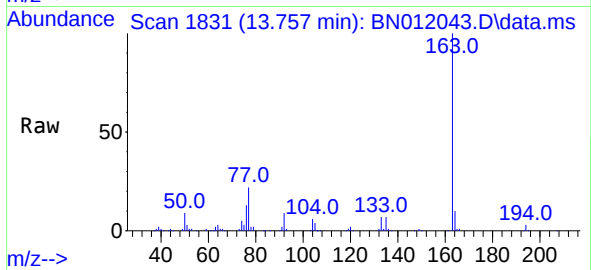

Tgt Ion:163 Resp: 269015

Ion	Ratio	Lower	Upper
163	100		
194	3.4	3.4	5.0
164	9.8	7.8	11.8

