

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100220\
 Data File : BN012040.D
 Acq On : 02 Oct 2020 17:14
 Operator : CG/JU
 Sample : PB132013BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK13

Integration Parameters: LSCINT.P

Integrator: RTE

Smoother: OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN100220.M

Title : SVOA CALIBRATION

Signal : TIC: BN012040.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.193	32	35	42	rVB	79039	102644	2.03%	0.174%
2	3.687	116	119	126	rBV7	5617	13328	0.26%	0.023%
3	3.911	154	157	163	rBV4	16440	23987	0.47%	0.041%
4	4.128	189	194	199	rBV	87450	112313	2.22%	0.191%
5	4.528	257	262	267	rBV	67847	89348	1.77%	0.152%
6	4.899	321	325	328	rVB4	6209	9262	0.18%	0.016%
7	5.493	425	426	432	rBV4	3676	5233	0.10%	0.009%
8	5.993	509	511	518	rVB4	3208	6033	0.12%	0.010%
9	6.075	522	525	529	rVB5	4883	6778	0.13%	0.012%
10	6.828	647	653	663	rBV	1114381	1704667	33.71%	2.894%
11	6.999	676	682	692	rVB	842170	1296205	25.63%	2.200%
12	7.193	708	715	723	rBV	1217875	1848846	36.56%	3.138%
13	7.657	787	794	803	rBV	1115439	1715646	33.93%	2.912%
14	8.357	905	913	925	rBV	1290062	2030720	40.16%	3.447%
15	8.804	981	989	1001	rBV	1024800	1645164	32.53%	2.793%
16	9.522	1102	1111	1121	rBV	840362	1367597	27.04%	2.321%
17	10.051	1194	1201	1210	rBV	1245425	2063582	40.81%	3.503%
18	10.434	1259	1266	1275	rBV	1431604	2292309	45.33%	3.891%
19	10.569	1282	1289	1304	rBV	1197160	2025307	40.05%	3.438%
20	10.663	1304	1305	1312	rVB6	5110	8121	0.16%	0.014%
21	12.028	1533	1537	1543	rVB4	16402	25944	0.51%	0.044%
22	13.710	1817	1823	1833	rBV	2196693	2906455	57.48%	4.934%
23	13.987	1863	1870	1883	rBV	2361474	3351488	66.28%	5.689%
24	14.298	1914	1923	1931	rBV	1981240	2873390	56.82%	4.877%
25	14.492	1950	1956	1971	rBV	889482	1298352	25.68%	2.204%
26	14.904	2023	2026	2028	rBV3	4874	5876	0.12%	0.010%
27	15.292	2086	2092	2105	rVV	2988284	4115560	81.39%	6.986%
28	15.410	2107	2112	2124	rVV	933150	1255034	24.82%	2.130%
29	15.534	2127	2133	2138	rVB4	36277	51376	1.02%	0.087%
30	16.081	2223	2226	2232	rBV5	10048	16295	0.32%	0.028%
31	16.833	2350	2354	2357	rVV2	8865	14433	0.29%	0.024%
32	16.980	2375	2379	2380	rBV3	4639	5420	0.11%	0.009%
33	17.045	2383	2390	2397	rVV	2406664	3177124	62.83%	5.393%
34	17.145	2400	2407	2426	rVB	2971415	4288037	84.80%	7.279%
35	17.669	2494	2496	2502	rVB6	4133	5681	0.11%	0.010%
36	17.951	2538	2544	2546	rBV7	10327	17100	0.34%	0.029%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100220\
 Data File : BN012040.D
 Acq On : 02 Oct 2020 17:14
 Operator : CG/JU
 Sample : PB132013BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK13

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN100220.M
 Title : SVOA CALIBRATION

37	18.016	2552	2555	2560	rBV3	12968	15783	0.31%	0.027%
38	18.716	2669	2674	2676	rBV5	7169	11921	0.24%	0.020%
39	18.939	2710	2712	2713	rBV2	6543	5273	0.10%	0.009%
40	18.957	2713	2715	2718	rVV3	6590	6601	0.13%	0.011%
41	19.004	2721	2723	2729	rBV6	9093	17059	0.34%	0.029%
42	19.075	2732	2735	2739	rVB3	23341	35625	0.70%	0.060%
43	19.216	2757	2759	2761	rBV3	7495	7759	0.15%	0.013%
44	19.333	2776	2779	2782	rBV2	21938	24734	0.49%	0.042%
45	19.380	2785	2787	2788	rBV2	12502	6239	0.12%	0.011%
46	19.398	2788	2790	2792	rBV3	7996	6244	0.12%	0.011%
47	19.445	2792	2798	2808	rBV	3713158	4840767	95.73%	8.217%
48	19.627	2827	2829	2830	rBV	11078	6173	0.12%	0.010%
49	21.033	3064	3068	3072	rBV	236789	311585	6.16%	0.529%
50	21.245	3099	3104	3111	rBV	2732671	3390599	67.05%	5.755%
51	23.315	3449	3456	3468	rBV	2625078	5056795	100.00%	8.584%
52	23.451	3473	3479	3487	rVB	1843720	3393460	67.11%	5.760%


Sum of corrected areas: 58911272

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100220\
Data File : BN012040.D
Acq On : 02 Oct 2020 17:14
Operator : CG/JU
Sample : PB132013BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK13

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN100220.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

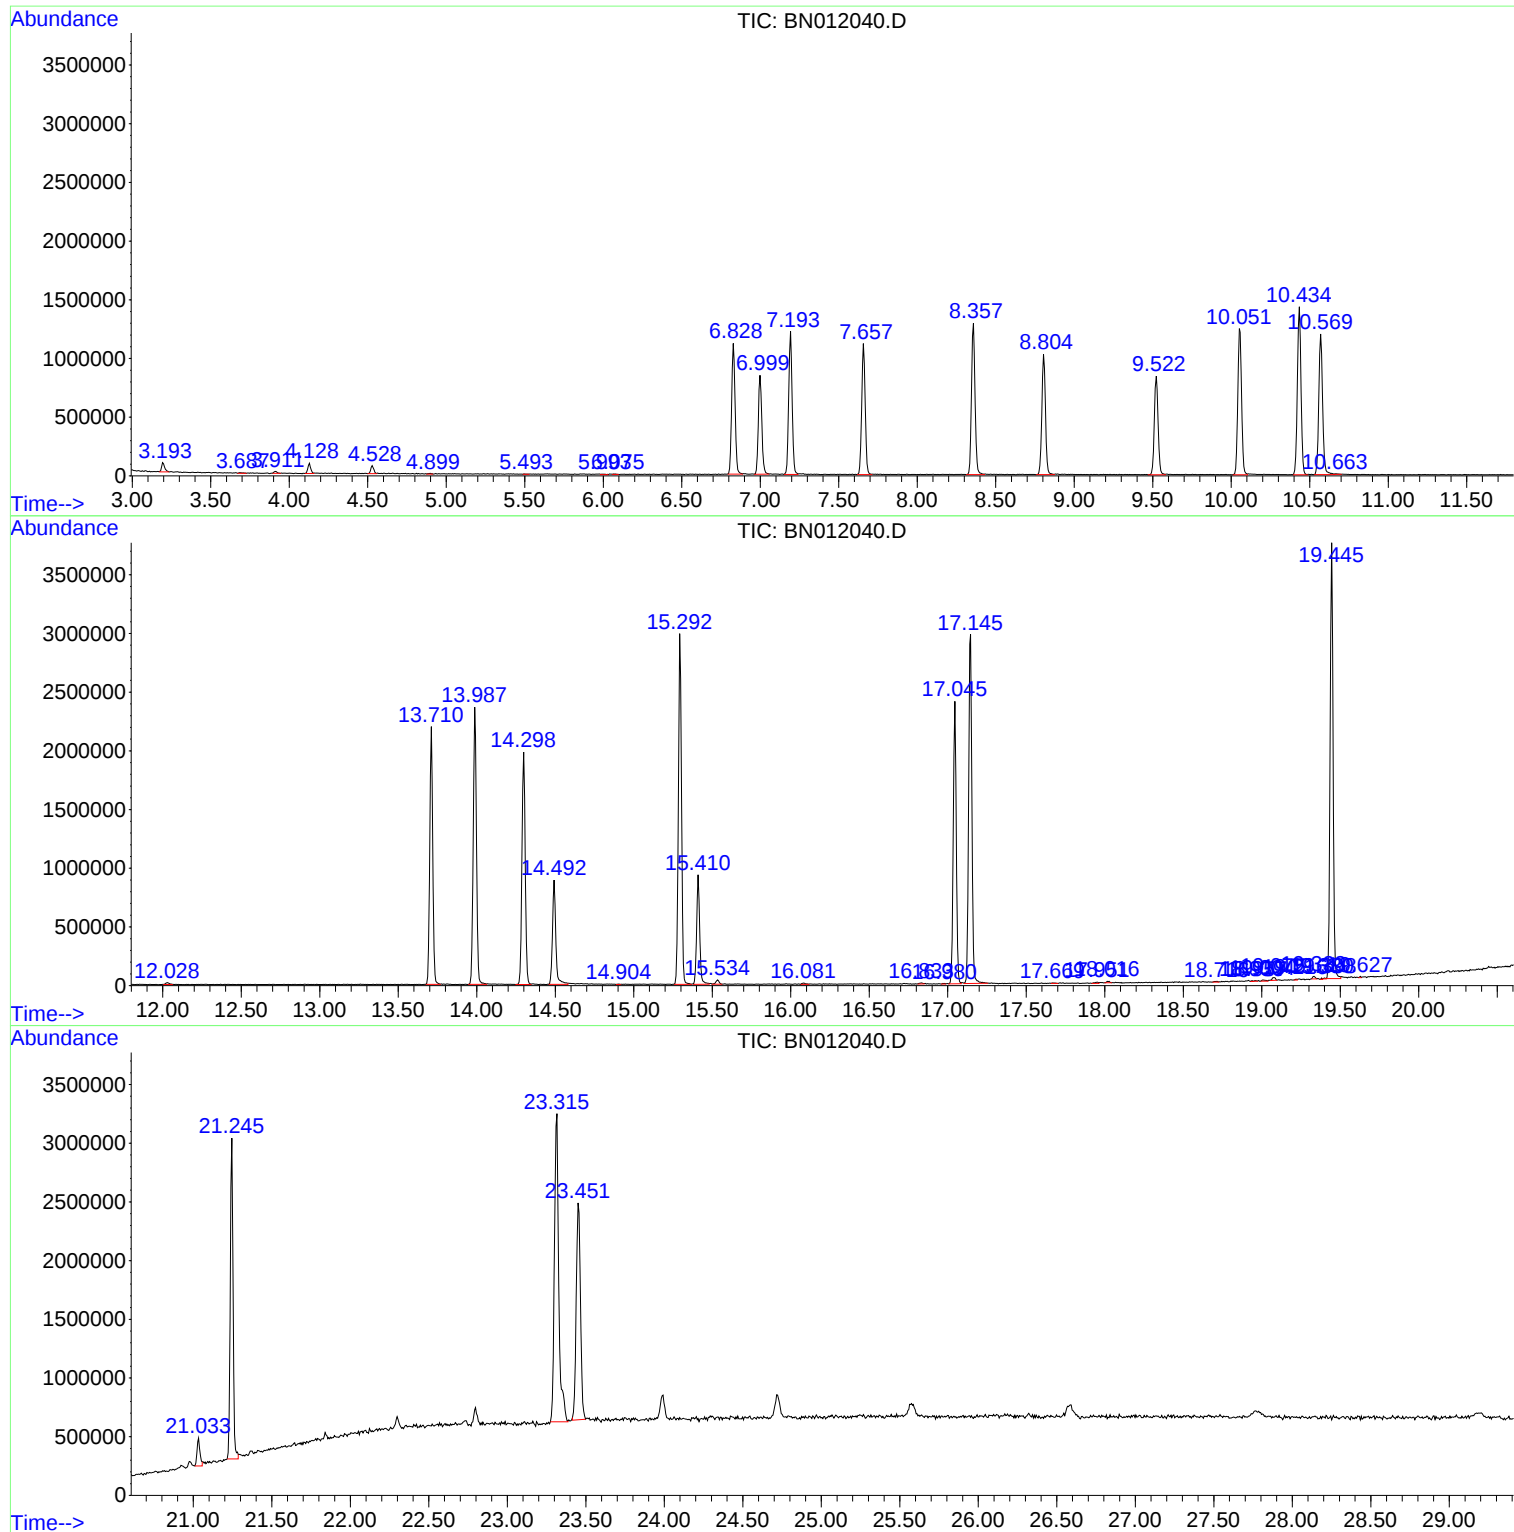

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100220\
Data File : BN012040.D
Acq On : 02 Oct 2020 17:14
Operator : CG/JU
Sample : PB132013BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK13

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN100220.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100220\
Data File : BN012040.D
Acq On : 02 Oct 2020 17:14
Operator : CG/JU
Sample : PB132013BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK13

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN100220.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------