

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100220\
 Data File : BN012052.D
 Acq On : 03 Oct 2020 00:32
 Operator : CG/JU
 Sample : L4166-02
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AB9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoother: OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN100220.M

Title : SVOA CALIBRATION

Signal : TIC: BN012052.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.193	32	35	43	rVB	63321	85208	2.00%	0.162%
2	3.911	154	157	163	rVV6	11934	18860	0.44%	0.036%
3	4.528	259	262	266	rVV5	5249	7891	0.18%	0.015%
4	4.575	268	270	274	rVB4	5493	7464	0.17%	0.014%
5	4.758	299	301	304	rVV3	5029	4780	0.11%	0.009%
6	4.811	308	310	313	rVV3	6869	6765	0.16%	0.013%
7	5.358	400	403	406	rVB4	4207	4917	0.12%	0.009%
8	6.428	581	585	587	rBV4	3353	5105	0.12%	0.010%
9	6.699	627	631	635	rBV6	4273	4798	0.11%	0.009%
10	6.828	647	653	663	rBV	928094	1451754	34.00%	2.757%
11	6.999	676	682	695	rVB	699942	1078424	25.25%	2.048%
12	7.193	708	715	725	rBV	997286	1542260	36.12%	2.929%
13	7.293	728	732	738	rBV3	18700	33138	0.78%	0.063%
14	7.657	786	794	803	rBV	1118280	1701742	39.85%	3.232%
15	7.722	803	805	809	rVB4	6254	7339	0.17%	0.014%
16	8.357	906	913	923	rBV	1099949	1710478	40.05%	3.249%
17	8.804	982	989	1000	rBV	847543	1355611	31.74%	2.575%
18	9.522	1104	1111	1120	rBV	679825	1111864	26.04%	2.112%
19	10.051	1194	1201	1210	rBV	1070235	1745316	40.87%	3.315%
20	10.110	1210	1211	1216	rVB5	5966	8007	0.19%	0.015%
21	10.369	1253	1255	1258	rBV4	3235	4685	0.11%	0.009%
22	10.434	1258	1266	1275	rBV	1373656	2229146	52.20%	4.234%
23	10.569	1282	1289	1303	rBV	989778	1715440	40.17%	3.258%
24	10.857	1336	1338	1341	rVB4	3922	4878	0.11%	0.009%
25	10.887	1341	1343	1350	rBV5	3269	6089	0.14%	0.012%
26	12.034	1533	1538	1541	rVV6	11395	19133	0.45%	0.036%
27	12.410	1597	1602	1605	rBV5	5275	6892	0.16%	0.013%
28	12.657	1638	1644	1646	rBV5	6091	9972	0.23%	0.019%
29	12.904	1682	1686	1692	rVV6	5475	9504	0.22%	0.018%
30	13.128	1721	1724	1728	rBV4	4127	4853	0.11%	0.009%
31	13.192	1730	1735	1741	rVV4	12385	20868	0.49%	0.040%
32	13.263	1743	1747	1750	rVB5	5098	7114	0.17%	0.014%
33	13.410	1768	1772	1776	rVB3	2760	5513	0.13%	0.010%
34	13.710	1817	1823	1827	rBV	1735383	2381119	55.76%	4.523%
35	13.757	1827	1831	1837	rVB	415502	564047	13.21%	1.071%
36	13.987	1864	1870	1883	rBV	2033445	2860134	66.98%	5.432%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100220\
 Data File : BN012052.D
 Acq On : 03 Oct 2020 00:32
 Operator : CG/JU
 Sample : L4166-02
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AB9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN100220.M
 Title : SVOA CALIBRATION

37	14.298	1916	1923	1931	rBV	1941312	2841582	66.54%	5.397%
38	14.492	1948	1956	1969	rBV	445333	726119	17.00%	1.379%
39	14.581	1969	1971	1974	rVB4	4559	4686	0.11%	0.009%
40	14.663	1983	1985	1989	rVB4	4230	4665	0.11%	0.009%
41	14.710	1989	1993	1996	rBV4	2749	5213	0.12%	0.010%
42	15.110	2057	2061	2065	rBV3	6293	11419	0.27%	0.022%
43	15.292	2083	2092	2099	rBV	2585114	3486200	81.64%	6.622%
44	15.410	2106	2112	2124	rBV	553364	766313	17.94%	1.455%
45	15.534	2127	2133	2139	rVB2	27657	40666	0.95%	0.077%
46	15.857	2185	2188	2189	rBV3	4664	4677	0.11%	0.009%
47	15.969	2204	2207	2211	rBV4	5687	6824	0.16%	0.013%
48	16.028	2216	2217	2222	rVV5	4442	4821	0.11%	0.009%
49	16.081	2222	2226	2230	rVV5	8096	11103	0.26%	0.021%
50	16.233	2250	2252	2256	rBV4	3550	5151	0.12%	0.010%
51	16.328	2265	2268	2271	rBV4	3691	5323	0.12%	0.010%
52	16.375	2274	2276	2281	rBV4	3701	5716	0.13%	0.011%
53	16.828	2350	2353	2358	rBV5	10409	18462	0.43%	0.035%
54	16.975	2374	2378	2379	rBV4	6898	10164	0.24%	0.019%
55	17.045	2383	2390	2399	rVV	2272164	3139797	73.52%	5.964%
56	17.139	2399	2406	2417	rBV2	2524759	3621772	84.81%	6.879%
57	17.345	2436	2441	2444	rBV5	7042	12238	0.29%	0.023%
58	17.469	2457	2462	2465	rBV6	3355	5237	0.12%	0.010%
59	17.586	2479	2482	2484	rBV4	4524	6515	0.15%	0.012%
60	17.675	2493	2497	2498	rBV4	4158	5634	0.13%	0.011%
61	17.945	2538	2543	2552	rBV4	115774	193368	4.53%	0.367%
62	18.022	2553	2556	2560	rVB	12604	19488	0.46%	0.037%
63	18.116	2568	2572	2575	rBV5	4006	6697	0.16%	0.013%
64	18.451	2627	2629	2631	rBV3	4949	4618	0.11%	0.009%
65	18.475	2631	2633	2634	rBV2	6126	4318	0.10%	0.008%
66	18.627	2657	2659	2662	rVB4	6940	5334	0.12%	0.010%
67	18.827	2690	2693	2695	rBV3	7727	9630	0.23%	0.018%
68	19.074	2731	2735	2740	rBV3	25090	40302	0.94%	0.077%
69	19.204	2755	2757	2758	rVV2	7957	4696	0.11%	0.009%
70	19.239	2759	2763	2769	rVV6	28082	48402	1.13%	0.092%
71	19.327	2774	2778	2785	rBV2	33607	52683	1.23%	0.100%
72	19.392	2787	2789	2791	rBV2	9788	10158	0.24%	0.019%
73	19.445	2792	2798	2806	rBV	2950414	4072568	95.37%	7.735%
74	20.957	3052	3055	3062	rBV4	229840	322639	7.56%	0.613%
75	21.027	3064	3067	3072	rVV	88227	109247	2.56%	0.207%
76	21.239	3098	3103	3108	rBV	2740568	3397283	79.55%	6.453%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100220\
Data File : BN012052.D
Acq On : 03 Oct 2020 00:32
Operator : CG/JU
Sample : L4166-02
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AB9

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN100220.M
Title : SVOA CALIBRATION

77	23.304	3448	3454	3466	rVB	2303919	4270410	100.00%	8.111%
78	23.445	3472	3478	3490	rVB2	1976404	3586403	83.98%	6.812%




Sum of corrected areas: 52649649

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100220\
Data File : BN012052.D
Acq On : 03 Oct 2020 00:32
Operator : CG/JU
Sample : L4166-02
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AB9

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN100220.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

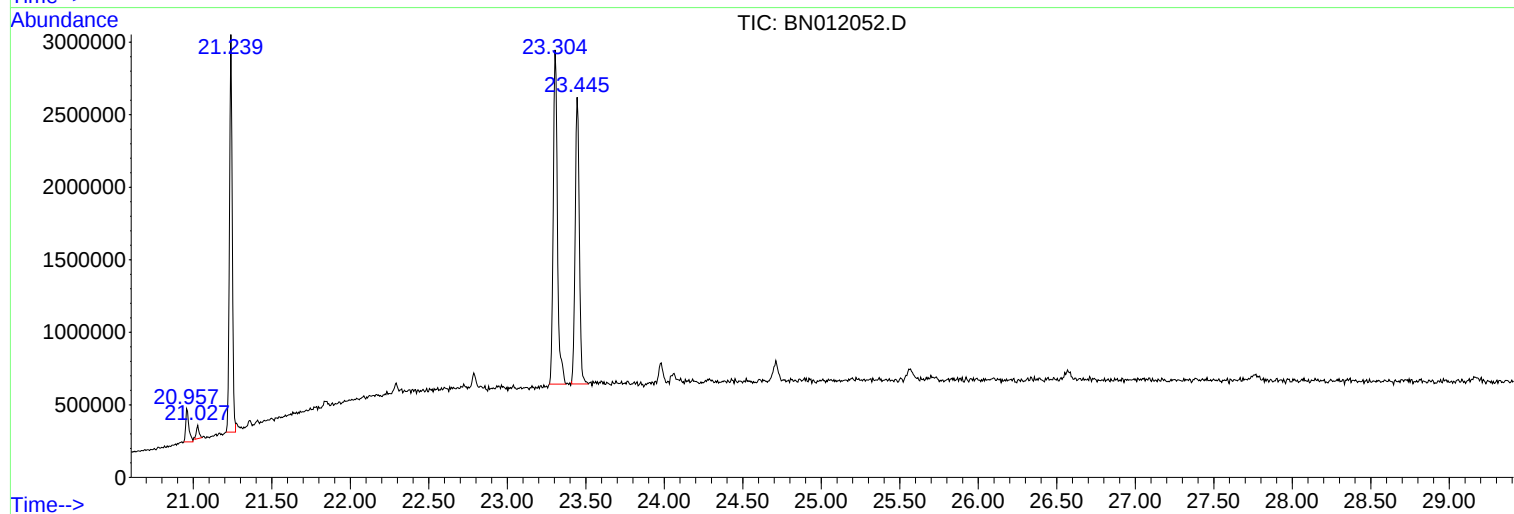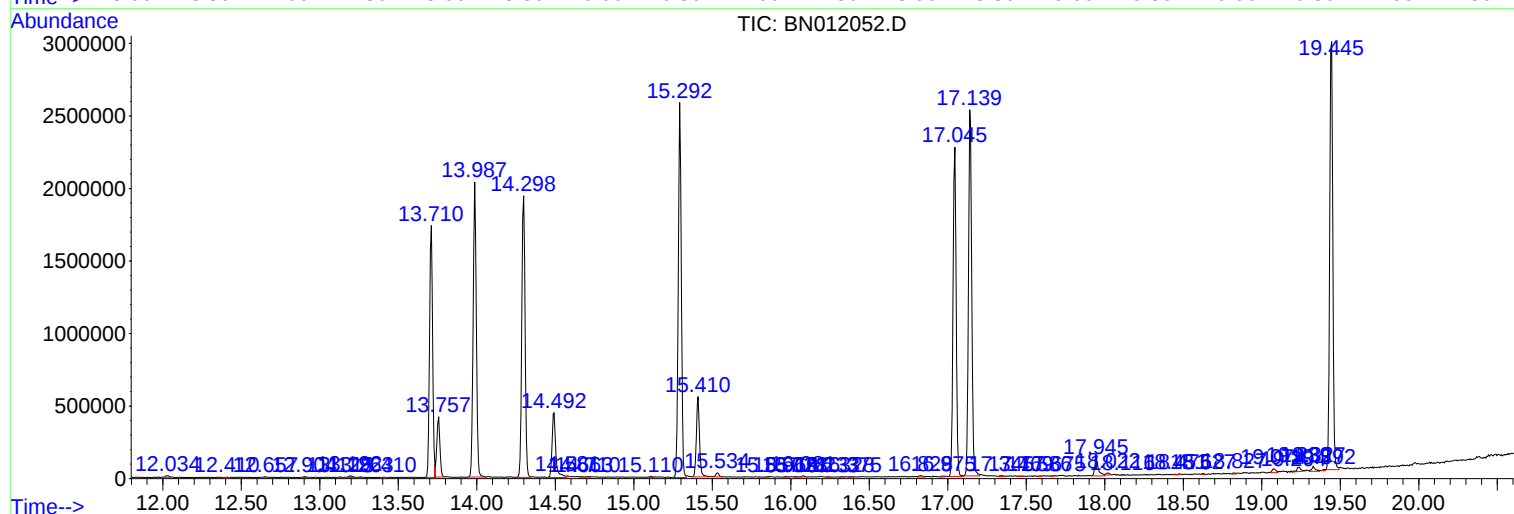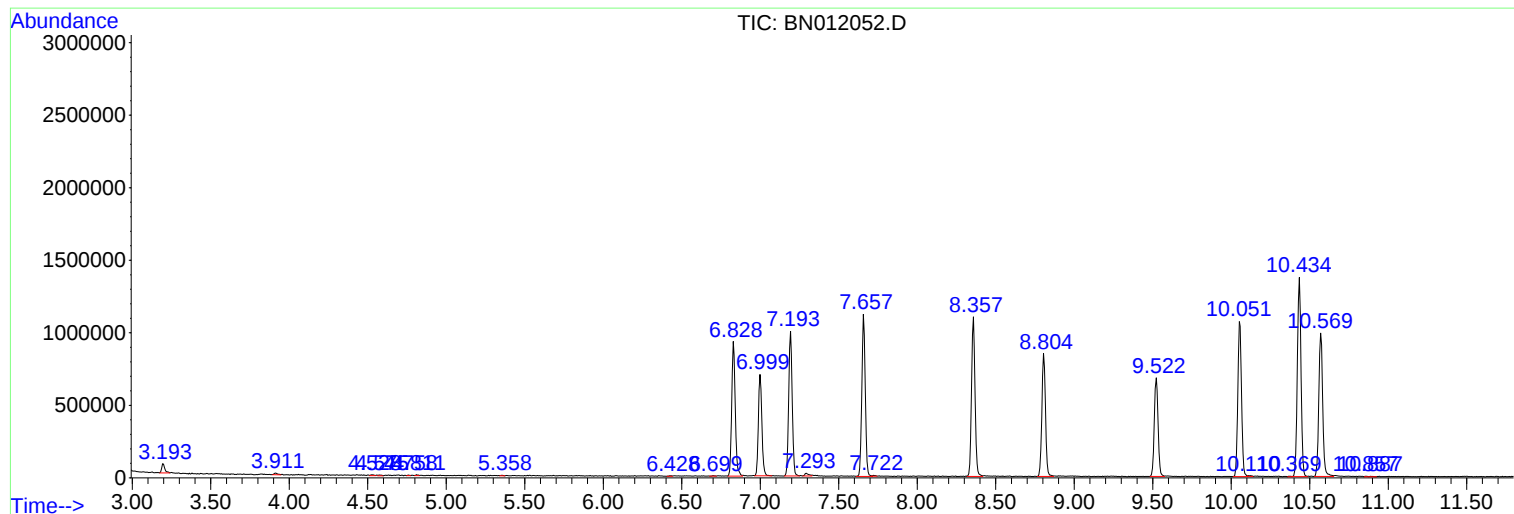

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100220\
Data File : BN012052.D
Acq On : 03 Oct 2020 00:32
Operator : CG/JU
Sample : L4166-02
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AB9

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN100220.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100220\
Data File : BN012052.D
Acq On : 03 Oct 2020 00:32
Operator : CG/JU
Sample : L4166-02
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AB9

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN100220.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
