




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100224\
Data File : BN034384.D
Acq On : 03 Oct 2024 23:46
Operator : RC/JU
Sample : P4084-11
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DCYM9

Manual IntegrationsAPPROVED

Quant Time: Oct 04 01:08:39 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Sep 30 14:14:38 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/05/2024
Supervised By :mohammad ahmed 10/05/2024

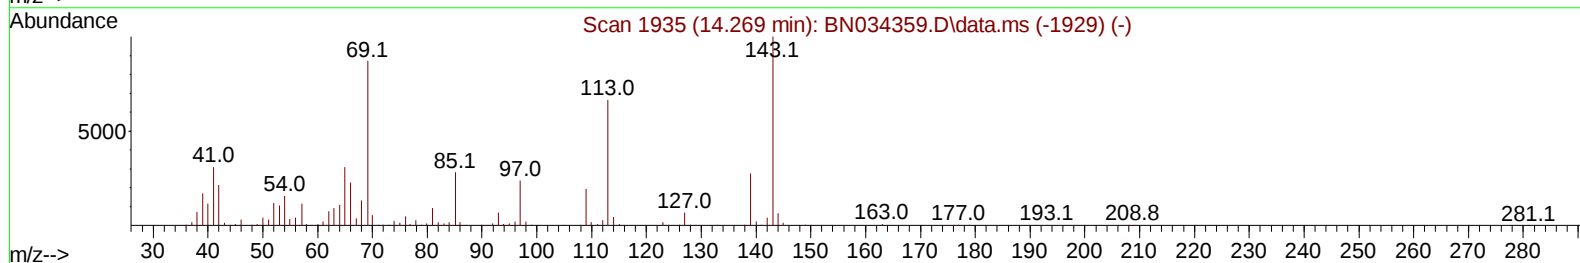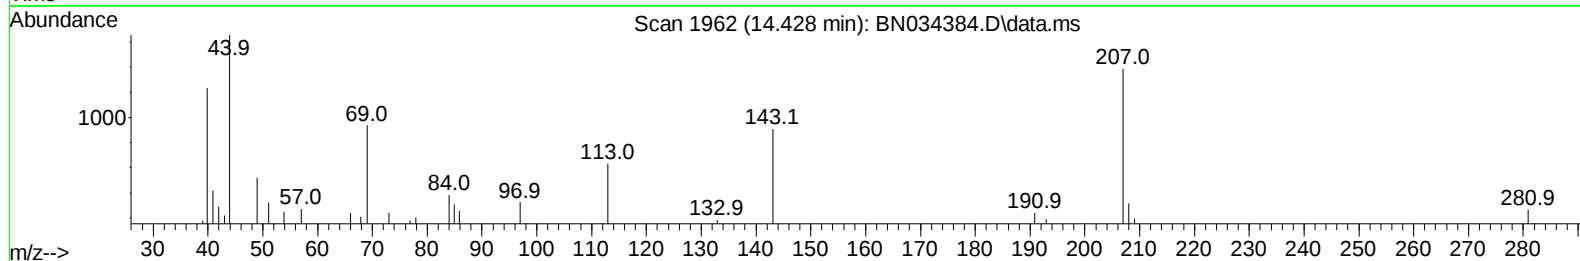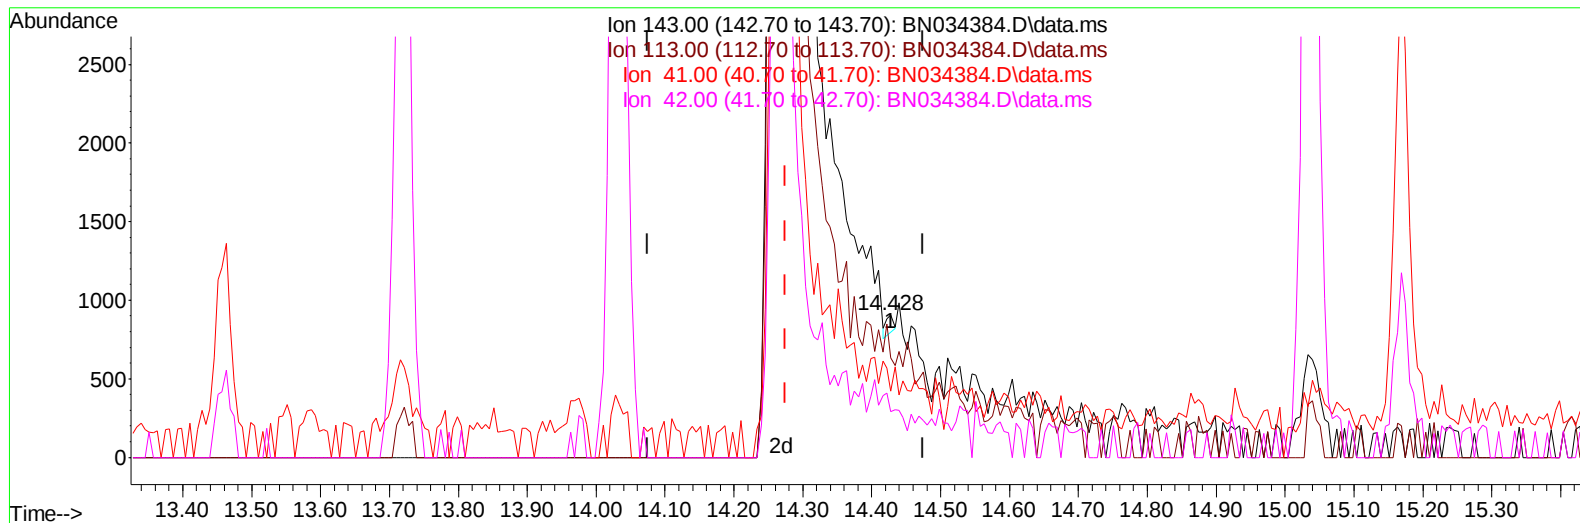

TIC: BN034384.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.428min (+ 0.153) 0.01 ng/u1

response 89

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	76.90	69.71
41.00	41.70	46.26
42.00	28.50	31.94




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100224\
Data File : BN034384.D
Acq On : 03 Oct 2024 23:46
Operator : RC/JU
Sample : P4084-11
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DCYM9

Manual IntegrationsAPPROVED

Quant Time: Oct 04 01:08:39 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Sep 30 14:14:38 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/05/2024
Supervised By :mohammad ahmed 10/05/2024

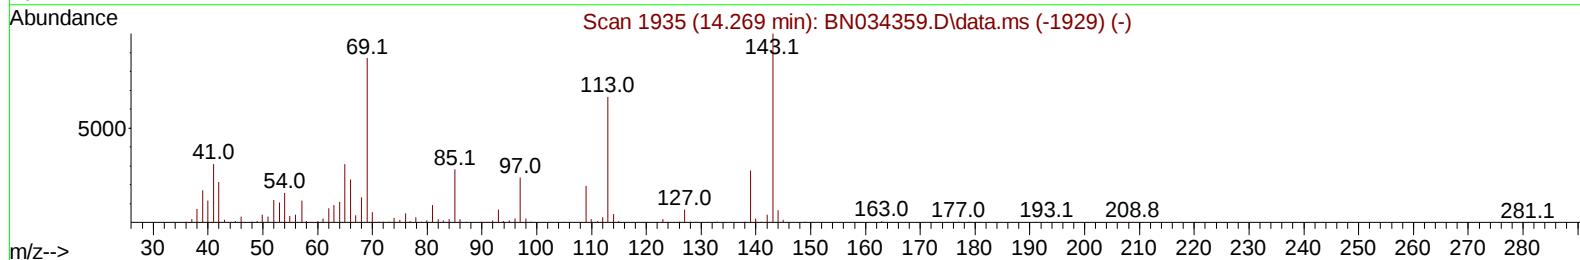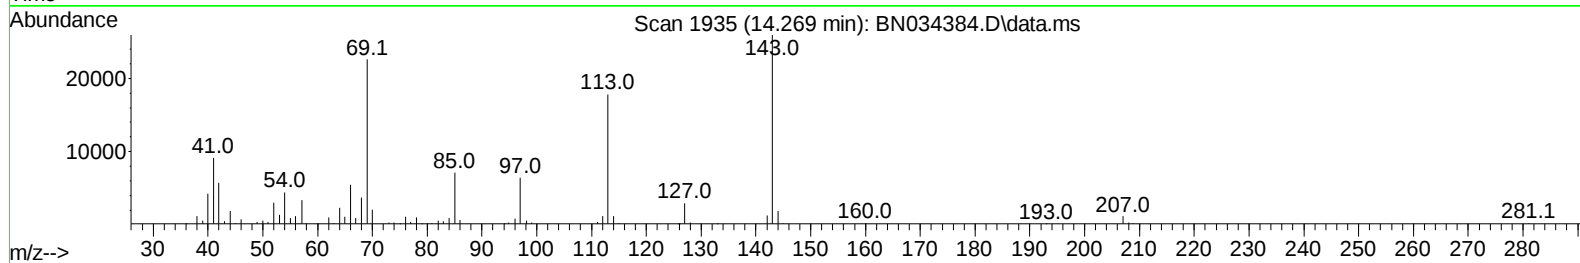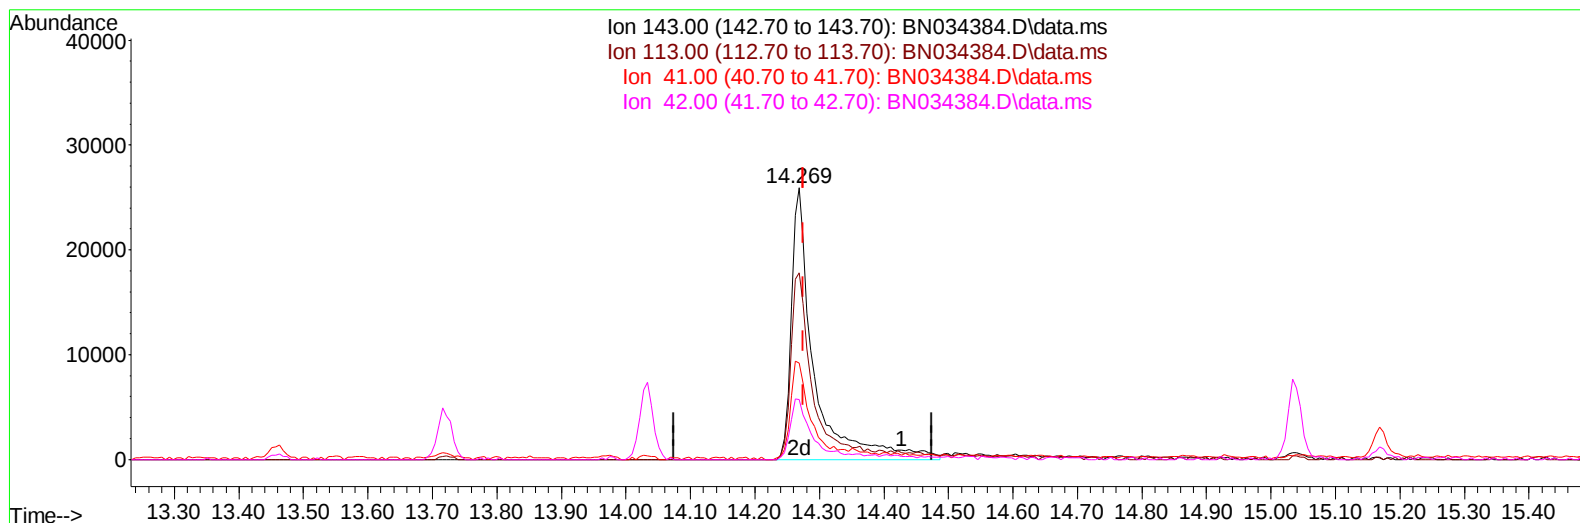

TIC: BN034384.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.269min (-0.006) 9.51 ng/ul m

response 62856

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	76.90	68.76
41.00	41.70	35.39
42.00	28.50	22.13#

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100224\
 Data File : BN034384.D
 Acq On : 03 Oct 2024 23:46
 Operator : RC/JU
 Sample : P4084-11
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DCYM9

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 10/05/2024
 Supervised By :mohammad ahmed 10/05/2024

Quant Time: Oct 04 01:12:05 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Sep 30 14:14:38 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.381	152	197324	20.000	ng/ul	0.00
20) Naphthalene-d8	10.134	136	736811	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.034	164	431091	20.000	ng/ul	0.00
64) Phenanthrene-d10	16.792	188	866261	20.000	ng/ul	0.00
79) Chrysene-d12	21.027	240	902396	20.000	ng/ul	0.00
88) Perylene-d12	23.733	264	1123869	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.005	96	14425	2.983	ng/uL	0.00
4) Pyridine-d5	3.393	84	157059	10.927	ng/ul	0.00
7) Phenol-d5	6.581	99	237000	13.533	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.734	67	147167	13.544	ng/ul	0.00
11) 2-Chlorophenol-d4	6.922	132	212324	15.403	ng/ul	0.00
15) 4-Methylphenol-d8	8.099	113	191276	13.274	ng/ul	0.00
21) Nitrobenzene-d5	8.522	128	97591	16.617	ng/ul	0.00
24) 2-Nitrophenol-d4	9.234	143	99252	16.435	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.769	165	181980	16.001	ng/ul	0.00
31) 4-Chloroaniline-d4	10.287	131	262472	15.244	ng/ul	0.00
46) Dimethylphthalate-d6	13.463	166	573688	17.807	ng/ul	0.00
49) Acenaphthylene-d8	13.722	160	667021	18.404	ng/ul	0.00
54) 4-Nitrophenol-d4	14.269	143	62856m	9.507	ng/ul	0.00
60) Fluorene-d10	15.039	176	511317	18.727	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.169	200	49789	9.640	ng/ul	0.00
73) Anthracene-d10	16.886	188	780969	19.176	ng/ul	-0.01
81) Pyrene-d10	19.198	212	960893	19.111	ng/ul	-0.01
92) Benzo(a)pyrene-d12	23.551	264	1119449	19.391	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100224\
Data File : BN034384.D
Acq On : 03 Oct 2024 23:46
Operator : RC/JU
Sample : P4084-11
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DCYM9

Manual IntegrationsAPPROVED

Quant Time: Oct 04 01:12:05 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Sep 30 14:14:38 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/05/2024
Supervised By :mohammad ahmed 10/05/2024

