

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100224\
 Data File : BN034335.D
 Acq On : 02 Oct 2024 13:40
 Operator : RC/JU
 Sample : P4016-13
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DCVW4

Quant Time: Oct 02 14:55:52 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Sep 30 14:14:38 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.387	152	250107	20.000	ng/ul	0.00
20) Naphthalene-d8	10.139	136	1010295	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.039	164	631314	20.000	ng/ul	0.00
64) Phenanthrene-d10	16.798	188	1232355	20.000	ng/ul	0.00
79) Chrysene-d12	21.033	240	1011649	20.000	ng/ul	# 0.00
88) Perylene-d12	23.745	264	1206239	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.005	96	19912	3.249	ng/uL	0.00
4) Pyridine-d5	3.393	84	247430	13.582	ng/ul	0.00
7) Phenol-d5	6.587	99	349527	15.747	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.740	67	206921	15.025	ng/ul	0.00
11) 2-Chlorophenol-d4	6.928	132	300207	17.182	ng/ul	0.00
15) 4-Methylphenol-d8	8.098	113	294217	16.109	ng/ul	0.00
21) Nitrobenzene-d5	8.528	128	139292	17.298	ng/ul	0.00
24) 2-Nitrophenol-d4	9.240	143	146538	17.697	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.775	165	276956	17.760	ng/ul	0.00
31) 4-Chloroaniline-d4	10.287	131	400620	16.969	ng/ul	0.00
46) Dimethylphthalate-d6	13.463	166	899498	19.065	ng/ul	0.00
49) Acenaphthylene-d8	13.728	160	990261	18.657	ng/ul	0.00
54) 4-Nitrophenol-d4	14.269	143	88027	9.091	ng/ul	0.00
60) Fluorene-d10	15.039	176	753515	18.845	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.175	200	81742	11.125	ng/ul	0.00
73) Anthracene-d10	16.892	188	1139403	19.666	ng/ul	0.00
81) Pyrene-d10	19.204	212	1237551	21.955	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.556	264	1213689	19.588	ng/ul	0.00
Target Compounds						
					Qvalue	
71) Pentachlorophenol	16.451	266	78213	8.085	ng/ul	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100224\
Data File : BN034335.D
Acq On : 02 Oct 2024 13:40
Operator : RC/JU
Sample : P4016-13
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DCVW4


Quant Time: Oct 02 14:55:52 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Sep 30 14:14:38 2024
Response via : Initial Calibration

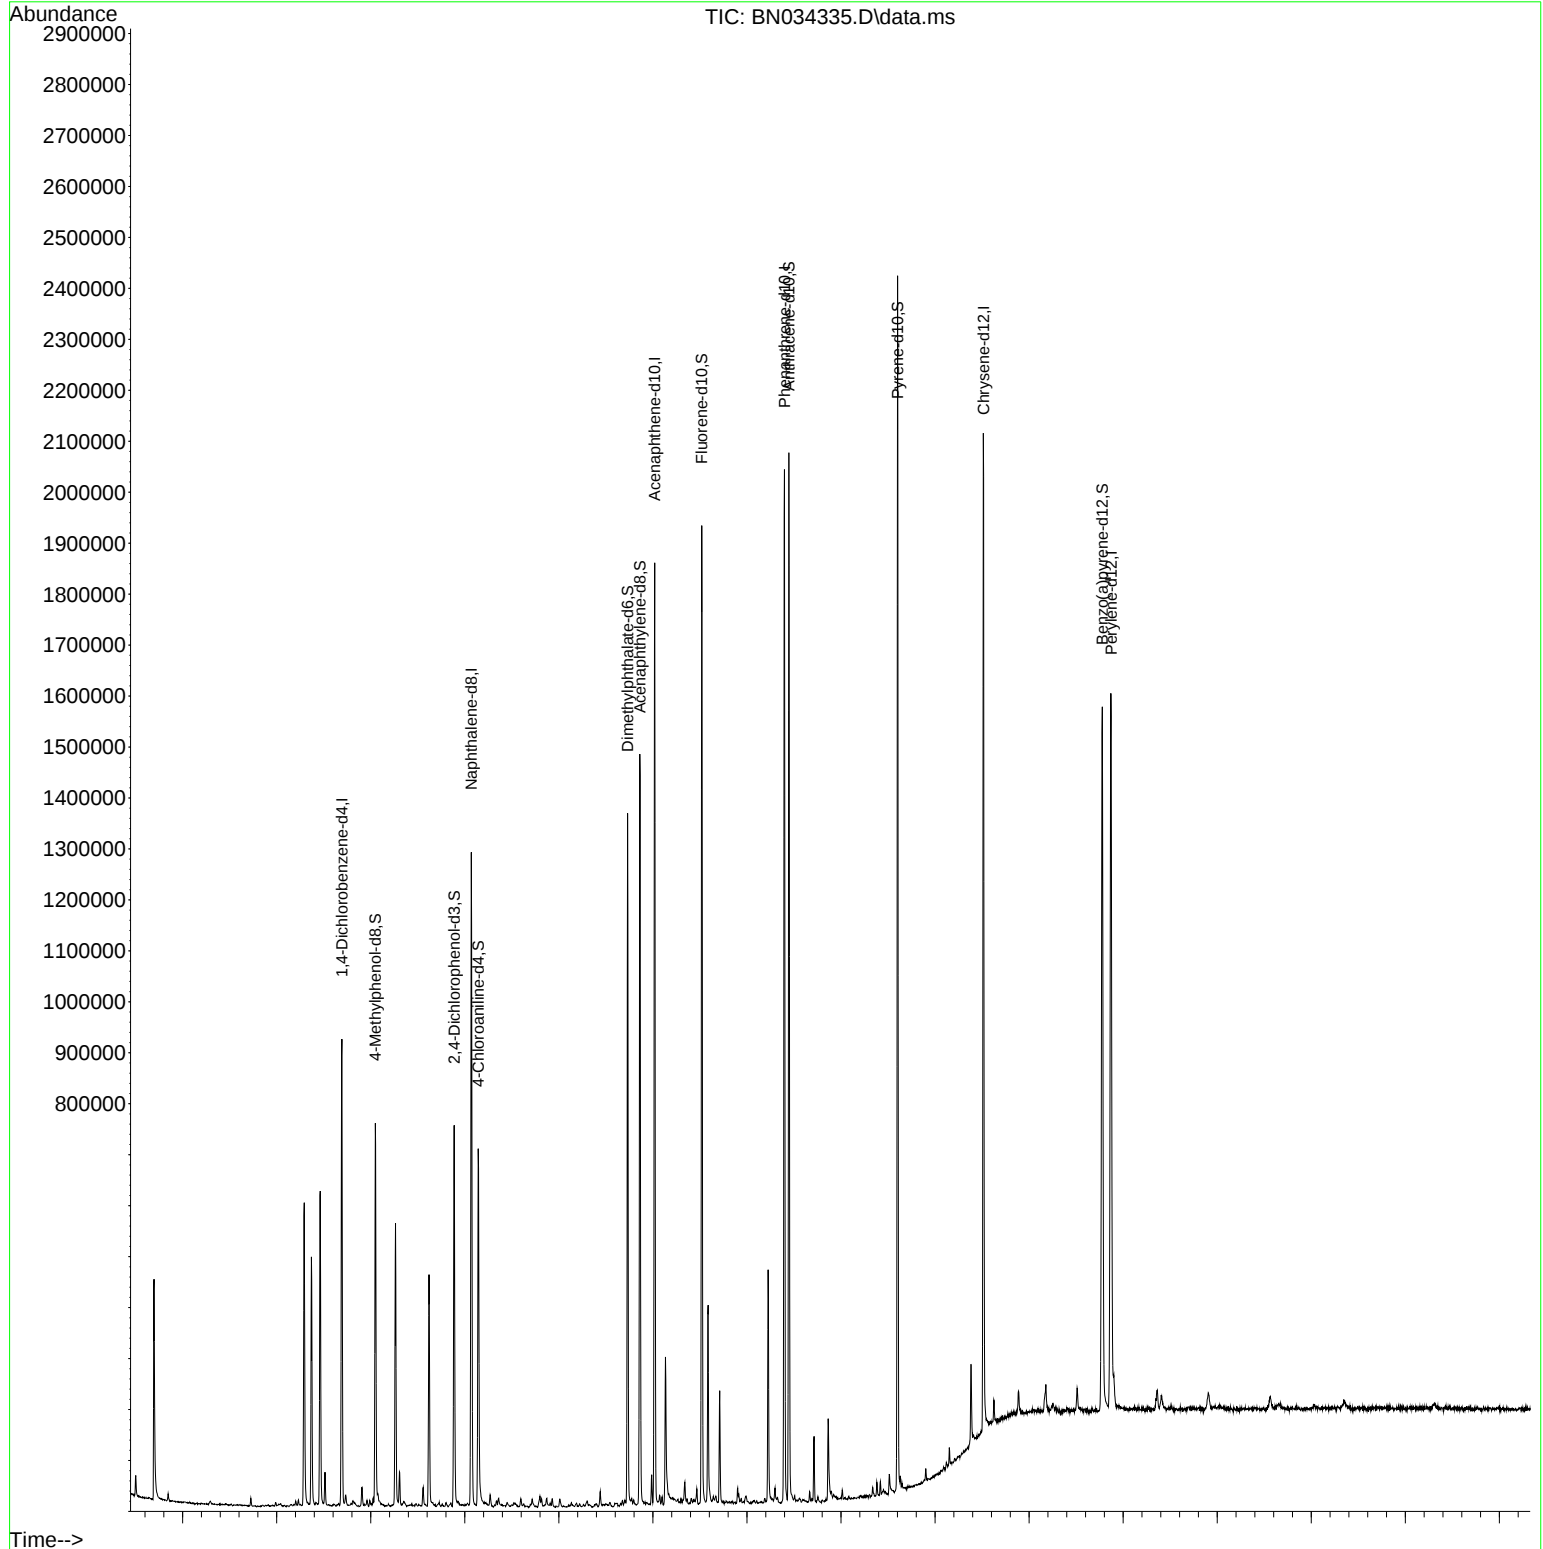

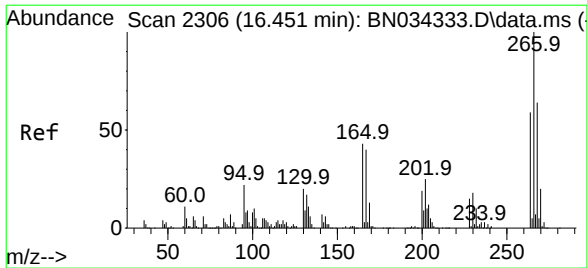

#71
Pentachlorophenol
Concen: 8.085 ng/ul
RT: 16.451 min Scan# 23
Delta R.T. -0.006 min
Lab File: BN034335.D
Acq: 02 Oct 2024 13:40

Instrument :
BNA_N
ClientSampleId :
DCVW4

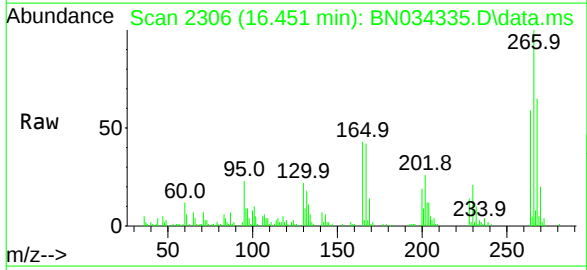

Tgt Ion:	266	Resp:	78213
Ion	Ratio	Lower	Upper
266	100		
264	58.9	51.1	76.7
268	64.6	52.8	79.2

