

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100224\
 Data File : BN034334.D
 Acq On : 02 Oct 2024 13:01
 Operator : RC/JU
 Sample : PB163456BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK456

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN034334.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.005	16	20	26	rVB	63544	80103	1.59%	0.161%
2	3.393	82	86	109	rBV	631056	1021025	20.32%	2.048%
3	3.693	133	137	142	rVB	19250	24853	0.49%	0.050%
4	6.587	622	629	644	rBV	747035	1230554	24.49%	2.468%
5	6.740	649	655	671	rVB	656087	1026873	20.44%	2.059%
6	6.922	679	686	698	rBV	831676	1335929	26.59%	2.679%
7	7.387	758	765	775	rBV	804212	1248348	24.85%	2.503%
8	8.099	880	886	906	rBV	946684	1572452	31.30%	3.153%
9	8.528	952	959	976	rVV	757515	1227870	24.44%	2.462%
10	9.240	1072	1080	1094	rBV	613004	989478	19.70%	1.984%
11	9.775	1164	1171	1184	rBV	947023	1574724	31.35%	3.158%
12	10.063	1216	1220	1224	rBV6	2900	5418	0.11%	0.011%
13	10.140	1226	1233	1244	rVB	1056984	1735897	34.55%	3.481%
14	10.287	1251	1258	1291	rBV	850720	1598514	31.82%	3.206%
15	11.745	1499	1506	1513	rBV	12212	23949	0.48%	0.048%
16	13.463	1791	1798	1817	rBV	1582195	2254191	44.87%	4.520%
17	13.722	1835	1842	1860	rBV	1852670	2796854	55.67%	5.609%
18	14.039	1889	1896	1909	rBV	1535158	2285450	45.49%	4.583%
19	14.269	1927	1935	1955	rBV	517099	928638	18.48%	1.862%
20	15.039	2060	2066	2083	rBV	2326701	3452914	68.73%	6.924%
21	15.175	2083	2089	2100	rVV	620727	847949	16.88%	1.700%
22	15.281	2104	2107	2114	rVB4	12237	20879	0.42%	0.042%
23	15.833	2197	2201	2207	rVB5	6681	8622	0.17%	0.017%
24	16.386	2291	2295	2297	rBV3	5514	8316	0.17%	0.017%
25	16.451	2303	2306	2309	rBV5	4896	6727	0.13%	0.013%
26	16.586	2325	2329	2333	rBV5	4042	7012	0.14%	0.014%
27	16.798	2358	2365	2375	rBV	1853344	2670568	53.16%	5.355%
28	16.892	2375	2381	2394	rVV2	2580254	3719344	74.04%	7.459%
29	17.845	2539	2543	2548	rBV7	4070	8126	0.16%	0.016%
30	18.763	2695	2699	2706	rBV2	32485	47431	0.94%	0.095%
31	18.839	2708	2712	2717	rVB	28659	37942	0.76%	0.076%
32	19.204	2768	2774	2791	rBV	3140958	4429564	88.17%	8.883%
33	21.033	3079	3085	3099	rBV	2062852	3081470	61.34%	6.179%
34	23.557	3506	3514	3530	rBV2	2259478	5023764	100.00%	10.075%
35	23.739	3537	3545	3553	rBV	1543008	3534275	70.35%	7.088%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100224\
Data File : BN034334.D
Acq On : 02 Oct 2024 13:01
Operator : RC/JU
Sample : PB163456BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK456

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 49866023

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100224\
Data File : BN034334.D
Acq On : 02 Oct 2024 13:01
Operator : RC/JU
Sample : PB163456BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK456

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

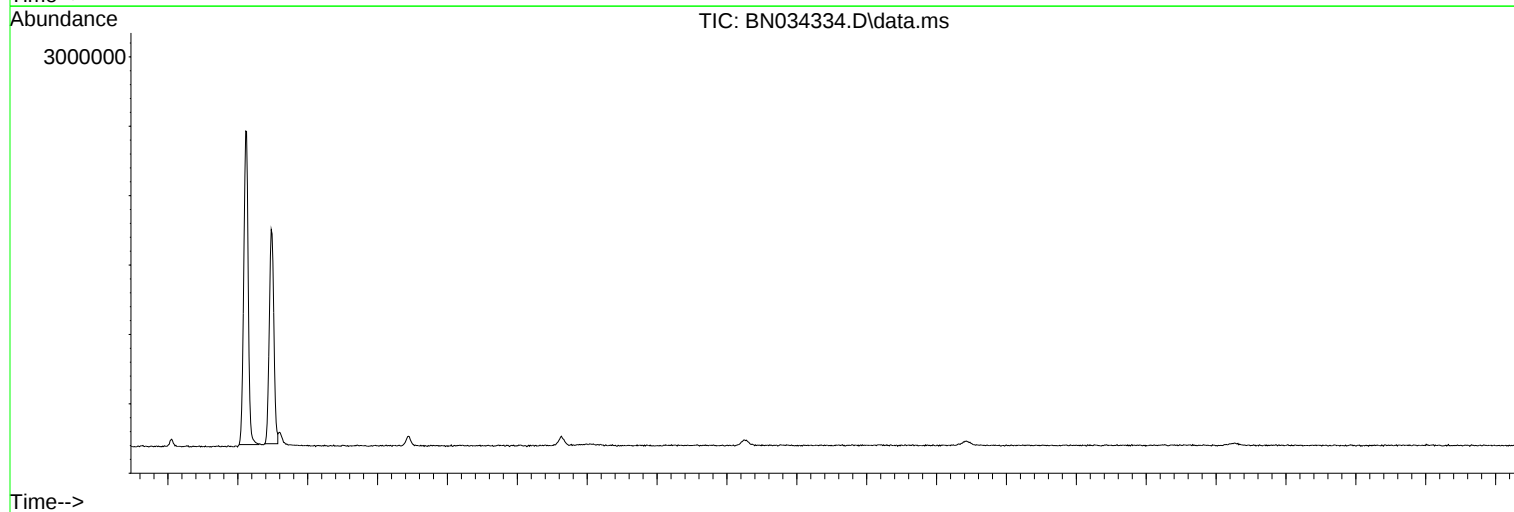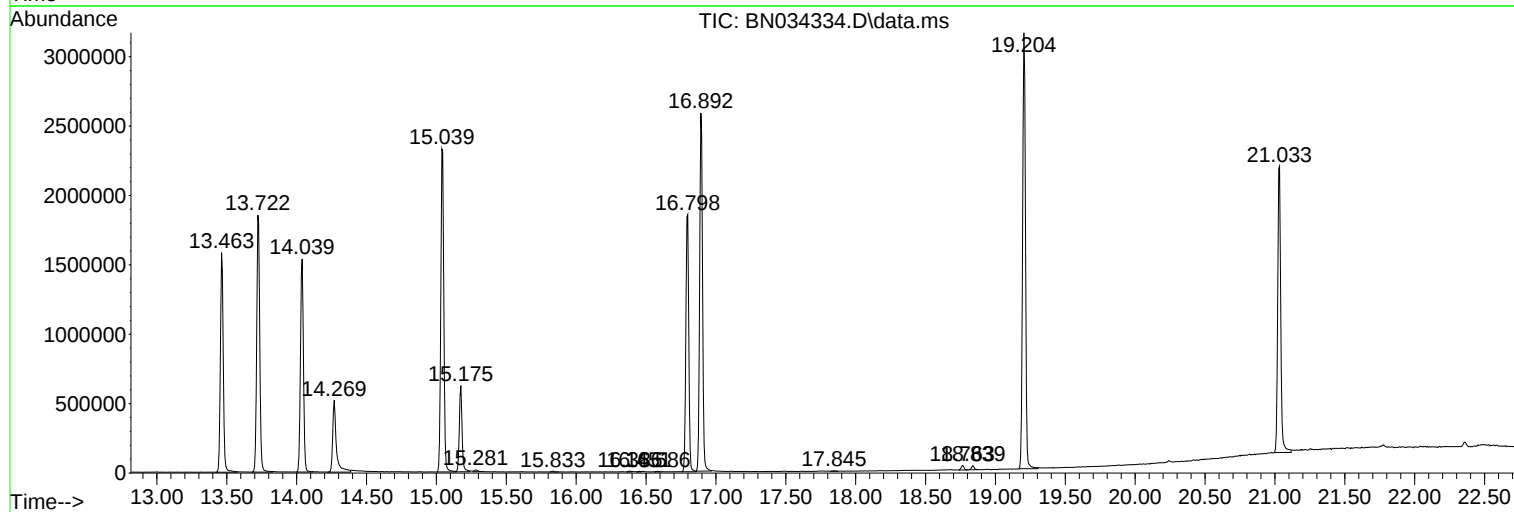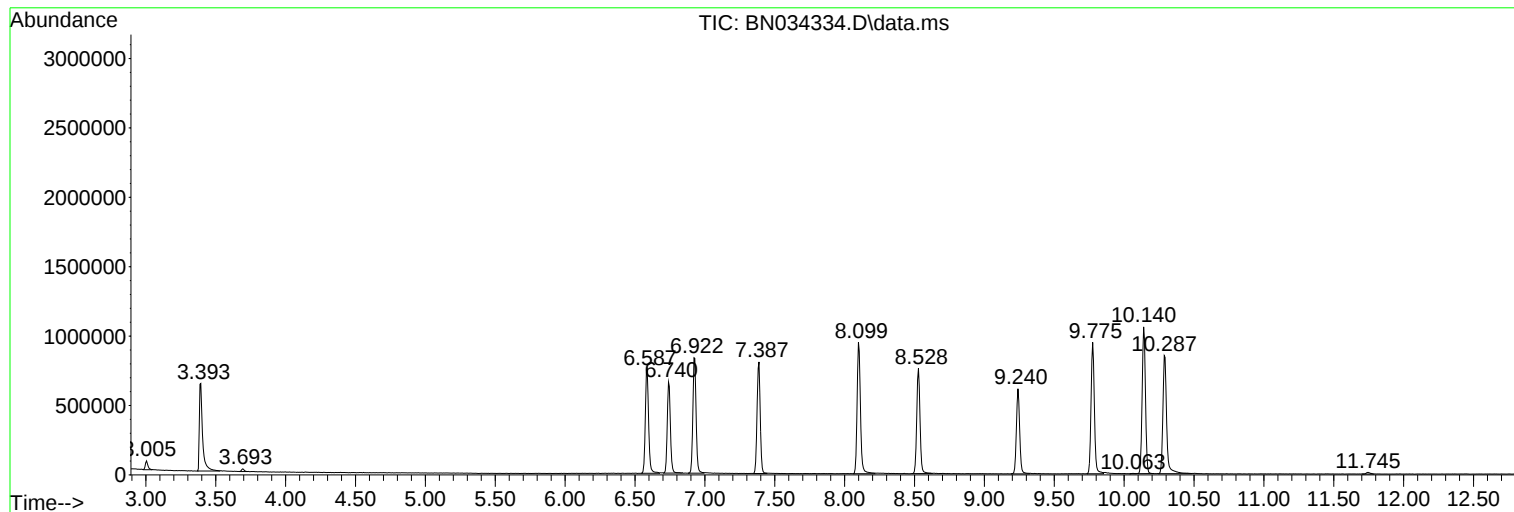

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100224\
Data File : BN034334.D
Acq On : 02 Oct 2024 13:01
Operator : RC/JU
Sample : PB163456BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK456

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100224\
Data File : BN034334.D
Acq On : 02 Oct 2024 13:01
Operator : RC/JU
Sample : PB163456BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK456

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc