

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100224\
Data File : BN034347.D
Acq On : 02 Oct 2024 22:50
Operator : RC/JU
Sample : PB163513BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK513

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
Title : SVOA CALIBRATION

Signal : TIC: BN034347.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.005	16	20	32	rVB	68200	96392	1.75%	0.173%
2	3.387	81	85	100	rBV	779982	1157365	21.01%	2.076%
3	3.693	133	137	143	rVB	23855	31032	0.56%	0.056%
4	6.587	621	629	640	rBV	933878	1457782	26.47%	2.615%
5	6.740	649	655	668	rVB	778431	1189832	21.60%	2.134%
6	6.922	680	686	703	rBV	983312	1588539	28.84%	2.849%
7	7.387	757	765	773	rBV	929286	1450002	26.32%	2.601%
8	8.099	879	886	903	rBV	1115467	1843413	33.47%	3.306%
9	8.528	948	959	974	rBV	893737	1419908	25.78%	2.547%
10	9.240	1072	1080	1092	rBV	731229	1164614	21.14%	2.089%
11	9.775	1164	1171	1183	rBV	1112458	1842827	33.46%	3.305%
12	10.140	1226	1233	1241	rBV	1267587	2049235	37.20%	3.676%
13	10.287	1250	1258	1279	rBV	1018859	1835885	33.33%	3.293%
14	11.745	1501	1506	1514	rBV	13025	26376	0.48%	0.047%
15	13.463	1791	1798	1817	rBV	1835946	2530222	45.94%	4.538%
16	13.722	1836	1842	1855	rBV	2119281	3221077	58.48%	5.777%
17	14.039	1889	1896	1913	rBV	1780758	2598904	47.18%	4.661%
18	14.269	1927	1935	1950	rBV	538543	944183	17.14%	1.694%
19	15.039	2060	2066	2080	rBV	2620635	3869765	70.26%	6.941%
20	15.175	2083	2089	2101	rVV	678183	940351	17.07%	1.687%
21	15.281	2104	2107	2113	rVB3	13010	20253	0.37%	0.036%
22	15.833	2197	2201	2206	rVB4	6365	8643	0.16%	0.016%
23	16.386	2290	2295	2302	rBV9	5052	9774	0.18%	0.018%
24	16.457	2302	2307	2308	rBV4	6867	7740	0.14%	0.014%
25	16.580	2324	2328	2335	rVB3	5334	8975	0.16%	0.016%
26	16.792	2358	2364	2375	rBV	1957583	2880430	52.29%	5.166%
27	16.892	2375	2381	2397	rVB2	2849211	4077436	74.03%	7.313%
28	18.033	2571	2575	2580	rBV6	4164	8065	0.15%	0.014%
29	18.763	2695	2699	2706	rBV2	36740	48231	0.88%	0.087%
30	18.839	2708	2712	2720	rVB	32626	46946	0.85%	0.084%
31	19.204	2767	2774	2787	rBV	3507090	4739745	86.05%	8.501%
32	21.027	3079	3084	3095	rBV	2326980	3213357	58.34%	5.764%
33	23.021	3419	3423	3429	rVB2	92659	155706	2.83%	0.279%
34	23.557	3505	3514	3532	rBV2	2559836	5508094	100.00%	9.879%
35	23.739	3537	3545	3552	rBV	1645773	3761716	68.29%	6.747%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100224\
Data File : BN034347.D
Acq On : 02 Oct 2024 22:50
Operator : RC/JU
Sample : PB163513BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK513

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 55752815

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100224\
Data File : BN034347.D
Acq On : 02 Oct 2024 22:50
Operator : RC/JU
Sample : PB163513BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK513

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

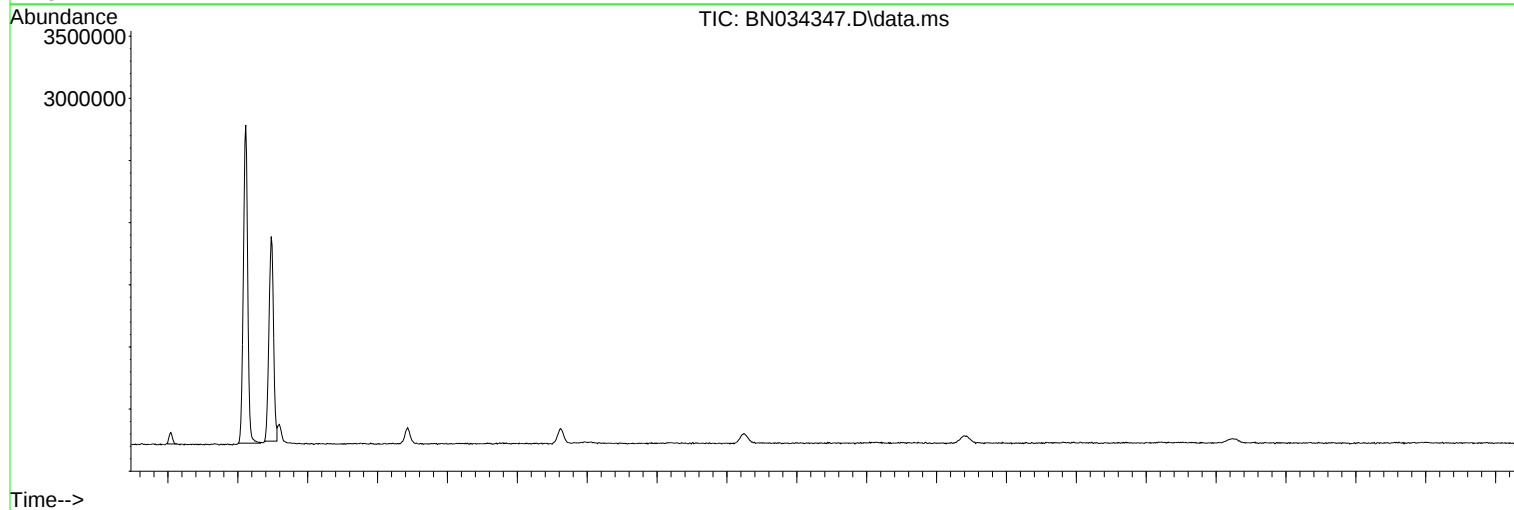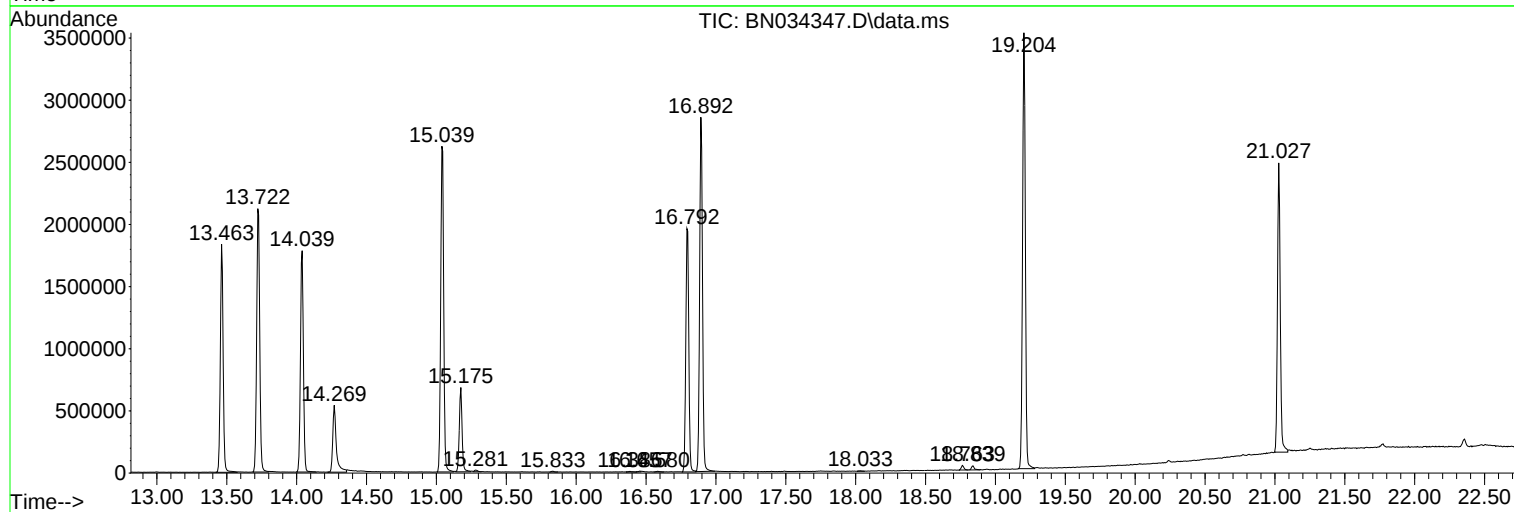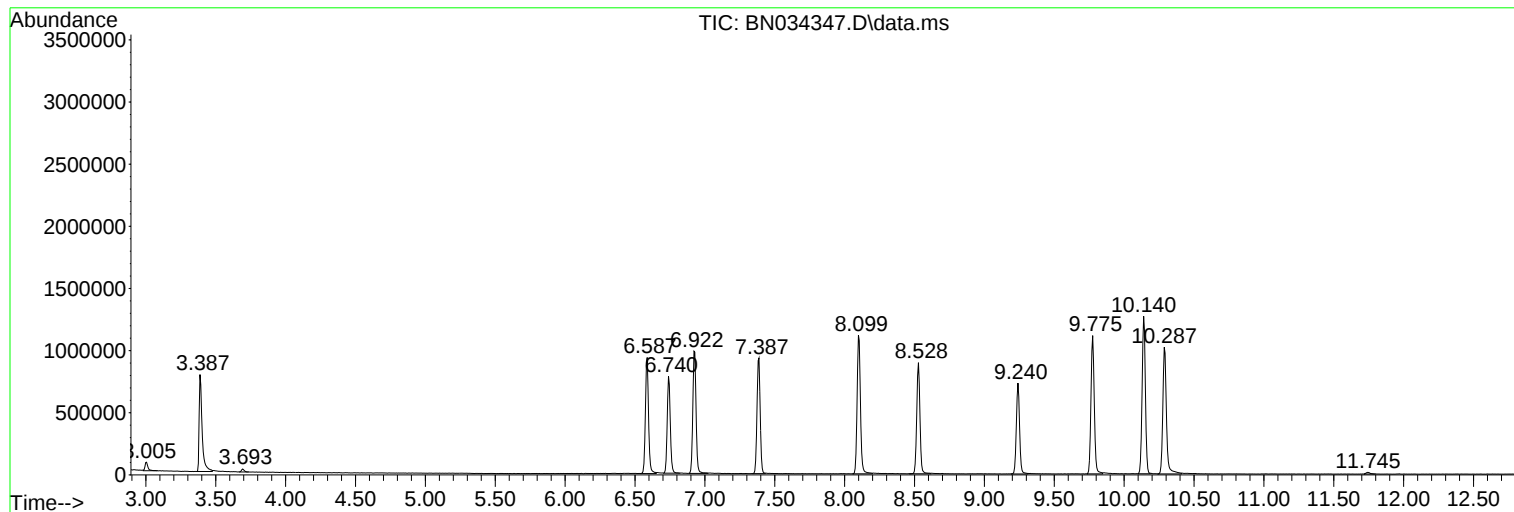

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100224\
Data File : BN034347.D
Acq On : 02 Oct 2024 22:50
Operator : RC/JU
Sample : PB163513BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK513

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100224\
Data File : BN034347.D
Acq On : 02 Oct 2024 22:50
Operator : RC/JU
Sample : PB163513BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK513

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc
