

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100224\
 Data File : BN034360.D
 Acq On : 03 Oct 2024 08:00
 Operator : RC/JU
 Sample : PB163489BL
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK489

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN034360.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.005	16	20	31	rVB	63832	92259	2.07%	0.182%
2	3.387	82	85	106	rBV	732260	1086515	24.43%	2.144%
3	3.693	133	137	143	rVB	17795	23559	0.53%	0.046%
4	6.581	620	628	645	rBV	806222	1280997	28.80%	2.528%
5	6.740	649	655	668	rVB	677755	1026877	23.09%	2.027%
6	6.922	679	686	698	rBV	922164	1414010	31.79%	2.791%
7	7.381	757	764	776	rBV	1083393	1679696	37.77%	3.315%
8	8.099	879	886	904	rBV	963940	1560872	35.10%	3.080%
9	8.522	950	958	969	rBV	719570	1194761	26.86%	2.358%
10	9.240	1072	1080	1092	rBV	583809	975071	21.92%	1.924%
11	9.769	1162	1170	1183	rBV	903661	1531467	34.44%	3.022%
12	10.140	1224	1233	1245	rBV	1422908	2321794	52.21%	4.582%
13	10.287	1250	1258	1282	rBV	835021	1534426	34.50%	3.028%
14	11.746	1499	1506	1513	rBV2	12298	24436	0.55%	0.048%
15	13.463	1791	1798	1814	rBV	1445597	2031545	45.68%	4.009%
16	13.722	1835	1842	1855	rBV	1819949	2615117	58.80%	5.161%
17	14.034	1889	1895	1907	rBV	1975001	2888577	64.95%	5.701%
18	14.269	1928	1935	1957	rBV	381905	761239	17.12%	1.502%
19	15.040	2060	2066	2081	rBV	2230109	3134747	70.49%	6.187%
20	15.169	2082	2088	2103	rVV	500632	720712	16.21%	1.422%
21	15.281	2103	2107	2112	rVB4	9852	14496	0.33%	0.029%
22	16.392	2289	2296	2300	rVV10	2476	5671	0.13%	0.011%
23	16.581	2325	2328	2332	rBV3	4104	5372	0.12%	0.011%
24	16.792	2358	2364	2374	rBV	2336341	3169973	71.28%	6.256%
25	16.892	2374	2381	2394	rVV	2295126	3238643	72.82%	6.392%
26	18.763	2695	2699	2703	rBV	27438	35747	0.80%	0.071%
27	18.839	2708	2712	2716	rVB	23478	32834	0.74%	0.065%
28	19.204	2767	2774	2786	rBV	2841580	3800944	85.46%	7.501%
29	21.027	3079	3084	3096	rBV	2573336	3599591	80.94%	7.104%
30	23.557	3505	3514	3527	rBV2	1981956	4447385	100.00%	8.777%
31	23.739	3536	3545	3563	rVB	1904970	4421297	99.41%	8.726%

Sum of corrected areas: 50670630




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100224\
Data File : BN034360.D
Acq On : 03 Oct 2024 08:00
Operator : RC/JU
Sample : PB163489BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK489

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

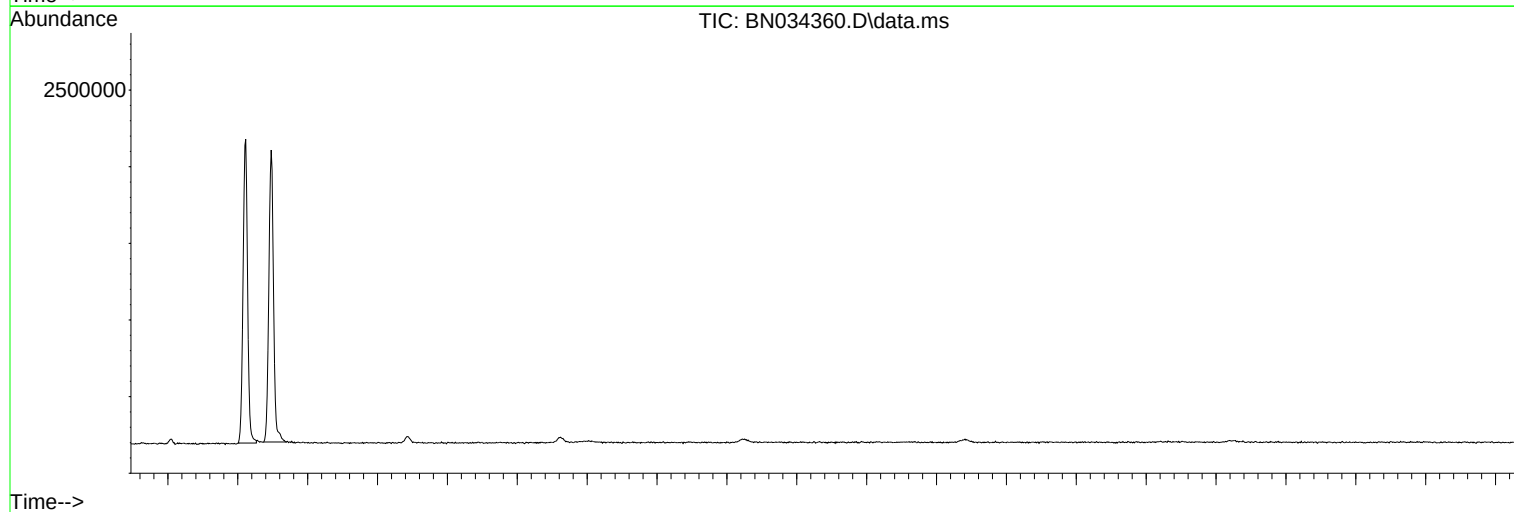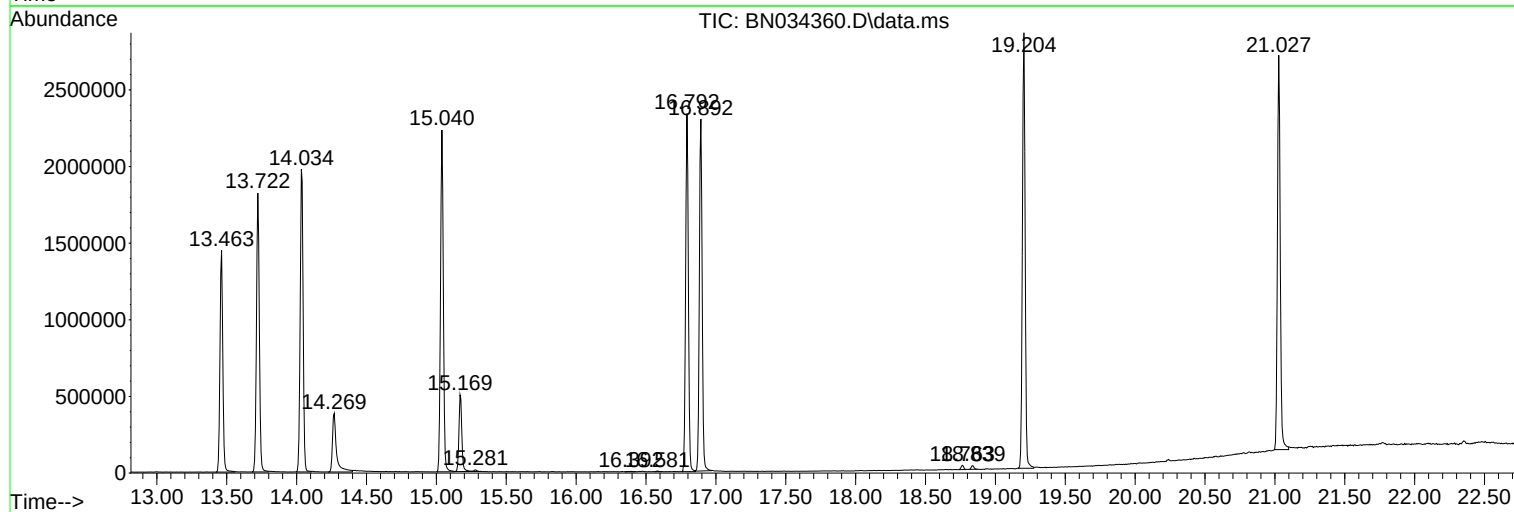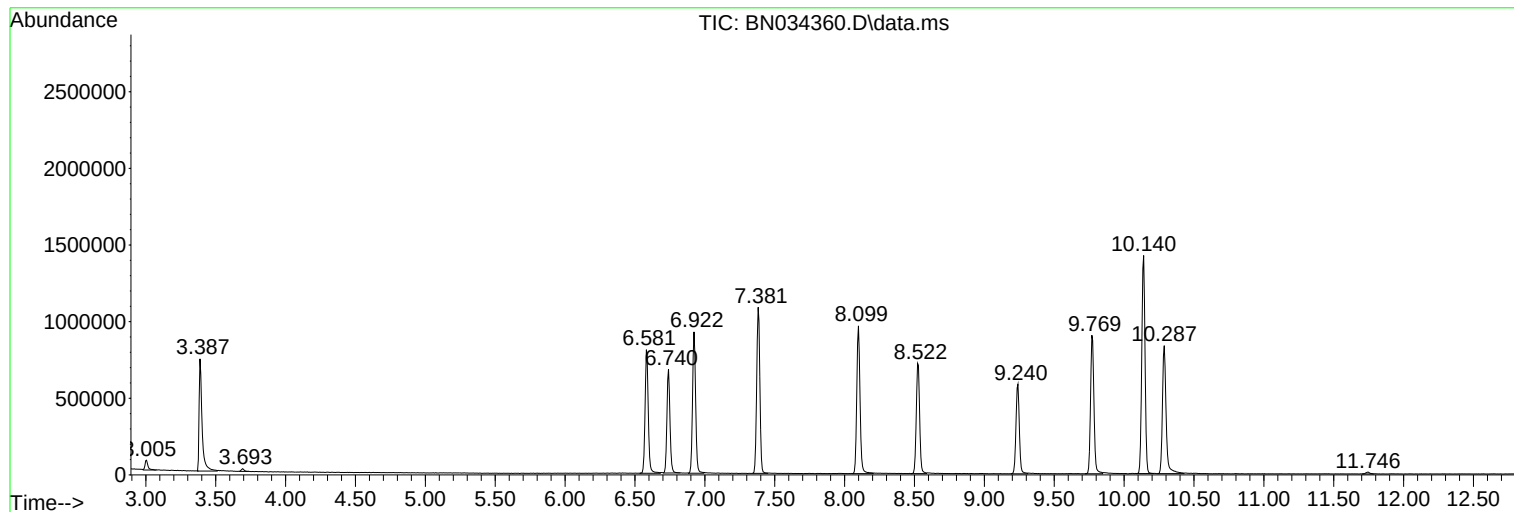

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100224\
Data File : BN034360.D
Acq On : 03 Oct 2024 08:00
Operator : RC/JU
Sample : PB163489BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK489

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100224\
Data File : BN034360.D
Acq On : 03 Oct 2024 08:00
Operator : RC/JU
Sample : PB163489BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK489

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc