

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100224\
 Data File : BN034364.D
 Acq On : 03 Oct 2024 10:37
 Operator : RC/JU
 Sample : P4016-15DL 20X
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DDC20DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN034364.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.411	87	89	97	rBV	12790	22999	0.41%	0.099%
2	3.693	133	137	141	rVB	9903	12532	0.23%	0.054%
3	5.446	431	435	443	rVB	21490	32218	0.58%	0.139%
4	5.975	521	525	530	rBV2	10558	13825	0.25%	0.060%
5	6.081	541	543	549	rVB5	7639	10622	0.19%	0.046%
6	6.405	594	598	602	rVB	13400	17765	0.32%	0.077%
7	6.458	602	607	610	rBV2	15950	21369	0.38%	0.092%
8	6.575	622	627	633	rBV4	17145	35700	0.64%	0.154%
9	6.740	649	655	659	rBV	19179	30828	0.56%	0.133%
10	6.922	681	686	693	rBV	21500	34696	0.62%	0.150%
11	7.022	698	703	710	rBV2	68743	103833	1.87%	0.449%
12	7.381	757	764	775	rBV	775350	1200171	21.62%	5.186%
13	7.646	806	809	819	rVV8	9401	27381	0.49%	0.118%
14	7.922	851	856	860	rVB2	15688	25209	0.45%	0.109%
15	7.975	862	865	869	rBV3	11679	15311	0.28%	0.066%
16	8.046	874	877	882	rVV2	16875	25554	0.46%	0.110%
17	8.105	882	887	891	rVV2	15826	29617	0.53%	0.128%
18	8.152	891	895	906	rVB3	16805	40112	0.72%	0.173%
19	8.334	920	926	930	rBV4	5817	13146	0.24%	0.057%
20	8.481	947	951	954	rVV5	9155	15845	0.29%	0.068%
21	8.528	954	959	964	rVV2	15181	31718	0.57%	0.137%
22	8.611	968	973	981	rVB	80507	118505	2.13%	0.512%
23	8.716	981	991	997	rVB	10433	33379	0.60%	0.144%
24	8.805	997	1006	1008	rBV10	6420	13676	0.25%	0.059%
25	9.058	1045	1049	1055	rVB5	4930	10699	0.19%	0.046%
26	9.240	1074	1080	1086	rBV5	12740	29247	0.53%	0.126%
27	9.305	1090	1091	1099	rVV6	6715	11712	0.21%	0.051%
28	9.452	1107	1116	1120	rBV4	9476	22997	0.41%	0.099%
29	9.516	1123	1127	1132	rBV7	8190	14430	0.26%	0.062%
30	9.599	1138	1141	1144	rBV2	9186	12098	0.22%	0.052%
31	9.699	1153	1158	1162	rBV5	7703	12260	0.22%	0.053%
32	9.781	1167	1172	1180	rVB3	14959	28640	0.52%	0.124%
33	10.140	1223	1233	1246	rBV	1033728	1774744	31.97%	7.669%
34	10.281	1251	1257	1263	rBV6	24440	54567	0.98%	0.236%
35	10.534	1295	1300	1308	rBV	30091	50194	0.90%	0.217%
36	10.840	1347	1352	1357	rVB5	9235	16431	0.30%	0.071%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100224\
 Data File : BN034364.D
 Acq On : 03 Oct 2024 10:37
 Operator : RC/JU
 Sample : P4016-15DL 20X
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DDC20DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
 Title : SVOA CALIBRATION

37	11.028	1375	1384	1390	rBV5	7188	24303	0.44%	0.105%
38	11.187	1406	1411	1418	rBV3	13186	33229	0.60%	0.144%
39	11.252	1418	1422	1428	rVB	36582	58250	1.05%	0.252%
40	11.428	1447	1452	1457	rBV4	13829	22867	0.41%	0.099%

41	11.599	1472	1481	1484	rBV	33689	62786	1.13%	0.271%
42	11.634	1484	1487	1491	rVV2	17575	24228	0.44%	0.105%
43	11.681	1491	1495	1501	rVB	11433	17130	0.31%	0.074%
44	11.822	1514	1519	1523	rVB5	5879	10390	0.19%	0.045%
45	12.040	1548	1556	1561	rBV5	8129	20376	0.37%	0.088%

46	12.257	1588	1593	1597	rBV4	11489	21105	0.38%	0.091%
47	12.434	1619	1623	1627	rVB6	7554	10610	0.19%	0.046%
48	12.581	1643	1648	1651	rBV2	13023	18193	0.33%	0.079%
49	12.875	1693	1698	1705	rBV	41802	65042	1.17%	0.281%
50	13.193	1745	1752	1758	rBV6	12367	30781	0.55%	0.133%

51	13.352	1775	1779	1783	rBV2	15683	23382	0.42%	0.101%
52	13.410	1783	1789	1793	rVV9	14933	28341	0.51%	0.122%
53	13.463	1793	1798	1804	rBV	43631	67442	1.21%	0.291%
54	13.546	1809	1812	1816	rVV2	15283	21555	0.39%	0.093%
55	13.593	1816	1820	1822	rVV4	9809	10959	0.20%	0.047%

56	13.722	1833	1842	1848	rVV	57193	101865	1.83%	0.440%
57	13.969	1880	1884	1889	rVV	230602	289711	5.22%	1.252%
58	14.034	1889	1895	1908	rVV	1460177	2168112	39.05%	9.369%
59	14.146	1908	1914	1917	rVB5	18389	26482	0.48%	0.114%
60	14.193	1917	1922	1928	rVB	61889	85621	1.54%	0.370%

61	14.275	1928	1936	1940	rBV7	13457	31777	0.57%	0.137%
62	14.528	1973	1979	1983	rVB4	10787	16978	0.31%	0.073%
63	14.593	1987	1990	1994	rBV4	17911	25493	0.46%	0.110%
64	14.640	1994	1998	2000	rBV3	31268	49207	0.89%	0.213%
65	14.675	2000	2004	2009	rVB3	80888	119406	2.15%	0.516%

66	14.816	2023	2028	2035	rBV	33461	52038	0.94%	0.225%
67	14.934	2040	2048	2052	rBV2	54682	88500	1.59%	0.382%
68	15.040	2061	2066	2071	rBV	72404	104088	1.87%	0.450%
69	15.157	2081	2086	2090	rBV	24178	41157	0.74%	0.178%
70	15.204	2090	2094	2100	rVB2	20607	36545	0.66%	0.158%

71	15.346	2110	2118	2122	rBV3	18153	39291	0.71%	0.170%
72	15.422	2128	2131	2138	rVB6	17745	28896	0.52%	0.125%
73	15.493	2138	2143	2148	rBV5	7395	14402	0.26%	0.062%
74	15.557	2148	2154	2159	rVB9	8065	16483	0.30%	0.071%
75	15.693	2172	2177	2180	rBV6	6550	11451	0.21%	0.049%

76	15.798	2190	2195	2198	rBV	54244	78918	1.42%	0.341%
----	--------	------	------	------	-----	-------	-------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100224\
 Data File : BN034364.D
 Acq On : 03 Oct 2024 10:37
 Operator : RC/JU
 Sample : P4016-15DL 20X
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DDC20DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
 Title : SVOA CALIBRATION

77	15.981	2220	2226	2232	rBV	8672	22797	0.41%	0.099%
78	16.151	2253	2255	2261	rVB7	8523	13220	0.24%	0.057%
79	16.451	2299	2306	2319	rBV	4090315	5551899	100.00%	23.992%
80	16.593	2326	2330	2335	rBV4	41453	63546	1.14%	0.275%
81	16.645	2337	2339	2346	rVB3	21621	29282	0.53%	0.127%
82	16.793	2358	2364	2376	rBV	1808043	2579006	46.45%	11.145%
83	16.893	2376	2381	2389	rVV	86126	149180	2.69%	0.645%
84	16.957	2389	2392	2398	rVB5	18904	26294	0.47%	0.114%
85	17.134	2419	2422	2425	rVB5	7833	10333	0.19%	0.045%
86	17.334	2451	2456	2459	rVV	37141	47182	0.85%	0.204%
87	17.381	2460	2464	2469	rVV	29157	44288	0.80%	0.191%
88	17.422	2469	2471	2475	rVB5	9041	11715	0.21%	0.051%
89	17.734	2518	2524	2526	rBV5	9280	19125	0.34%	0.083%
90	17.775	2529	2531	2537	rVB7	6449	10545	0.19%	0.046%
91	18.028	2569	2574	2578	rVB	26475	34739	0.63%	0.150%
92	18.404	2633	2638	2641	rBV7	7319	11556	0.21%	0.050%
93	18.610	2669	2673	2675	rBV5	8065	10989	0.20%	0.047%
94	18.669	2680	2683	2689	rVB	24462	30464	0.55%	0.132%
95	19.204	2767	2774	2780	rBV2	97249	147445	2.66%	0.637%
96	19.263	2780	2784	2786	rBV2	15882	17708	0.32%	0.077%
97	19.798	2872	2875	2882	rVB5	20581	26475	0.48%	0.114%
98	20.304	2959	2961	2964	rVB2	20476	19103	0.34%	0.083%
99	21.028	3079	3084	3095	rBV	2163326	2957636	53.27%	12.781%
100	23.739	3537	3545	3553	rBV	1476646	3344879	60.25%	14.454%



Sum of corrected areas: 23140826

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100224\
Data File : BN034364.D
Acq On : 03 Oct 2024 10:37
Operator : RC/JU
Sample : P4016-15DL 20X
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DDC20DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

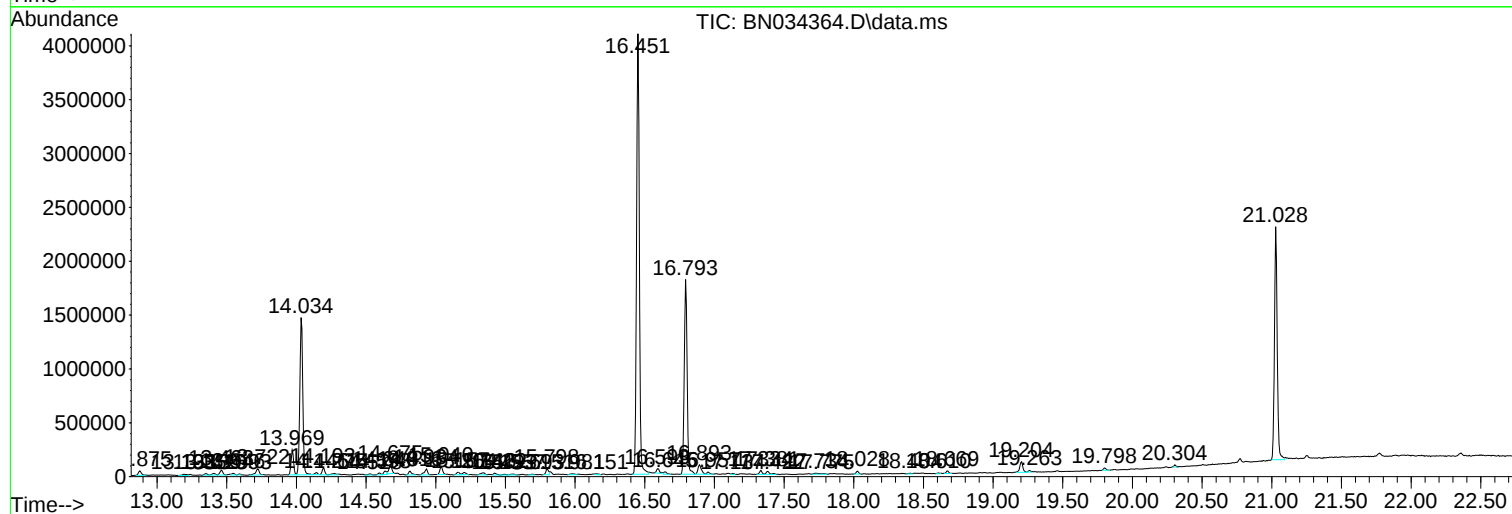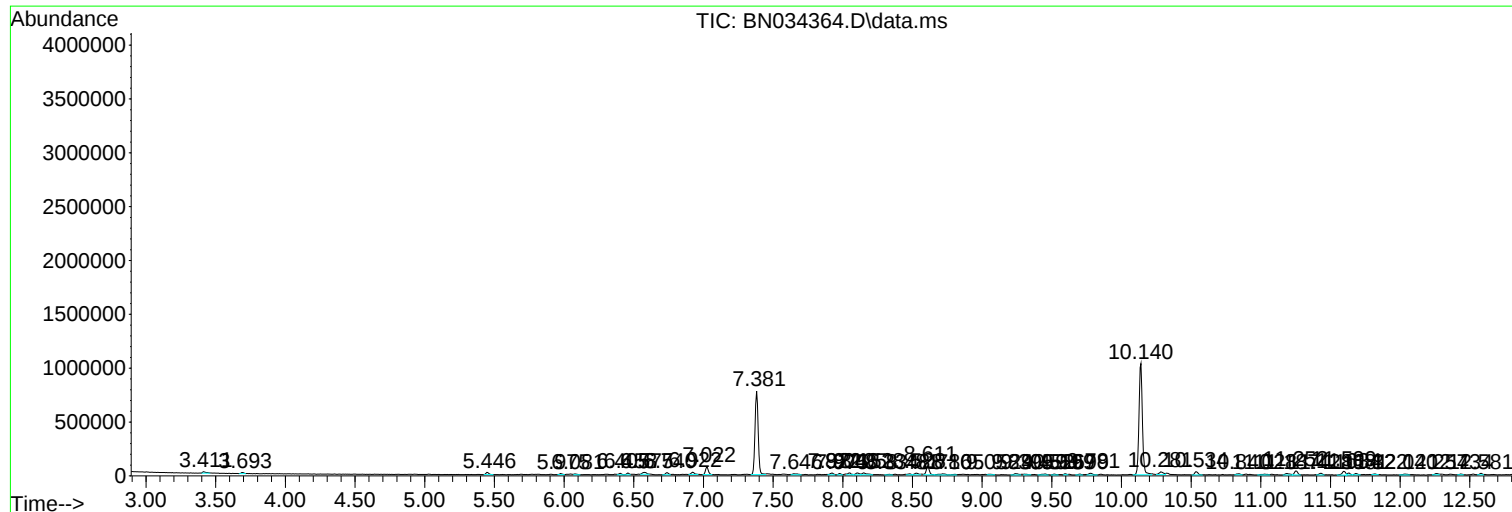

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100224\
Data File : BN034364.D
Acq On : 03 Oct 2024 10:37
Operator : RC/JU
Sample : P4016-15DL 20X
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DDC20DL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
13.969	2.67 ng/ul	289711	Acenaphthene-d10	14.034

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Heptane, 3-ethyl-5-methyl-	142	C10H22	052896-90-9	80
2			2-Ethylhexyl mercaptoacetate	204	C10H20O2S	007659-86-1	72
3			Octane, 3,6-dimethyl-	142	C10H22	015869-94-0	72
4			Decane, 5,6-dipropyl-	226	C16H34	119209-20-0	72
5			Oxalic acid, 2-ethylhexyl nonyl ...	328	C19H36O4	1000309-39-2	72

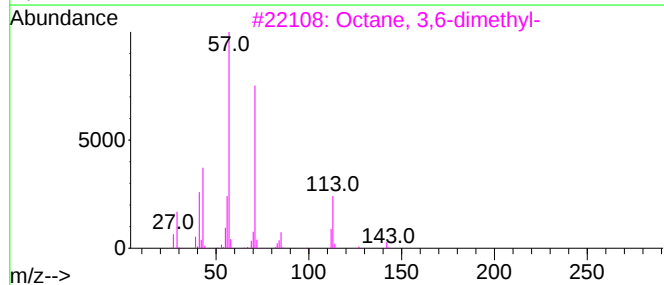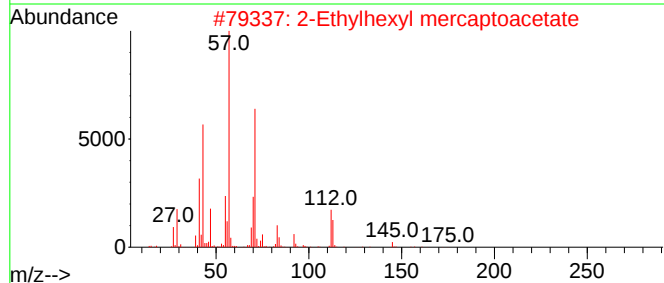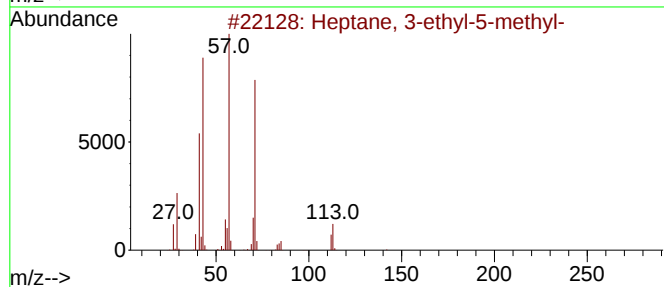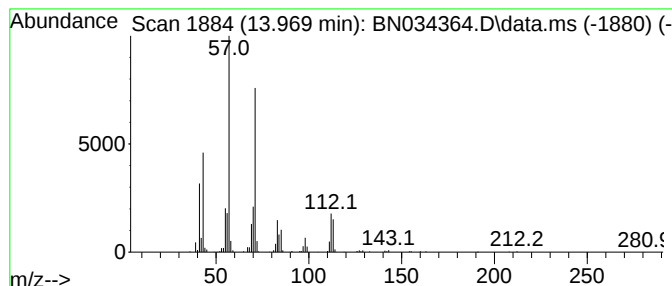

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100224\
Data File : BN034364.D
Acq On : 03 Oct 2024 10:37
Operator : RC/JU
Sample : P4016-15DL 20X
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DDC20DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	13.969	2.7	ng/u1	289711	3	14.034	2168110	20.0