

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100224\
 Data File : BN034374.D
 Acq On : 03 Oct 2024 17:13
 Operator : RC/JU
 Sample : PB163635BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK635

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN034374.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.005	16	20	29	rVB	51169	73485	2.33%	0.216%
2	3.387	82	85	105	rBV	525168	822634	26.11%	2.419%
3	3.693	134	137	144	rVB	11650	16317	0.52%	0.048%
4	6.040	532	536	542	rBV8	1591	3231	0.10%	0.010%
5	6.581	622	628	639	rBV	611360	970792	30.82%	2.855%
6	6.740	648	655	663	rBV	514254	798654	25.35%	2.348%
7	6.922	679	686	702	rBV	712756	1093195	34.70%	3.214%
8	7.381	757	764	773	rBV	648614	1009717	32.05%	2.969%
9	8.098	879	886	900	rBV	708131	1190936	37.80%	3.502%
10	8.522	951	958	973	rBV	571410	926940	29.42%	2.726%
11	9.234	1073	1079	1090	rBV	431433	725848	23.04%	2.134%
12	9.769	1162	1170	1184	rBV	702291	1186671	37.67%	3.489%
13	10.134	1225	1232	1245	rVB	799606	1334032	42.35%	3.923%
14	10.286	1250	1258	1276	rBV	625714	1143614	36.30%	3.363%
15	11.745	1499	1506	1512	rBV3	8331	15702	0.50%	0.046%
16	13.463	1791	1798	1807	rBV	1013433	1473551	46.78%	4.333%
17	13.722	1835	1842	1863	rBV	1302365	1939379	61.56%	5.703%
18	14.033	1889	1895	1904	rBV	1059122	1590168	50.48%	4.676%
19	14.269	1928	1935	1947	rBV	233264	464016	14.73%	1.364%
20	15.039	2058	2066	2081	rBV	1609389	2320440	73.66%	6.823%
21	15.169	2083	2088	2100	rVV	316036	462523	14.68%	1.360%
22	15.280	2104	2107	2111	rVB3	6913	11292	0.36%	0.033%
23	16.586	2324	2329	2334	rVB5	2846	5450	0.17%	0.016%
24	16.792	2358	2364	2371	rBV	1301149	1737495	55.15%	5.109%
25	16.892	2375	2381	2401	rVB	1660864	2360235	74.92%	6.940%
26	18.762	2695	2699	2705	rBV3	18734	29647	0.94%	0.087%
27	18.839	2708	2712	2716	rVB2	16074	23427	0.74%	0.069%
28	19.204	2768	2774	2784	rBV	2127577	2762348	87.69%	8.122%
29	21.027	3079	3084	3097	rBV	1405548	2020897	64.15%	5.942%
30	23.556	3506	3514	3525	rBV	1440030	3150292	100.00%	9.263%
31	23.739	3537	3545	3553	rBV2	1038346	2346086	74.47%	6.898%




Sum of corrected areas: 34009014

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100224\
Data File : BN034374.D
Acq On : 03 Oct 2024 17:13
Operator : RC/JU
Sample : PB163635BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK635

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

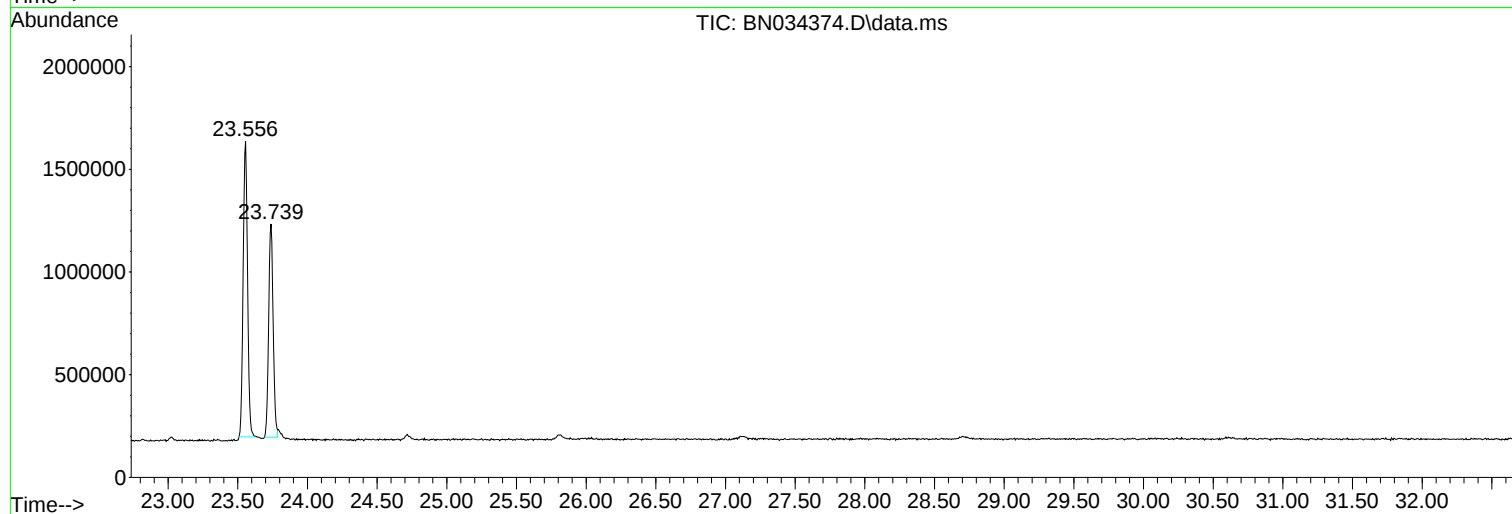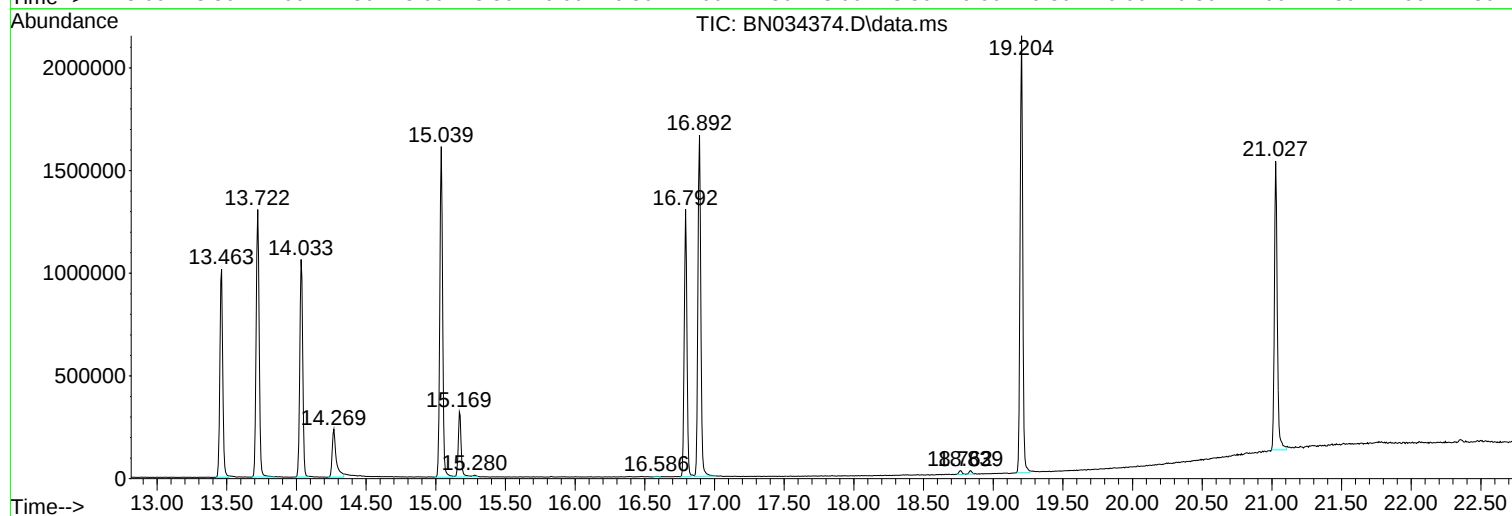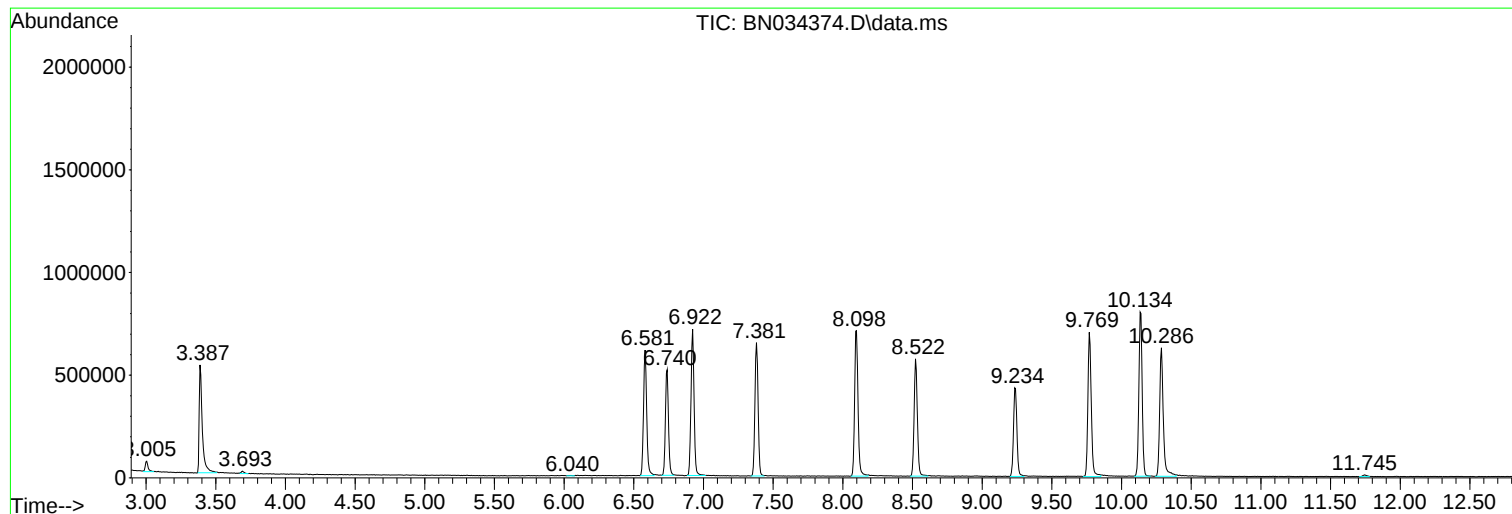

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100224\
Data File : BN034374.D
Acq On : 03 Oct 2024 17:13
Operator : RC/JU
Sample : PB163635BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK635

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100224\
Data File : BN034374.D
Acq On : 03 Oct 2024 17:13
Operator : RC/JU
Sample : PB163635BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK635

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091124.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc