

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN100224\  
 Data File : BN034380.D  
 Acq On : 03 Oct 2024 21:09  
 Operator : RC/JU  
 Sample : P4017-12DL 10X  
 Misc :  
 ALS Vial : 9 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 DDC94DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\SFAM-EPA-BN091124.MA.M  
 Title : SVOA CALIBRATION

Signal : TIC: BN034380.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 3.405       | 84            | 88          | 99           | rBV      | 51295          | 93973         | 1.96%           | 0.324%        |
| 2         | 3.693       | 134           | 137         | 147          | rVB      | 13328          | 21115         | 0.44%           | 0.073%        |
| 3         | 4.010       | 186           | 191         | 202          | rVB      | 44595          | 67251         | 1.40%           | 0.232%        |
| 4         | 5.975       | 520           | 525         | 529          | rBV5     | 9797           | 15250         | 0.32%           | 0.053%        |
| 5         | 6.404       | 594           | 598         | 603          | rVV2     | 13035          | 18647         | 0.39%           | 0.064%        |
| 6         | 6.457       | 603           | 607         | 611          | rVV2     | 15496          | 20042         | 0.42%           | 0.069%        |
| 7         | 6.581       | 621           | 628         | 641          | rVB2     | 80790          | 158800        | 3.31%           | 0.547%        |
| 8         | 6.740       | 647           | 655         | 665          | rVB      | 72367          | 121511        | 2.54%           | 0.419%        |
| 9         | 6.922       | 680           | 686         | 698          | rVB      | 89142          | 162135        | 3.38%           | 0.559%        |
| 10        | 7.022       | 698           | 703         | 709          | rBV      | 56632          | 84162         | 1.76%           | 0.290%        |
| 11        | 7.316       | 750           | 753         | 757          | rVV3     | 11850          | 18753         | 0.39%           | 0.065%        |
| 12        | 7.381       | 757           | 764         | 773          | rVV      | 952380         | 1485111       | 30.99%          | 5.117%        |
| 13        | 7.463       | 773           | 778         | 783          | rVB4     | 12315          | 27365         | 0.57%           | 0.094%        |
| 14        | 7.581       | 793           | 798         | 805          | rVB3     | 13575          | 25608         | 0.53%           | 0.088%        |
| 15        | 7.651       | 805           | 810         | 819          | rVB7     | 14739          | 36566         | 0.76%           | 0.126%        |
| 16        | 7.822       | 835           | 839         | 842          | rBV4     | 10505          | 16335         | 0.34%           | 0.056%        |
| 17        | 7.916       | 846           | 855         | 861          | rVB3     | 27041          | 51942         | 1.08%           | 0.179%        |
| 18        | 7.975       | 861           | 865         | 870          | rBV      | 20666          | 30050         | 0.63%           | 0.104%        |
| 19        | 8.045       | 873           | 877         | 881          | rVV2     | 29700          | 41923         | 0.87%           | 0.144%        |
| 20        | 8.098       | 881           | 886         | 891          | rVV2     | 73403          | 129236        | 2.70%           | 0.445%        |
| 21        | 8.151       | 891           | 895         | 904          | rVB2     | 32026          | 58006         | 1.21%           | 0.200%        |
| 22        | 8.522       | 953           | 958         | 964          | rVV      | 62690          | 111974        | 2.34%           | 0.386%        |
| 23        | 8.610       | 968           | 973         | 981          | rVB      | 89597          | 137673        | 2.87%           | 0.474%        |
| 24        | 8.722       | 989           | 992         | 998          | rVB7     | 13344          | 22852         | 0.48%           | 0.079%        |
| 25        | 8.951       | 1024          | 1031        | 1037         | rBV10    | 6982           | 13760         | 0.29%           | 0.047%        |
| 26        | 9.239       | 1074          | 1080        | 1086         | rBV      | 50609          | 93279         | 1.95%           | 0.321%        |
| 27        | 9.451       | 1109          | 1116        | 1121         | rVV5     | 9069           | 19818         | 0.41%           | 0.068%        |
| 28        | 9.516       | 1123          | 1127        | 1131         | rBV6     | 9116           | 13754         | 0.29%           | 0.047%        |
| 29        | 9.598       | 1136          | 1141        | 1150         | rVB4     | 13518          | 25400         | 0.53%           | 0.088%        |
| 30        | 9.775       | 1164          | 1171        | 1179         | rVV      | 76919          | 143389        | 2.99%           | 0.494%        |
| 31        | 10.134      | 1224          | 1232        | 1251         | rBV      | 1300348        | 2301201       | 48.03%          | 7.929%        |
| 32        | 10.281      | 1251          | 1257        | 1279         | rVV3     | 163248         | 358329        | 7.48%           | 1.235%        |
| 33        | 10.451      | 1279          | 1286        | 1291         | rVB4     | 12348          | 22692         | 0.47%           | 0.078%        |
| 34        | 10.545      | 1296          | 1302        | 1311         | rVB6     | 12031          | 30800         | 0.64%           | 0.106%        |
| 35        | 10.669      | 1314          | 1323        | 1336         | rBV      | 68679          | 124032        | 2.59%           | 0.427%        |
| 36        | 11.039      | 1381          | 1386        | 1390         | rVV2     | 20086          | 34203         | 0.71%           | 0.118%        |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN100224\  
 Data File : BN034380.D  
 Acq On : 03 Oct 2024 21:09  
 Operator : RC/JU  
 Sample : P4017-12DL 10X  
 Misc :  
 ALS Vial : 9 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 DDC94DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\SFAM-EPA-BN091124.MA.M  
 Title : SVOA CALIBRATION

|    |        |      |      |      |       |         |         |        |        |
|----|--------|------|------|------|-------|---------|---------|--------|--------|
| 37 | 11.081 | 1390 | 1393 | 1399 | rVB4  | 9120    | 13458   | 0.28%  | 0.046% |
| 38 | 11.181 | 1406 | 1410 | 1417 | rBV4  | 8324    | 15421   | 0.32%  | 0.053% |
| 39 | 11.286 | 1423 | 1428 | 1435 | rVB5  | 9693    | 17491   | 0.37%  | 0.060% |
| 40 | 11.392 | 1438 | 1446 | 1449 | rBV5  | 11650   | 21445   | 0.45%  | 0.074% |
| 41 | 11.428 | 1449 | 1452 | 1457 | rVB5  | 14054   | 19760   | 0.41%  | 0.068% |
| 42 | 11.510 | 1462 | 1466 | 1472 | rVB3  | 9925    | 17000   | 0.35%  | 0.059% |
| 43 | 11.575 | 1472 | 1477 | 1479 | rBV2  | 23811   | 39970   | 0.83%  | 0.138% |
| 44 | 11.686 | 1492 | 1496 | 1502 | rBV4  | 10367   | 18136   | 0.38%  | 0.062% |
| 45 | 12.016 | 1547 | 1552 | 1562 | rBV   | 59680   | 106742  | 2.23%  | 0.368% |
| 46 | 12.263 | 1590 | 1594 | 1605 | rVV2  | 20825   | 39636   | 0.83%  | 0.137% |
| 47 | 12.363 | 1605 | 1611 | 1615 | rVV5  | 16593   | 30155   | 0.63%  | 0.104% |
| 48 | 12.410 | 1615 | 1619 | 1627 | rVV5  | 8722    | 20109   | 0.42%  | 0.069% |
| 49 | 12.592 | 1644 | 1650 | 1656 | rVB6  | 15213   | 29810   | 0.62%  | 0.103% |
| 50 | 12.763 | 1672 | 1679 | 1685 | rBV9  | 9123    | 20830   | 0.43%  | 0.072% |
| 51 | 12.875 | 1688 | 1698 | 1703 | rVV3  | 33844   | 66496   | 1.39%  | 0.229% |
| 52 | 12.922 | 1703 | 1706 | 1709 | rVV3  | 10513   | 15992   | 0.33%  | 0.055% |
| 53 | 13.086 | 1727 | 1734 | 1740 | rBV3  | 33243   | 62425   | 1.30%  | 0.215% |
| 54 | 13.198 | 1745 | 1753 | 1755 | rBV8  | 9042    | 21732   | 0.45%  | 0.075% |
| 55 | 13.228 | 1755 | 1758 | 1762 | rVV2  | 10638   | 17433   | 0.36%  | 0.060% |
| 56 | 13.351 | 1773 | 1779 | 1783 | rBV5  | 14144   | 29858   | 0.62%  | 0.103% |
| 57 | 13.404 | 1783 | 1788 | 1792 | rVV8  | 11188   | 22012   | 0.46%  | 0.076% |
| 58 | 13.463 | 1792 | 1798 | 1806 | rVV   | 174401  | 260663  | 5.44%  | 0.898% |
| 59 | 13.592 | 1815 | 1820 | 1828 | rVB4  | 27836   | 50147   | 1.05%  | 0.173% |
| 60 | 13.722 | 1834 | 1842 | 1850 | rVV   | 209653  | 353400  | 7.38%  | 1.218% |
| 61 | 13.786 | 1850 | 1853 | 1858 | rVB   | 20082   | 25019   | 0.52%  | 0.086% |
| 62 | 13.969 | 1878 | 1884 | 1888 | rBV   | 79013   | 111679  | 2.33%  | 0.385% |
| 63 | 14.033 | 1888 | 1895 | 1907 | rVB   | 2042132 | 2829093 | 59.04% | 9.748% |
| 64 | 14.304 | 1930 | 1941 | 1945 | rVV6  | 28594   | 66140   | 1.38%  | 0.228% |
| 65 | 14.527 | 1974 | 1979 | 1982 | rBV4  | 10312   | 14120   | 0.29%  | 0.049% |
| 66 | 14.592 | 1987 | 1990 | 1995 | rBV6  | 25159   | 34762   | 0.73%  | 0.120% |
| 67 | 14.675 | 1995 | 2004 | 2017 | rVB2  | 131450  | 291766  | 6.09%  | 1.005% |
| 68 | 14.798 | 2021 | 2025 | 2030 | rBV7  | 22232   | 33992   | 0.71%  | 0.117% |
| 69 | 14.851 | 2030 | 2034 | 2039 | rVB8  | 11140   | 17784   | 0.37%  | 0.061% |
| 70 | 14.933 | 2043 | 2048 | 2054 | rVB   | 42541   | 55475   | 1.16%  | 0.191% |
| 71 | 15.004 | 2055 | 2060 | 2061 | rBV5  | 9772    | 14560   | 0.30%  | 0.050% |
| 72 | 15.039 | 2061 | 2066 | 2079 | rVB   | 300281  | 448139  | 9.35%  | 1.544% |
| 73 | 15.169 | 2079 | 2088 | 2092 | rVB6  | 44767   | 102696  | 2.14%  | 0.354% |
| 74 | 15.327 | 2110 | 2115 | 2121 | rBV7  | 27649   | 61863   | 1.29%  | 0.213% |
| 75 | 15.416 | 2126 | 2130 | 2139 | rVV   | 82266   | 136033  | 2.84%  | 0.469% |
| 76 | 15.486 | 2139 | 2142 | 2150 | rVV10 | 6785    | 16116   | 0.34%  | 0.056% |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN100224\  
 Data File : BN034380.D  
 Acq On : 03 Oct 2024 21:09  
 Operator : RC/JU  
 Sample : P4017-12DL 10X  
 Misc :  
 ALS Vial : 9 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 DDC94DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\SFAM-EPA-BN091124.MA.M  
 Title : SVOA CALIBRATION

|     |        |      |      |      |      |         |         |         |         |
|-----|--------|------|------|------|------|---------|---------|---------|---------|
| 77  | 15.557 | 2150 | 2154 | 2159 | rVB7 | 9309    | 16334   | 0.34%   | 0.056%  |
| 78  | 15.798 | 2189 | 2195 | 2198 | rBV2 | 48418   | 69277   | 1.45%   | 0.239%  |
| 79  | 16.163 | 2251 | 2257 | 2261 | rBV8 | 8563    | 14984   | 0.31%   | 0.052%  |
| 80  | 16.451 | 2299 | 2306 | 2319 | rBV  | 1972175 | 2810634 | 58.66%  | 9.684%  |
| 81  | 16.592 | 2325 | 2330 | 2335 | rVV3 | 41432   | 57852   | 1.21%   | 0.199%  |
| 82  | 16.651 | 2336 | 2340 | 2344 | rVB3 | 13419   | 21073   | 0.44%   | 0.073%  |
| 83  | 16.792 | 2358 | 2364 | 2376 | rBV  | 2434653 | 3397654 | 70.91%  | 11.707% |
| 84  | 16.892 | 2376 | 2381 | 2392 | rVB  | 324445  | 462889  | 9.66%   | 1.595%  |
| 85  | 17.333 | 2452 | 2456 | 2461 | rBV  | 38995   | 50835   | 1.06%   | 0.175%  |
| 86  | 17.374 | 2461 | 2463 | 2468 | rVV4 | 11529   | 15811   | 0.33%   | 0.054%  |
| 87  | 17.421 | 2468 | 2471 | 2479 | rVB3 | 28002   | 37009   | 0.77%   | 0.128%  |
| 88  | 17.727 | 2518 | 2523 | 2529 | rBV5 | 24462   | 47251   | 0.99%   | 0.163%  |
| 89  | 17.857 | 2542 | 2545 | 2550 | rVB2 | 11531   | 14729   | 0.31%   | 0.051%  |
| 90  | 18.027 | 2569 | 2574 | 2579 | rBV  | 28713   | 39810   | 0.83%   | 0.137%  |
| 91  | 18.492 | 2648 | 2653 | 2656 | rBV6 | 8329    | 16612   | 0.35%   | 0.057%  |
| 92  | 18.604 | 2669 | 2672 | 2676 | rBV3 | 10419   | 14110   | 0.29%   | 0.049%  |
| 93  | 18.674 | 2680 | 2684 | 2687 | rVB2 | 23730   | 29101   | 0.61%   | 0.100%  |
| 94  | 18.868 | 2712 | 2717 | 2720 | rVV  | 28201   | 38383   | 0.80%   | 0.132%  |
| 95  | 19.198 | 2767 | 2773 | 2781 | rBV  | 414028  | 610108  | 12.73%  | 2.102%  |
| 96  | 19.262 | 2781 | 2784 | 2787 | rVB2 | 22881   | 25063   | 0.52%   | 0.086%  |
| 97  | 19.804 | 2872 | 2876 | 2879 | rVB3 | 19222   | 24365   | 0.51%   | 0.084%  |
| 98  | 21.027 | 3078 | 3084 | 3094 | rBV  | 2908882 | 4141358 | 86.43%  | 14.270% |
| 99  | 23.545 | 3507 | 3512 | 3525 | rVB  | 257240  | 568981  | 11.87%  | 1.961%  |
| 100 | 23.733 | 3536 | 3544 | 3553 | rBV  | 2112381 | 4791570 | 100.00% | 16.510% |




Sum of corrected areas: 29022088

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN100224\  
Data File : BN034380.D  
Acq On : 03 Oct 2024 21:09  
Operator : RC/JU  
Sample : P4017-12DL 10X  
Misc :  
ALS Vial : 9 Sample Multiplier: 1

Instrument :  
BNA\_N  
ClientSampleId :  
DDC94DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\SFAM-EPA-BN091124.MA.M  
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

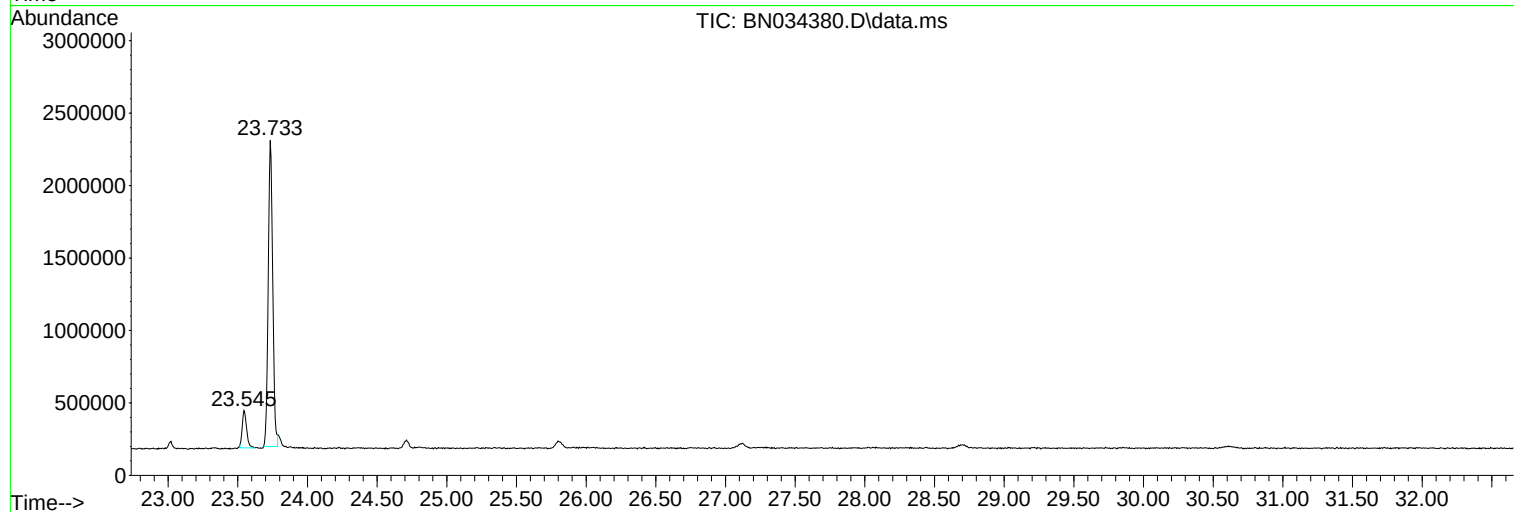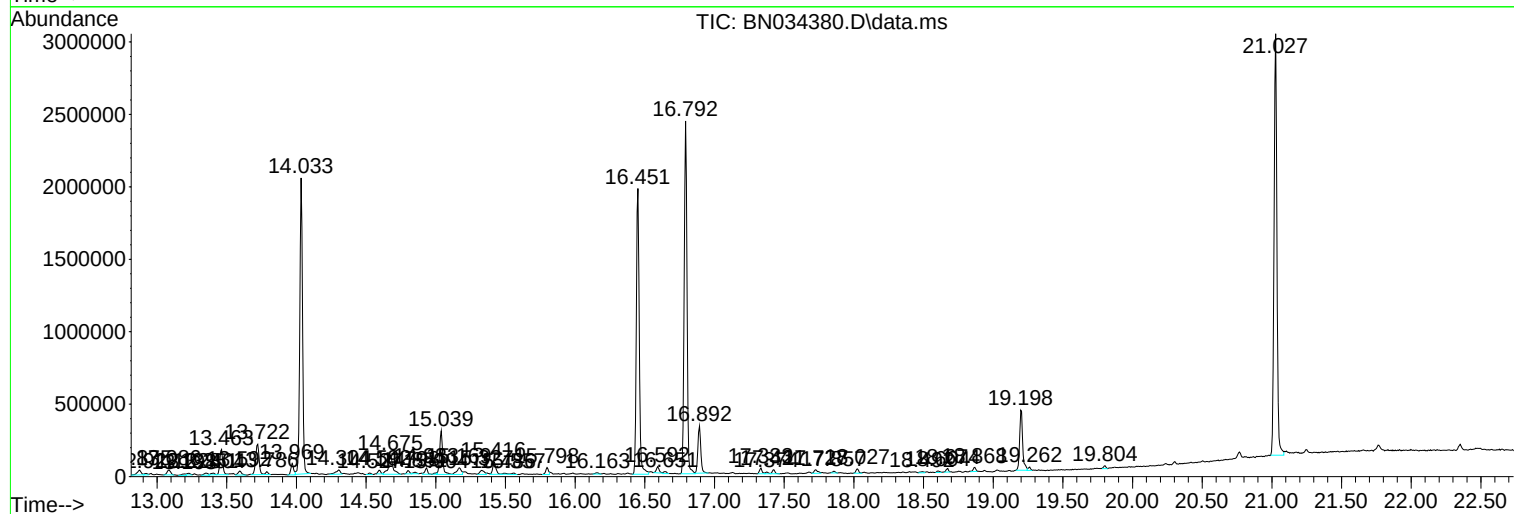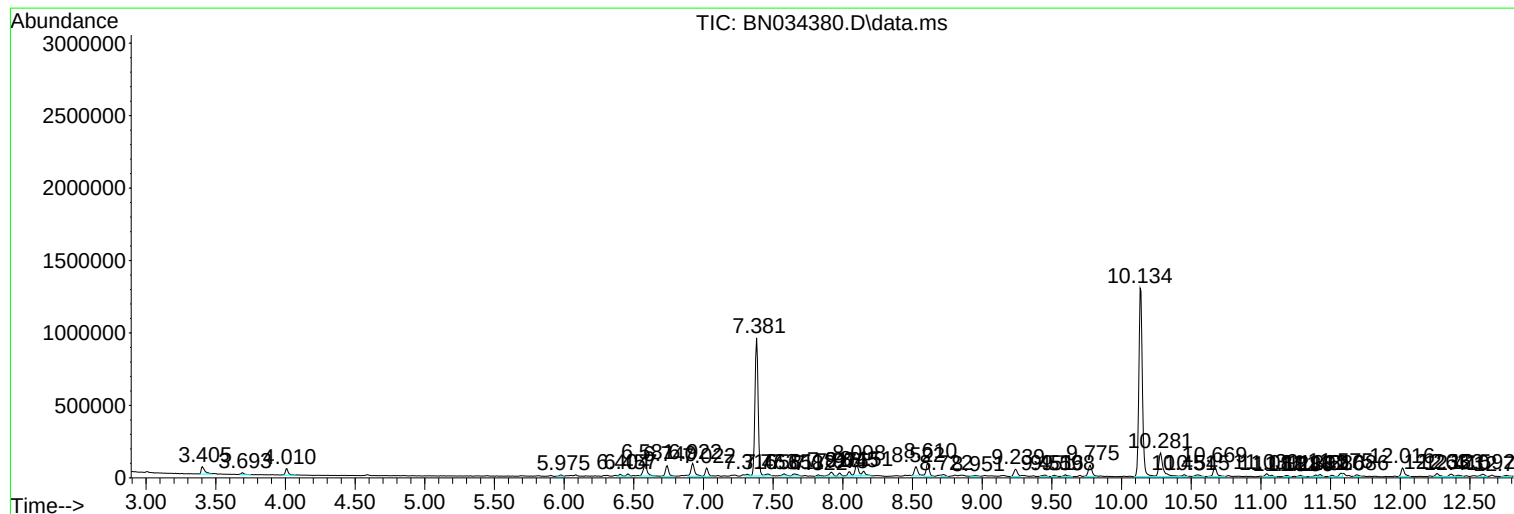

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN100224\  
Data File : BN034380.D  
Acq On : 03 Oct 2024 21:09  
Operator : RC/JU  
Sample : P4017-12DL 10X  
Misc :  
ALS Vial : 9 Sample Multiplier: 1

Instrument :  
BNA\_N  
ClientSampleId :  
DDC94DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\SFAM-EPA-BN091124.MA.M  
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN100224\  
Data File : BN034380.D  
Acq On : 03 Oct 2024 21:09  
Operator : RC/JU  
Sample : P4017-12DL 10X  
Misc :  
ALS Vial : 9 Sample Multiplier: 1

Instrument :  
BNA\_N  
ClientSampleId :  
DDC94DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\SFAM-EPA-BN091124.MA.M  
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|