

Data Path : Z:\SVOASRV\HPCHEM1\BNA\_N\DATA\BN100319\  
 Data File : BN008001.D  
 Acq On : 04 Oct 2019 03:34  
 Operator : JU  
 Sample : K5077-18  
 Misc :  
 ALS Vial : 18 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 PST-024-B268-092519

Quant Time: Oct 04 05:42:58 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_N\METHODS\8270-SIM-BN091819.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Thu Oct 03 18:39:49 2019

Response via : Initial Calibration

| Internal Standards        | R.T.  | QIon | Response | Conc | Units | Dev(Min) |
|---------------------------|-------|------|----------|------|-------|----------|
| 1) 1,4-Dichlorobenzene-d4 | 7.69  | 152  | 4689     | 0.40 | ng    | -0.02    |
| 7) Naphthalene-d8         | 10.46 | 136  | 19549    | 0.40 | ng    | -0.01    |
| 13) Acenaphthene-d10      | 14.31 | 164  | 12346    | 0.40 | ng    | -0.01    |
| 19) Phenanthrene-d10      | 17.06 | 188  | 26811    | 0.40 | ng    | -0.01    |
| 27) Chrysene-d12          | 21.25 | 240  | 28978    | 0.40 | ng    | -0.02    |
| 34) Perylene-d12          | 23.46 | 264  | 31452    | 0.40 | ng    | -0.03    |

#### System Monitoring Compounds

|                             |       |     |       |      |    |       |
|-----------------------------|-------|-----|-------|------|----|-------|
| 4) 2-Fluorophenol           | 5.31  | 112 | 4473  | 0.28 | ng | 0.00  |
| 5) Phenol-d6                | 6.87  | 99  | 6379  | 0.32 | ng | 0.00  |
| 8) Nitrobenzene-d5          | 8.82  | 82  | 4649  | 0.27 | ng | -0.01 |
| 11) 2-Methylnaphthalene-d10 | 12.05 | 152 | 10131 | 0.31 | ng | -0.02 |
| 14) 2,4,6-Tribromophenol    | 15.81 | 330 | 1957  | 0.29 | ng | -0.01 |
| 15) 2-Fluorobiphenyl        | 12.93 | 172 | 13808 | 0.27 | ng | -0.01 |
| 25) Fluoranthene-d10        | 19.09 | 212 | 28379 | 0.31 | ng | -0.01 |
| 29) Terphenyl-d14           | 19.69 | 244 | 22804 | 0.32 | ng | -0.02 |

#### Target Compounds


|                                |       |     |       |       |    | Qvalue |
|--------------------------------|-------|-----|-------|-------|----|--------|
| 3) n-Nitrosodimethylamine      | 2.98  | 42  | 4823  | 2.015 | ng | 85     |
| 16) Acenaphthylene             | 14.02 | 152 | 5443  | 0.083 | ng | 96     |
| 18) Fluorene                   | 15.36 | 166 | 1097  | 0.020 | ng | # 86   |
| 23) Phenanthrene               | 17.09 | 178 | 21879 | 0.262 | ng | 99     |
| 24) Anthracene                 | 17.19 | 178 | 4395  | 0.058 | ng | 99     |
| 26) Fluoranthene               | 19.12 | 202 | 63735 | 0.614 | ng | 99     |
| 28) Pyrene                     | 19.49 | 202 | 61484 | 0.622 | ng | 96     |
| 30) Benzo(a)anthracene         | 21.28 | 228 | 33923 | 0.318 | ng | 93     |
| 31) Chrysene                   | 21.28 | 228 | 33860 | 0.326 | ng | 96     |
| 32) Bis(2-ethylhexyl)phthalate | 21.17 | 149 | 6154  | 0.112 | ng | 95     |
| 33) Indeno(1,2,3-cd)pyrene     | 25.67 | 276 | 25556 | 0.196 | ng | 95     |
| 35) Benzo(b)fluoranthene       | 22.81 | 252 | 53644 | 0.491 | ng | # 64   |
| 36) Benzo(k)fluoranthene       | 22.81 | 252 | 53644 | 0.497 | ng | # 64   |
| 37) Benzo(a)pyrene             | 23.37 | 252 | 30858 | 0.301 | ng | # 83   |
| 38) Dibenzo(a,h)anthracene     | 25.68 | 278 | 5982  | 0.057 | ng | # 38   |
| 39) Benzo(g,h,i)perylene       | 26.35 | 276 | 25932 | 0.250 | ng | # 90   |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA\_N\DATA\BN100319\  
Data File : BN008001.D  
Acq On : 04 Oct 2019 03:34  
Operator : JU  
Sample : K5077-18  
Misc :  
ALS Vial : 18 Sample Multiplier: 1

Instrument :  
BNA\_N  
ClientSampleId :  
PST-024-B268-092519

Quant Time: Oct 04 05:42:58 2019  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_N\METHODS\8270-SIM-BN091819.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Oct 03 18:39:49 2019  
Response via : Initial Calibration

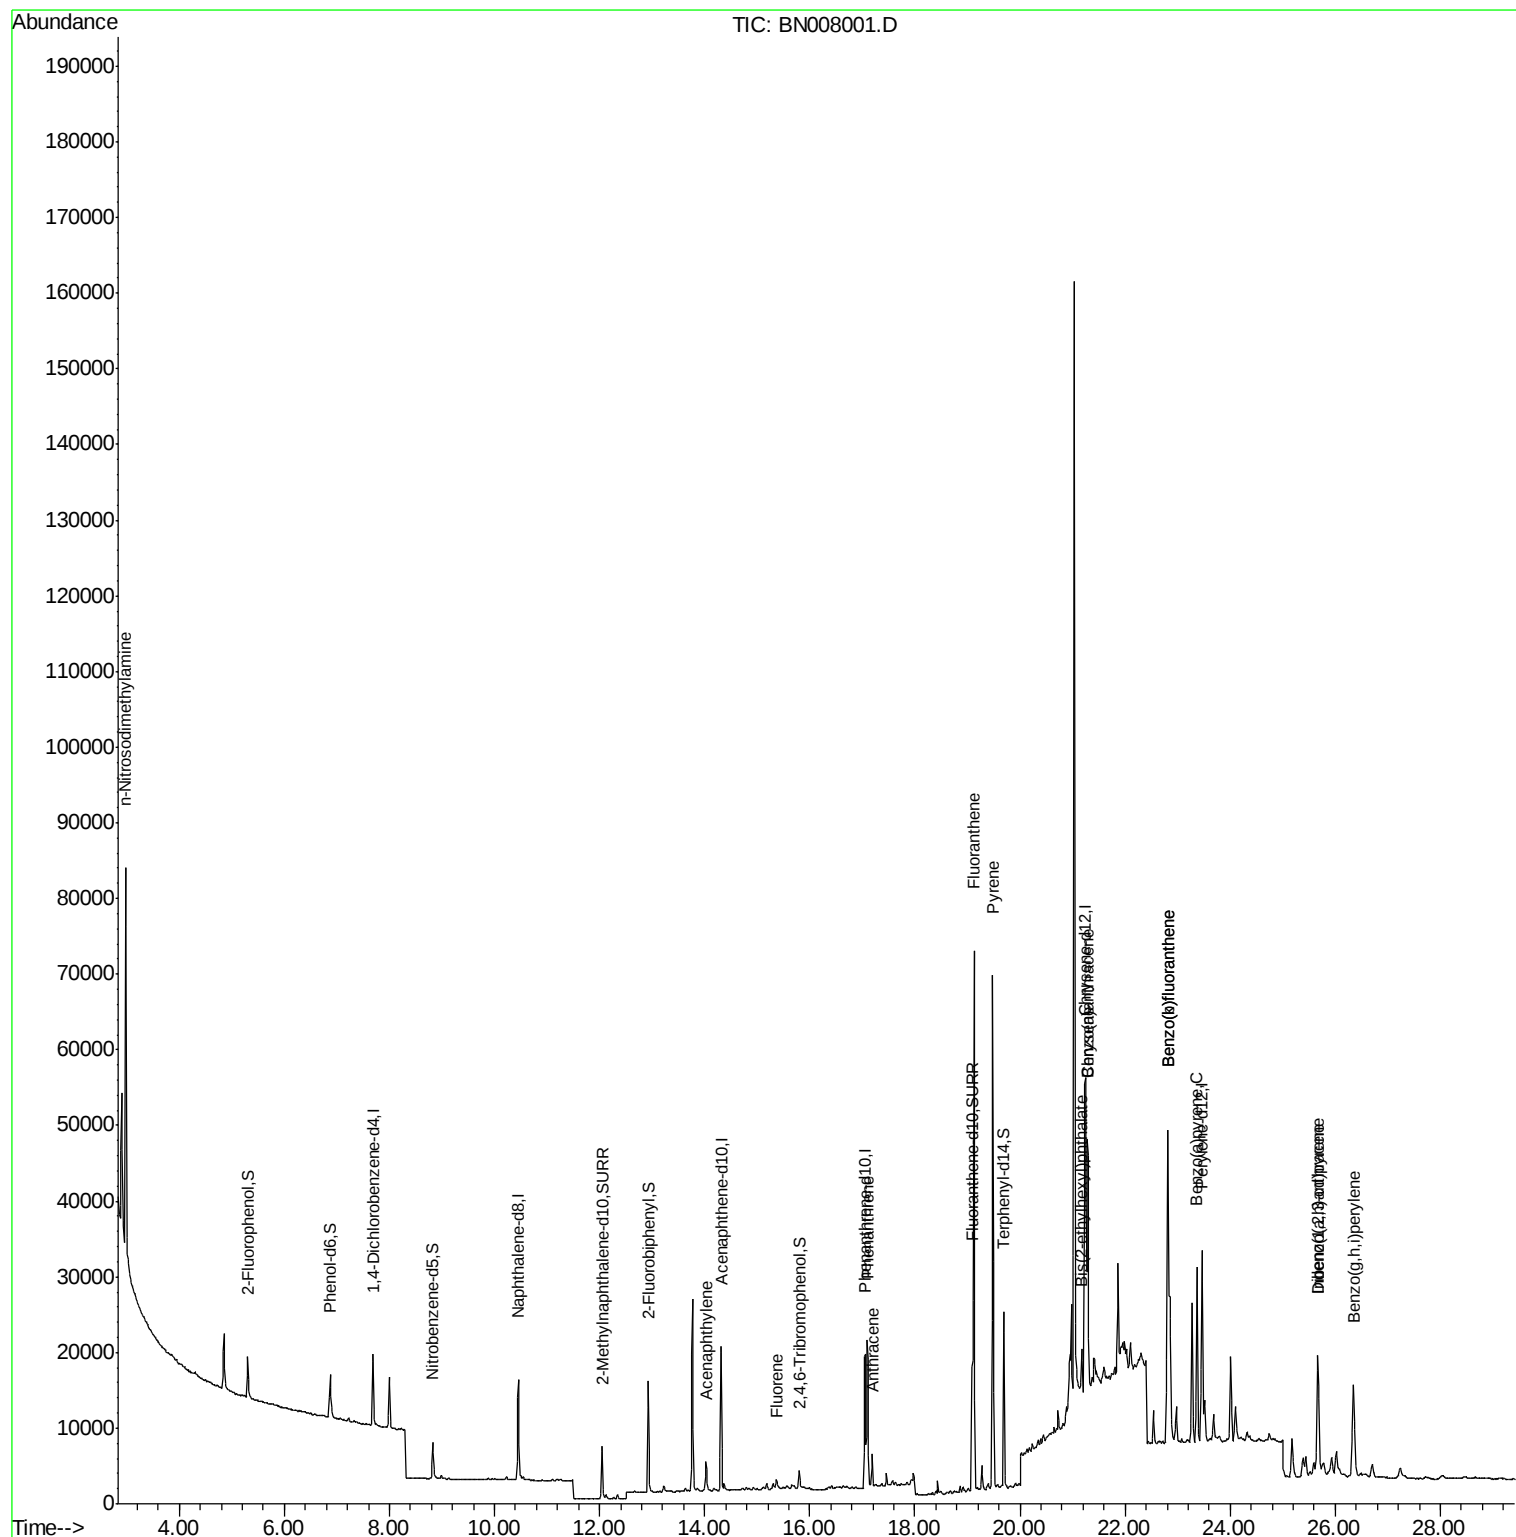




#1




1,4-Dichlorobenzene-d4  
Concen: 0.400 ng  
RT: 7.69 min Scan# 603  
Delta R.T. -0.02 min  
Lab File: BN008001.D  
Acq: 04 Oct 2019 03:34

Instrument :  
BNA\_N  
ClientSampleId :  
PST-024-B268-092519

Tgt Ion: 152 Resp: 4689  
Ion Ratio Lower Upper  
152 100  
150 149.9 125.6 188.4  
115 64.4 53.3 79.9

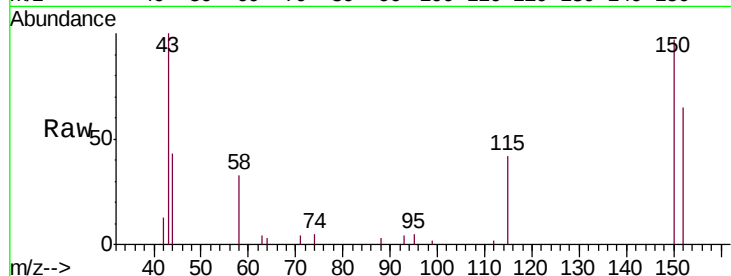


Abundance Ion 152.00 (151.70 to 152.70): E  
Ion 150.00 (149.70 to 150.70): E  
Ion 115.00 (114.70 to 115.70): E

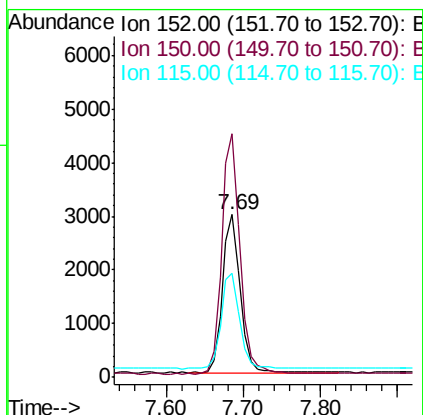



#3


n-Nitrosodimethylamine  
Concen: 2.015 ng  
RT: 2.98 min Scan# 19  
Delta R.T. -0.02 min  
Lab File: BN008001.D  
Acq: 04 Oct 2019 03:34

Tgt Ion: 42 Resp: 4823  
Ion Ratio Lower Upper  
42 100  
74 128.3 87.9 131.9  
44 31.8 29.4 44.0



Abundance Ion 42.00 (41.70 to 42.70): BNC  
Ion 74.00 (73.70 to 74.70): BNC  
Ion 44.00 (43.70 to 44.70): BNC

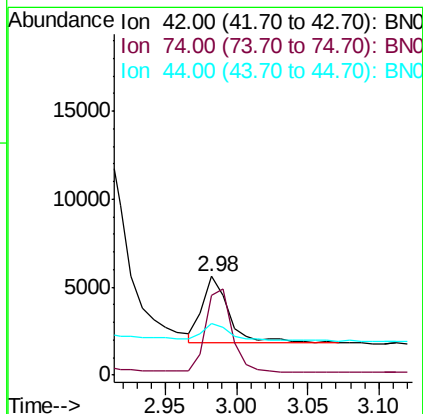

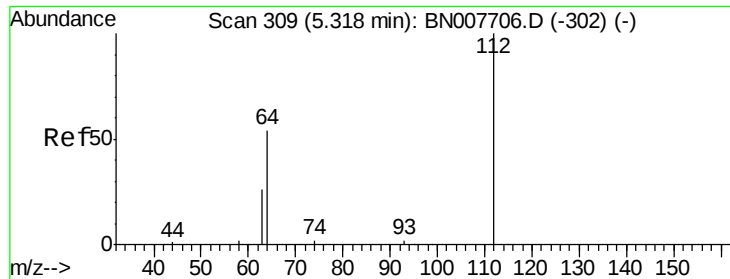

#4

2-Fluorophenol

Concen: 0.277 ng

RT: 5.31 min Scan# 308

Delta R.T. -0.01 min

Lab File: BN008001.D

Acq: 04 Oct 2019 03:34

Instrument :

BNA\_N

ClientSampleId :

PST-024-B268-092519


Tgt Ion: 112 Resp: 4473

Ion Ratio Lower Upper

112 100

64 59.4 46.6 70.0




63 28.9 23.1 34.7

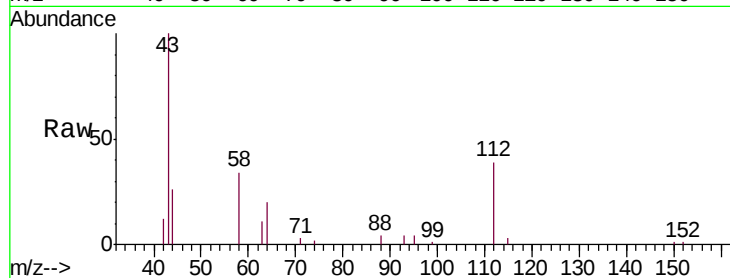

Abundance Ion 112.00 (111.70 to 112.70): BNC

Ion 64.00 (63.70 to 64.70): BNC

Ion 63.00 (62.70 to 63.70): BNC

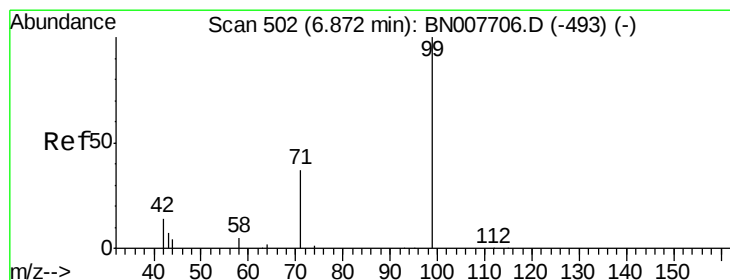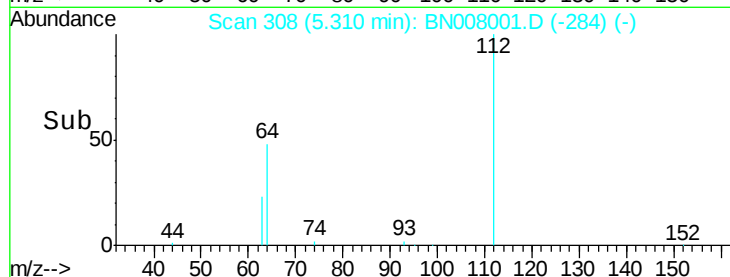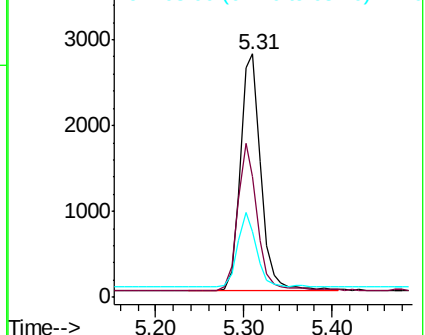

#5

Phenol-d6

Concen: 0.316 ng

RT: 6.87 min Scan# 502

Delta R.T. 0.00 min

Lab File: BN008001.D

Acq: 04 Oct 2019 03:34


Tgt Ion: 99 Resp: 6379

Ion Ratio Lower Upper

99 100

42 15.7 12.8 19.2



71 36.0 27.6 41.4

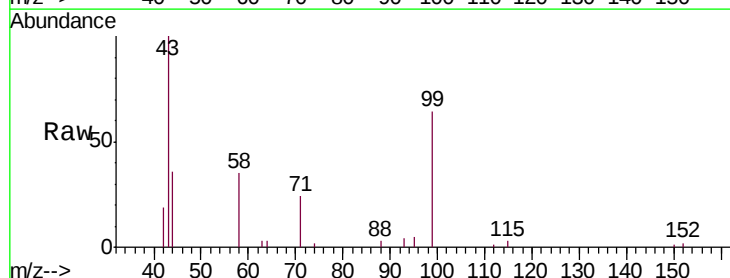

Abundance Ion 99.00 (98.70 to 99.70): BNC

Ion 42.00 (41.70 to 42.70): BNC

Ion 71.00 (70.70 to 71.70): BNC

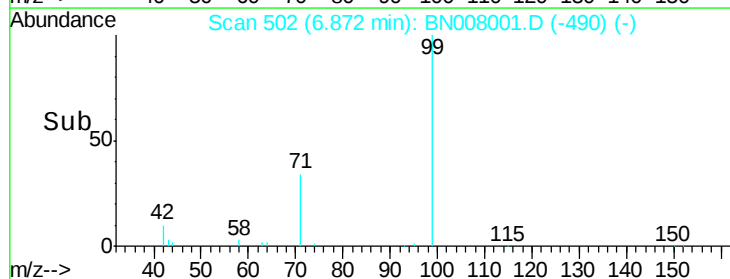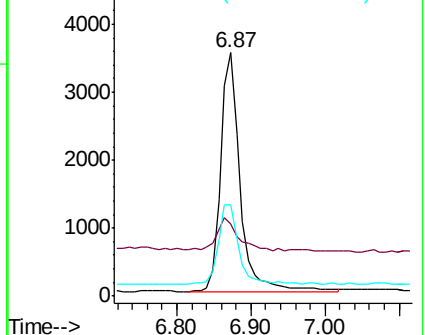



#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.46 min Scan# 850

Delta R.T. -0.01 min

Lab File: BN008001.D

Acq: 04 Oct 2019 03:34

Instrument :

BNA\_N

ClientSampleId :

PST-024-B268-092519

Tgt Ion:136 Resp: 19549


Ion Ratio Lower Upper

136 100

137 11.3 9.2 13.8

54 5.5 5.8 8.8#

68 6.2 6.5 9.7#

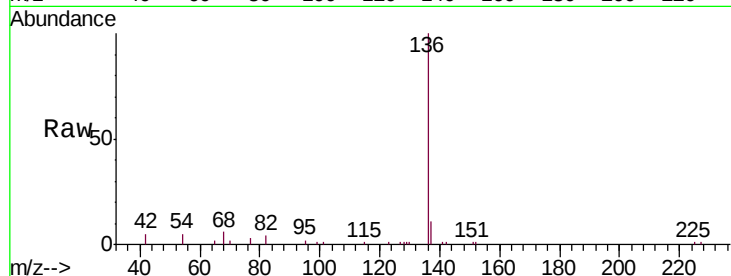




Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BNC

Ion 68.00 (67.70 to 68.70): BNC

Time-->

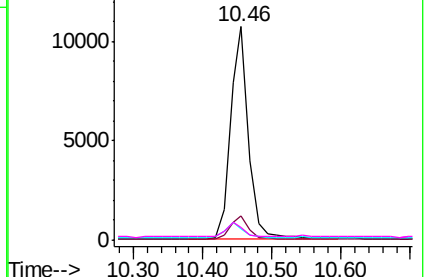

#8

Nitrobenzene-d5

Concen: 0.272 ng

RT: 8.82 min Scan# 721

Delta R.T. -0.01 min

Lab File: BN008001.D

Acq: 04 Oct 2019 03:34


Tgt Ion: 82 Resp: 4649

Ion Ratio Lower Upper

82 100

128 36.5 24.5 36.7

54 42.5 35.2 52.8





Abundance Ion 82.00 (81.70 to 82.70): BNC

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BNC

Time-->



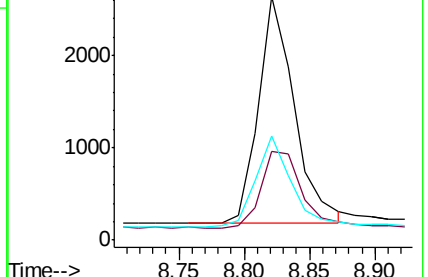





#11  
 2-Methylnaphthalene-d10  
 Concen: 0.308 ng  
 RT: 12.05 min Scan# 1054  
 Delta R.T. -0.02 min  
 Lab File: BN008001.D  
 Acq: 04 Oct 2019 03:34




Instrument :  
 BNA\_N  
 ClientSampleId :  
 PST-024-B268-092519


Tgt Ion:152 Resp: 10131  
 Ion Ratio Lower Upper  
 152 100  
 151 19.0 15.4 23.2

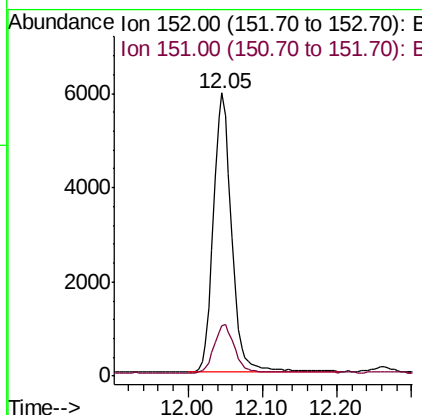

#13  
 Acenaphthene-d10  
 Concen: 0.400 ng  
 RT: 14.31 min Scan# 1320  
 Delta R.T. -0.01 min  
 Lab File: BN008001.D  
 Acq: 04 Oct 2019 03:34

Tgt Ion:164 Resp: 12346  
 Ion Ratio Lower Upper  
 164 100  
 162 98.5 81.7 122.5  
 160 43.2 37.0 55.4



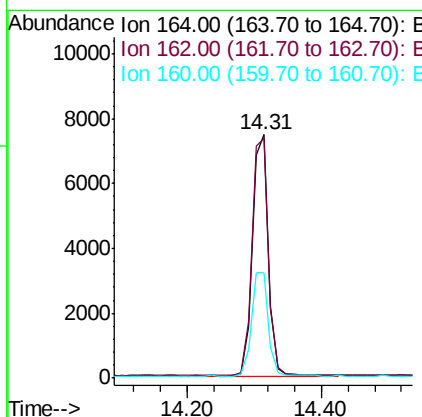



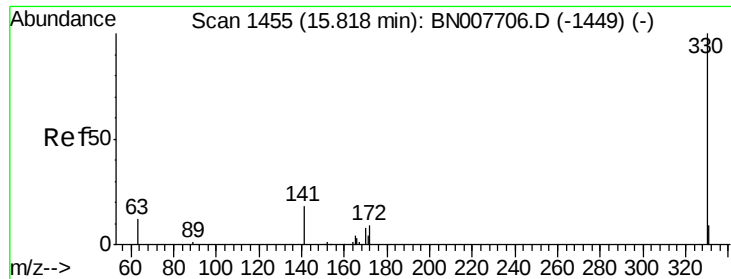

#14  
 2,4,6-Tribromophenol  
 Concen: 0.291 ng  
 RT: 15.81 min Scan# 1454  
 Delta R.T. -0.01 min  
 Lab File: BN008001.D  
 Acq: 04 Oct 2019 03:34




Instrument :  
 BNA\_N  
 ClientSampleId :  
 PST-024-B268-092519


Tgt Ion: 330 Resp: 1957  
 Ion Ratio Lower Upper  
 330 100  
 332 0.0 0.0 0.0  
 141 33.1 28.7 43.1

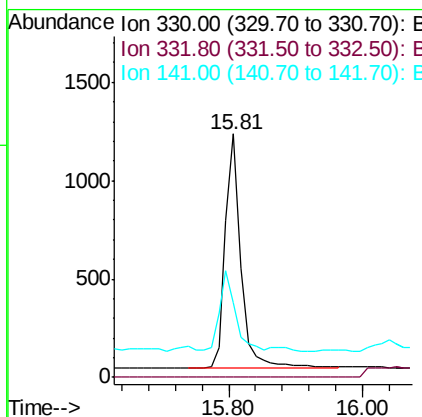

#15  
 2-Fluorobiphenyl  
 Concen: 0.272 ng  
 RT: 12.93 min Scan# 1196  
 Delta R.T. -0.01 min  
 Lab File: BN008001.D  
 Acq: 04 Oct 2019 03:34

Tgt Ion: 172 Resp: 13808  
 Ion Ratio Lower Upper  
 172 100  
 171 34.6 28.8 43.2  
 170 22.7 19.5 29.3

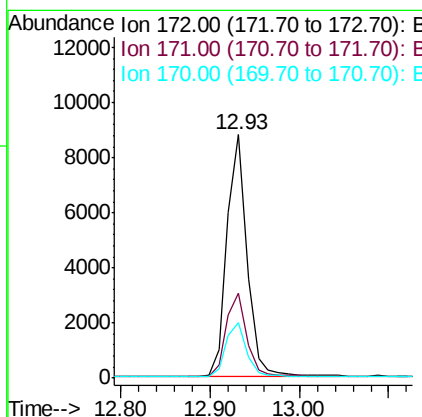



#16

Acenaphthylene

Concen: 0.083 ng

RT: 14.02 min Scan# 1294

Delta R.T. -0.02 min

Lab File: BN008001.D

Acq: 04 Oct 2019 03:34

Instrument :

BNA\_N

ClientSampleId :

PST-024-B268-092519


Tgt Ion:152 Resp: 5443

Ion Ratio Lower Upper

152 100

151 17.4 15.5 23.3




153 14.1 10.4 15.6

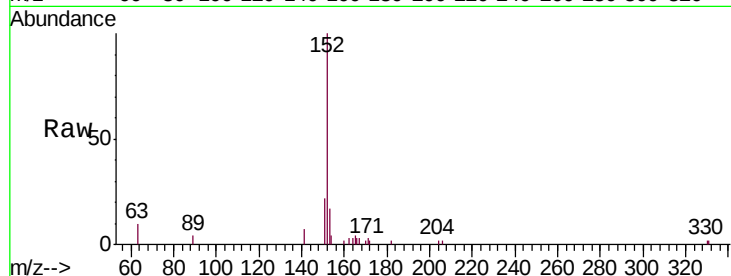

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E

Ion 153.00 (152.70 to 153.70): E

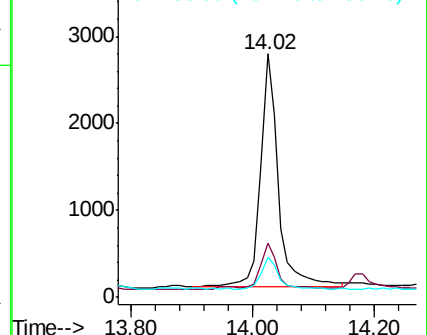

#18

Fluorene

Concen: 0.020 ng

RT: 15.36 min Scan# 1414

Delta R.T. -0.01 min

Lab File: BN008001.D

Acq: 04 Oct 2019 03:34


Tgt Ion:166 Resp: 1097

Ion Ratio Lower Upper

166 100

165 112.1 78.0 117.0



167 18.2 10.9 16.3#




Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E




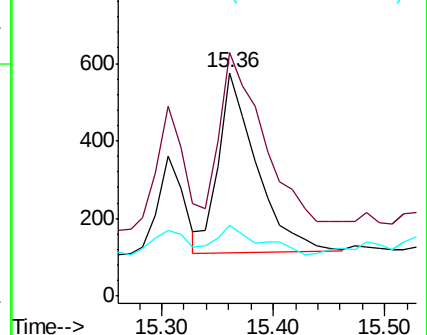




#19  
Phenanthrene-d10  
Concen: 0.400 ng  
RT: 17.06 min Scan# 1571  
Delta R.T. -0.01 min  
Lab File: BN008001.D  
Acq: 04 Oct 2019 03:34




Instrument :  
BNA\_N  
ClientSampleId :  
PST-024-B268-092519


Tgt Ion:188 Resp: 26811  
Ion Ratio Lower Upper  
188 100  
94 0.0 0.0 0.0  
80 7.8 7.4 11.2

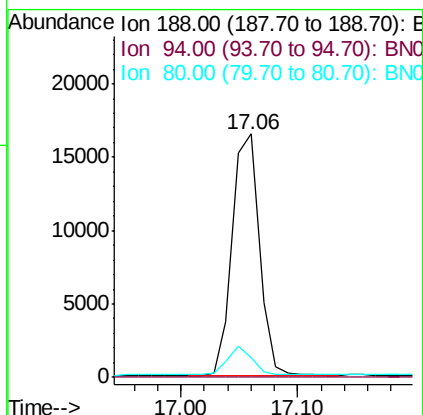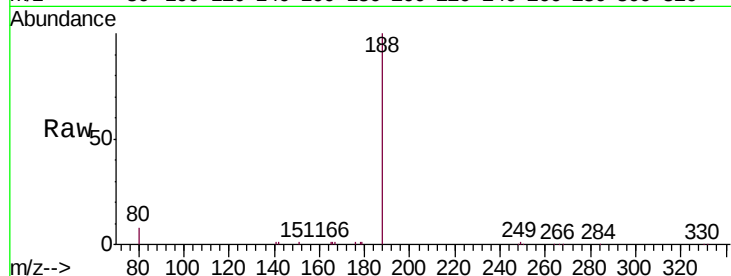

#23  
Phenanthrene  
Concen: 0.262 ng  
RT: 17.09 min Scan# 1574  
Delta R.T. -0.02 min  
Lab File: BN008001.D  
Acq: 04 Oct 2019 03:34

Tgt Ion:178 Resp: 21879  
Ion Ratio Lower Upper  
178 100  
176 18.9 14.9 22.3  
179 15.4 12.5 18.7

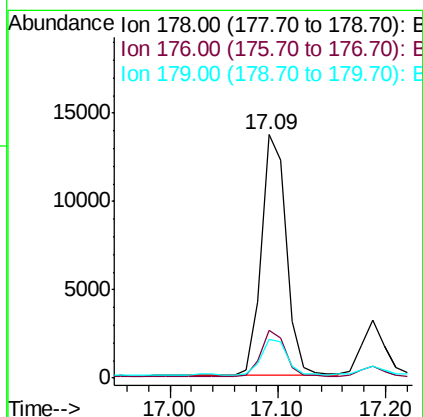



#24

Anthracene

Concen: 0.058 ng

RT: 17.19 min Scan# 1583

Delta R.T. -0.01 min

Lab File: BN008001.D

Acq: 04 Oct 2019 03:34

Instrument :

BNA\_N

ClientSampleId :

PST-024-B268-092519


Tgt Ion:178 Resp: 4395

Ion Ratio Lower Upper

178 100

176 18.5 14.6 21.8


179 16.3 12.2 18.4

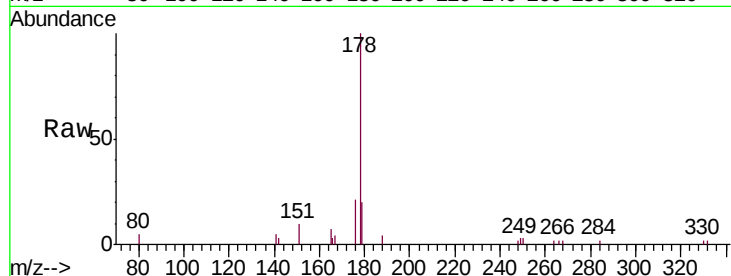



Abundance Ion 178.00 (177.70 to 178.70): E

Ion 176.00 (175.70 to 176.70): E

Ion 179.00 (178.70 to 179.70): E

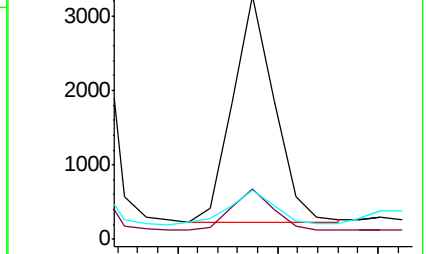

Time-->



#25

Fluoranthene-d10

Concen: 0.314 ng

RT: 19.09 min Scan# 1879

Delta R.T. -0.01 min

Lab File: BN008001.D

Acq: 04 Oct 2019 03:34


Tgt Ion:212 Resp: 28379

Ion Ratio Lower Upper

212 100

106 11.3 9.4 14.0


104 6.4 5.3 7.9




Abundance Ion 212.00 (211.70 to 212.70): E


Ion 106.00 (105.70 to 106.70): E

Ion 104.00 (103.70 to 104.70): E

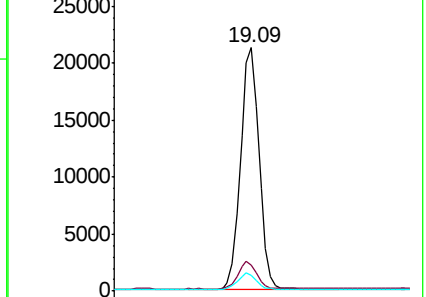

Time-->









#26  
Fluoranthene  
Concen: 0.614 ng  
RT: 19.12 min Scan# 1885  
Delta R.T. -0.01 min  
Lab File: BN008001.D  
Acq: 04 Oct 2019 03:34




Instrument :  
BNA\_N  
ClientSampleId :  
PST-024-B268-092519


Tgt Ion:202 Resp: 63735  
Ion Ratio Lower Upper  
202 100  
101 10.2 8.4 12.6  
203 17.5 13.8 20.8

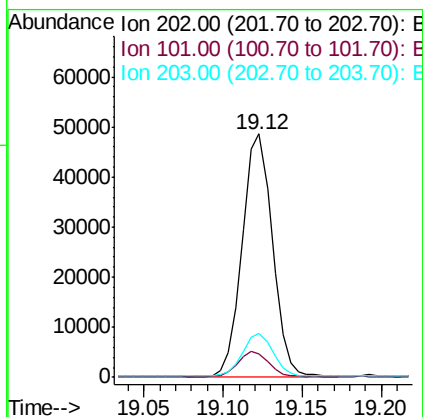

#27  
Chrysene-d12  
Concen: 0.400 ng  
RT: 21.25 min Scan# 2180  
Delta R.T. -0.02 min  
Lab File: BN008001.D  
Acq: 04 Oct 2019 03:34

Tgt Ion:240 Resp: 28978  
Ion Ratio Lower Upper  
240 100  
120 10.5 5.4 8.2#  
236 27.8 21.0 31.4

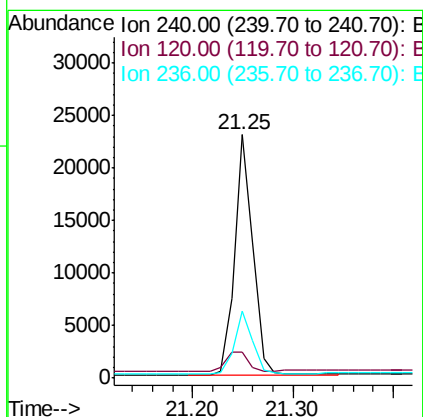



#28

Pyrene

Concen: 0.622 ng

RT: 19.49 min Scan# 1958

Delta R.T. -0.01 min

Lab File: BN008001.D

Acq: 04 Oct 2019 03:34





Instrument :

BNA\_N

ClientSampleId :

PST-024-B268-092519

|          |       |       |       |
|----------|-------|-------|-------|
| Tgt Ion: | 202   | Resp: | 61484 |
| Ion      | Ratio | Lower | Upper |
| 202      | 100   |       |       |
| 200      | 20.6  | 16.4  | 24.6  |
| 203      | 21.0  | 14.1  | 21.1  |

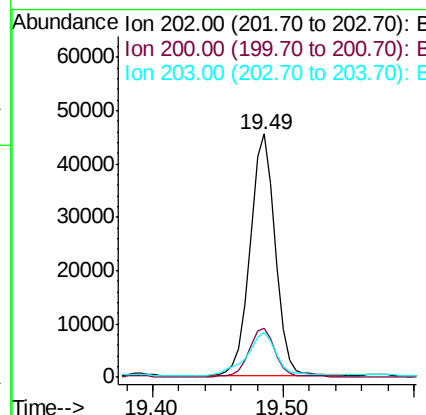

#29

Terphenyl-d14

Concen: 0.320 ng




RT: 19.69 min Scan# 2000


Delta R.T. -0.02 min

Lab File: BN008001.D

Acq: 04 Oct 2019 03:34

|          |       |       |       |
|----------|-------|-------|-------|
| Tgt Ion: | 244   | Resp: | 22804 |
| Ion      | Ratio | Lower | Upper |
| 244      | 100   |       |       |
| 212      | 7.5   | 5.9   | 8.9   |
| 122      | 10.8  | 7.4   | 11.2  |

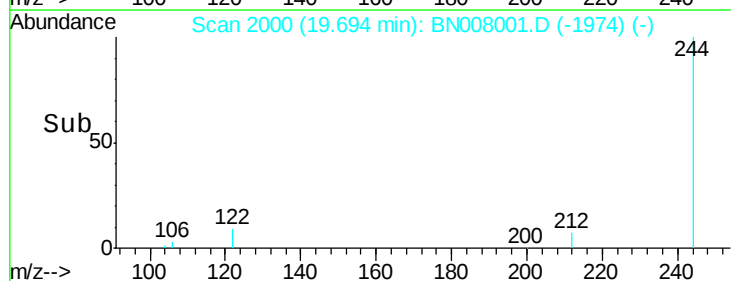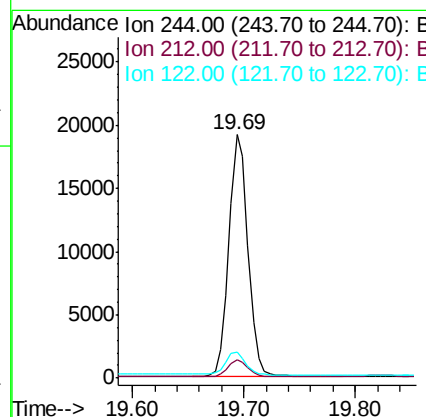



#30

Benzo(a)anthracene

Concen: 0.318 ng

RT: 21.28 min Scan# 2183

Delta R.T. 0.03 min

Lab File: BN008001.D

Acq: 04 Oct 2019 03:34

Instrument :

BNA\_N

ClientSampleId :

PST-024-B268-092519


Tgt Ion:228 Resp: 33923

Ion Ratio Lower Upper

228 100

226 32.3 22.1 33.1




229 21.8 15.8 23.6



Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

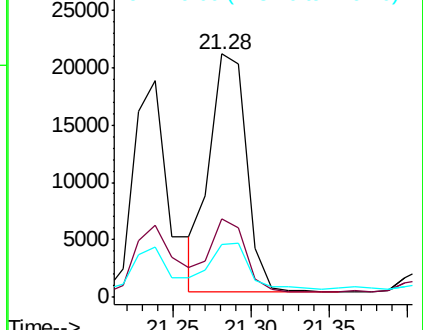

#31

Chrysene

Concen: 0.326 ng

RT: 21.28 min Scan# 2183

Delta R.T. -0.02 min

Lab File: BN008001.D

Acq: 04 Oct 2019 03:34


Tgt Ion:228 Resp: 33860

Ion Ratio Lower Upper

228 100

226 32.3 23.9 35.9



229 21.8 15.8 23.6




Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

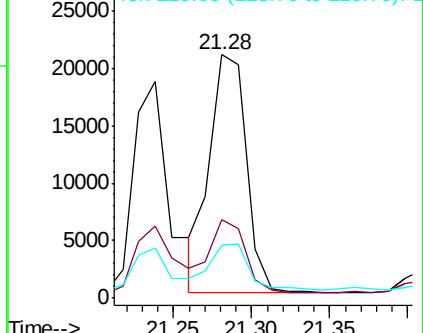



#32

Bis(2-ethylhexyl)phthalate

Concen: 0.112 ng

RT: 21.17 min Scan# 2173

Delta R.T. -0.03 min

Lab File: BN008001.D

Acq: 04 Oct 2019 03:34

Instrument :

BNA\_N

ClientSampleId :

PST-024-B268-092519


Tgt Ion:149 Resp: 6154

Ion Ratio Lower Upper

149 100

167 26.5 23.7 35.5




279 4.4 4.2 6.2



Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

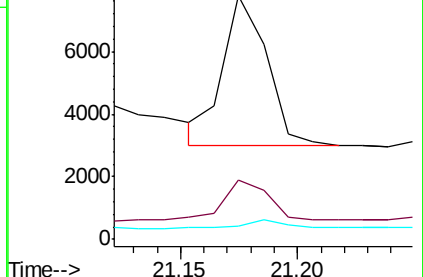

#33

Indeno(1,2,3-cd)pyrene

Concen: 0.196 ng

RT: 25.67 min Scan# 3243

Delta R.T. -0.03 min

Lab File: BN008001.D

Acq: 04 Oct 2019 03:34


Tgt Ion:276 Resp: 25556

Ion Ratio Lower Upper

276 100

138 17.5 17.1 25.7



277 24.3 20.0 30.0




Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

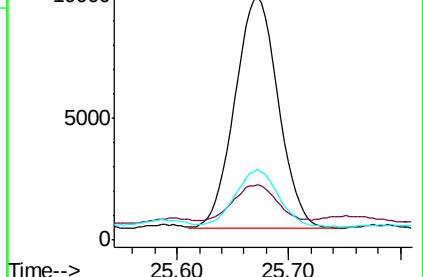

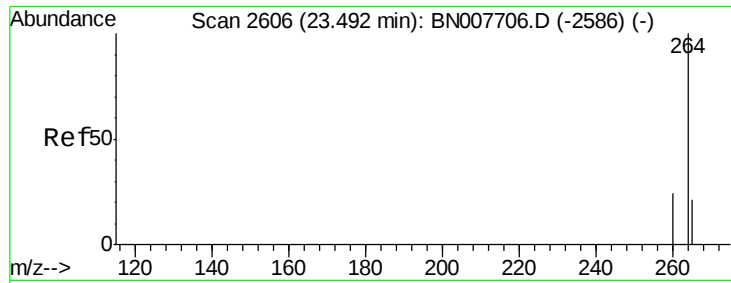

#34

Perylene-d12

Concen: 0.400 ng

RT: 23.46 min Scan# 2598

Delta R.T. -0.03 min

Lab File: BN008001.D

Acq: 04 Oct 2019 03:34

Instrument :

BNA\_N

ClientSampleId :

PST-024-B268-092519


Tgt Ion:264 Resp: 31452

Ion Ratio Lower Upper

264 100

260 25.4 19.3 28.9




265 40.8 26.9 40.3#

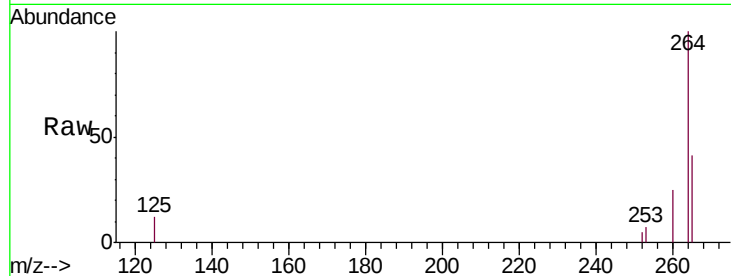

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

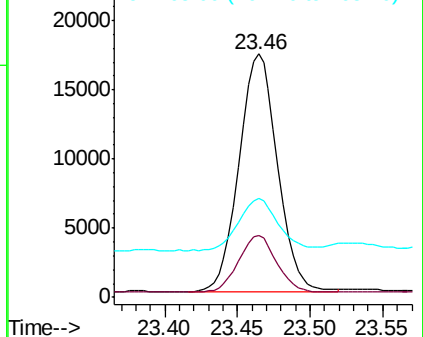

#35

Benzo(b)fluoranthene

Concen: 0.491 ng

RT: 22.81 min Scan# 2406

Delta R.T. -0.02 min

Lab File: BN008001.D

Acq: 04 Oct 2019 03:34


Tgt Ion:252 Resp: 53644

Ion Ratio Lower Upper

252 100

253 30.8 18.3 27.5#



125 40.4 8.2 12.4#




Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E




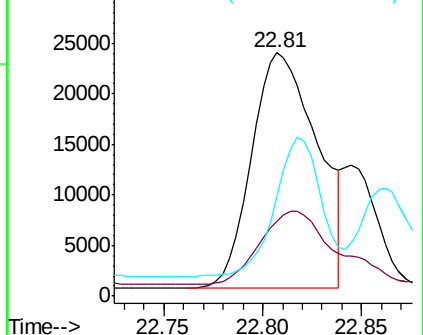




#36  
Benzo(k)fluoranthene  
Concen: 0.497 ng  
RT: 22.81 min Scan# 2406  
Delta R.T. -0.07 min  
Lab File: BN008001.D  
Acq: 04 Oct 2019 03:34




Instrument :  
BNA\_N  
ClientSampleId :  
PST-024-B268-092519


Tgt Ion:252 Resp: 53644  
Ion Ratio Lower Upper  
252 100  
253 30.8 18.5 27.7#  
125 40.4 8.4 12.6#

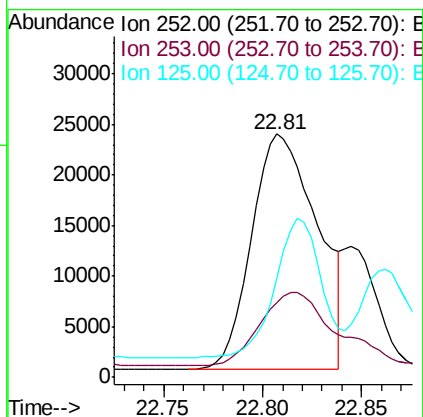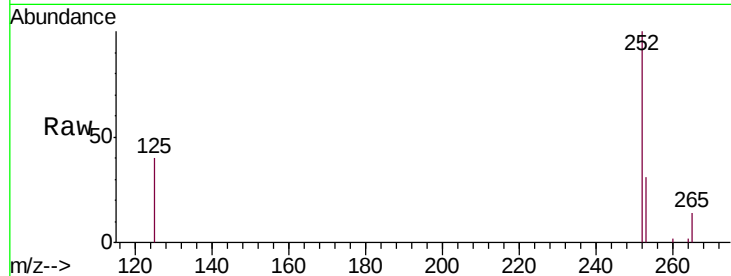

#37  
Benzo(a)pyrene  
Concen: 0.301 ng  
RT: 23.37 min Scan# 2570  
Delta R.T. -0.02 min  
Lab File: BN008001.D  
Acq: 04 Oct 2019 03:34

Tgt Ion:252 Resp: 30858  
Ion Ratio Lower Upper  
252 100  
253 28.0 18.6 27.8#  
125 23.5 9.4 14.0#

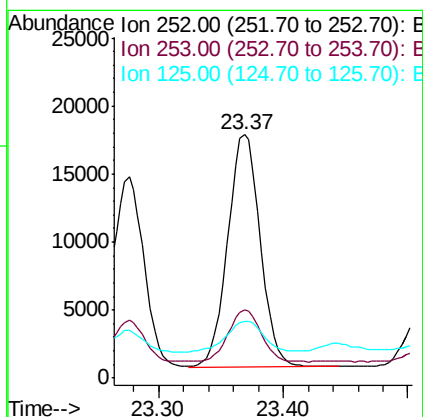



#38

Dibenzo(a,h)anthracene

Concen: 0.057 ng

RT: 25.68 min Scan# 3245

Delta R.T. -0.04 min

Lab File: BN008001.D

Acq: 04 Oct 2019 03:34

Instrument :

BNA\_N

ClientSampleId :

PST-024-B268-092519


Tgt Ion: 278 Resp: 5982

Ion Ratio Lower Upper

278 100

139 51.4 11.8 17.6#




279 46.6 19.4 29.2#



Abundance Ion 278.00 (277.70 to 278.70): E

Ion 139.00 (138.70 to 139.70): E

Ion 279.00 (278.70 to 279.70): E

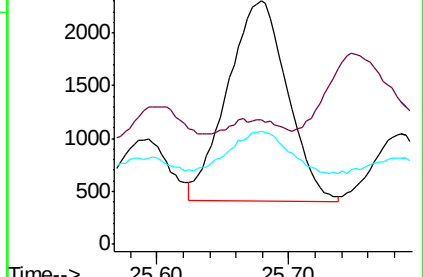

#39

Benzo(g,h,i)perylene

Concen: 0.250 ng

RT: 26.35 min Scan# 3440

Delta R.T. -0.03 min

Lab File: BN008001.D

Acq: 04 Oct 2019 03:34


Tgt Ion: 276 Resp: 25932

Ion Ratio Lower Upper

276 100

277 29.1 19.8 29.8

138 23.7 15.1 22.7#



Abundance Ion 276.00 (275.70 to 276.70): E

Ion 277.00 (276.70 to 277.70): E

Ion 138.00 (137.70 to 138.70): E

