


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN100319\
 Data File : BN007984.D
 Acq On : 03 Oct 2019 17:24
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN091819.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Oct 03 18:39:49 2019

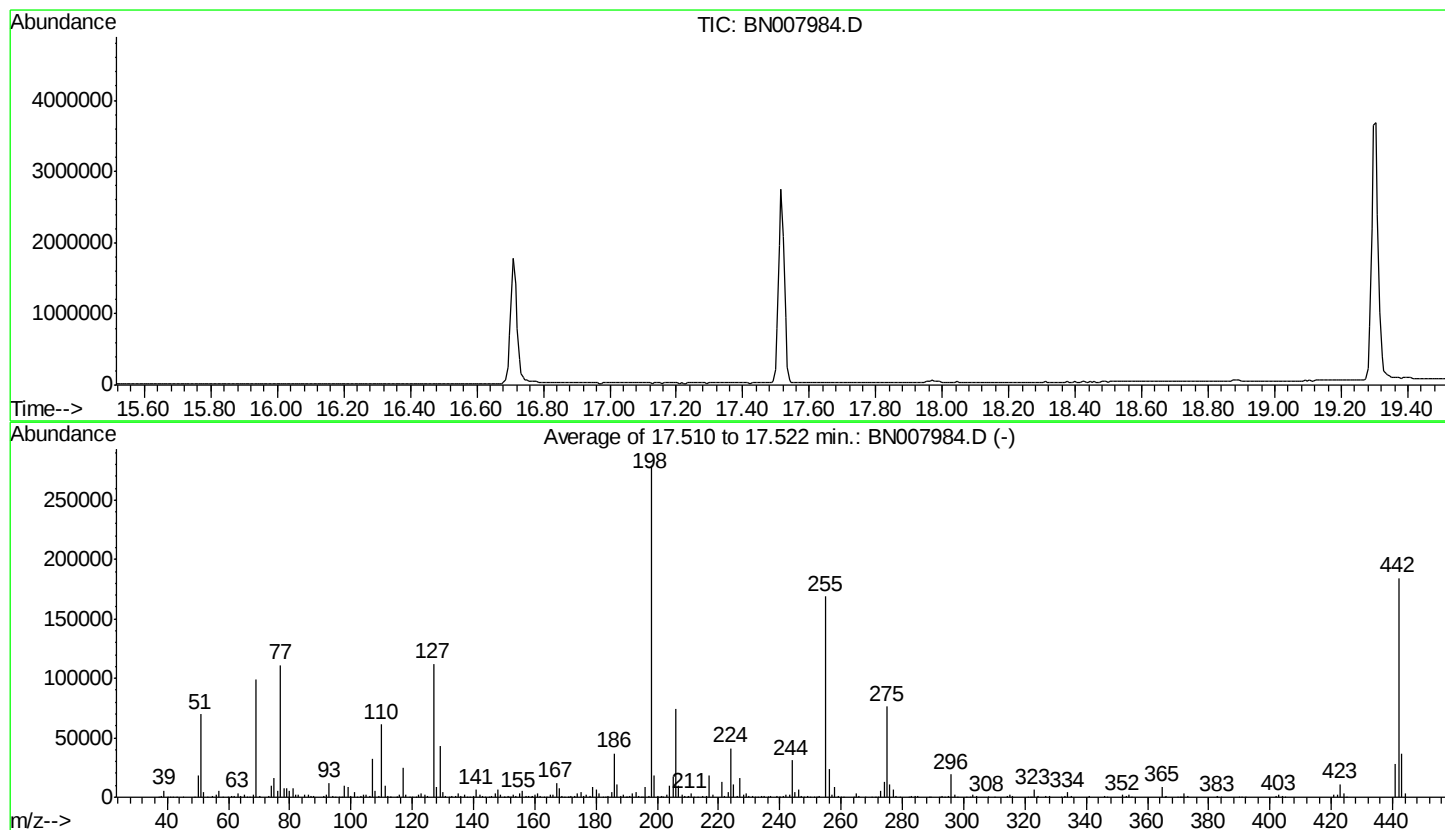

AutoFind: Scans 2469, 2470, 2471; Background Corrected with Scan 2462

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.1	69950	PASS
68	69	0.00	2	1.9	1863	PASS
69	198	0.00	100	35.4	98615	PASS
70	69	0.00	2	0.8	800	PASS
127	198	10	80	40.3	112488	PASS
197	198	0.00	2	0.3	852	PASS
198	198	100	100	100.0	278869	PASS
199	198	5	9	6.7	18804	PASS
275	198	10	60	27.3	76269	PASS
365	198	1	100	3.1	8695	PASS
441	198	0.01	100	10.2	28394	PASS
442	198	50	100	66.1	184248	PASS
443	442	15	24	19.6	36154	PASS