
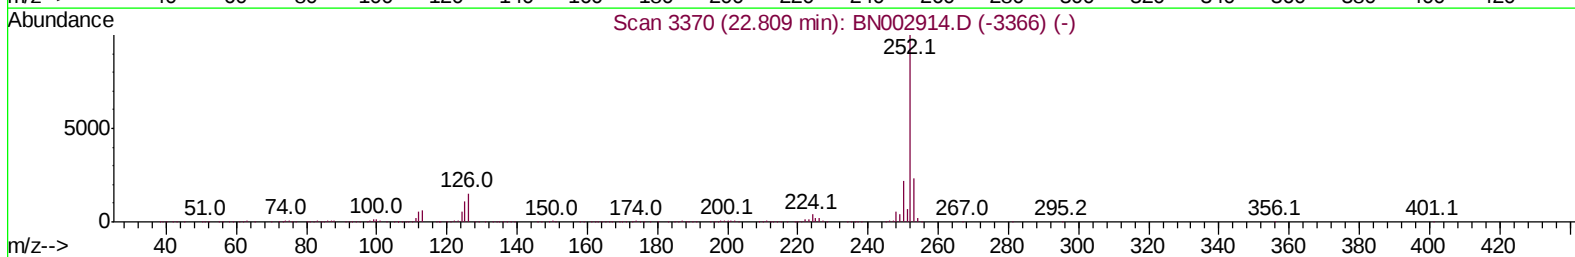
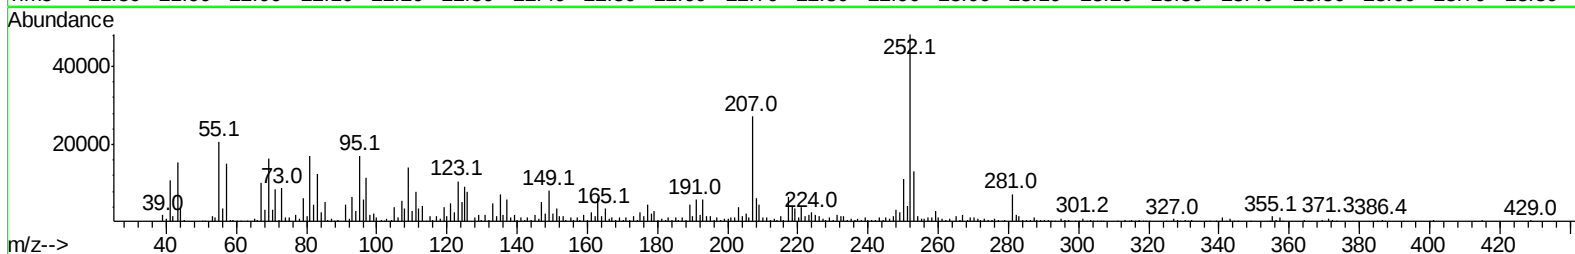


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN100418\
Data File : BN002915.D
Acq On : 03 Oct 2018 23:44
Operator : MJ/SJ
Sample : J5115-15
Misc :
ALS Vial : 18 Sample Multiplier: 1

Quant Time: Oct 04 04:29:41 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN091418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 04 04:26:52 2018
Response via : Initial Calibration

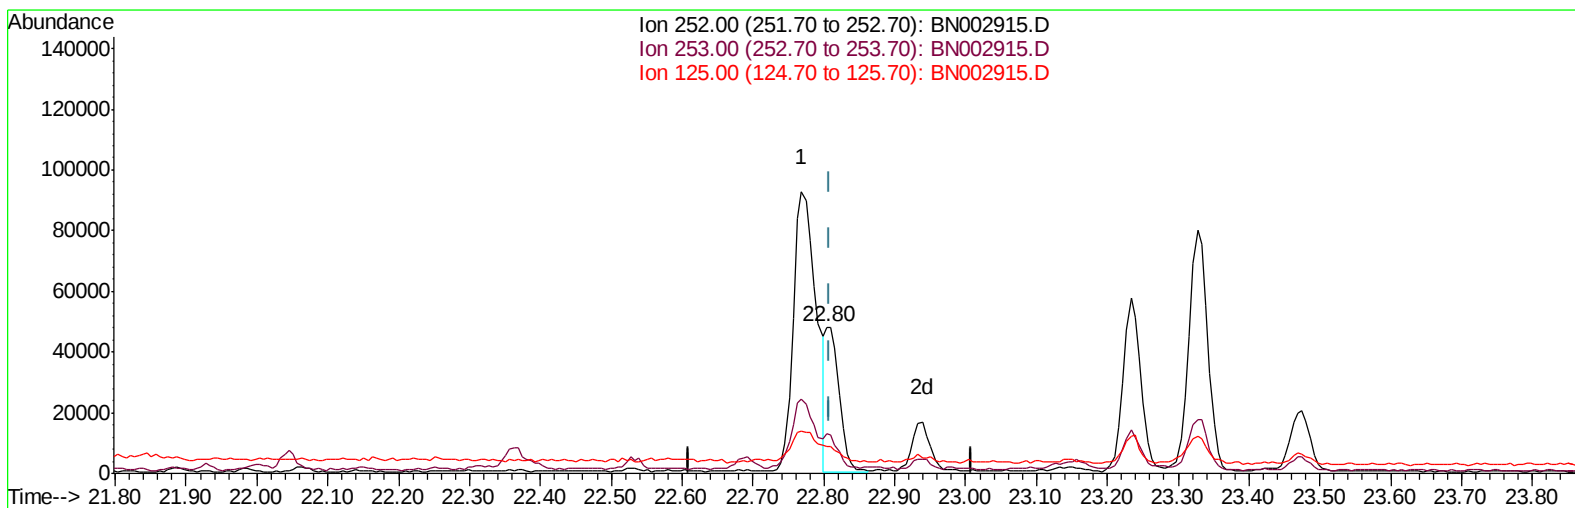

TIC: BN002915.D

(88) Benzo(k)fluoranthene

22.804min (-0.005) 1.97ng/ul m

response 66708

Ion	Exp%	Act%
252.00	100	100
253.00	22.30	26.93#
125.00	10.40	18.72#
0.00	0.00	0.00