
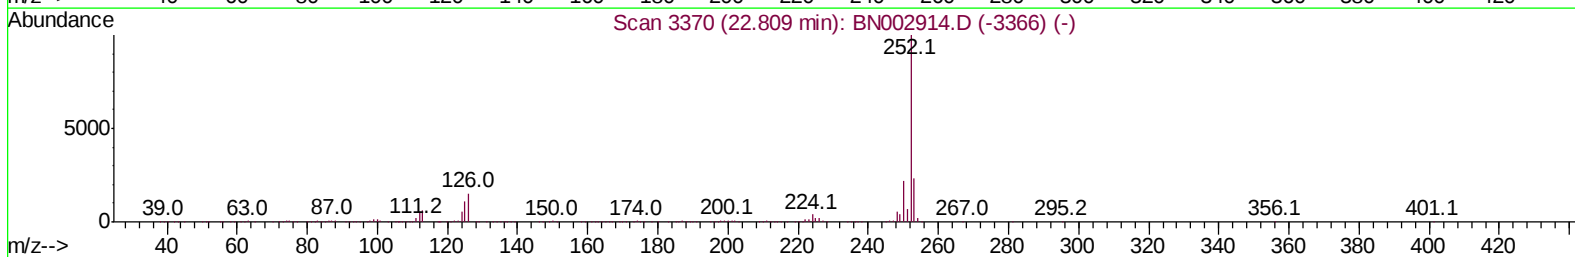
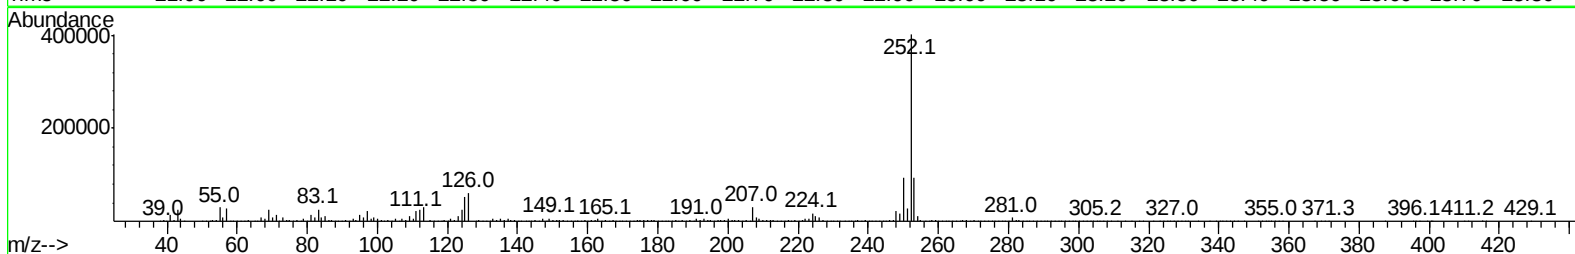


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN100418\
Data File : BN002920.D
Acq On : 04 Oct 2018 02:39
Operator : MJ/SJ
Sample : J5115-20
Misc :
ALS Vial : 23 Sample Multiplier: 1

Quant Time: Oct 04 04:30:32 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN091418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 04 04:26:52 2018
Response via : Initial Calibration

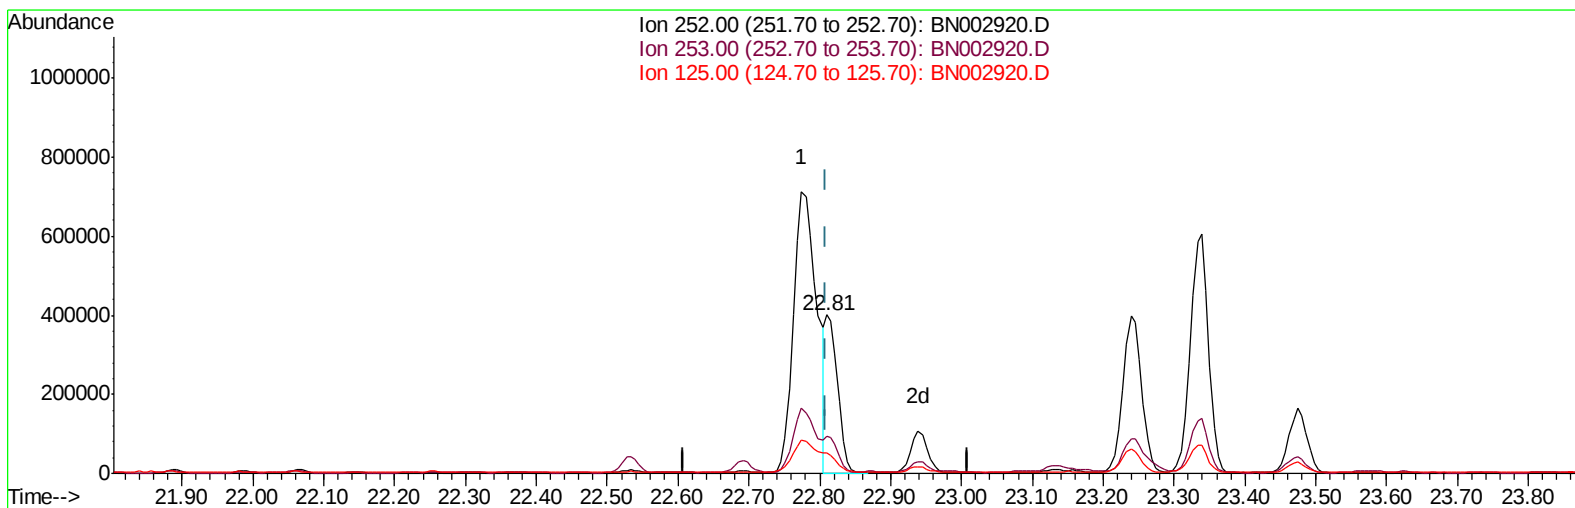

TIC: BN002920.D

(88) Benzo(k)fluoranthene

22.810min (+0.000) 14.11ng/ul m

response 490536

Ion	Exp%	Act%
252.00	100	100
253.00	22.30	23.57
125.00	10.40	13.12#
0.00	0.00	0.00