
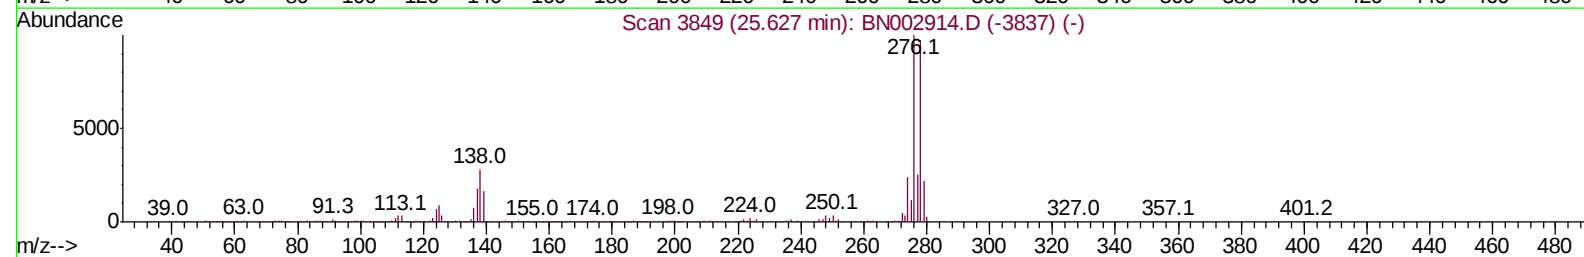
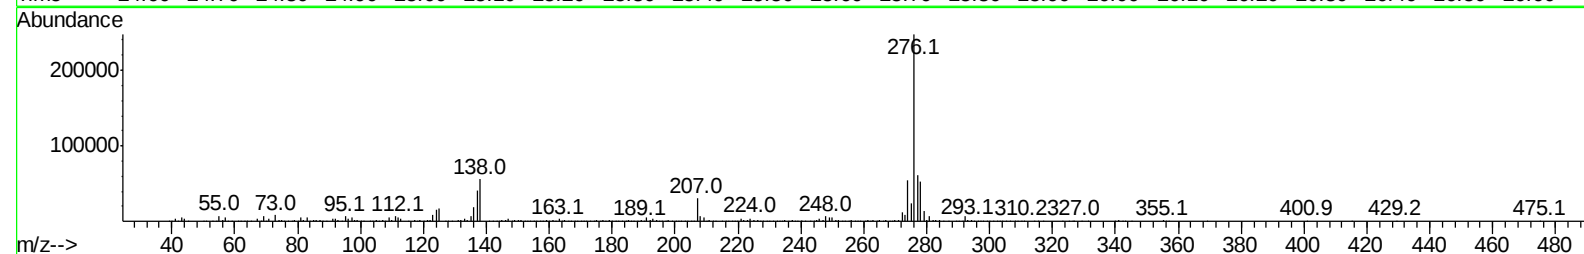


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN100418\
Data File : BN002920.D
Acq On : 04 Oct 2018 02:39
Operator : MJ/SJ
Sample : J5115-20
Misc :
ALS Vial : 23 Sample Multiplier: 1

Quant Time: Oct 04 04:30:32 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN091418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 04 04:26:52 2018
Response via : Initial Calibration

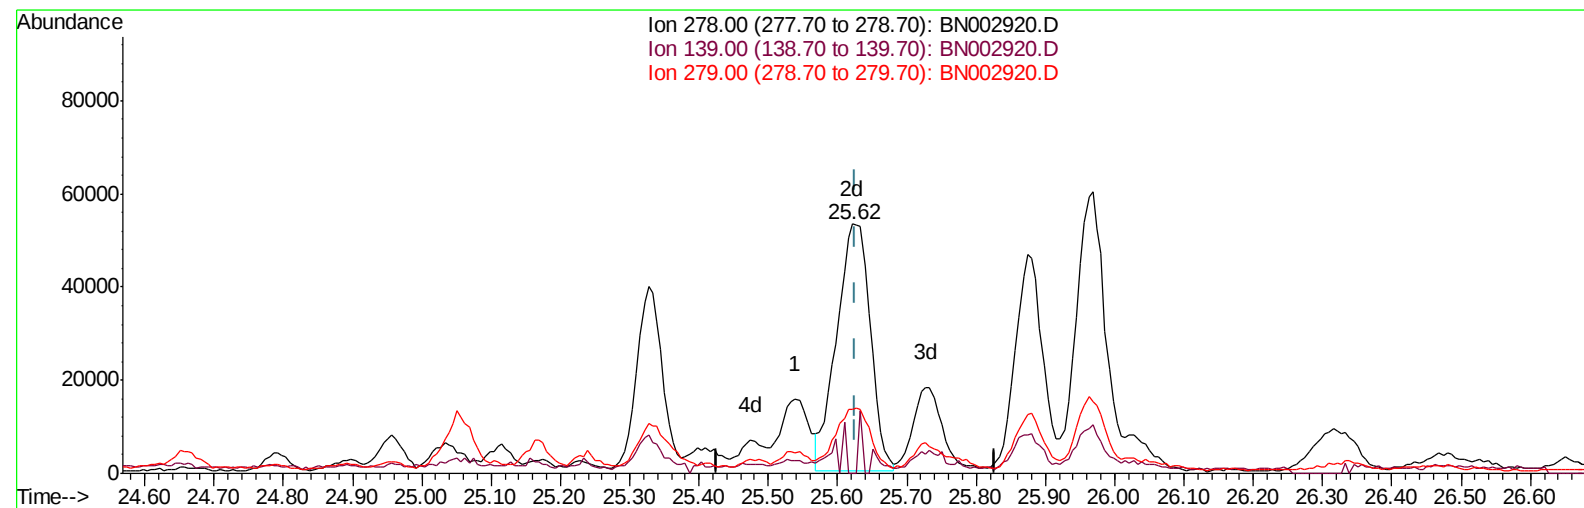

TIC: BN002920.D

(92) Dibenzo(a,h)anthracene

25.621min (-0.006) 5.06ng/ul m

response 177766

Ion	Exp%	Act%
278.00	100	100
139.00	15.90	0.00#
279.00	23.40	25.70
0.00	0.00	0.00