

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN100418\
 Data File : BN002899.D
 Acq On : 03 Oct 2018 14:17
 Operator : MJ/SJ
 Sample : PB113375BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Oct 04 02:50:55 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN091418MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 04 02:50:09 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	99314	20.00	ng/ul	0.00
18) Naphthalene-d8	10.39	136	440388	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.26	164	268546	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.02	188	635521	20.00	ng/ul	0.00
77) Chrysene-d12	21.22	240	727626	20.00	ng/ul	0.00
85) Perylene-d12	23.43	264	714179	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.20	96	15183	7.05	ng/uL	0.00
5) Phenol-d5	6.81	99	285419	33.84	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.97	67	188782	36.04	ng/ul	0.00
9) 2-Chlorophenol-d4	7.16	132	243967	35.15	ng/ul	0.00
13) 4-Methylphenol-d8	8.33	113	234946	35.97	ng/ul	0.00
19) Nitrobenzene-d5	8.78	128	120965	35.46	ng/ul	0.00
22) 2-Nitrophenol-d4	9.49	143	139856	36.23	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.03	165	234861	33.70	ng/ul	0.00
29) 4-Chloroaniline-d4	10.54	131	334289	41.46	ng/ul	0.00
43) Dimethylphthalate-d6	13.67	166	834230	39.69	ng/ul	0.00
46) Acenaphthylene-d8	13.95	160	1032073	37.60	ng/ul	0.00
51) 4-Nitrophenol-d4	14.50	143	110391	31.76	ng/ul	0.00
57) Fluorene-d10	15.26	176	731299	39.71	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.41	200	122529	30.82	ng/ul	0.00
70) Anthracene-d10	17.12	188	1168815	38.52	ng/ul	0.00
78) Pyrene-d10	19.42	212	1330757	34.66	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.29	264	1439172	38.28	ng/ul	0.00

Target Compounds


				Ovalue	
15) N-Nitroso-di-n-propylamine	8.33	70	5320	1.052	ng/ul# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN100418\
Data File : BN002899.D
Acq On : 03 Oct 2018 14:17
Operator : MJ/SJ
Sample : PB113375BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Oct 04 02:50:55 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN091418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 04 02:50:09 2018
Response via : Initial Calibration

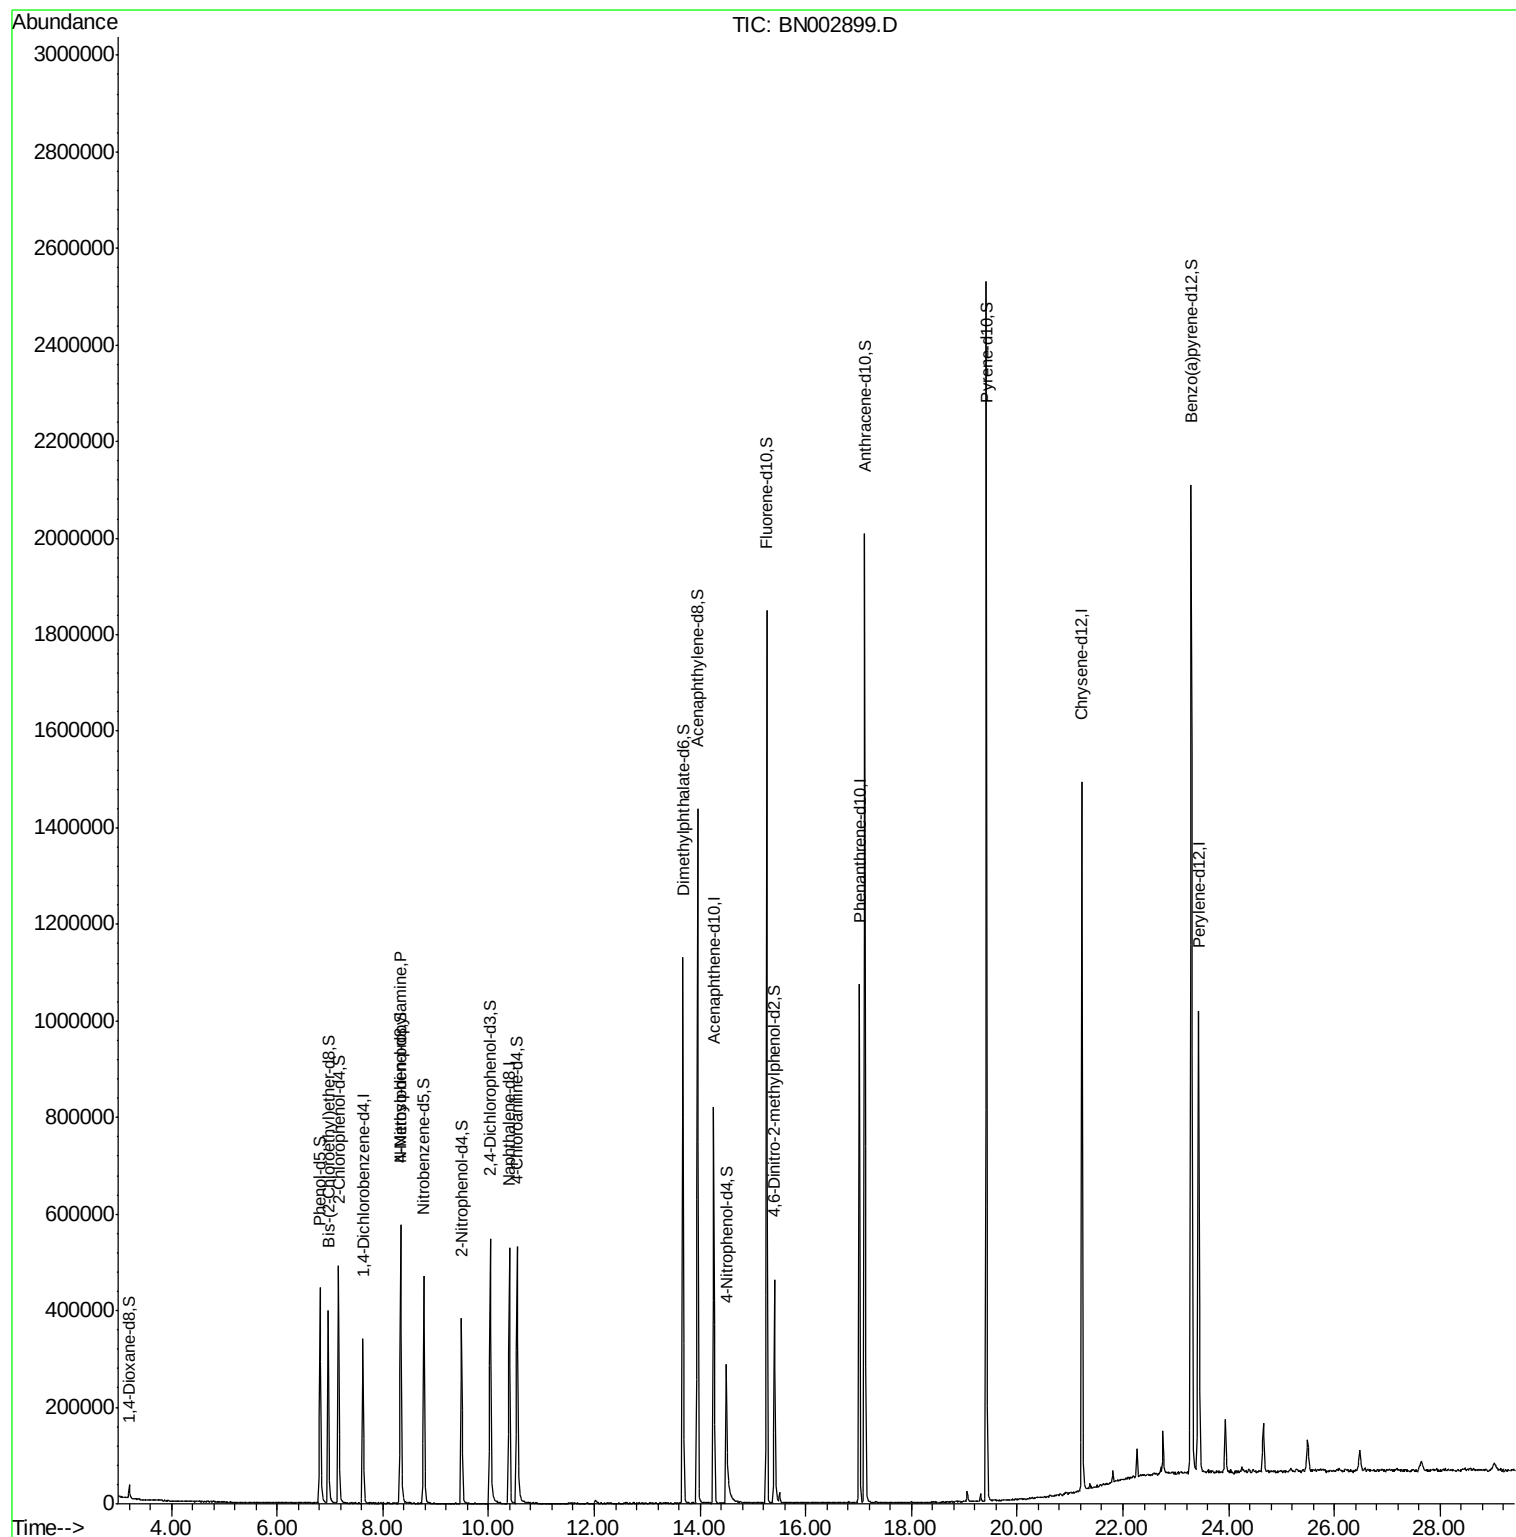

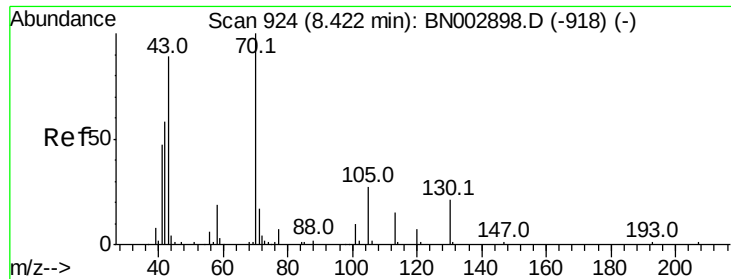

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.052 ng/ul
 RT: 8.33 min Scan# 909
 Delta R.T. -0.09 min
 Lab File: BN002899.D
 Acq: 03 Oct 2018 14:17

Instrument :
 BNA_N
 ClientSampleId :

Tot Ion: 70 Resp: 5320
 Ion Ratio Lower Upper
 70 100
 42 400.2 47.7 71.5#
 101 0.0 8.0 12.0#
 130 0.0 16.0 24.0#

