

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN100418\
 Data File : BN002908.D
 Acq On : 03 Oct 2018 19:40
 Operator : MJ/SJ
 Sample : PB113373BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Oct 04 02:52:12 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN091418MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 04 02:50:09 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	113042	20.00	ng/ul	0.00
18) Naphthalene-d8	10.39	136	512289	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.26	164	313458	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.02	188	730696	20.00	ng/ul	0.00
77) Chrysene-d12	21.22	240	763592	20.00	ng/ul	0.00
85) Perylene-d12	23.43	264	675958	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.20	96	16220	6.62	ng/uL	0.00
5) Phenol-d5	6.82	99	341009	35.52	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.97	67	218610	36.67	ng/ul	0.00
9) 2-Chlorophenol-d4	7.16	132	285448	36.13	ng/ul	0.00
13) 4-Methylphenol-d8	8.33	113	284970	38.33	ng/ul	0.00
19) Nitrobenzene-d5	8.78	128	149248	37.61	ng/ul	0.00
22) 2-Nitrophenol-d4	9.49	143	174253	38.80	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.03	165	288400	35.58	ng/ul	0.00
29) 4-Chloroaniline-d4	10.54	131	396761	42.30	ng/ul	0.00
43) Dimethylphthalate-d6	13.67	166	992366	40.44	ng/ul	0.00
46) Acenaphthylene-d8	13.95	160	1239444	38.69	ng/ul	0.00
51) 4-Nitrophenol-d4	14.50	143	153286	37.78	ng/ul	0.00
57) Fluorene-d10	15.26	176	859999	40.01	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.40	200	155688	34.06	ng/ul	0.00
70) Anthracene-d10	17.11	188	1366083	39.16	ng/ul	0.00
78) Pyrene-d10	19.42	212	1506479	37.39	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.30	264	1394188	39.18	ng/ul	0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
15) N-Nitroso-di-n-propylamine	8.34	70	6678	1.160	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN100418\
Data File : BN002908.D
Acq On : 03 Oct 2018 19:40
Operator : MJ/SJ
Sample : PB113373BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Oct 04 02:52:12 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN091418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 04 02:50:09 2018
Response via : Initial Calibration

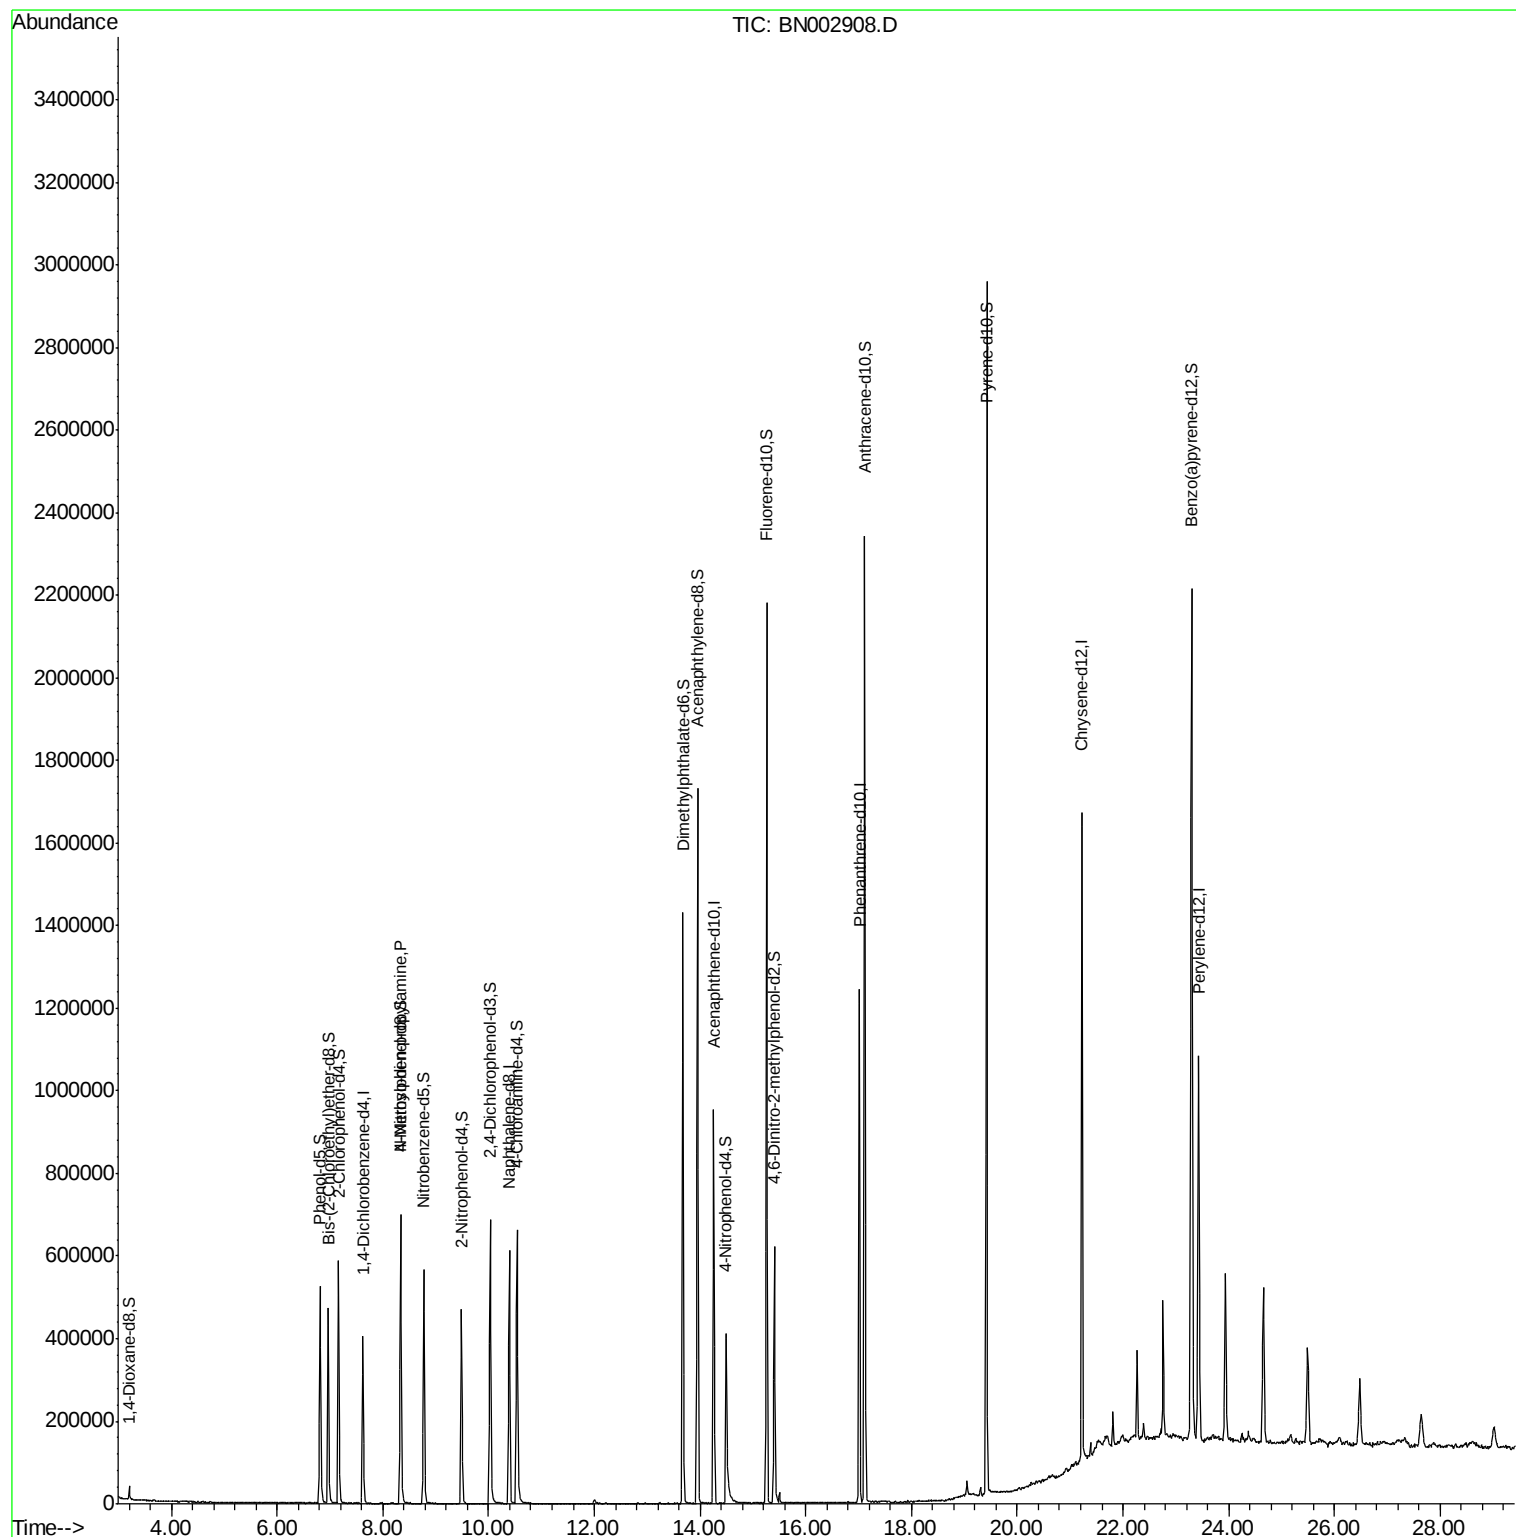

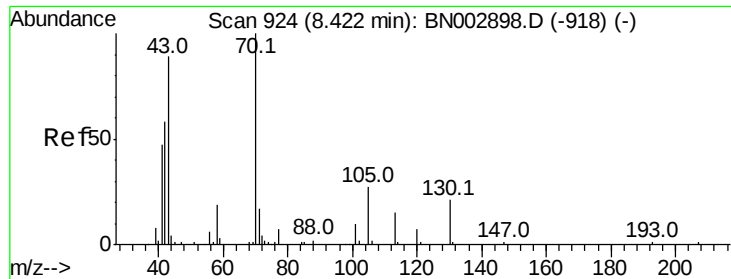

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.160 ng/ul
 RT: 8.34 min Scan# 910
 Delta R.T. -0.08 min
 Lab File: BN002908.D
 Acq: 03 Oct 2018 19:40

Instrument :
 BNA_N
 ClientSampleId :

Tot Ion: 70 Resp: 6678
 Ion Ratio Lower Upper
 70 100
 42 329.0 47.7 71.5#
 101 0.0 8.0 12.0#
 130 0.0 16.0 24.0#

