

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN100418\
 Data File : BN002900.D
 Acq On : 03 Oct 2018 14:53
 Operator : MJ/SJ
 Sample : J5116-02
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JLC53

Quant Time: Oct 04 02:50:59 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN091418MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 04 02:50:09 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	132872	20.00	ng/ul	0.00
18) Naphthalene-d8	10.39	136	585100	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.26	164	353194	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.02	188	803709	20.00	ng/ul	0.00
77) Chrysene-d12	21.22	240	850692	20.00	ng/ul	0.00
85) Perylene-d12	23.42	264	759980	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.20	96	11958	4.15	ng/uL	0.00
5) Phenol-d5	6.81	99	258262	22.89	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.97	67	171599	24.49	ng/ul	0.00
9) 2-Chlorophenol-d4	7.16	132	222271	23.93	ng/ul	0.00
13) 4-Methylphenol-d8	8.33	113	208282	23.83	ng/ul	0.00
19) Nitrobenzene-d5	8.78	128	109166	24.09	ng/ul	0.00
22) 2-Nitrophenol-d4	9.49	143	125516	24.47	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.03	165	211906	22.89	ng/ul	0.00
29) 4-Chloroaniline-d4	10.54	131	257734	24.06	ng/ul	0.00
43) Dimethylphthalate-d6	13.67	166	703518	25.45	ng/ul	0.00
46) Acenaphthylene-d8	13.95	160	894807	24.79	ng/ul	0.00
51) 4-Nitrophenol-d4	14.50	143	71618	15.67	ng/ul	0.01
57) Fluorene-d10	15.26	176	632054	26.10	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.40	200	87904	17.49	ng/ul	0.00
70) Anthracene-d10	17.11	188	988030	25.75	ng/ul	0.00
78) Pyrene-d10	19.42	212	1087463	24.22	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.29	264	1016678	25.42	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.73	163	160422	5.945	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN100418\
Data File : BN002900.D
Acq On : 03 Oct 2018 14:53
Operator : MJ/SJ
Sample : J5116-02
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
JLC53

Quant Time: Oct 04 02:50:59 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN091418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 04 02:50:09 2018
Response via : Initial Calibration

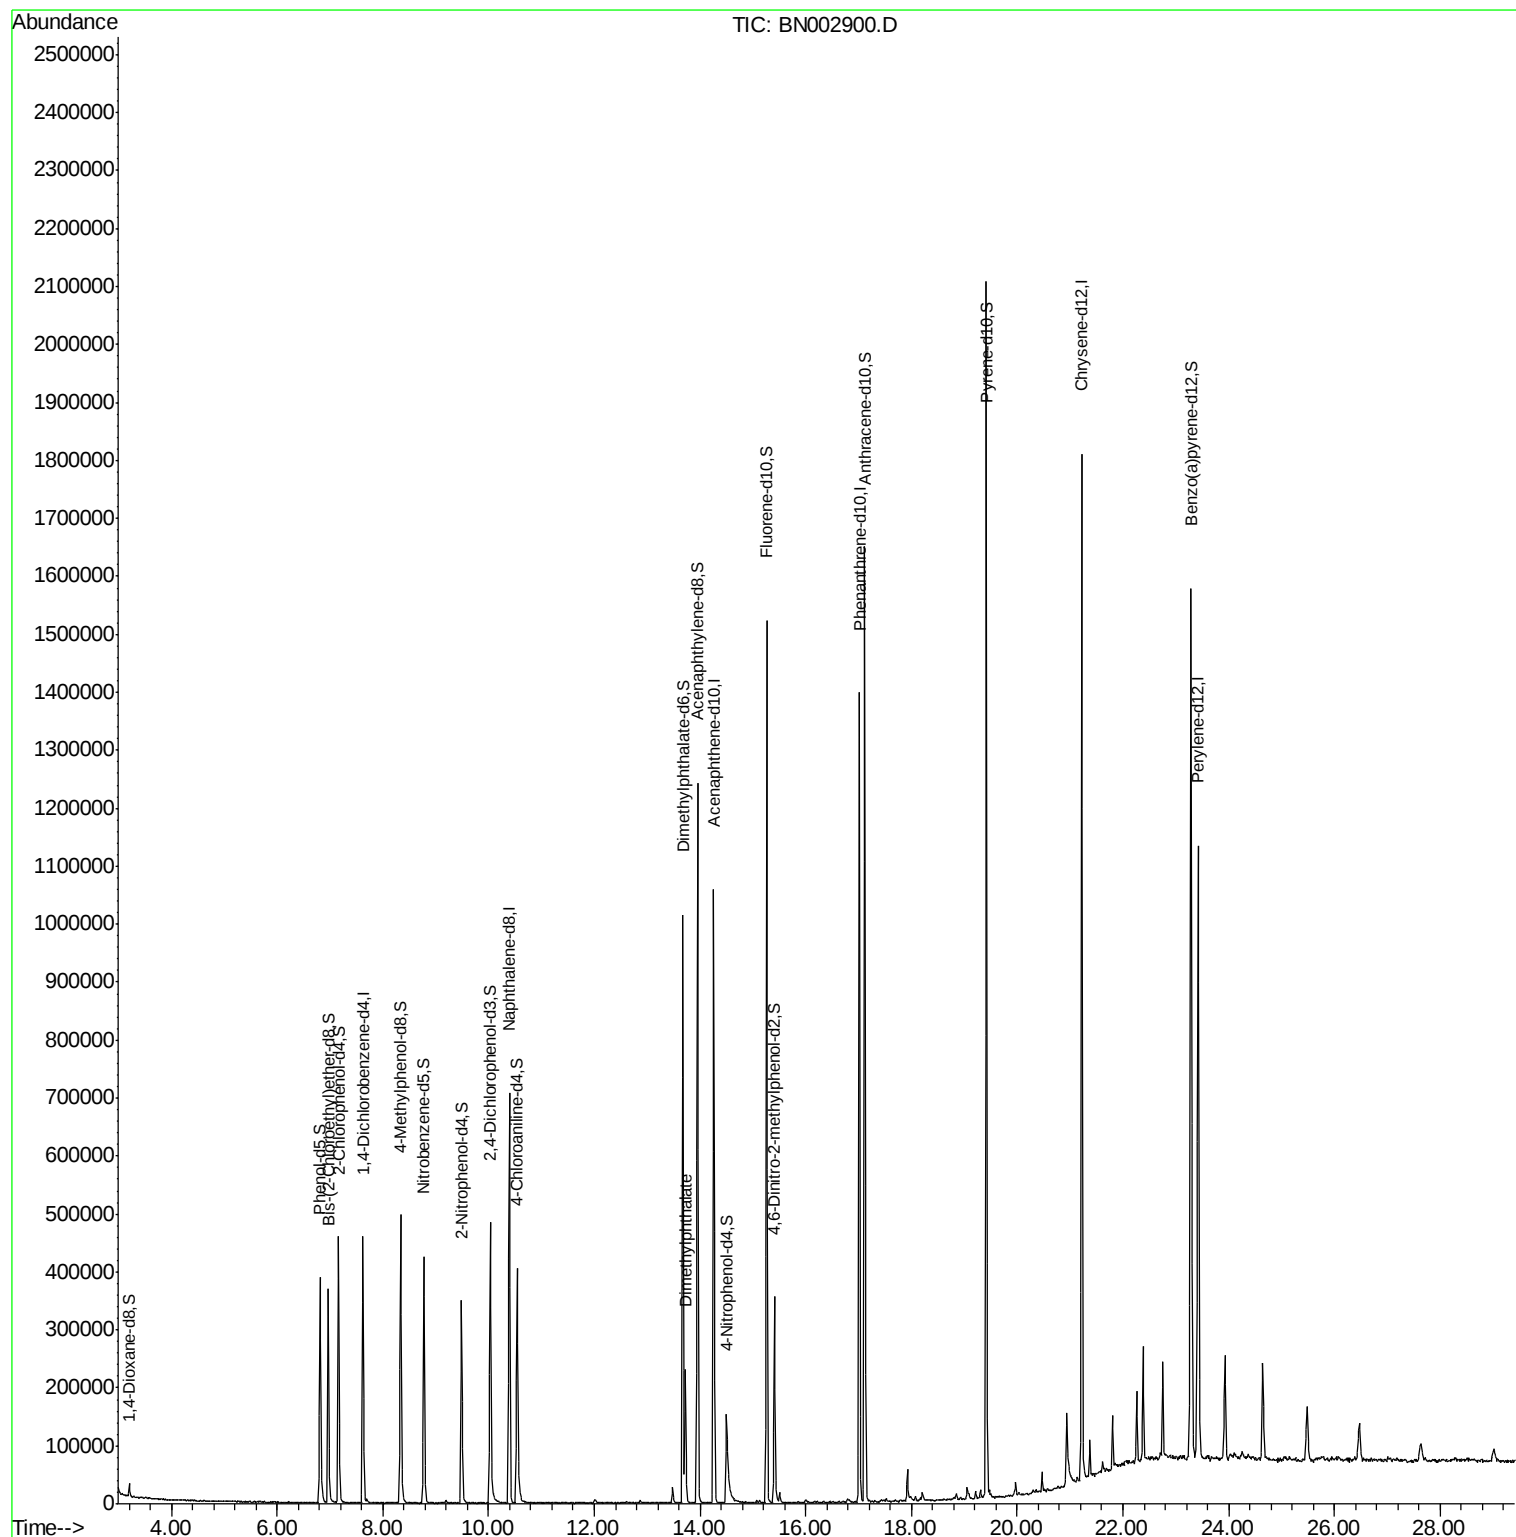

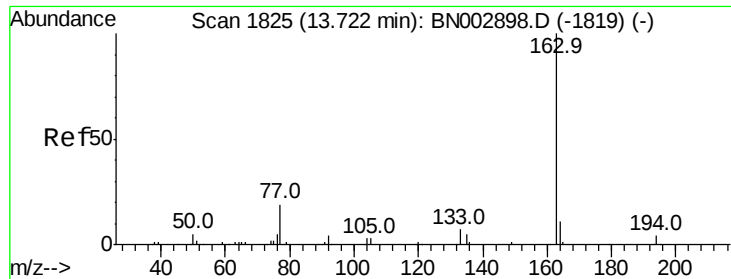

#44

Dimethylphthalate

Concen: 5.945 ng/ul

RT: 13.73 min Scan# 1826

Delta R.T. 0.01 min

Lab File: BN002900.D

Acq: 03 Oct 2018 14:53

Instrument :

BNA_N

ClientSampleId :

JLC53


Tot Ion:163 Resp: 160422

Ion Ratio Lower Upper

163 100

194 4.2 3.5 5.3

164 9.8 8.1 12.1

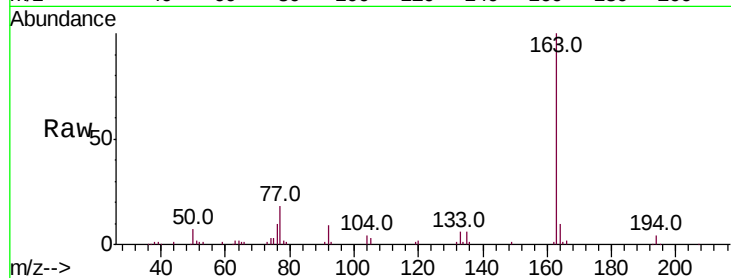

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

