

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN100418\
 Data File : BN002902.D
 Acq On : 03 Oct 2018 16:03
 Operator : MJ/SJ
 Sample : J5116-07
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JLC56

Quant Time: Oct 04 03:06:39 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN091418MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 04 02:50:09 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	91580	20.00	ng/ul	0.00
18) Naphthalene-d8	10.39	136	415264	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.26	164	249544	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.01	188	582148	20.00	ng/ul	0.00
77) Chrysene-d12	21.22	240	674497	20.00	ng/ul	0.00
85) Perylene-d12	23.43	264	662500	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.20	96	9926	5.00	ng/uL	0.00
5) Phenol-d5	6.82	99	222508	28.61	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.97	67	146105	30.25	ng/ul	0.00
9) 2-Chlorophenol-d4	7.16	132	187658	29.32	ng/ul	0.00
13) 4-Methylphenol-d8	8.33	113	183593	30.48	ng/ul	0.00
19) Nitrobenzene-d5	8.78	128	91311	28.39	ng/ul	0.00
22) 2-Nitrophenol-d4	9.49	143	105350	28.94	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.03	165	180976	27.54	ng/ul	0.00
29) 4-Chloroaniline-d4	10.54	131	251869	33.13	ng/ul	0.00
43) Dimethylphthalate-d6	13.67	166	618051	31.64	ng/ul	0.00
46) Acenaphthylene-d8	13.95	160	781449	30.64	ng/ul	0.00
51) 4-Nitrophenol-d4	14.52	143	44479	13.77	ng/ul	0.02
57) Fluorene-d10	15.26	176	562231	32.85	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.41	200	48728	13.38	ng/ul	0.00
70) Anthracene-d10	17.11	188	883045	31.77	ng/ul	0.00
78) Pyrene-d10	19.42	212	1031435	28.98	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.29	264	1125717	32.28	ng/ul	0.00

Target Compounds


					Ovalue
6) Phenol	6.85	94	12059	1.538 ng/ul	92
44) Dimethylphthalate	13.72	163	166320	8.724 ng/ul	99
69) Phenanthrene	17.06	178	40922	1.276 ng/ul	98
75) Di-n-butylphthalate	17.99	149	70835	2.115 ng/ul	99
76) Fluoranthene	19.09	202	87472	2.556 ng/ul	98
79) Pyrene	19.45	202	78403	1.758 ng/ul#	97
83) Bis(2-ethylhexyl)phthalate	21.14	149	27101	1.006 ng/ul#	99
84) Chrysene	21.26	228	52531	1.336 ng/ul	98
87) Benzo(b)fluoranthene	22.77	252	58204	1.439 ng/ul#	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN100418\
Data File : BN002902.D
Acq On : 03 Oct 2018 16:03
Operator : MJ/SJ
Sample : J5116-07
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
JLC56

Quant Time: Oct 04 03:06:39 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN091418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 04 02:50:09 2018
Response via : Initial Calibration

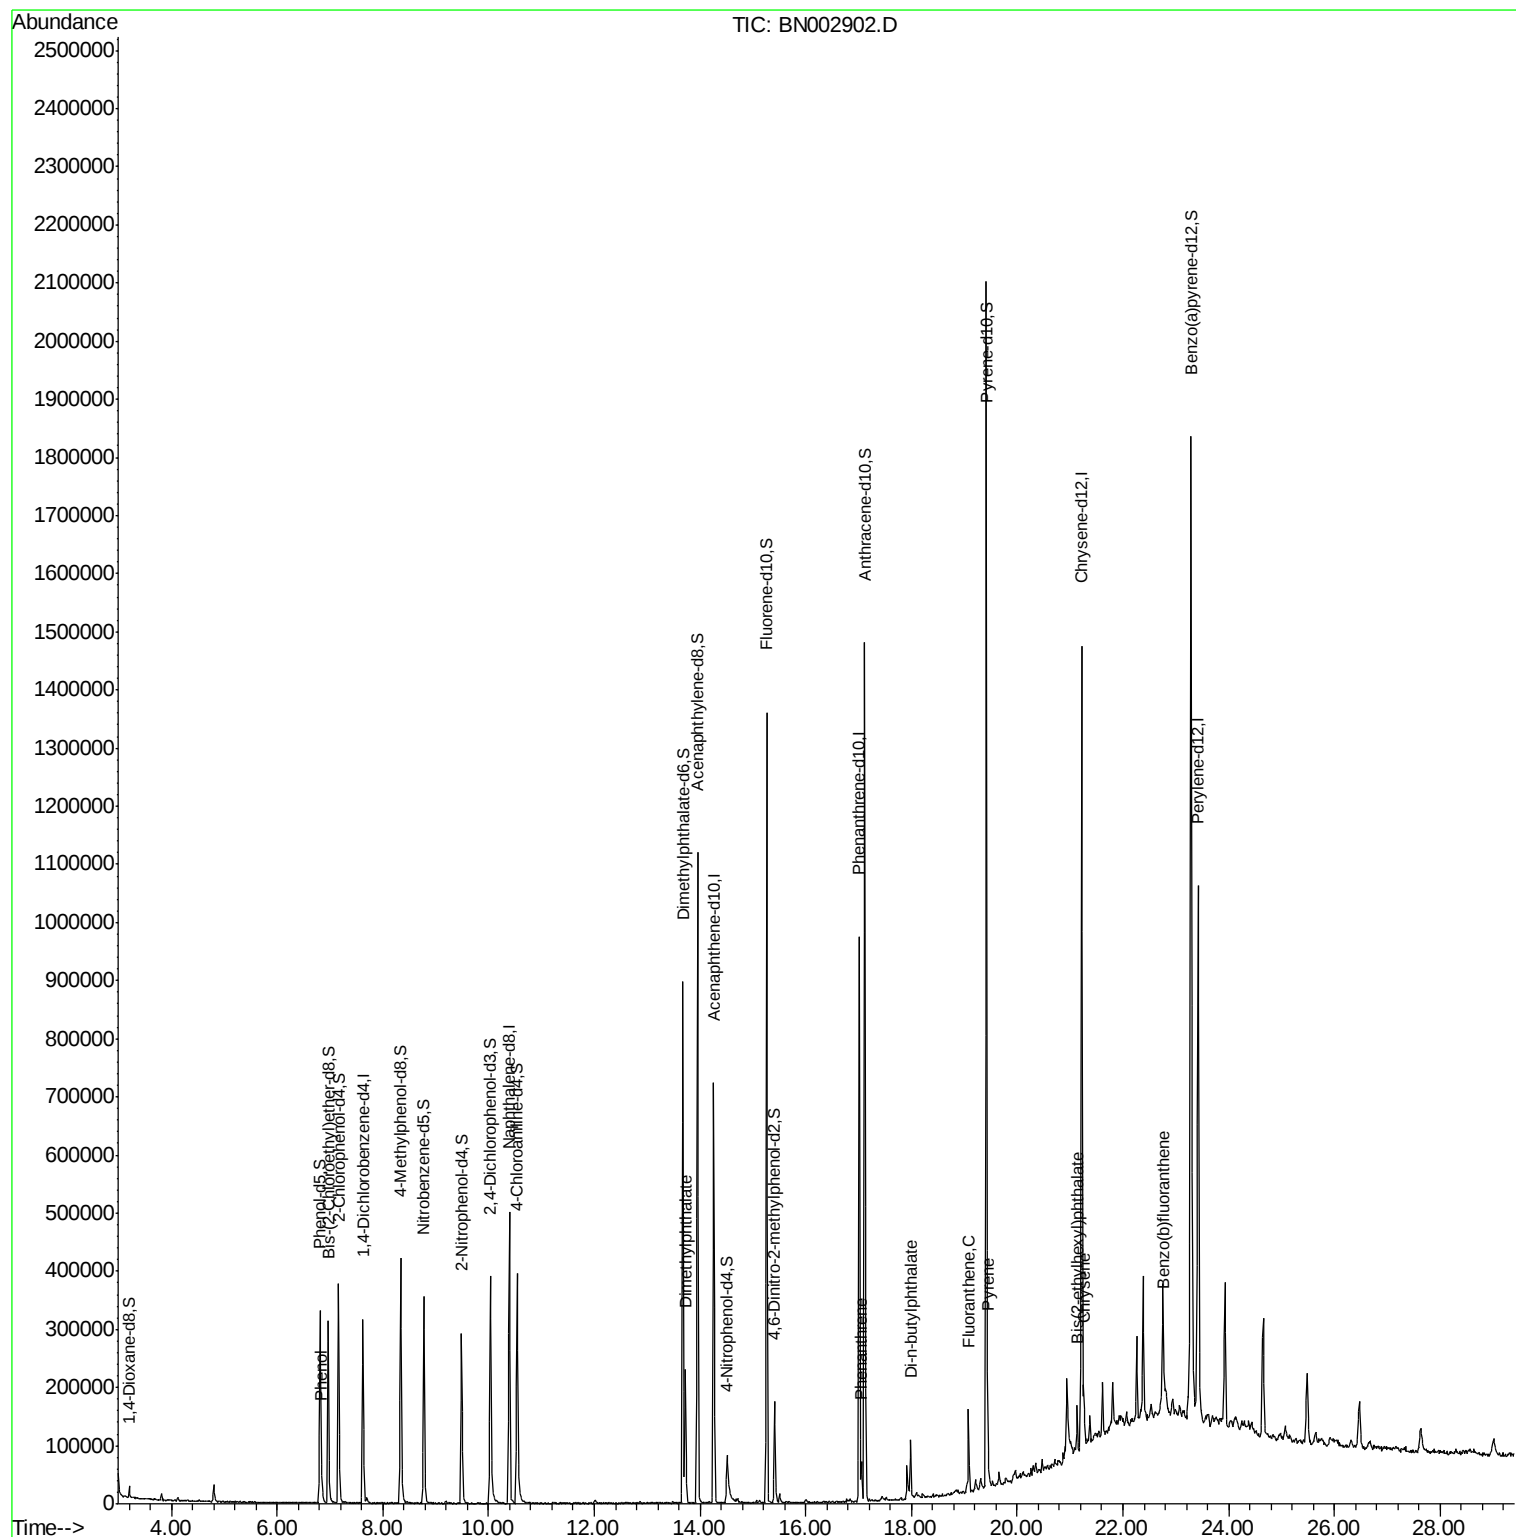

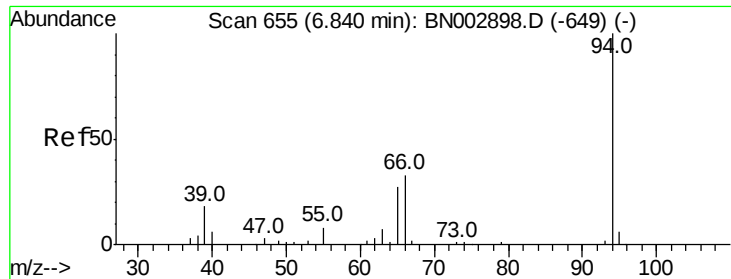





#6

Phenol

Concen: 1.538 ng/ul
 RT: 6.85 min Scan# 656
 Delta R.T. 0.01 min
 Lab File: BN002902.D
 Acq: 03 Oct 2018 16:03

Instrument :
 BNA_N
 ClientSampleId :
 JLC56

Tot Ion	Ratio	Lower	Upper
94	100		
65	29.9	23.1	34.7
66	44.4	29.8	44.6

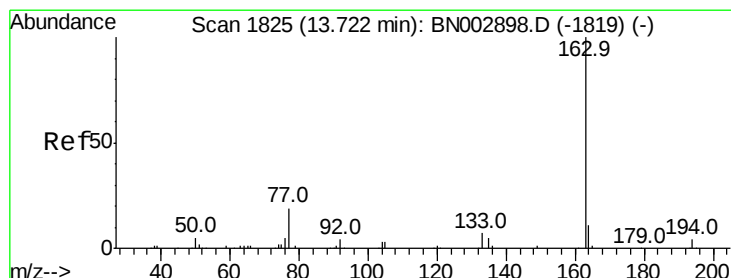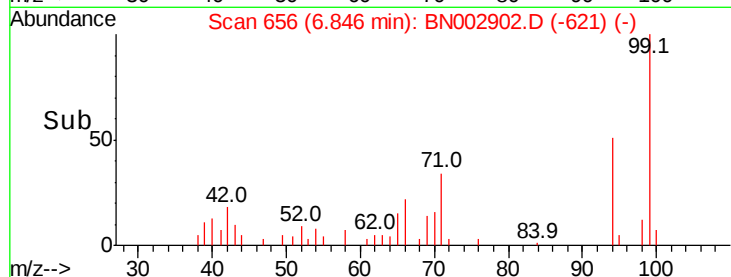
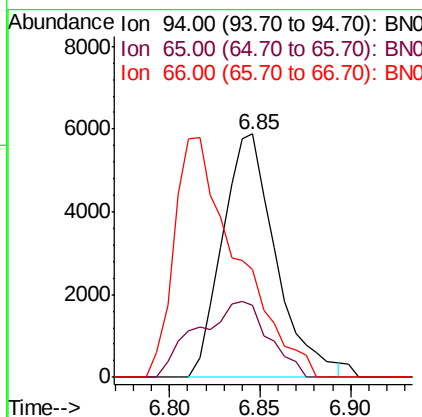
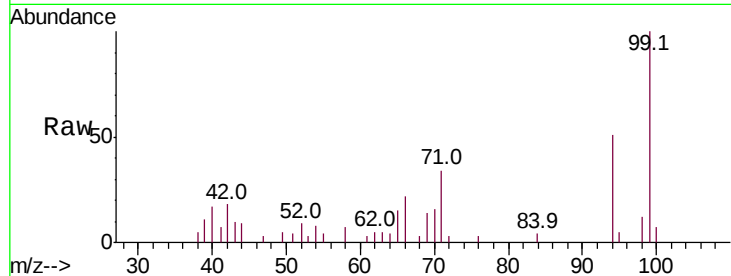



#44

Dimethylphthalate

Concen: 8.724 ng/ul
 RT: 13.72 min Scan# 1825
 Delta R.T. 0.00 min
 Lab File: BN002902.D
 Acq: 03 Oct 2018 16:03

Tgt Ion	Ratio	Lower	Upper
163	100		
194	4.2	3.5	5.3
164	9.9	8.1	12.1

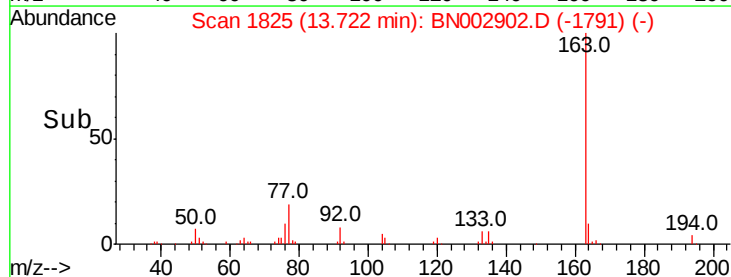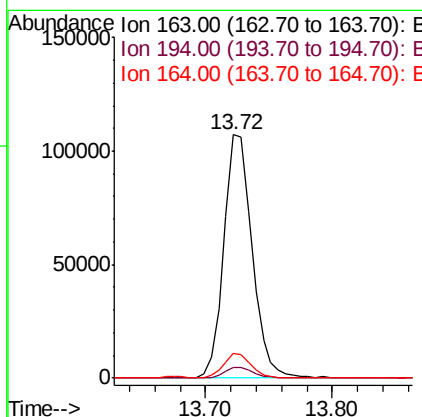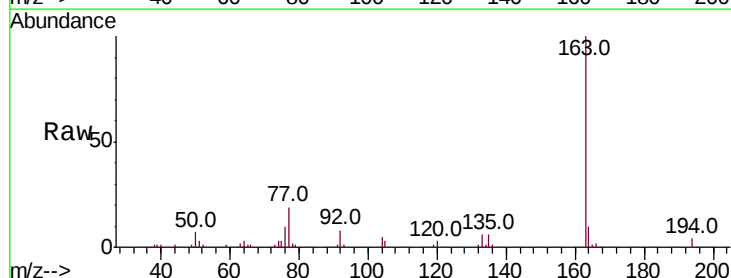

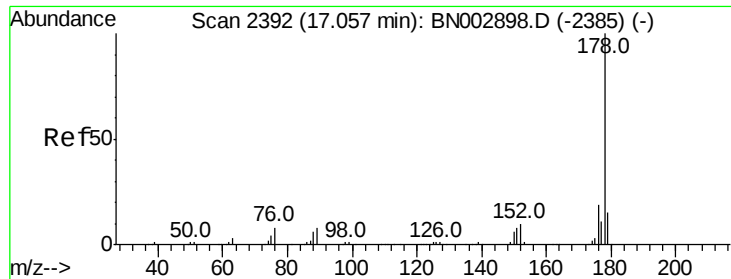

#69

Phenanthrene

Concen: 1.276 ng/ul

RT: 17.06 min Scan# 2392

Delta R.T. 0.00 min

Lab File: BN002902.D

Acq: 03 Oct 2018 16:03

Instrument :

BNA_N

ClientSampleId :

JLC56


Tot Ion:178 Resp: 40922

Ion Ratio Lower Upper

178 100

179 14.3 12.2 18.4




176 19.3 15.0 22.6

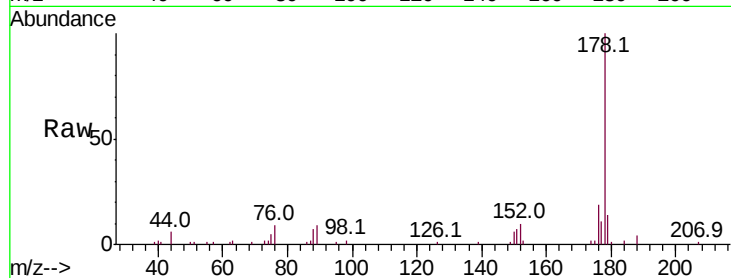

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

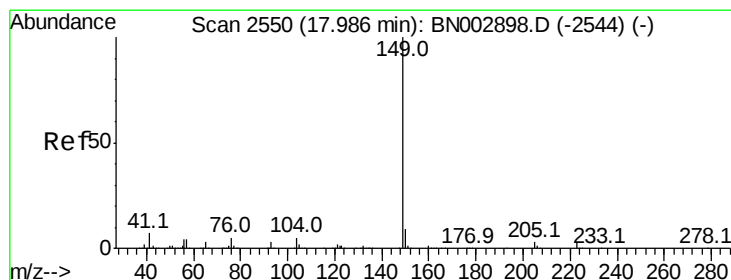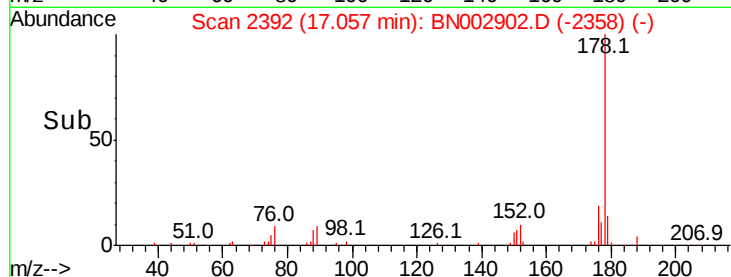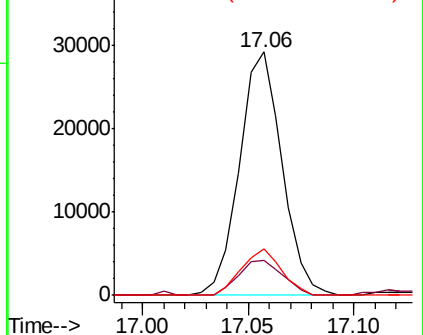

#75

Di-n-butylphthalate

Concen: 2.115 ng/ul

RT: 17.99 min Scan# 2550

Delta R.T. 0.00 min

Lab File: BN002902.D

Acq: 03 Oct 2018 16:03


Tgt Ion:149 Resp: 70835

Ion Ratio Lower Upper

149 100

150 9.2 7.3 10.9



104 5.0 3.7 5.5

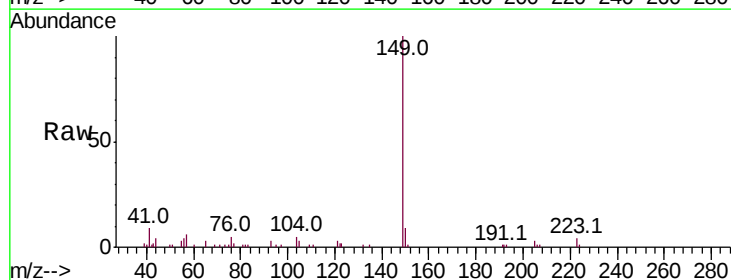


Abundance Ion 149.00 (148.70 to 149.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 104.00 (103.70 to 104.70): E



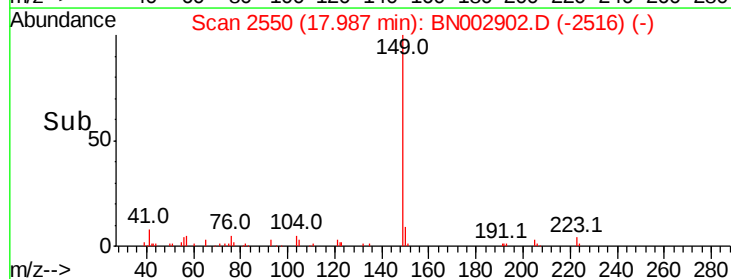
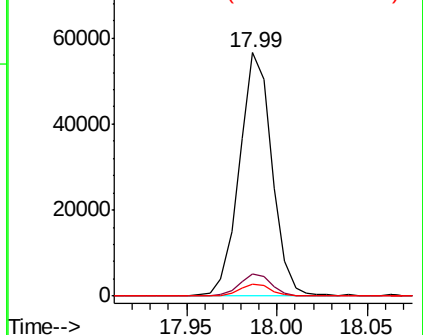


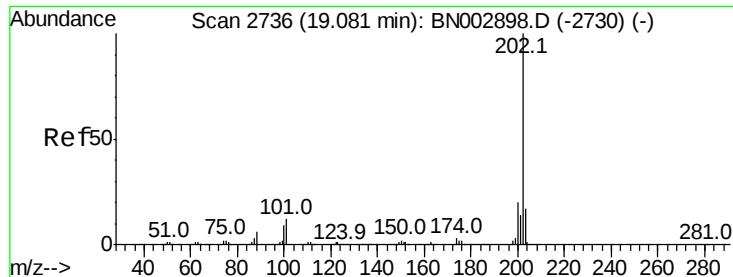

#76
Fluoranthene
Concen: 2.556 ng/ul
RT: 19.09 min Scan# 2737
Delta R.T. 0.01 min
Lab File: BN002902.D
Acq: 03 Oct 2018 16:03




Instrument :
BNA_N
ClientSampleId :
JLC56


Tot Ion	Ratio	Lower	Upper
202	100		
101	11.0	9.4	14.2
100	9.8	7.0	10.6

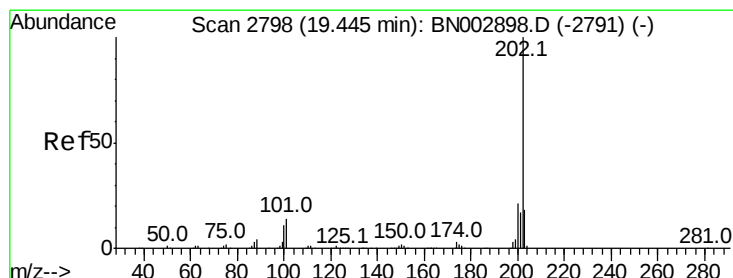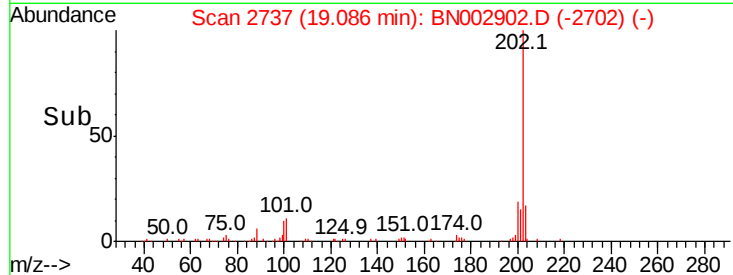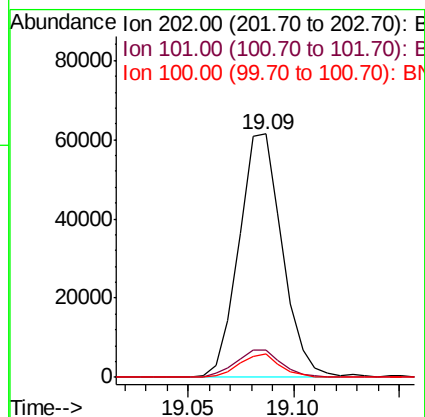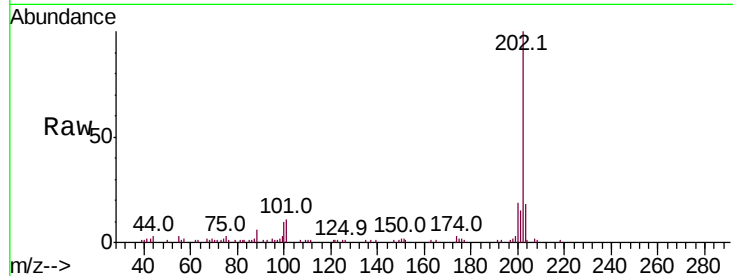

#79
Pyrene
Concen: 1.758 ng/ul
RT: 19.45 min Scan# 2798
Delta R.T. 0.00 min
Lab File: BN002902.D
Acq: 03 Oct 2018 16:03

Tgt Ion	Ratio	Lower	Upper
202	100		
101	12.9	10.8	16.2
100	12.3	8.2	12.2#

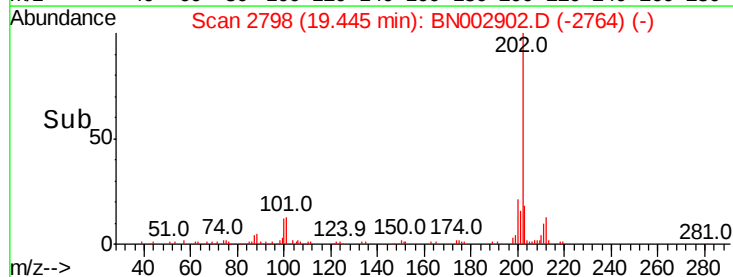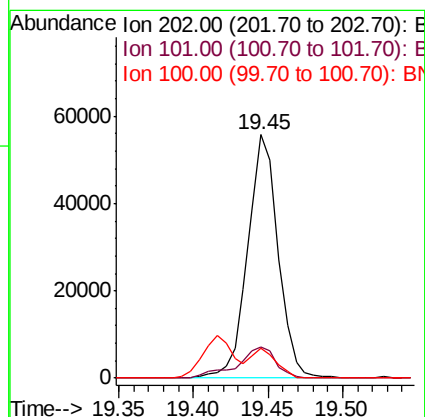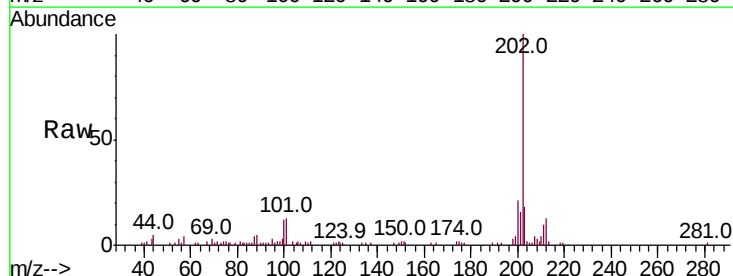


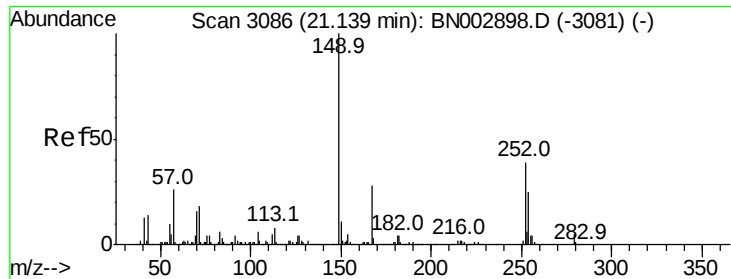




#83
 Bis(2-ethylhexyl)phthalate
 Concen: 1.006 ng/ul
 RT: 21.14 min Scan# 3086
 Delta R.T. 0.00 min
 Lab File: BN002902.D
 Acq: 03 Oct 2018 16:03

Instrument :
 BNA_N
 ClientSampleId :
 JLC56

Tot Ion:149 Resp: 27101
 Ion Ratio Lower Upper
 149 100
 167 27.1 22.0 33.0
 279 5.2 3.3 4.9#

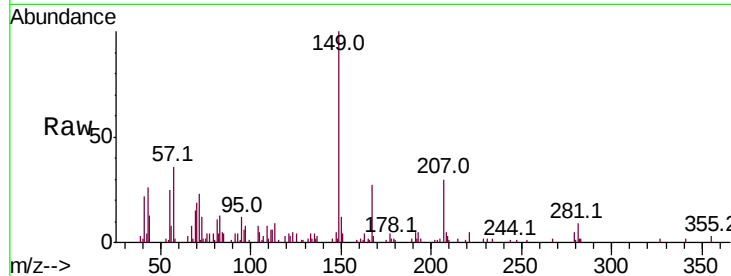


Abundance Ion 149.00 (148.70 to 149.70): E
 Ion 167.00 (166.70 to 167.70): E
 Ion 279.00 (278.70 to 279.70): E

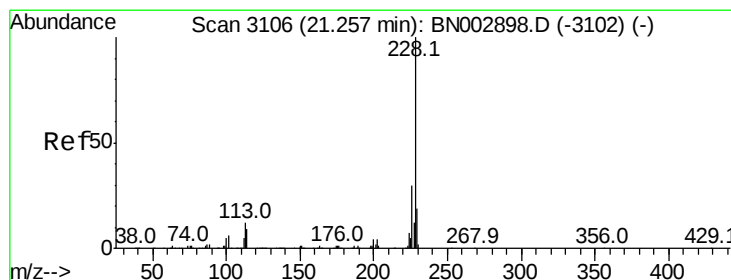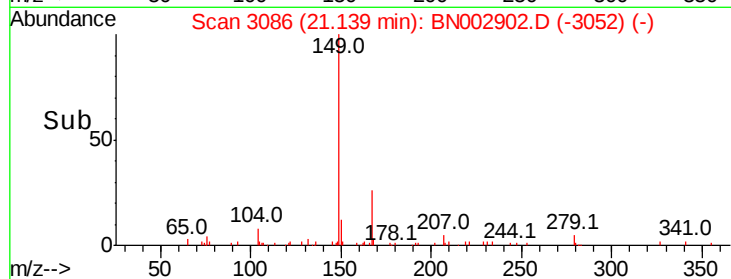
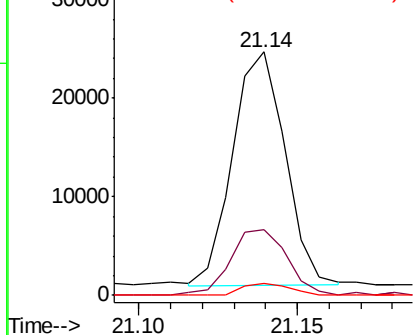



#84
 Chrysene
 Concen: 1.336 ng/ul
 RT: 21.26 min Scan# 3106
 Delta R.T. 0.00 min
 Lab File: BN002902.D
 Acq: 03 Oct 2018 16:03

Tgt Ion:228 Resp: 52531
 Ion Ratio Lower Upper
 228 100
 226 31.0 23.4 35.0
 229 19.9 15.7 23.5

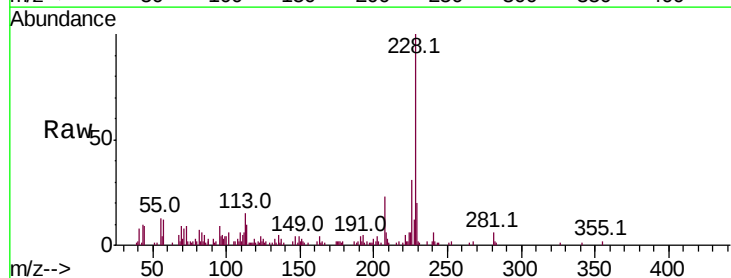

Abundance Ion 228.00 (227.70 to 228.70): E
 Ion 226.00 (225.70 to 226.70): E
 Ion 229.00 (228.70 to 229.70): E

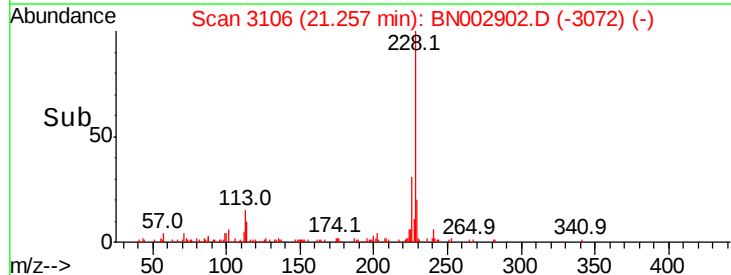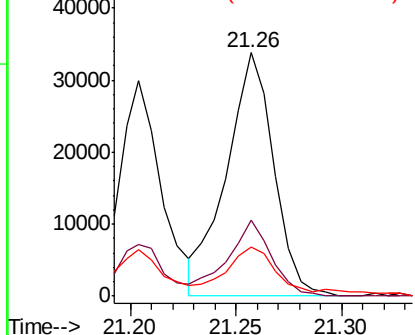

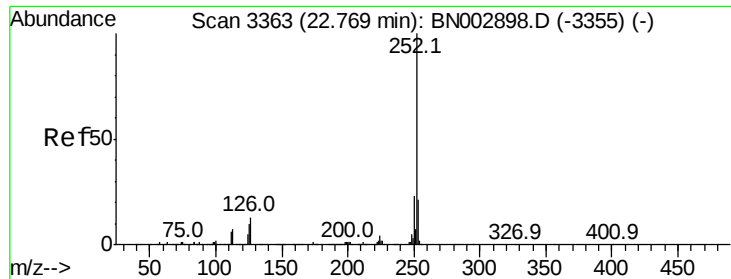

#87

Benzo(b)fluoranthene

Concen: 1.439 ng/ul

RT: 22.77 min Scan# 3364

Delta R.T. 0.01 min

Lab File: BN002902.D

Acq: 03 Oct 2018 16:03

Instrument :

BNA_N

ClientSampleId :

JLC56


Tot Ion:252 Resp: 58204

Ion Ratio Lower Upper

252 100

253 20.3 17.0 25.4

125 15.2 8.0 12.0#

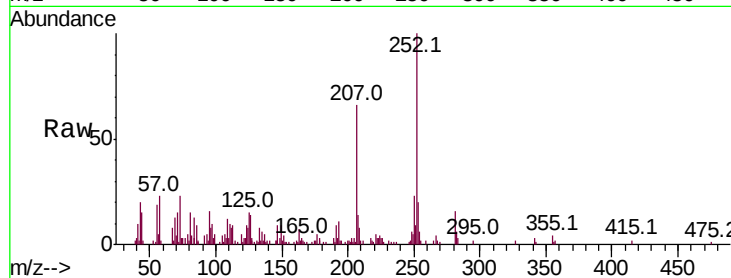

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

