

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN100418\
 Data File : BN002910.D
 Acq On : 03 Oct 2018 20:50
 Operator : MJ/SJ
 Sample : J5115-17
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JLC60

Quant Time: Oct 04 02:52:24 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN091418MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 04 02:50:09 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	115906	20.00	ng/ul	0.00
18) Naphthalene-d8	10.39	136	530927	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.26	164	322001	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.02	188	726814	20.00	ng/ul	0.00
77) Chrysene-d12	21.22	240	789246	20.00	ng/ul	0.00
85) Perylene-d12	23.42	264	729637	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.20	96	7886	3.14	ng/uL	0.00
5) Phenol-d5	6.82	99	193977	19.71	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.97	67	122506	20.04	ng/ul	0.00
9) 2-Chlorophenol-d4	7.16	132	161122	19.89	ng/ul	0.00
13) 4-Methylphenol-d8	8.33	113	155291	20.37	ng/ul	0.00
19) Nitrobenzene-d5	8.78	128	78617	19.12	ng/ul	0.00
22) 2-Nitrophenol-d4	9.49	143	92506	19.88	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.03	165	153540	18.28	ng/ul	0.00
29) 4-Chloroaniline-d4	10.54	131	209854	21.59	ng/ul	0.00
43) Dimethylphthalate-d6	13.67	166	538290	21.36	ng/ul	0.00
46) Acenaphthylene-d8	13.95	160	692779	21.05	ng/ul	0.00
51) 4-Nitrophenol-d4	14.50	143	64492	15.47	ng/ul	0.01
57) Fluorene-d10	15.26	176	501892	22.73	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.40	200	77723	17.10	ng/ul	0.00
70) Anthracene-d10	17.12	188	775457	22.35	ng/ul	0.00
78) Pyrene-d10	19.42	212	878134	21.08	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.29	264	876444	22.82	ng/ul	0.00


Target Compounds					Ovalue	
6) Phenol	6.84	94	19337	1.948	ng/ul	93
44) Dimethylphthalate	13.72	163	129045	5.246	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN100418\
Data File : BN002910.D
Acq On : 03 Oct 2018 20:50
Operator : MJ/SJ
Sample : J5115-17
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
JLC60

Quant Time: Oct 04 02:52:24 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN091418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 04 02:50:09 2018
Response via : Initial Calibration

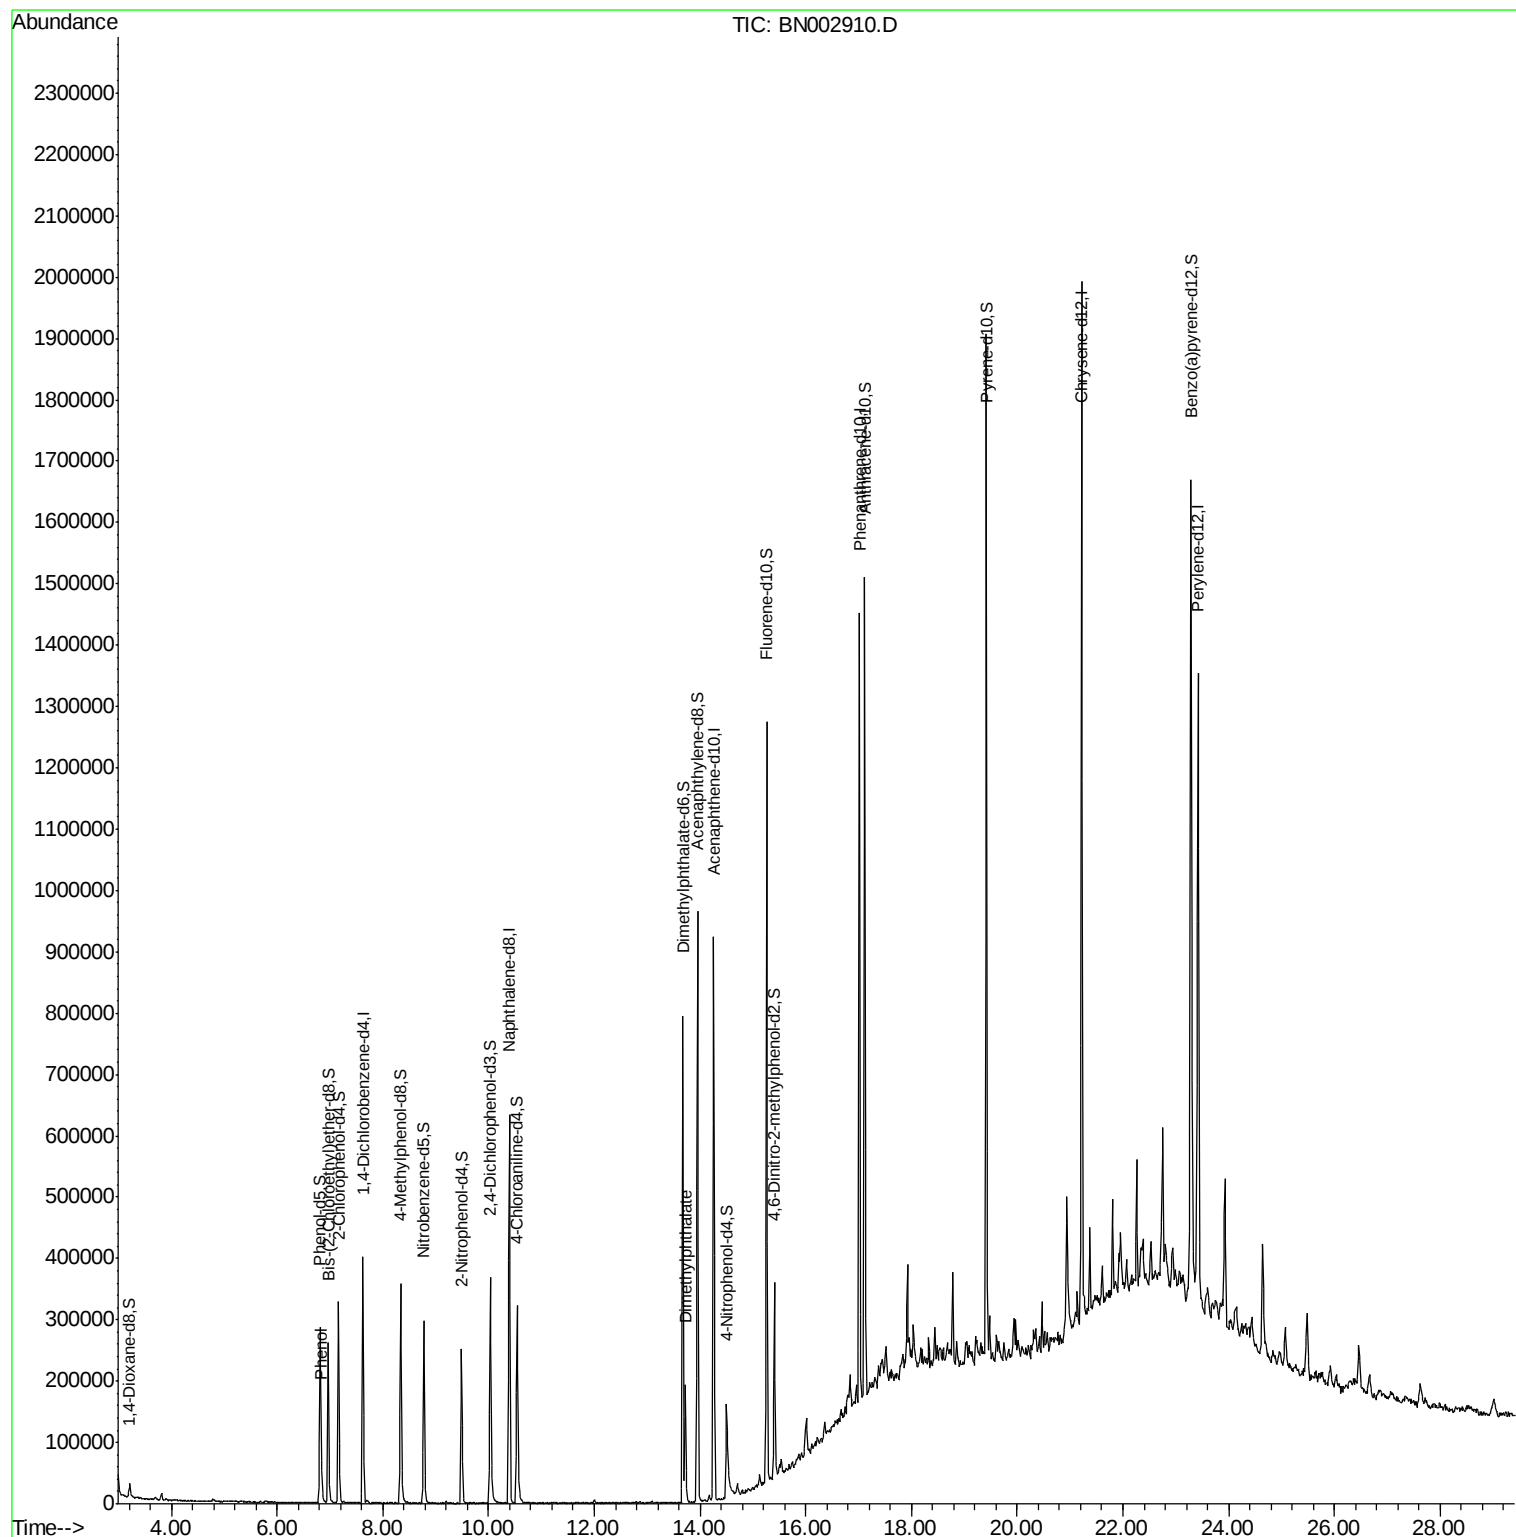

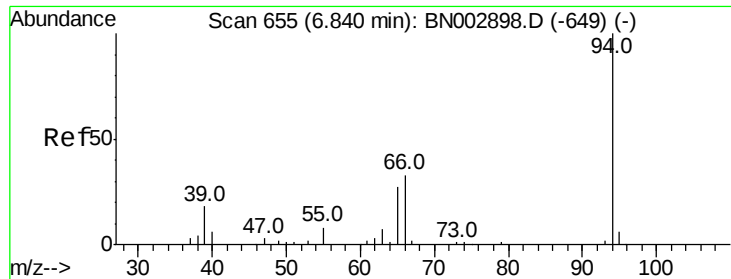

#6

Phenol

Concen: 1.948 ng/ul

RT: 6.84 min Scan# 655

Delta R.T. 0.00 min

Lab File: BN002910.D

Acq: 03 Oct 2018 20:50

Instrument :

BNA_N

ClientSampleId :

JLC60


Tot Ion: 94 Resp: 19337

Ion Ratio Lower Upper

94 100

65 28.0 23.1 34.7




66 44.2 29.8 44.6

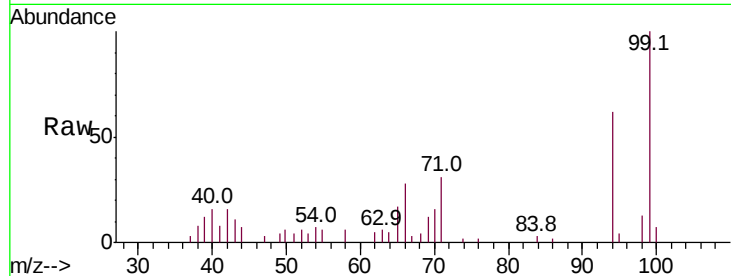

Abundance Ion 94.00 (93.70 to 94.70): BN002898.D (-649) (-)

Ion 65.00 (64.70 to 65.70): BN002898.D (-649) (-)

Ion 66.00 (65.70 to 66.70): BN002898.D (-649) (-)

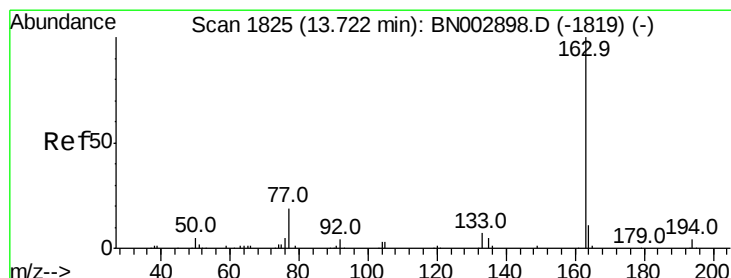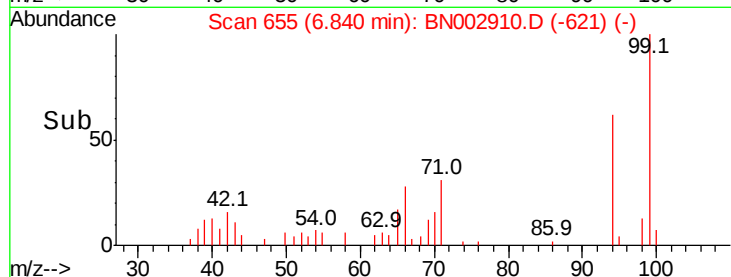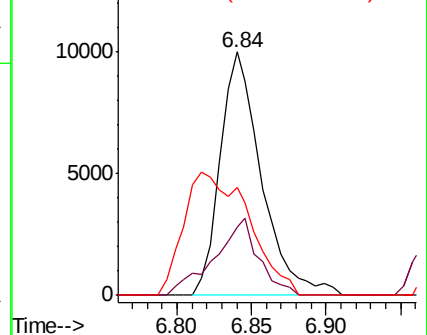

#44

Dimethylphthalate

Concen: 5.246 ng/ul

RT: 13.72 min Scan# 1825

Delta R.T. 0.00 min

Lab File: BN002910.D

Acq: 03 Oct 2018 20:50


Tgt Ion:163 Resp: 129045

Ion Ratio Lower Upper

163 100

194 4.6 3.5 5.3

164 11.0 8.1 12.1

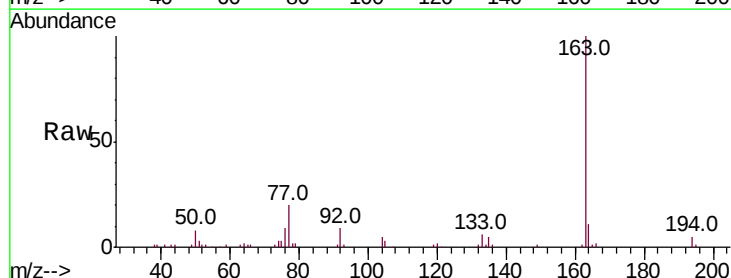

Abundance Ion 163.00 (162.70 to 163.70): BN002898.D (-1819) (-)

Ion 194.00 (193.70 to 194.70): BN002898.D (-1819) (-)

Ion 164.00 (163.70 to 164.70): BN002898.D (-1819) (-)

