

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN100418\
 Data File : BN002912.D
 Acq On : 03 Oct 2018 21:59
 Operator : MJ/SJ
 Sample : J5115-12
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JLC43

Quant Time: Oct 04 02:52:39 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN091418MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 04 02:50:09 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	115396	20.00	ng/ul	0.00
18) Naphthalene-d8	10.39	136	521758	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.26	164	313577	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.02	188	729103	20.00	ng/ul	0.00
77) Chrysene-d12	21.22	240	798141	20.00	ng/ul	0.00
85) Perylene-d12	23.43	264	708172	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.20	96	7420	2.97	ng/uL	0.00
5) Phenol-d5	6.81	99	184247	18.80	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.97	67	117800	19.36	ng/ul	0.00
9) 2-Chlorophenol-d4	7.16	132	157137	19.48	ng/ul	0.00
13) 4-Methylphenol-d8	8.33	113	144041	18.98	ng/ul	0.00
19) Nitrobenzene-d5	8.78	128	77859	19.26	ng/ul	0.00
22) 2-Nitrophenol-d4	9.49	143	90402	19.76	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.03	165	152156	18.43	ng/ul	0.00
29) 4-Chloroaniline-d4	10.54	131	191299	20.03	ng/ul	0.00
43) Dimethylphthalate-d6	13.67	166	501058	20.41	ng/ul	0.00
46) Acenaphthylene-d8	13.95	160	646130	20.16	ng/ul	0.00
51) 4-Nitrophenol-d4	14.50	143	65048	16.03	ng/ul	0.01
57) Fluorene-d10	15.26	176	458500	21.32	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.40	200	68480	15.02	ng/ul	0.00
70) Anthracene-d10	17.11	188	716469	20.58	ng/ul	0.00
78) Pyrene-d10	19.42	212	836269	19.86	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.29	264	780929	20.95	ng/ul	0.00

Target Compounds


					Ovalue
6) Phenol	6.85	94	11057	1.119 ng/ul	92
44) Dimethylphthalate	13.72	163	149783	6.252 ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN100418\
Data File : BN002912.D
Acq On : 03 Oct 2018 21:59
Operator : MJ/SJ
Sample : J5115-12
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
JLC43

Quant Time: Oct 04 02:52:39 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN091418MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 04 02:50:09 2018
Response via : Initial Calibration

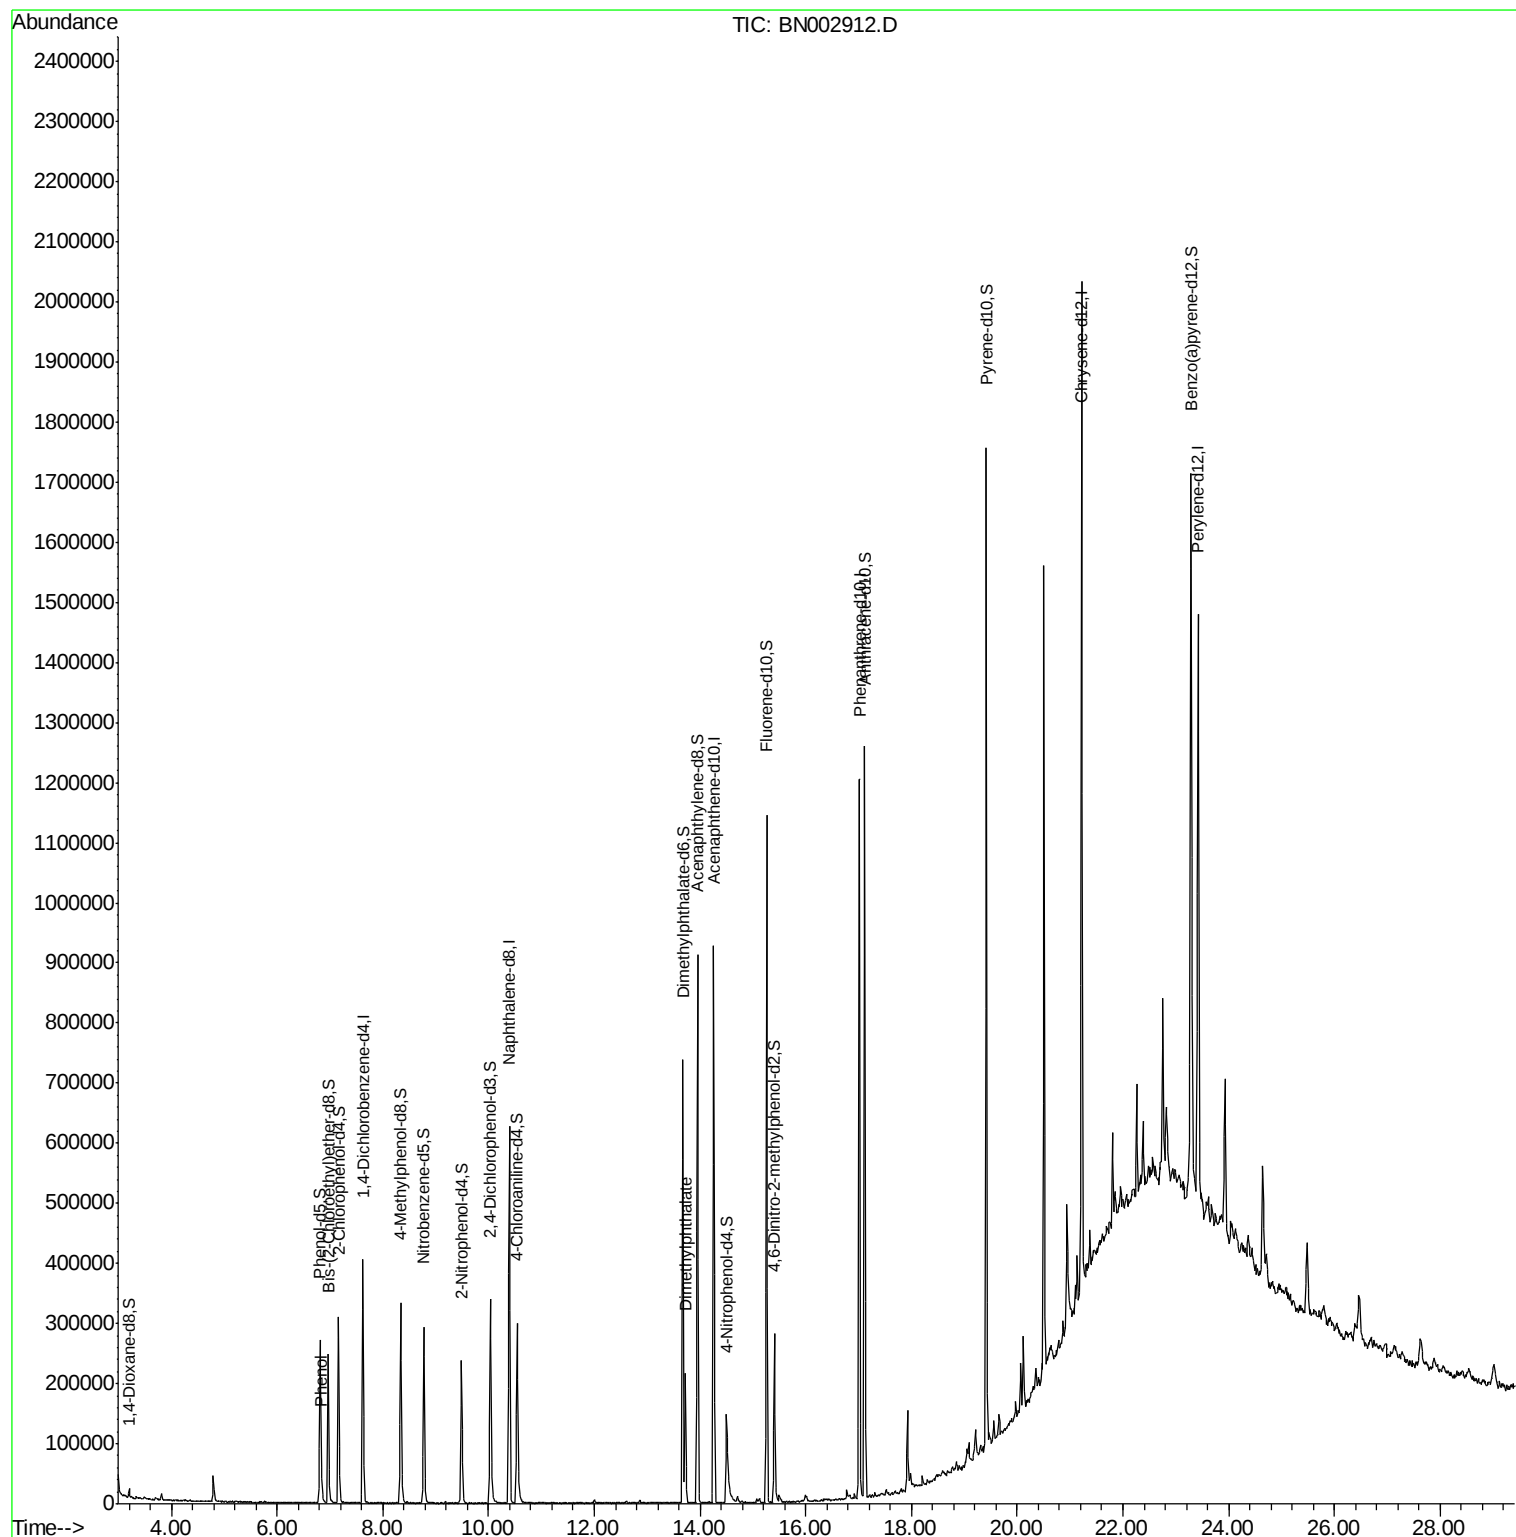

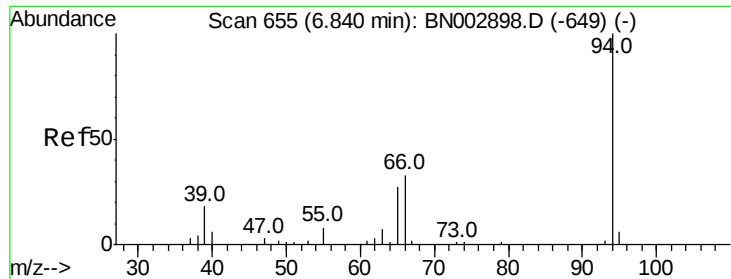





#6

Phenol

Concen: 1.119 ng/ul
 RT: 6.85 min Scan# 656
 Delta R.T. 0.01 min
 Lab File: BN002912.D
 Acq: 03 Oct 2018 21:59

Instrument :
 BNA_N
 ClientSampleId :
 JLC43

Tot Ion: 94 Resp: 11057
 Ion Ratio Lower Upper
 94 100
 65 24.2 23.1 34.7
 66 42.1 29.8 44.6

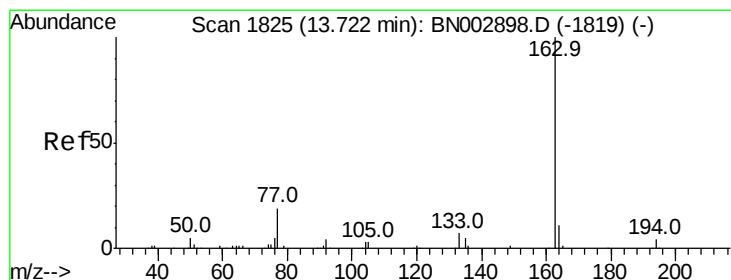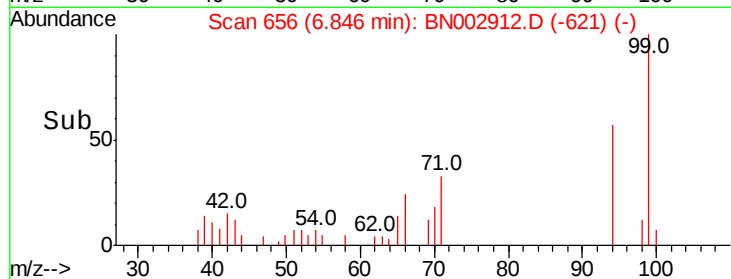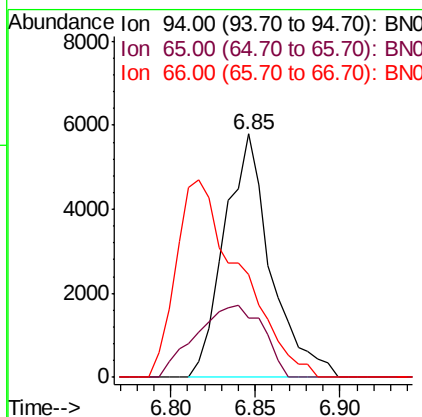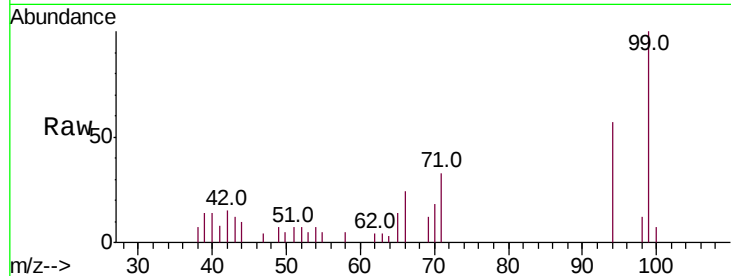

#44

Dimethylphthalate

Concen: 6.252 ng/ul
 RT: 13.72 min Scan# 1825
 Delta R.T. 0.00 min
 Lab File: BN002912.D
 Acq: 03 Oct 2018 21:59

Tgt Ion:163 Resp: 149783
 Ion Ratio Lower Upper
 163 100
 194 4.5 3.5 5.3
 164 9.1 8.1 12.1

