

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100421\
 Data File : BN016725.D
 Acq On : 05 Oct 2021 01:37
 Operator : CG/JU
 Sample : SSTDCCC0.4
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4

Quant Time: Oct 05 03:35:26 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN100421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 04 17:52:33 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.642	152	26590	0.400	ng	0.00
7) Naphthalene-d8	10.406	136	117422	0.400	ng	0.00
13) Acenaphthene-d10	14.268	164	61432	0.400	ng	0.00
19) Phenanthrene-d10	17.029	188	113524	0.400	ng	0.00
29) Chrysene-d12	21.238	240	112908	0.400	ng	# 0.00
35) Perylene-d12	23.488	264	118004	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.254	112	25357	0.374	ng	0.00
5) Phenol-d6	6.821	99	27864	0.370	ng	0.00
8) Nitrobenzene-d5	8.784	82	27155	0.330	ng	0.00
11) 2-Methylnaphthalene-d10	12.007	152	65660	0.375	ng	0.00
14) 2,4,6-Tribromophenol	15.778	330	9370	0.382	ng	0.00
15) 2-Fluorobiphenyl	12.898	172	92451	0.376	ng	0.00
27) Fluoranthene-d10	19.068	212	114281	0.368	ng	0.00
31) Terphenyl-d14	19.678	244	98435	0.390	ng	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.253	88	4657	0.375	ng	# 73
3) n-Nitrosodimethylamine	3.576	42	7357	0.367	ng	99
6) bis(2-Chloroethyl)ether	7.080	93	28258	0.391	ng	100
9) Naphthalene	10.457	128	120496	0.375	ng	100
10) Hexachlorobutadiene	10.748	225	22728	0.378	ng	# 100
12) 2-Methylnaphthalene	12.078	142	78054	0.382	ng	100
16) Acenaphthylene	13.989	152	96947	0.357	ng	100
17) Acenaphthene	14.332	154	66949	0.374	ng	99
18) Fluorene	15.321	166	81550	0.377	ng	100
20) 4,6-Dinitro-2-methylph...	15.410	198	2495	0.523	ng	# 72
21) 4-Bromophenyl-phenylether	16.226	248	25943	0.375	ng	96
22) Hexachlorobenzene	16.336	284	30394	0.388	ng	100
23) Atrazine	16.506	200	17421	0.318	ng	99
24) Pentachlorophenol	16.689	266	8090	0.551	ng	99
25) Phenanthrene	17.066	178	129178	0.387	ng	100
26) Anthracene	17.163	178	106644	0.358	ng	100
28) Fluoranthene	19.097	202	142900	0.386	ng	100
30) Pyrene	19.465	202	142536	0.384	ng	100
32) Benzo(a)anthracene	21.216	228	133072	0.380	ng	99
33) Chrysene	21.270	228	142906	0.402	ng	99
34) Bis(2-ethylhexyl)phtha...	21.174	149	54319	0.256	ng	99
36) Indeno(1,2,3-cd)pyrene	25.774	276	168955	0.451	ng	99
37) Benzo(b)fluoranthene	22.810	252	146373	0.384	ng	100
38) Benzo(k)fluoranthene	22.854	252	148545	0.405	ng	98
39) Benzo(a)pyrene	23.388	252	132712	0.389	ng	99
40) Dibenzo(a,h)anthracene	25.795	278	134978	0.454	ng	99
41) Benzo(g,h,i)perylene	26.469	276	147637	0.444	ng	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100421\
Data File : BN016725.D
Acq On : 05 Oct 2021 01:37
Operator : CG/JU
Sample : SSTDCCC0.4
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Quant Time: Oct 05 03:35:26 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN100421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 04 17:52:33 2021
Response via : Initial Calibration









#1
1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.642 min Scan# 495
Delta R.T. 0.000 min
Lab File: BN016725.D
Acq: 05 Oct 2021 01:37




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:152 Resp: 26590
Ion Ratio Lower Upper
152 100
150 155.1 123.3 184.9
115 58.0 47.0 70.6



#2
1,4-Dioxane
Concen: 0.375 ng
RT: 3.253 min Scan# 19
Delta R.T. -0.000 min
Lab File: BN016725.D
Acq: 05 Oct 2021 01:37

Tgt Ion: 88 Resp: 4657
Ion Ratio Lower Upper
88 100
43 31.1 61.7 92.5#
58 78.1 62.2 93.2







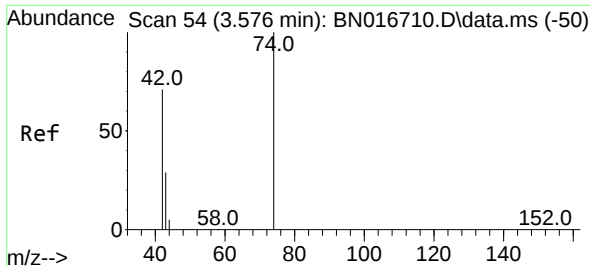

#3
n-Nitrosodimethylamine
Concen: 0.367 ng
RT: 3.576 min Scan# 54
Delta R.T. 0.000 min
Lab File: BN016725.D
Acq: 05 Oct 2021 01:37




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion: 42 Resp: 7357
Ion Ratio Lower Upper
42 100
74 153.8 124.0 186.0
44 6.9 5.6 8.4

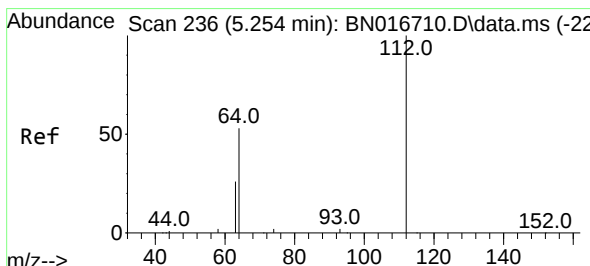

#4
2-Fluorophenol
Concen: 0.374 ng
RT: 5.254 min Scan# 236
Delta R.T. -0.000 min
Lab File: BN016725.D
Acq: 05 Oct 2021 01:37

Tgt Ion: 112 Resp: 25357
Ion Ratio Lower Upper
112 100
64 53.3 42.9 64.3
63 26.9 21.5 32.3







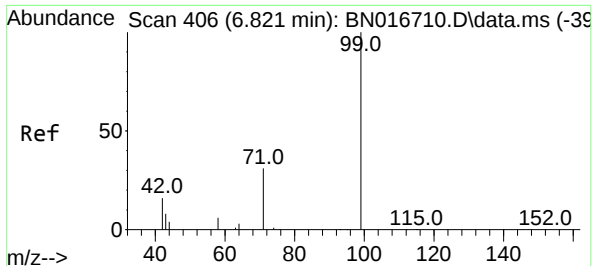

#5
Phenol-d6
Concen: 0.370 ng
RT: 6.821 min Scan# 406
Delta R.T. 0.000 min
Lab File: BN016725.D
Acq: 05 Oct 2021 01:37




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion: 99 Resp: 27864
Ion Ratio Lower Upper
99 100
42 16.7 13.4 20.2
71 29.9 24.0 36.0



#6
bis(2-Chloroethyl)ether
Concen: 0.391 ng
RT: 7.080 min Scan# 434
Delta R.T. 0.000 min
Lab File: BN016725.D
Acq: 05 Oct 2021 01:37

Tgt Ion: 93 Resp: 28258
Ion Ratio Lower Upper
93 100
63 73.2 59.0 88.6
95 33.0 26.4 39.6









#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.406 min Scan# 733
Delta R.T. 0.000 min
Lab File: BN016725.D
Acq: 05 Oct 2021 01:37




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:	136	Resp:	117422
Ion Ratio	Lower	Upper	
136	100		
137	11.0	8.9	13.3
54	6.8	6.5	9.7
68	5.8	5.3	7.9



#8
Nitrobenzene-d5
Concen: 0.330 ng
RT: 8.784 min Scan# 605
Delta R.T. 0.000 min
Lab File: BN016725.D
Acq: 05 Oct 2021 01:37

Tgt Ion:	82	Resp:	27155
Ion Ratio	Lower	Upper	
82	100		
128	44.0	33.8	50.6
54	46.7	38.5	57.7









#9
Naphthalene
Concen: 0.375 ng
RT: 10.457 min Scan# 737
Delta R.T. 0.000 min
Lab File: BN016725.D
Acq: 05 Oct 2021 01:37




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:128 Resp: 120496
Ion Ratio Lower Upper
128 100
129 11.0 8.7 13.1
127 12.9 10.3 15.5



#10
Hexachlorobutadiene
Concen: 0.378 ng
RT: 10.748 min Scan# 760
Delta R.T. 0.000 min
Lab File: BN016725.D
Acq: 05 Oct 2021 01:37

Tgt Ion:225 Resp: 22728
Ion Ratio Lower Upper
225 100
223 0.0 0.0 0.0
227 64.0 51.1 76.7









#11
2-Methylnaphthalene-d10
Concen: 0.375 ng
RT: 12.007 min Scan# 932
Delta R.T. 0.000 min
Lab File: BN016725.D
Acq: 05 Oct 2021 01:37




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:152 Resp: 65660
Ion Ratio Lower Upper
152 100
151 20.2 16.2 24.4



#12
2-Methylnaphthalene
Concen: 0.382 ng
RT: 12.078 min Scan# 948
Delta R.T. -0.004 min
Lab File: BN016725.D
Acq: 05 Oct 2021 01:37

Tgt Ion:142 Resp: 78054
Ion Ratio Lower Upper
142 100
141 88.6 70.6 106.0
115 32.7 26.1 39.1









#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.268 min Scan# 1183
Delta R.T. -0.000 min
Lab File: BN016725.D
Acq: 05 Oct 2021 01:37




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:164 Resp: 61432
Ion Ratio Lower Upper
164 100
162 102.4 82.6 124.0
160 46.5 38.2 57.2



#14
2,4,6-Tribromophenol
Concen: 0.382 ng
RT: 15.778 min Scan# 1302
Delta R.T. 0.000 min
Lab File: BN016725.D
Acq: 05 Oct 2021 01:37

Tgt Ion:330 Resp: 9370
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 30.1 24.2 36.2









#15
2-Fluorobiphenyl
Concen: 0.376 ng
RT: 12.898 min Scan# 1075
Delta R.T. 0.000 min
Lab File: BN016725.D
Acq: 05 Oct 2021 01:37




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:	172	Resp:	92451
Ion	Ratio	Lower	Upper
172	100		
171	33.4	26.9	40.3
170	21.4	17.4	26.0



#16
Acenaphthylene
Concen: 0.357 ng
RT: 13.989 min Scan# 1161
Delta R.T. 0.000 min
Lab File: BN016725.D
Acq: 05 Oct 2021 01:37

Tgt Ion:	152	Resp:	96947
Ion	Ratio	Lower	Upper
152	100		
151	19.4	15.5	23.3
153	13.0	10.4	15.6









#17
Acenaphthene
Concen: 0.374 ng
RT: 14.332 min Scan# 1188
Delta R.T. 0.000 min
Lab File: BN016725.D
Acq: 05 Oct 2021 01:37




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:154 Resp: 66949
Ion Ratio Lower Upper
154 100
153 113.9 90.1 135.1
152 55.0 43.6 65.4



#18
Fluorene
Concen: 0.377 ng
RT: 15.321 min Scan# 1266
Delta R.T. 0.000 min
Lab File: BN016725.D
Acq: 05 Oct 2021 01:37

Tgt Ion:166 Resp: 81550
Ion Ratio Lower Upper
166 100
165 97.2 78.1 117.1
167 13.3 10.7 16.1









#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.029 min Scan# 1404
Delta R.T. 0.000 min
Lab File: BN016725.D
Acq: 05 Oct 2021 01:37




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:188 Resp: 113524
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 6.9 5.8 8.8



#20
4,6-Dinitro-2-methylphenol
Concen: 0.523 ng
RT: 15.410 min Scan# 1273
Delta R.T. -0.013 min
Lab File: BN016725.D
Acq: 05 Oct 2021 01:37

Tgt Ion:198 Resp: 2495
Ion Ratio Lower Upper
198 100
182 17.0 26.2 39.2#
77 0.0 0.0 0.0









#21
4-Bromophenyl-phenylether
Concen: 0.375 ng
RT: 16.226 min Scan# 1338
Delta R.T. 0.000 min
Lab File: BN016725.D
Acq: 05 Oct 2021 01:37




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:248 Resp: 25943
Ion Ratio Lower Upper
248 100
250 97.0 76.2 114.4
141 50.4 45.6 68.4



#22
Hexachlorobenzene
Concen: 0.388 ng
RT: 16.336 min Scan# 1347
Delta R.T. -0.000 min
Lab File: BN016725.D
Acq: 05 Oct 2021 01:37

Tgt Ion:284 Resp: 30394
Ion Ratio Lower Upper
284 100
142 31.8 25.8 38.6
249 29.3 23.3 34.9









#23
Atrazine
Concen: 0.318 ng
RT: 16.506 min Scan# 1361
Delta R.T. 0.000 min
Lab File: BN016725.D
Acq: 05 Oct 2021 01:37




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:200 Resp: 17421
Ion Ratio Lower Upper
200 100
173 24.4 20.1 30.1
215 48.7 38.8 58.2



#24
Pentachlorophenol
Concen: 0.551 ng
RT: 16.689 min Scan# 1376
Delta R.T. -0.000 min
Lab File: BN016725.D
Acq: 05 Oct 2021 01:37

Tgt Ion:266 Resp: 8090
Ion Ratio Lower Upper
266 100
264 62.9 49.3 73.9
268 64.0 51.8 77.8









#25
Phenanthrene
Concen: 0.387 ng
RT: 17.066 min Scan# 1407
Delta R.T. 0.000 min
Lab File: BN016725.D
Acq: 05 Oct 2021 01:37




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:178 Resp: 129178
Ion Ratio Lower Upper
178 100
176 18.8 15.0 22.6
179 15.4 12.4 18.6



#26
Anthracene
Concen: 0.358 ng
RT: 17.163 min Scan# 1415
Delta R.T. 0.000 min
Lab File: BN016725.D
Acq: 05 Oct 2021 01:37

Tgt Ion:178 Resp: 106644
Ion Ratio Lower Upper
178 100
176 18.5 14.5 21.7
179 15.3 12.2 18.4









#27
Fluoranthene-d10
Concen: 0.368 ng
RT: 19.068 min Scan# 1697
Delta R.T. 0.000 min
Lab File: BN016725.D
Acq: 05 Oct 2021 01:37




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:212 Resp: 114281
Ion Ratio Lower Upper
212 100
106 13.3 10.6 16.0
104 7.2 5.8 8.8



#28
Fluoranthene
Concen: 0.386 ng
RT: 19.097 min Scan# 1703
Delta R.T. -0.000 min
Lab File: BN016725.D
Acq: 05 Oct 2021 01:37

Tgt Ion:202 Resp: 142900
Ion Ratio Lower Upper
202 100
101 11.1 8.9 13.3
203 17.4 13.8 20.8









#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.238 min Scan# 2002
Delta R.T. 0.000 min
Lab File: BN016725.D
Acq: 05 Oct 2021 01:37




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:240 Resp: 112908
Ion Ratio Lower Upper
240 100
120 6.6 6.6 10.0#
236 25.6 20.7 31.1



#30
Pyrene
Concen: 0.384 ng
RT: 19.465 min Scan# 1777
Delta R.T. 0.000 min
Lab File: BN016725.D
Acq: 05 Oct 2021 01:37

Tgt Ion:202 Resp: 142536
Ion Ratio Lower Upper
202 100
200 20.7 16.5 24.7
203 17.5 13.9 20.9









#31
Terphenyl-d14
Concen: 0.390 ng
RT: 19.678 min Scan# 1820
Delta R.T. -0.005 min
Lab File: BN016725.D
Acq: 05 Oct 2021 01:37




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:244 Resp: 98435
Ion Ratio Lower Upper
244 100
212 7.3 5.8 8.6
122 12.6 8.9 13.3



#32
Benzo(a)anthracene
Concen: 0.380 ng
RT: 21.216 min Scan# 2000
Delta R.T. -0.000 min
Lab File: BN016725.D
Acq: 05 Oct 2021 01:37

Tgt Ion:228 Resp: 133072
Ion Ratio Lower Upper
228 100
226 27.0 22.3 33.5
229 19.2 15.4 23.0









#33
Chrysene
Concen: 0.402 ng
RT: 21.270 min Scan# 2005
Delta R.T. -0.000 min
Lab File: BN016725.D
Acq: 05 Oct 2021 01:37




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:228 Resp: 142906
Ion Ratio Lower Upper
228 100
226 29.9 24.2 36.4
229 19.4 15.4 23.0



#34
Bis(2-ethylhexyl)phthalate
Concen: 0.256 ng
RT: 21.174 min Scan# 1996
Delta R.T. -0.000 min
Lab File: BN016725.D
Acq: 05 Oct 2021 01:37


Tgt Ion:149 Resp: 54319
Ion Ratio Lower Upper
149 100
167 27.5 22.2 33.4
279 4.1 3.4 5.2








#35
 Perylene-d12
 Concen: 0.400 ng
 RT: 23.488 min Scan# 2428
 Delta R.T. -0.007 min
 Lab File: BN016725.D
 Acq: 05 Oct 2021 01:37

Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4







Tgt Ion:264 Resp: 118004
 Ion Ratio Lower Upper
 264 100
 260 24.7 19.8 29.6
 265 23.3 20.3 30.5



#36
 Indeno(1,2,3-cd)pyrene
 Concen: 0.451 ng
 RT: 25.774 min Scan# 3096
 Delta R.T. -0.007 min
 Lab File: BN016725.D
 Acq: 05 Oct 2021 01:37


Tgt Ion:276 Resp: 168955
 Ion Ratio Lower Upper
 276 100
 138 25.1 19.2 28.8
 277 25.1 20.0 30.0








#37
Benzo(b)fluoranthene
Concen: 0.384 ng
RT: 22.810 min Scan# 2230
Delta R.T. -0.003 min
Lab File: BN016725.D
Acq: 05 Oct 2021 01:37

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4







Tgt Ion:252 Resp: 146373
Ion Ratio Lower Upper
252 100
253 22.3 17.8 26.8
125 10.0 8.3 12.5



#38
Benzo(k)fluoranthene
Concen: 0.405 ng
RT: 22.854 min Scan# 2243
Delta R.T. -0.007 min
Lab File: BN016725.D
Acq: 05 Oct 2021 01:37

Tgt Ion:252 Resp: 148545
Ion Ratio Lower Upper
252 100
253 22.4 17.8 26.8
125 12.4 8.5 12.7









#39
Benzo(a)pyrene
Concen: 0.389 ng
RT: 23.388 min Scan# 2399
Delta R.T. -0.003 min
Lab File: BN016725.D
Acq: 05 Oct 2021 01:37




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:252 Resp: 132712
Ion Ratio Lower Upper
252 100
253 22.0 17.9 26.9
125 11.1 9.4 14.2



#40
Dibenzo(a,h)anthracene
Concen: 0.454 ng
RT: 25.795 min Scan# 3102
Delta R.T. -0.003 min
Lab File: BN016725.D
Acq: 05 Oct 2021 01:37

Tgt Ion:278 Resp: 134978
Ion Ratio Lower Upper
278 100
139 17.5 13.1 19.7
279 24.1 19.3 28.9





#41
Benzo(g,h,i)perylene
Concen: 0.444 ng
RT: 26.469 min Scan# 3299
Delta R.T. -0.007 min
Lab File: BN016725.D
Acq: 05 Oct 2021 01:37

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion:276 Resp: 147637
Ion Ratio Lower Upper
276 100
277 23.9 19.0 28.4
138 20.9 17.0 25.6

