

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100421\
 Data File : BN016740.D
 Acq On : 05 Oct 2021 10:36
 Operator : CG/JU
 Sample : SSTDCCC0.4
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4EC

Quant Time: Oct 05 11:05:46 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN100421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 04 17:52:33 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.642	152	23318	0.400	ng	0.00
7) Naphthalene-d8	10.406	136	103566	0.400	ng	# 0.00
13) Acenaphthene-d10	14.269	164	53161	0.400	ng	0.00
19) Phenanthrene-d10	17.029	188	101328	0.400	ng	0.00
29) Chrysene-d12	21.238	240	104040	0.400	ng	0.00
35) Perylene-d12	23.488	264	112545	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.263	112	23073	0.388	ng	0.00
5) Phenol-d6	6.822	99	25424	0.385	ng	0.00
8) Nitrobenzene-d5	8.784	82	26497	0.365	ng	0.00
11) 2-Methylnaphthalene-d10	12.003	152	57274	0.371	ng	0.00
14) 2,4,6-Tribromophenol	15.766	330	9161	0.416	ng	-0.01
15) 2-Fluorobiphenyl	12.886	172	81229	0.382	ng	-0.01
27) Fluoranthene-d10	19.068	212	104750	0.378	ng	0.00
31) Terphenyl-d14	19.678	244	89479	0.384	ng	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.253	88	4003	0.368	ng	# 65
3) n-Nitrosodimethylamine	3.594	42	6657	0.379	ng	# 99
6) bis(2-Chloroethyl)ether	7.080	93	25009	0.395	ng	100
9) Naphthalene	10.457	128	105724	0.373	ng	100
10) Hexachlorobutadiene	10.749	225	20257	0.382	ng	# 100
12) 2-Methylnaphthalene	12.078	142	68761	0.382	ng	100
16) Acenaphthylene	13.989	152	86733	0.370	ng	100
17) Acenaphthene	14.332	154	58192	0.375	ng	99
18) Fluorene	15.322	166	70674	0.378	ng	100
20) 4,6-Dinitro-2-methylph...	15.410	198	1756	0.472	ng	# 74
21) 4-Bromophenyl-phenylether	16.226	248	22867	0.371	ng	# 91
22) Hexachlorobenzene	16.336	284	26871	0.384	ng	99
23) Atrazine	16.506	200	16704	0.342	ng	97
24) Pentachlorophenol	16.677	266	8457	0.587	ng	99
25) Phenanthrene	17.066	178	113254	0.380	ng	100
26) Anthracene	17.151	178	97070	0.365	ng	100
28) Fluoranthene	19.097	202	130172	0.394	ng	100
30) Pyrene	19.460	202	131569	0.385	ng	100
32) Benzo(a)anthracene	21.217	228	128403	0.398	ng	99
33) Chrysene	21.270	228	134591	0.411	ng	100
34) Bis(2-ethylhexyl)phtha...	21.174	149	61550	0.315	ng	100
36) Indeno(1,2,3-cd)pyrene	25.771	276	164679	0.461	ng	99
37) Benzo(b)fluoranthene	22.810	252	141299	0.388	ng	99
38) Benzo(k)fluoranthene	22.858	252	141648	0.405	ng	99
39) Benzo(a)pyrene	23.388	252	129955	0.399	ng	99
40) Dibenzo(a,h)anthracene	25.791	278	132506	0.467	ng	99
41) Benzo(g,h,i)perylene	26.469	276	141791	0.447	ng	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100421\
Data File : BN016740.D
Acq On : 05 Oct 2021 10:36
Operator : CG/JU
Sample : SSTDCCC0.4
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Quant Time: Oct 05 11:05:46 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN100421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 04 17:52:33 2021
Response via : Initial Calibration

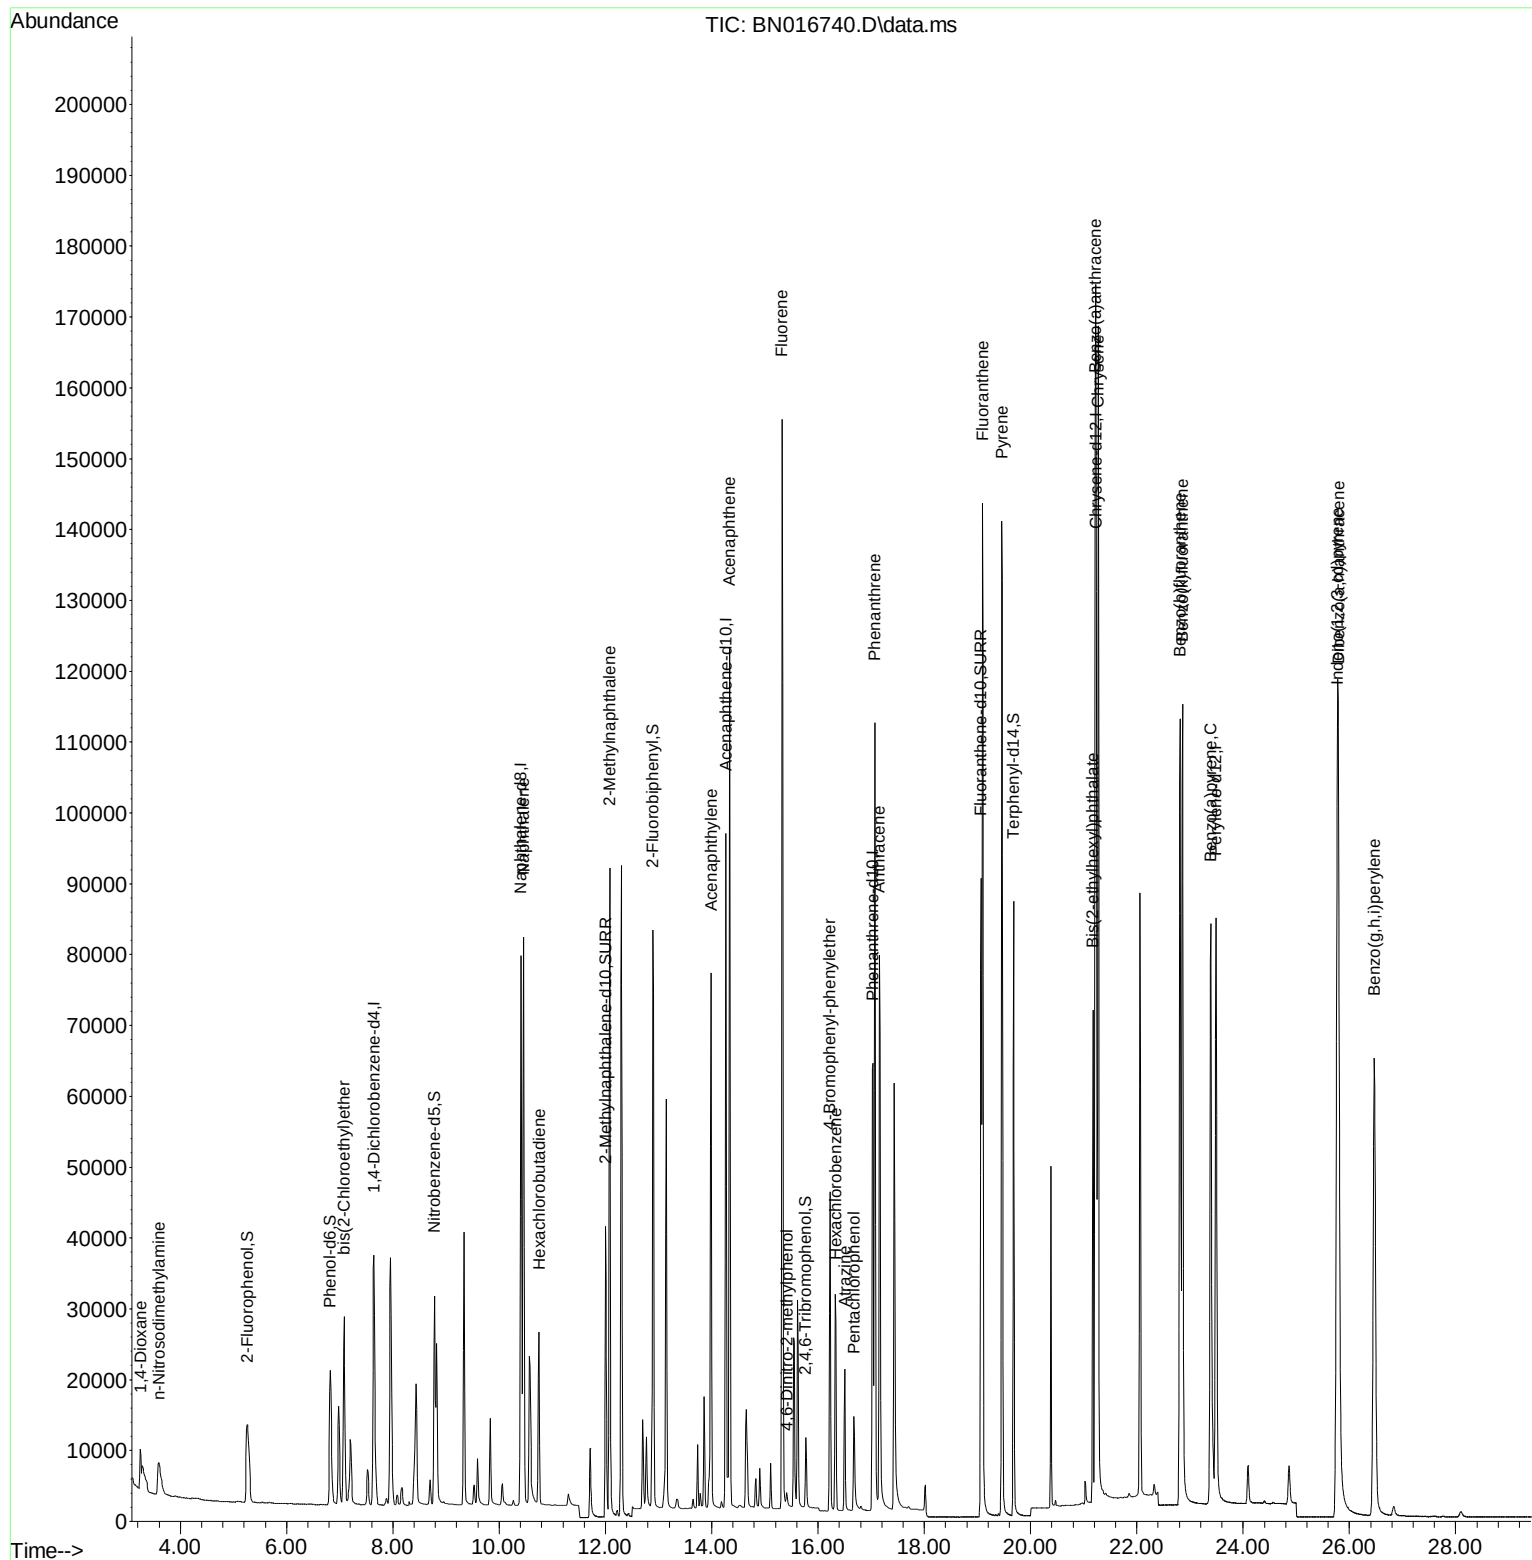


Abundance Scan 495 (7.642 min): BN016710.D\data.ms (-487) (#1)





1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.642 min Scan# 495
Delta R.T. 0.000 min
Lab File: BN016740.D
Acq: 05 Oct 2021 10:36


Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

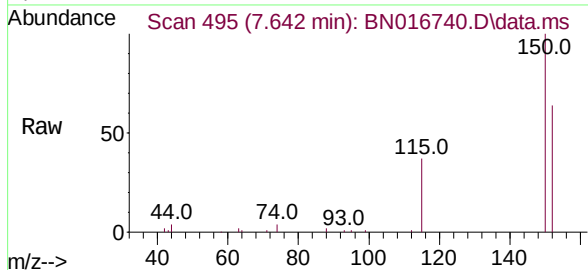

Tgt Ion:	152	Resp:	23318
Ion	Ratio	Lower	Upper
152	100		
150	155.5	123.3	184.9
115	58.0	47.0	70.6



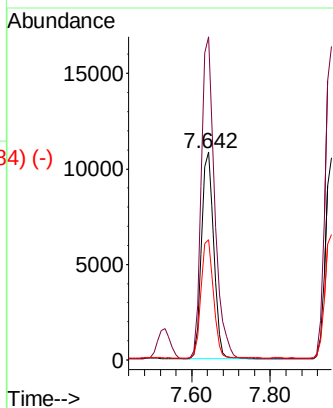



Abundance Scan 19 (3.253 min): BN016710.D\data.ms (-16) (#2)

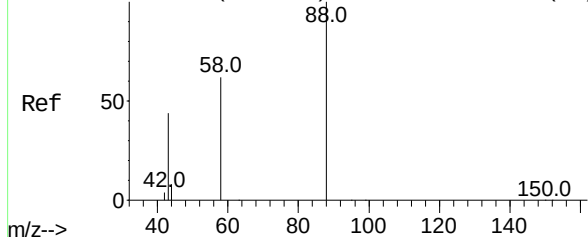

1,4-Dioxane
Concen: 0.368 ng
RT: 3.253 min Scan# 19
Delta R.T. 0.000 min
Lab File: BN016740.D
Acq: 05 Oct 2021 10:36

Tgt Ion:	88	Resp:	4003
Ion	Ratio	Lower	Upper
88	100		
43	27.0	61.7	92.5#
58	66.6	62.2	93.2


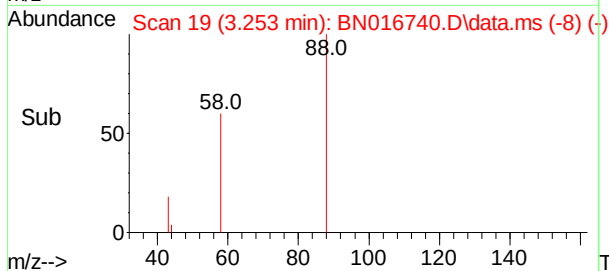




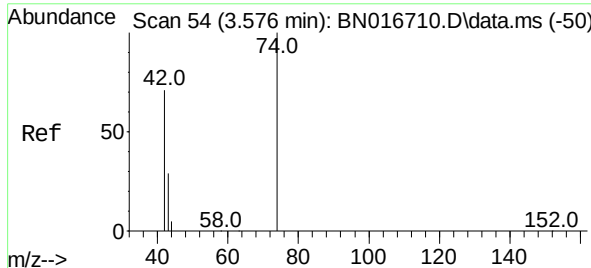

n-Nitrosodimethylamine
 Concen: 0.379 ng
 RT: 3.594 min Scan# 56
 Delta R.T. 0.019 min
 Lab File: BN016740.D
 Acq: 05 Oct 2021 10:36




Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4EC


Tgt Ion: 42 Resp: 6657
 Ion Ratio Lower Upper
 42 100
 74 153.7 124.0 186.0
 44 8.9 5.6 8.4#

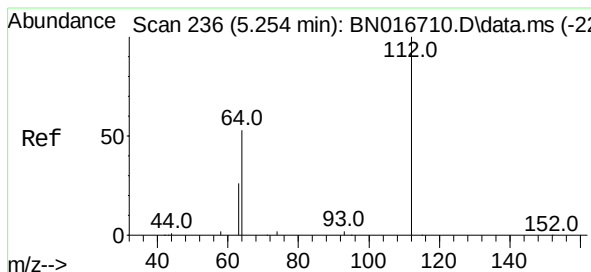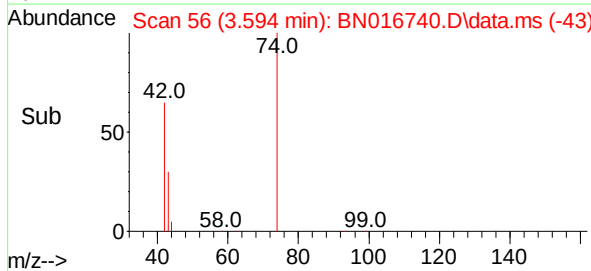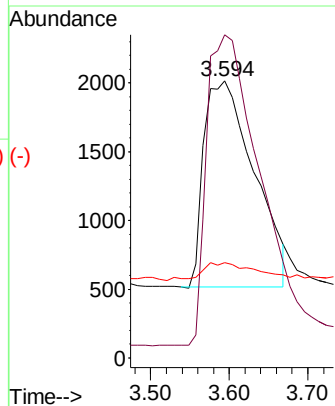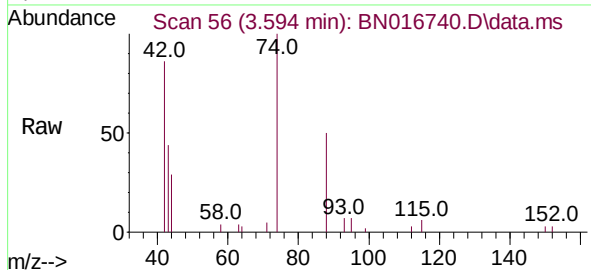

2-Fluorophenol
 Concen: 0.388 ng
 RT: 5.263 min Scan# 237
 Delta R.T. 0.009 min
 Lab File: BN016740.D
 Acq: 05 Oct 2021 10:36

Tgt Ion: 112 Resp: 23073
 Ion Ratio Lower Upper
 112 100
 64 54.2 42.9 64.3
 63 27.3 21.5 32.3


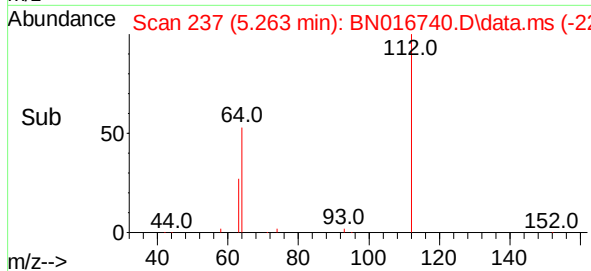
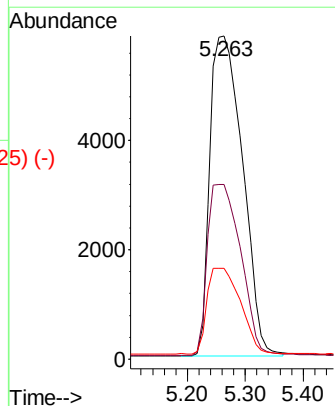
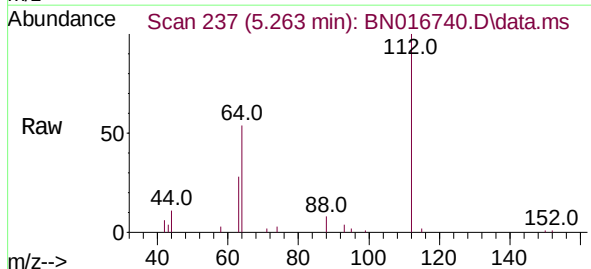


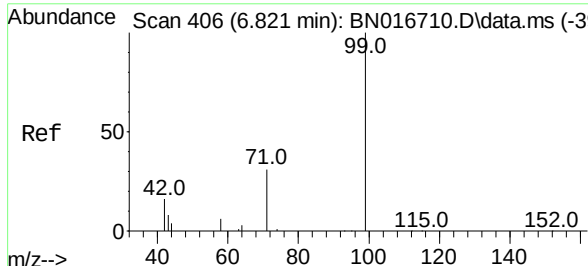

Phenol-d6
 Concen: 0.385 ng
 RT: 6.822 min Scan# 406
 Delta R.T. 0.000 min
 Lab File: BN016740.D
 Acq: 05 Oct 2021 10:36




Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4EC


Tgt Ion:	99	Resp:	25424
Ion	Ratio	Lower	Upper
99	100		
42	16.9	13.4	20.2
71	30.3	24.0	36.0

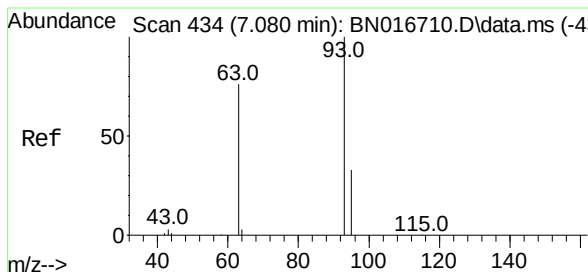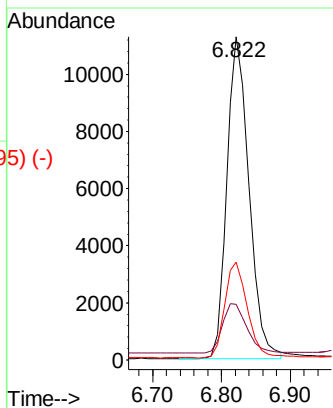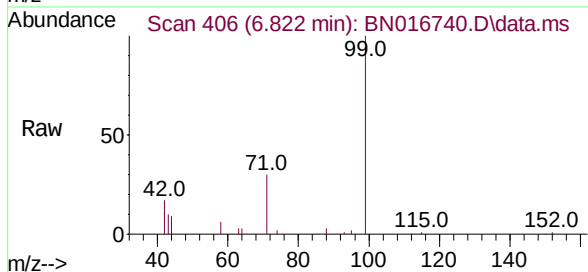

bis(2-Chloroethyl)ether
 Concen: 0.395 ng
 RT: 7.080 min Scan# 434
 Delta R.T. 0.000 min
 Lab File: BN016740.D
 Acq: 05 Oct 2021 10:36

Tgt Ion:	93	Resp:	25009
Ion	Ratio	Lower	Upper
93	100		
63	74.0	59.0	88.6
95	33.1	26.4	39.6







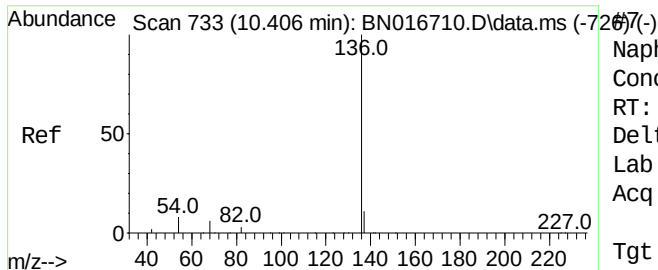

Naphthalene-d8
 Concen: 0.400 ng
 RT: 10.406 min Scan# 733
 Delta R.T. 0.000 min
 Lab File: BN016740.D
 Acq: 05 Oct 2021 10:36




Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4EC

Tgt Ion:	136	Resp:	103566
Ion	Ratio	Lower	Upper
136	100		
137	10.8	8.9	13.3
54	6.4	6.5	9.7#
68	5.5	5.3	7.9

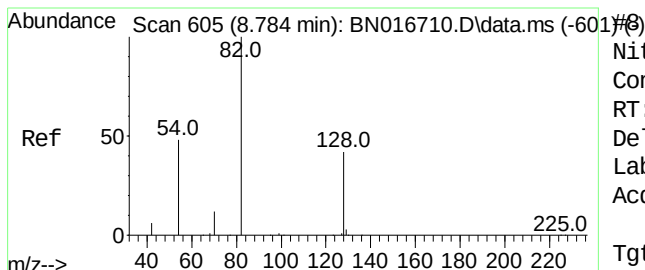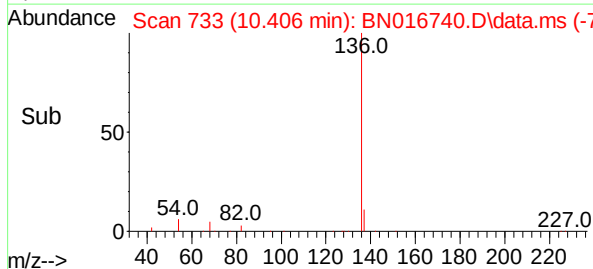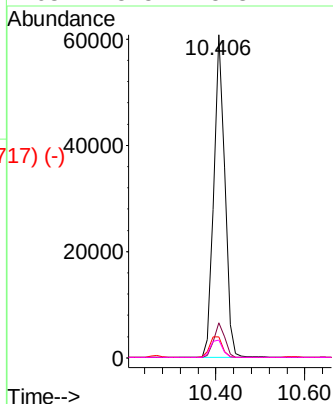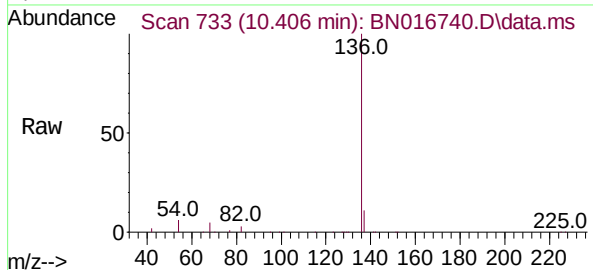


Nitrobenzene-d5
 Concen: 0.365 ng
 RT: 8.784 min Scan# 605
 Delta R.T. 0.000 min
 Lab File: BN016740.D
 Acq: 05 Oct 2021 10:36

Tgt Ion:	82	Resp:	26497
Ion	Ratio	Lower	Upper
82	100		
128	44.9	33.8	50.6
54	44.6	38.5	57.7

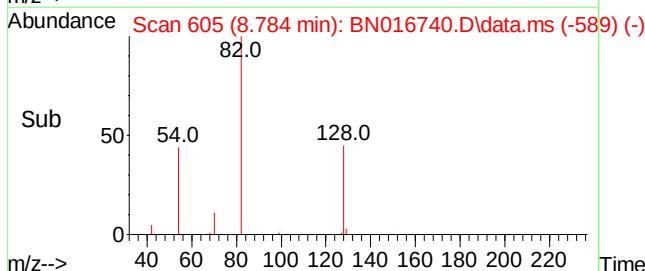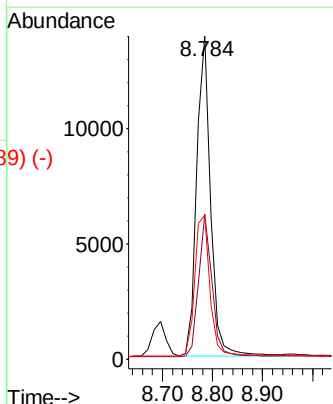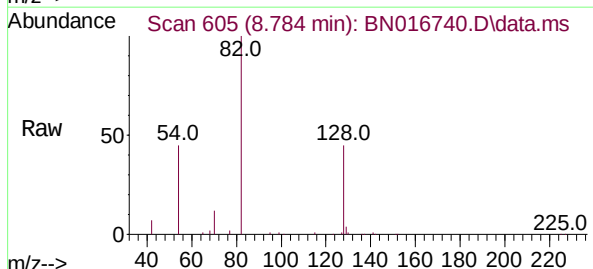




Abundance Scan 737 (10.457 min): BN016710.D\data.ms (-737) (-)

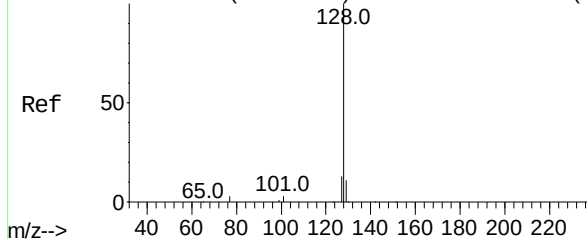


Naphthalene
Concen: 0.373 ng
RT: 10.457 min Scan# 737
Delta R.T. 0.000 min
Lab File: BN016740.D
Acq: 05 Oct 2021 10:36

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Tgt Ion:128	Resp: 105724
Ion Ratio	Lower Upper
128 100	
129 11.0	8.7 13.1
127 12.9	10.3 15.5

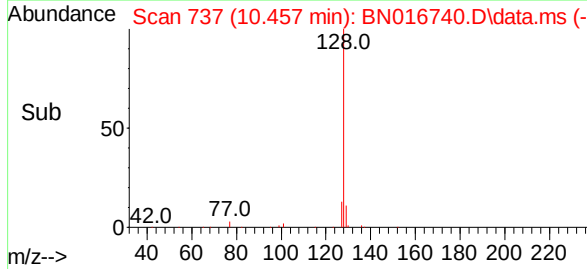

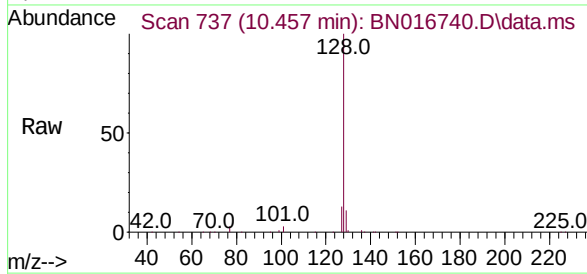


Abundance Scan 760 (10.749 min): BN016710.D\data.ms (-755) (-)

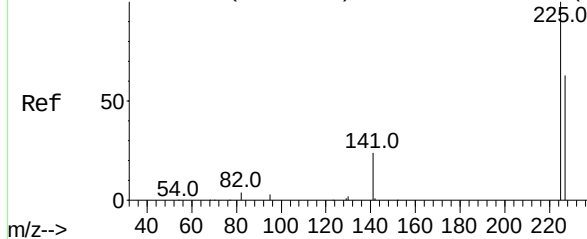


Hexachlorobutadiene
Concen: 0.382 ng
RT: 10.749 min Scan# 760
Delta R.T. 0.000 min
Lab File: BN016740.D
Acq: 05 Oct 2021 10:36

Tgt Ion:225	Resp: 20257
Ion Ratio	Lower Upper
225 100	
223 0.0	0.0 0.0
227 64.3	51.1 76.7

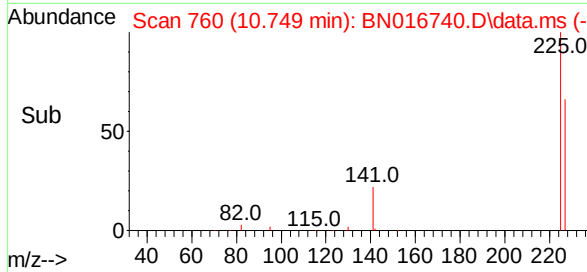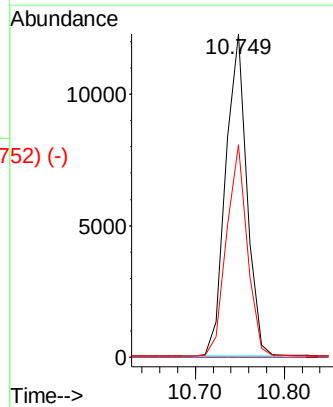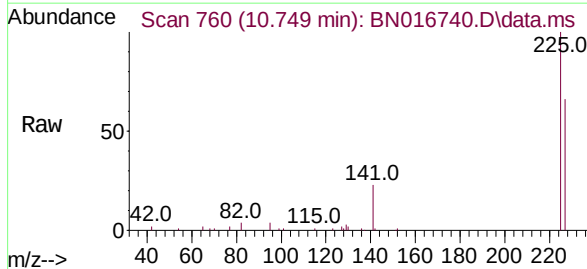


Abundance Scan 932 (12.007 min): BN016710.D\data.ms (-927) (-)





2-Methylnaphthalene-d10
Concen: 0.371 ng
RT: 12.003 min Scan# 931
Delta R.T. -0.004 min
Lab File: BN016740.D
Acq: 05 Oct 2021 10:36


Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

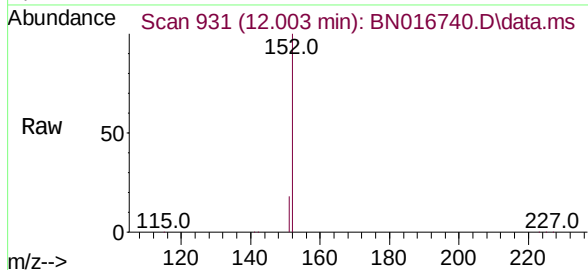


Tgt Ion:152 Resp: 57274
Ion Ratio Lower Upper
152 100
151 20.4 16.2 24.4





Abundance Scan 949 (12.082 min): BN016710.D\data.ms (-937) (-)



2-Methylnaphthalene
Concen: 0.382 ng
RT: 12.078 min Scan# 948
Delta R.T. -0.004 min
Lab File: BN016740.D
Acq: 05 Oct 2021 10:36




Tgt Ion:142 Resp: 68761
Ion Ratio Lower Upper
142 100
141 88.0 70.6 106.0
115 32.3 26.1 39.1






Abundance Scan 1183 (14.268 min): BN016710.D\data.ms (-1175) (-)

Acenaphthene-d10
Concen: 0.400 ng
RT: 14.269 min Scan# 1183
Delta R.T. 0.000 min
Lab File: BN016740.D
Acq: 05 Oct 2021 10:36

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

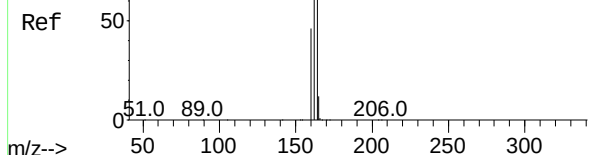





Tgt Ion:	164	Resp:	53161
Ion	Ratio	Lower	Upper
164	100		
162	102.2	82.6	124.0
160	46.4	38.2	57.2

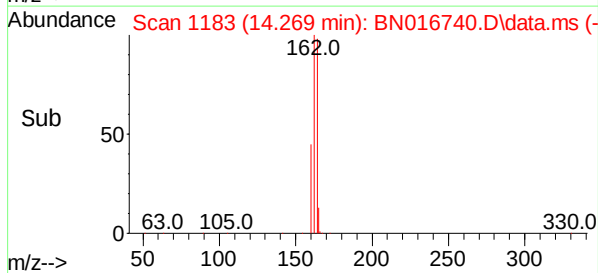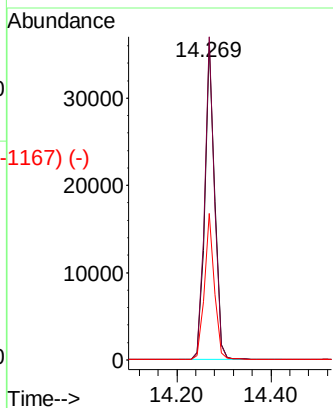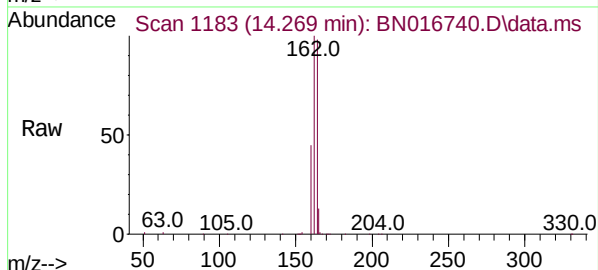


Abundance Scan 1302 (15.778 min): BN016710.D\data.ms (-1294) (-)

2,4,6-Tribromophenol
Concen: 0.416 ng
RT: 15.766 min Scan# 1301
Delta R.T. -0.012 min
Lab File: BN016740.D
Acq: 05 Oct 2021 10:36

Tgt Ion:	330	Resp:	9161
Ion	Ratio	Lower	Upper
330	100		
332	0.0	0.0	0.0
141	30.2	24.2	36.2

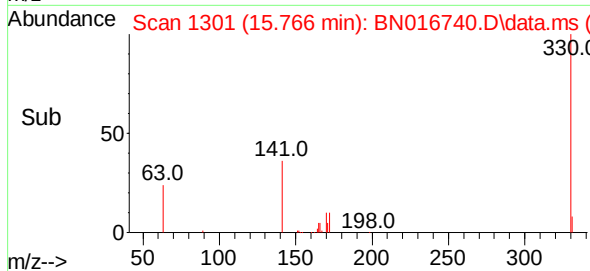

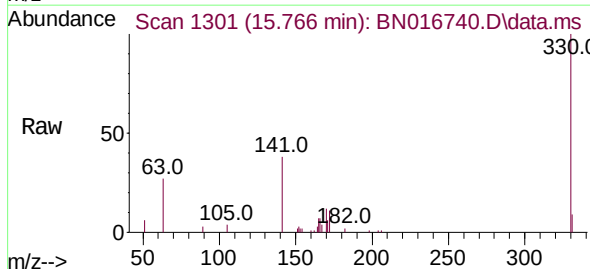
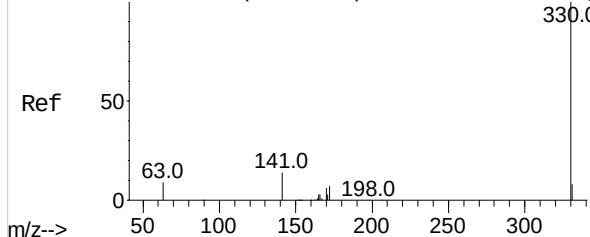


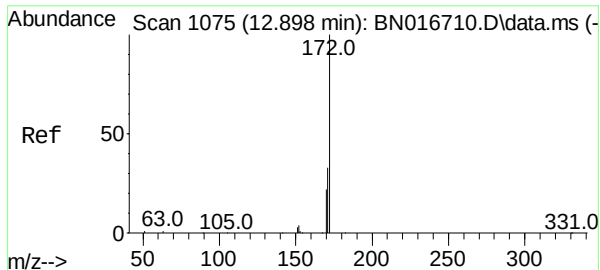

Scan 1075 (12.898 min): BN016710.D\data.ms (-1075) (-)
 2-Fluorobiphenyl
 Concen: 0.382 ng
 RT: 12.886 min Scan# 1074
 Delta R.T. -0.012 min
 Lab File: BN016740.D
 Acq: 05 Oct 2021 10:36




Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4EC

Tgt Ion:	172	Resp:	81229
Ion	Ratio	Lower	Upper
172	100		
171	35.8	26.9	40.3
170	24.4	17.4	26.0

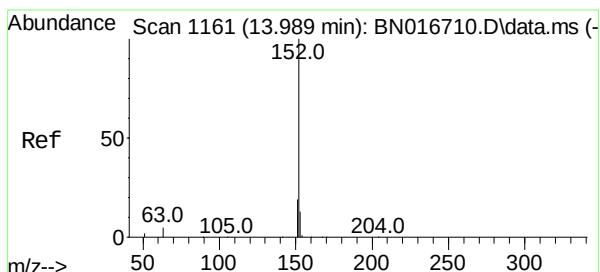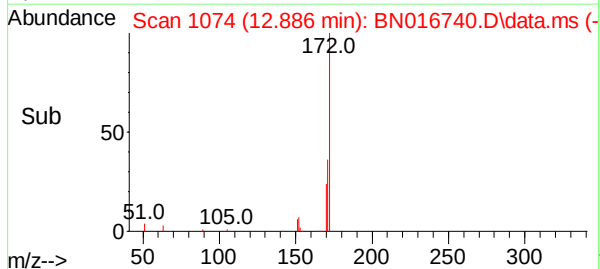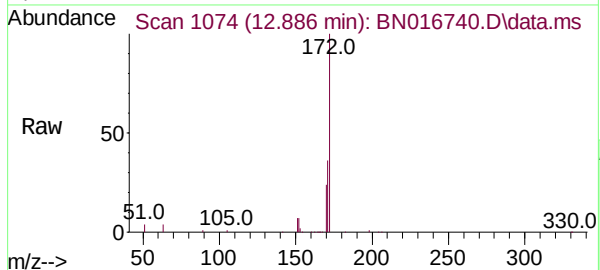

Scan 1161 (13.989 min): BN016710.D\data.ms (-1161) (-)
 Acenaphthylene
 Concen: 0.370 ng
 RT: 13.989 min Scan# 1161
 Delta R.T. 0.000 min
 Lab File: BN016740.D
 Acq: 05 Oct 2021 10:36


Tgt Ion:	152	Resp:	86733
Ion	Ratio	Lower	Upper
152	100		
151	19.5	15.5	23.3
153	13.1	10.4	15.6

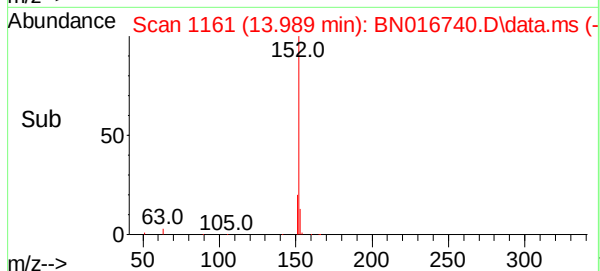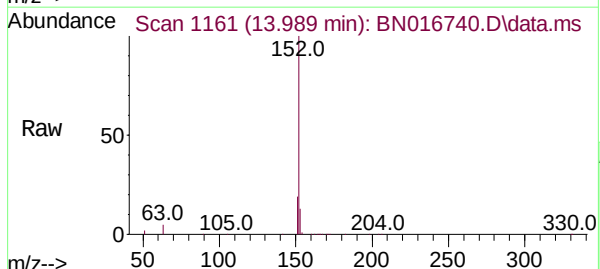



Abundance Scan 1188 (14.332 min): BN016710.D\data.ms (-1187) (-)

Acenaphthene
Concen: 0.375 ng
RT: 14.332 min Scan# 1188
Delta R.T. 0.000 min
Lab File: BN016740.D
Acq: 05 Oct 2021 10:36


Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

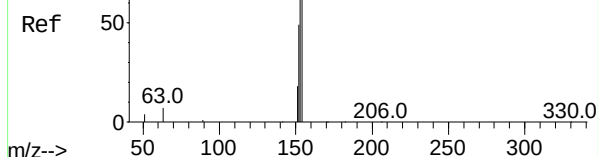

Tgt Ion:	154	Resp:	58192
Ion Ratio	Lower	Upper	
154	100		
153	113.7	90.1	135.1
152	55.2	43.6	65.4

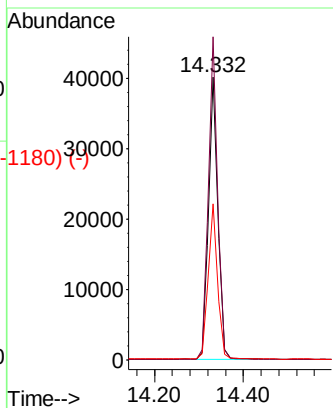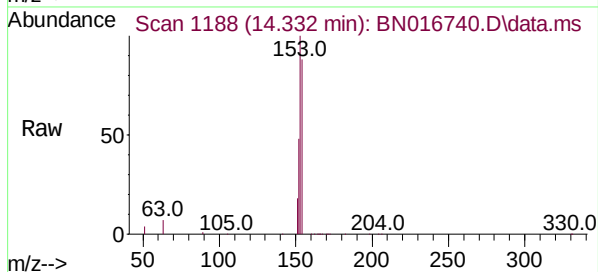



Abundance Scan 1188 (14.332 min): BN016740.D\data.ms (-1180) (-)

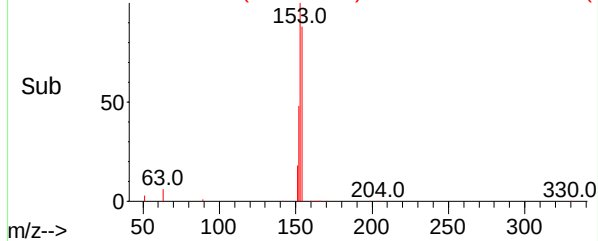


Abundance Scan 1266 (15.322 min): BN016710.D\data.ms (-1265) (-)

Fluorene
Concen: 0.378 ng
RT: 15.322 min Scan# 1266
Delta R.T. 0.001 min
Lab File: BN016740.D
Acq: 05 Oct 2021 10:36

Tgt Ion:	166	Resp:	70674
Ion Ratio	Lower	Upper	
166	100		
165	97.7	78.1	117.1
167	13.4	10.7	16.1

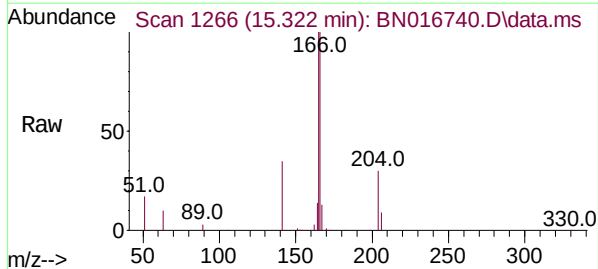


Abundance Scan 1266 (15.322 min): BN016740.D\data.ms (-1250) (-)

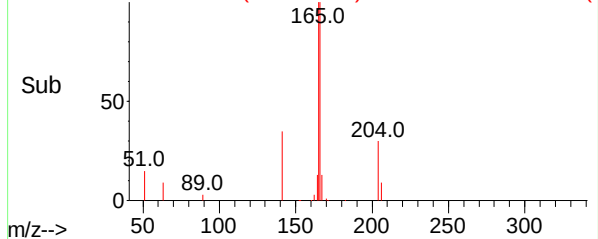



Abundance Scan 1404 (17.029 min): BN016710.D\data.ms (-1388) (-)

Phenanthrene-d10
Concen: 0.400 ng
RT: 17.029 min Scan# 1404
Delta R.T. 0.000 min
Lab File: BN016740.D
Acq: 05 Oct 2021 10:36


Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

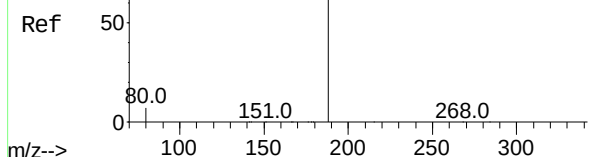

Tgt Ion	Ratio	Lower	Upper
188	100		
94	0.0	0.0	0.0
80	6.2	5.8	8.8

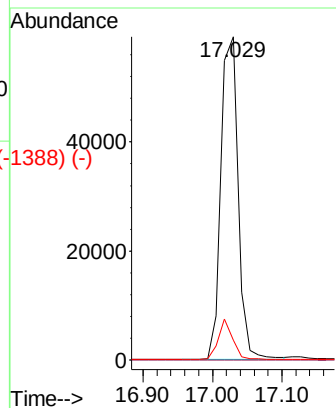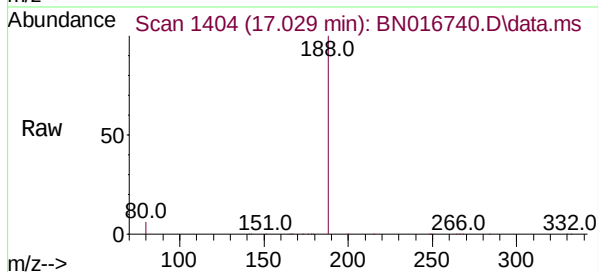


Abundance Scan 1404 (17.029 min): BN016740.D\data.ms (-1388) (-)


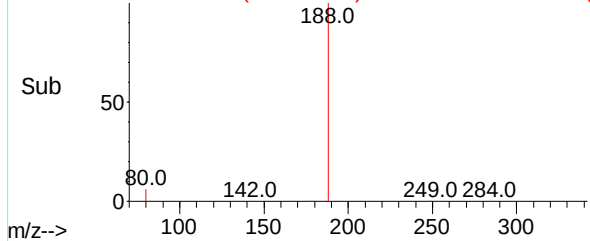


Abundance Scan 1274 (15.423 min): BN016710.D\data.ms (-1266) (-)


4,6-Dinitro-2-methylphenol
Concen: 0.472 ng
RT: 15.410 min Scan# 1273
Delta R.T. -0.013 min
Lab File: BN016740.D
Acq: 05 Oct 2021 10:36

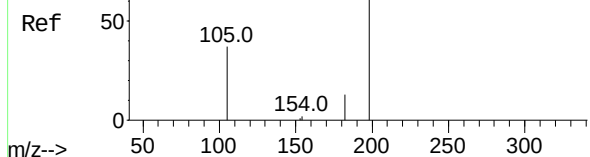


Tgt Ion	Ratio	Lower	Upper
198	100		
182	17.9	26.2	39.2#
77	0.0	0.0	0.0

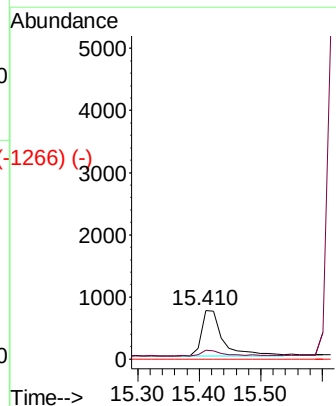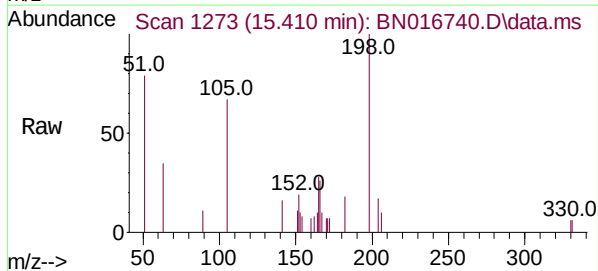

Abundance Scan 1273 (15.410 min): BN016740.D\data.ms (-1266) (-)

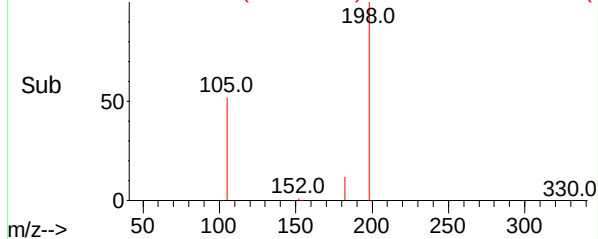




Abundance Scan 1338 (16.226 min): BN016710.D\data.ms (-1324) (-)




4-Bromophenyl-phenylether
Concen: 0.371 ng
RT: 16.226 min Scan# 1338
Delta R.T. 0.000 min
Lab File: BN016740.D
Acq: 05 Oct 2021 10:36

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Tgt Ion:	248	Resp:	22867
Ion Ratio	Lower	Upper	
248	100		
250	99.7	76.2	114.4
141	44.8	45.6	68.4#


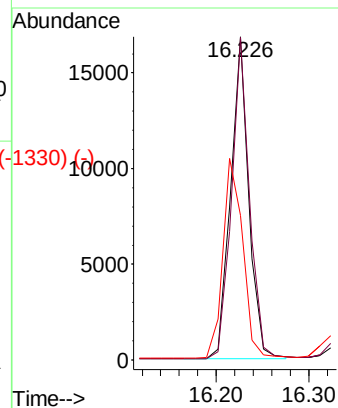
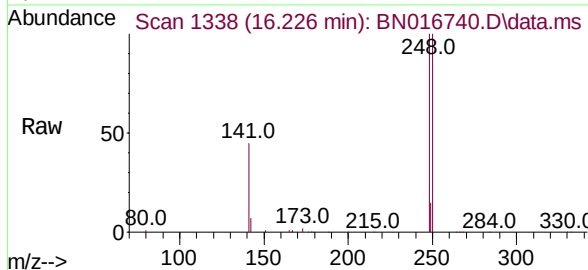



Abundance Scan 1347 (16.336 min): BN016710.D\data.ms (-1322) (-)



Hexachlorobenzene
Concen: 0.384 ng
RT: 16.336 min Scan# 1347
Delta R.T. 0.000 min
Lab File: BN016740.D
Acq: 05 Oct 2021 10:36

Tgt Ion:	284	Resp:	26871
Ion Ratio	Lower	Upper	
284	100		
142	31.7	25.8	38.6
249	29.0	23.3	34.9



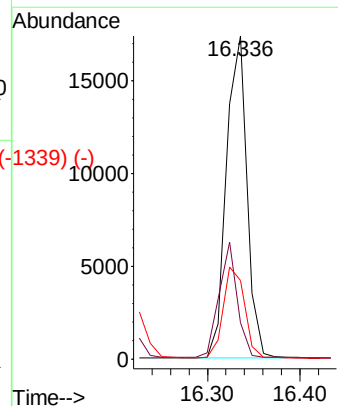



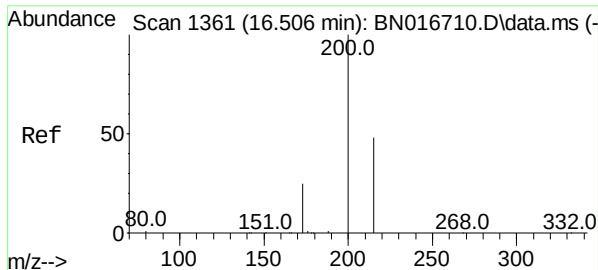

#23 (-)
Atrazine
Concen: 0.342 ng
RT: 16.506 min Scan# 1361
Delta R.T. 0.000 min
Lab File: BN016740.D
Acq: 05 Oct 2021 10:36




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Tgt Ion:	200	Resp:	16704
Ion	Ratio	Lower	Upper
200	100		
173	22.2	20.1	30.1
215	50.0	38.8	58.2

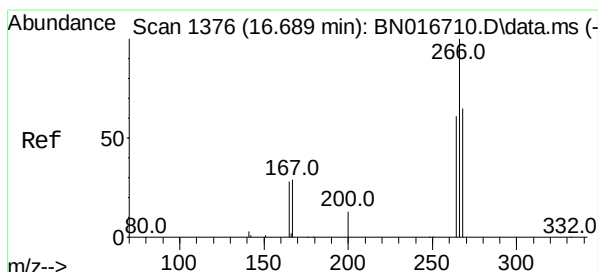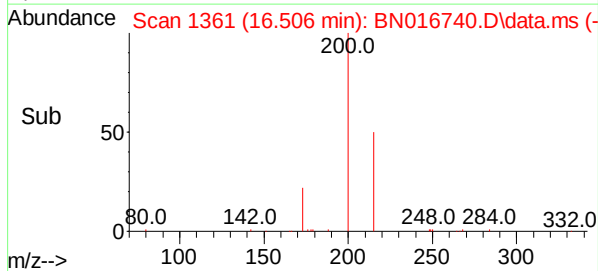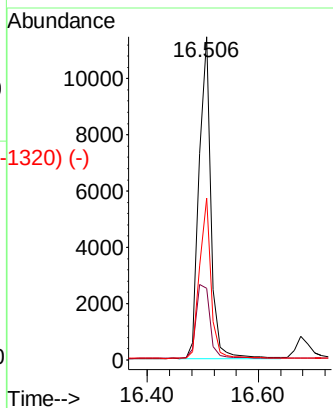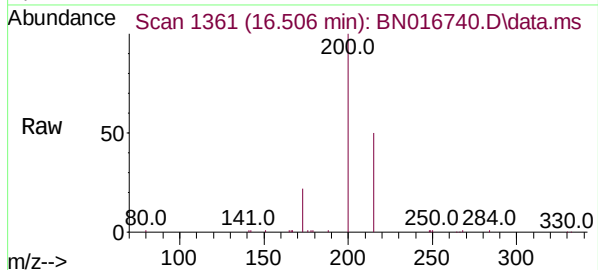


#24 (-)
Pentachlorophenol
Concen: 0.587 ng
RT: 16.677 min Scan# 1375
Delta R.T. -0.012 min
Lab File: BN016740.D
Acq: 05 Oct 2021 10:36

Tgt Ion:	266	Resp:	8457
Ion	Ratio	Lower	Upper
266	100		
264	62.7	49.3	73.9
268	63.8	51.8	77.8

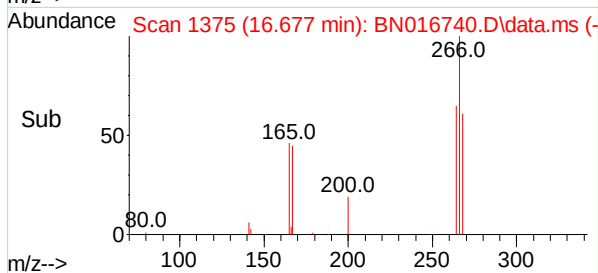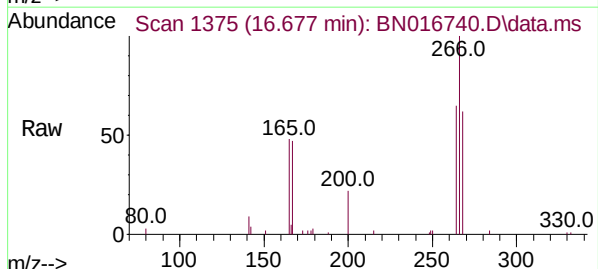




Abundance Scan 1407 (17.066 min): BN016710.D\data.ms (-1325) (-)

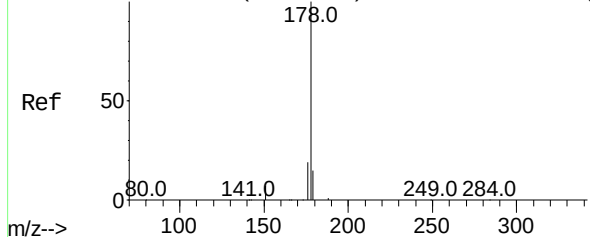


Phenanthrene
Concen: 0.380 ng
RT: 17.066 min Scan# 1407
Delta R.T. 0.000 min
Lab File: BN016740.D
Acq: 05 Oct 2021 10:36

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Tgt Ion:	178	Resp:	113254
Ion	Ratio	Lower	Upper
178	100		
176	18.8	15.0	22.6
179	15.4	12.4	18.6

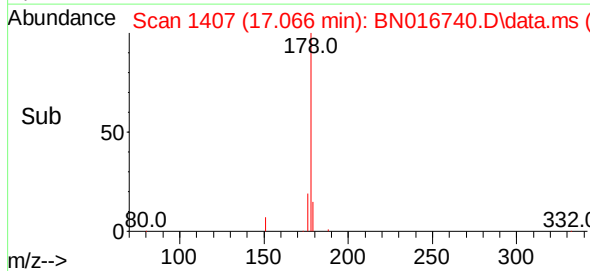
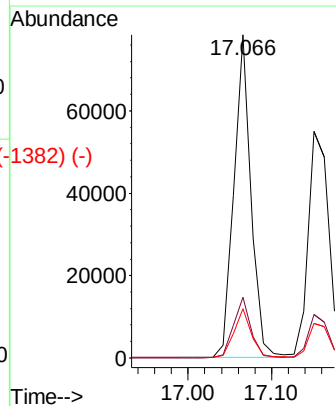
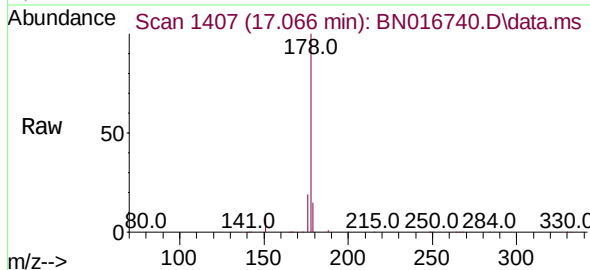


Abundance Scan 1415 (17.163 min): BN016710.D\data.ms (-1428) (-)

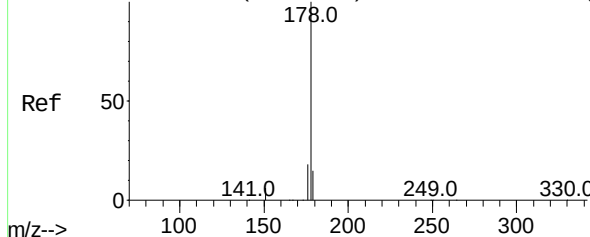

Anthracene
Concen: 0.365 ng
RT: 17.151 min Scan# 1414
Delta R.T. -0.012 min
Lab File: BN016740.D
Acq: 05 Oct 2021 10:36


Tgt Ion:	178	Resp:	97070
Ion	Ratio	Lower	Upper
178	100		
176	18.4	14.5	21.7
179	15.3	12.2	18.4

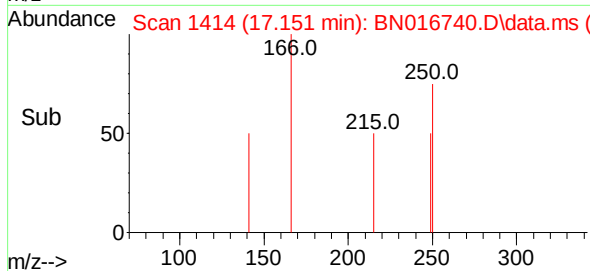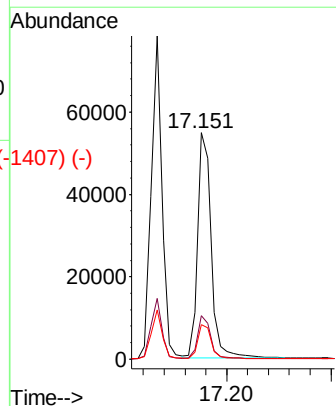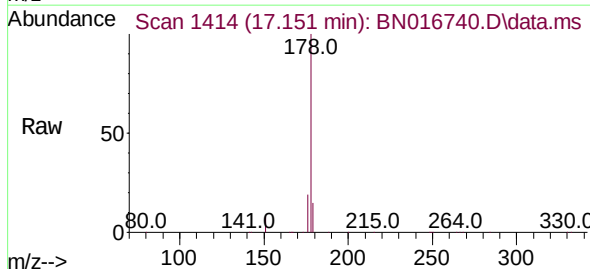



Abundance Scan 1697 (19.068 min): BN016710.D\data.ms (-1627) (-)

Fluoranthene-d10
Concen: 0.378 ng
RT: 19.068 min Scan# 1697
Delta R.T. 0.000 min
Lab File: BN016740.D
Acq: 05 Oct 2021 10:36


Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

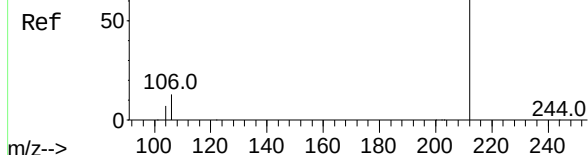

Tgt Ion:	212	Resp:	104750
Ion Ratio	Lower	Upper	
212	100		
106	13.3	10.6	16.0
104	7.2	5.8	8.8

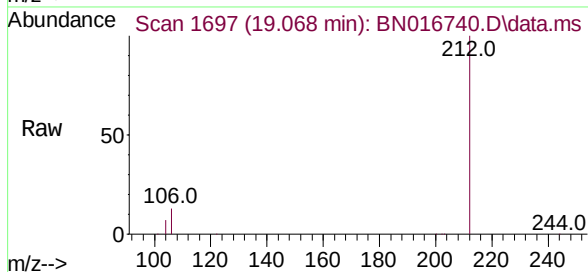



Abundance Scan 1697 (19.068 min): BN016740.D\data.ms (-1677) (-)




Abundance Scan 1703 (19.097 min): BN016710.D\data.ms (-1628) (-)

Fluoranthene
Concen: 0.394 ng
RT: 19.097 min Scan# 1703
Delta R.T. 0.000 min
Lab File: BN016740.D
Acq: 05 Oct 2021 10:36

Tgt Ion:	202	Resp:	130172
Ion Ratio	Lower	Upper	
202	100		
101	11.1	8.9	13.3
203	17.2	13.8	20.8




Abundance Scan 1703 (19.097 min): BN016740.D\data.ms (-1663) (-)

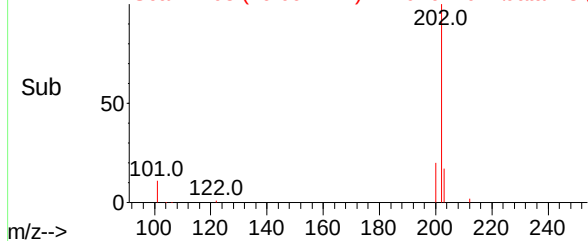




Abundance Scan 2002 (21.238 min): BN016710.D\data.ms (-1929) (-)

Chrysene-d12
Concen: 0.400 ng
RT: 21.238 min Scan# 2002
Delta R.T. 0.000 min
Lab File: BN016740.D
Acq: 05 Oct 2021 10:36

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

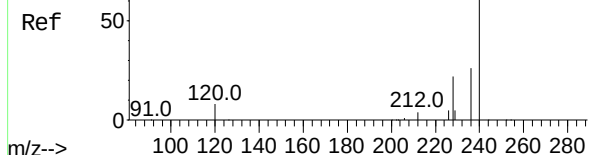


Tgt Ion:	240	Resp:	104040
Ion	Ratio	Lower	Upper
240	100		
120	7.0	6.6	10.0
236	25.7	20.7	31.1

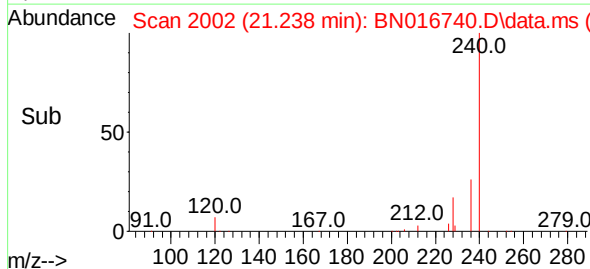
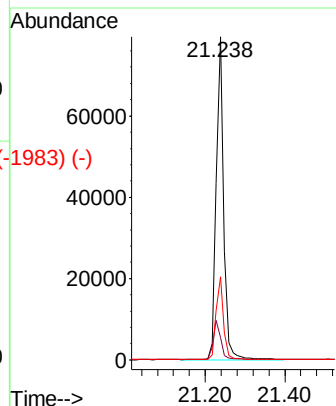
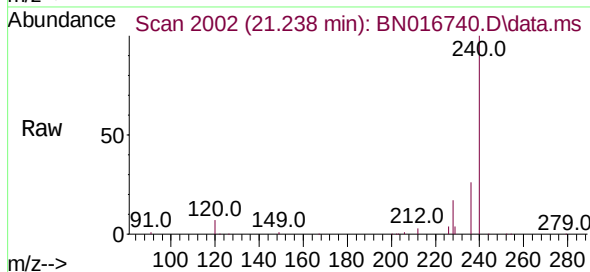


Abundance Scan 1777 (19.465 min): BN016710.D\data.ms (-1737) (-)

Pyrene
Concen: 0.385 ng
RT: 19.460 min Scan# 1776
Delta R.T. -0.005 min
Lab File: BN016740.D
Acq: 05 Oct 2021 10:36

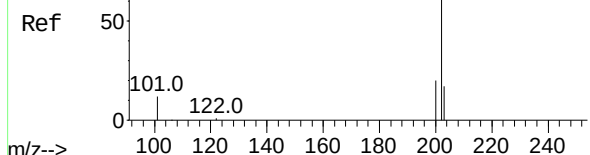


Tgt Ion:	202	Resp:	131569
Ion	Ratio	Lower	Upper
202	100		
200	20.7	16.5	24.7
203	17.5	13.9	20.9

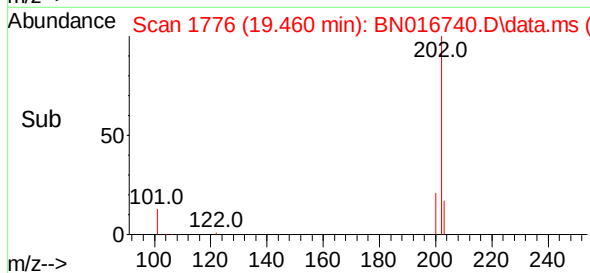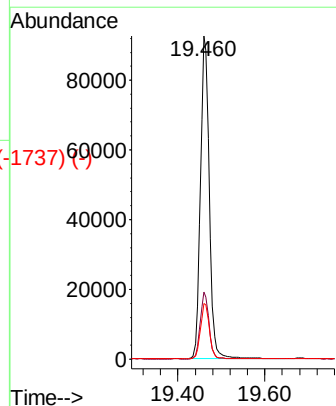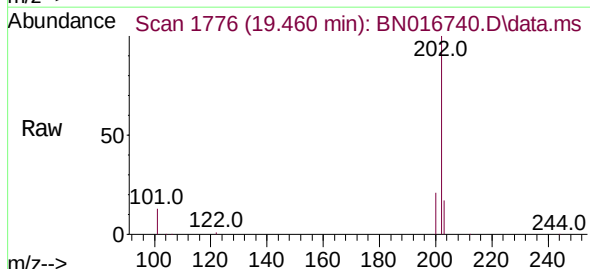




Abundance Scan 1821 (19.683 min): BN016710.D\data.ms (-181) (-)

Terphenyl-d14
Concen: 0.384 ng
RT: 19.678 min Scan# 1820
Delta R.T. -0.005 min
Lab File: BN016740.D
Acq: 05 Oct 2021 10:36

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

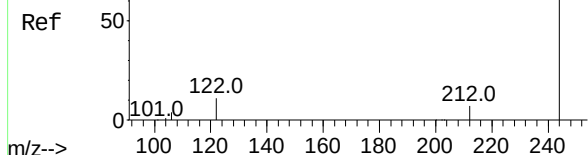


Tgt Ion	Ratio	Lower	Upper
244	100		
212	7.3	5.8	8.6
122	12.6	8.9	13.3



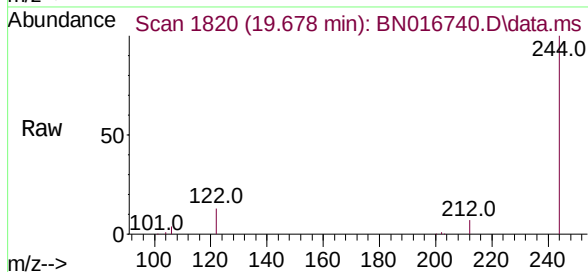


Abundance Scan 2000 (21.216 min): BN016710.D\data.ms (-1932) (-)


Benzo(a)anthracene
Concen: 0.398 ng
RT: 21.217 min Scan# 2000
Delta R.T. 0.000 min
Lab File: BN016740.D
Acq: 05 Oct 2021 10:36

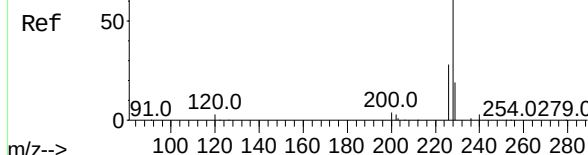

Tgt Ion	Ratio	Lower	Upper
228	100		
226	27.3	22.3	33.5
229	19.2	15.4	23.0

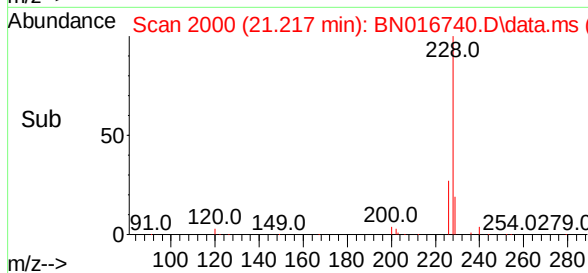




Abundance Scan 2005 (21.270 min): BN016710.D\data.ms (-2003) (-)

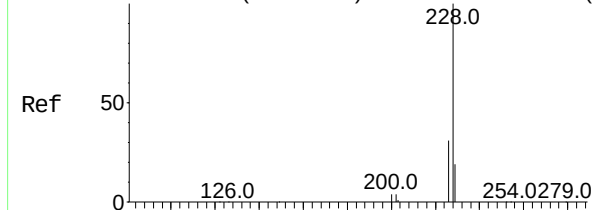


Chrysene
Concen: 0.411 ng
RT: 21.270 min Scan# 2005
Delta R.T. 0.000 min
Lab File: BN016740.D
Acq: 05 Oct 2021 10:36

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Tgt Ion:	228	Resp:	134591
Ion	Ratio	Lower	Upper
228	100		
226	29.9	24.2	36.4
229	19.3	15.4	23.0

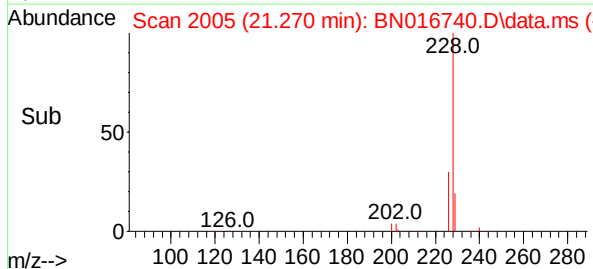

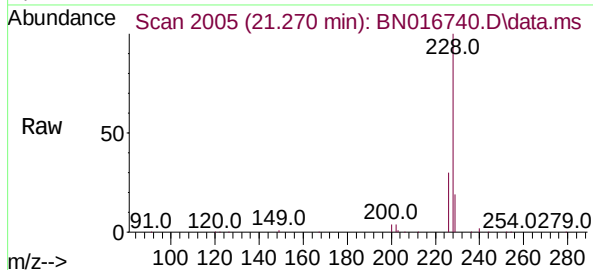


Abundance Scan 1996 (21.174 min): BN016710.D\data.ms (-1996) (-)

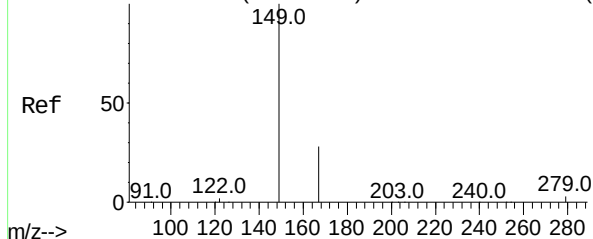

Bis(2-ethylhexyl)phthalate
Concen: 0.315 ng
RT: 21.174 min Scan# 1996
Delta R.T. 0.000 min
Lab File: BN016740.D
Acq: 05 Oct 2021 10:36




Tgt Ion:	149	Resp:	61550
Ion	Ratio	Lower	Upper
149	100		
167	27.9	22.2	33.4
279	4.2	3.4	5.2

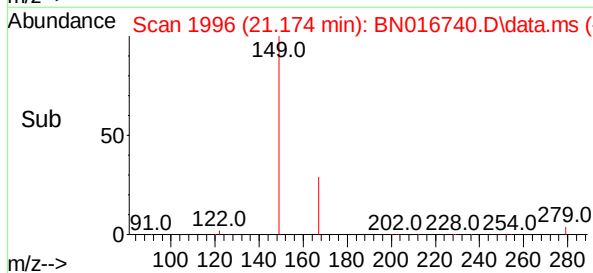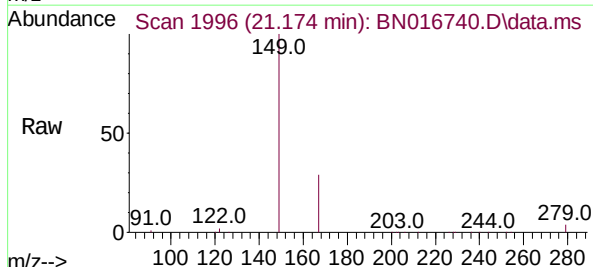


Abundance Scan 2430 (23.494 min): BN016710.D\data.ms (-2430) (-)

Perylene-d12
Concen: 0.400 ng
RT: 23.488 min Scan# 2428
Delta R.T. -0.007 min
Lab File: BN016740.D
Acq: 05 Oct 2021 10:36

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


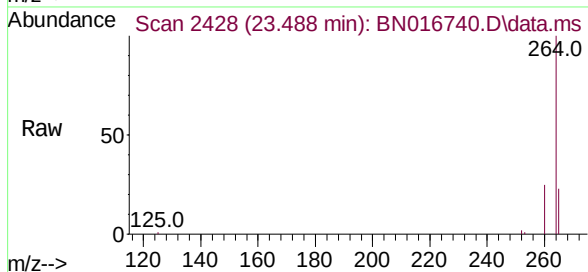
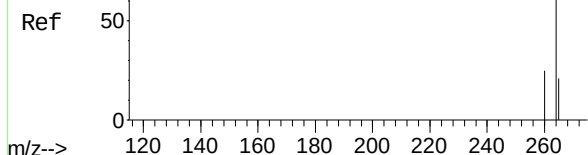


Tgt Ion	Ratio	Lower	Upper
264	100		
260	24.7	19.8	29.6
265	23.3	20.3	30.5

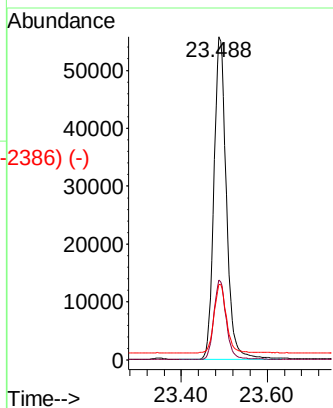


Abundance Scan 3098 (25.781 min): BN016710.D\data.ms (-3098) (-)


Indeno(1,2,3-cd)pyrene
Concen: 0.461 ng
RT: 25.771 min Scan# 3095
Delta R.T. -0.010 min
Lab File: BN016740.D
Acq: 05 Oct 2021 10:36

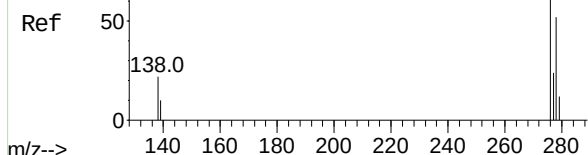

Tgt Ion	Ratio	Lower	Upper
276	100		
138	24.8	19.2	28.8
277	25.0	20.0	30.0





Abundance Scan 2231 (22.813 min): BN016710.D\data.ms (-2173) (-)




Benzo(b)fluoranthene
Concen: 0.388 ng
RT: 22.810 min Scan# 2230
Delta R.T. -0.003 min
Lab File: BN016740.D
Acq: 05 Oct 2021 10:36

Tgt Ion:	252	Resp:	141299
Ion Ratio	Lower	Upper	
252	100		
253	22.1	17.8	26.8
125	9.9	8.3	12.5


Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

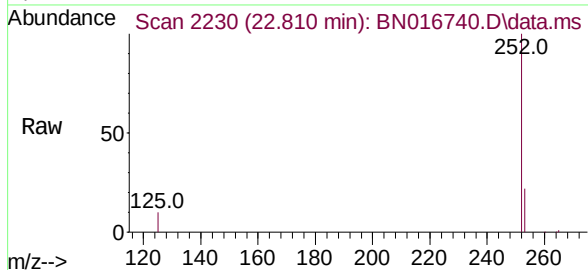

Abundance Scan 2230 (22.810 min): BN016740.D\data.ms (-2173) (-)





Abundance Scan 2245 (22.861 min): BN016710.D\data.ms (-2238) (-)




Benzo(k)fluoranthene
Concen: 0.405 ng
RT: 22.858 min Scan# 2244
Delta R.T. -0.003 min
Lab File: BN016740.D
Acq: 05 Oct 2021 10:36

Tgt Ion:	252	Resp:	141648
Ion Ratio	Lower	Upper	
252	100		
253	22.6	17.8	26.8
125	11.4	8.5	12.7




Abundance Scan 2244 (22.858 min): BN016740.D\data.ms (-2230) (-)

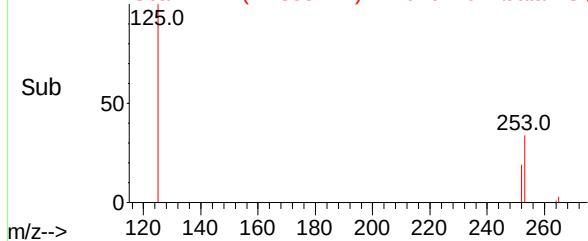




Abundance Scan 2400 (23.392 min): BN016710.D\data.ms (-2339) (-)

Benzo(a)pyrene
Concen: 0.399 ng
RT: 23.388 min Scan# 2399
Delta R.T. -0.003 min
Lab File: BN016740.D
Acq: 05 Oct 2021 10:36

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

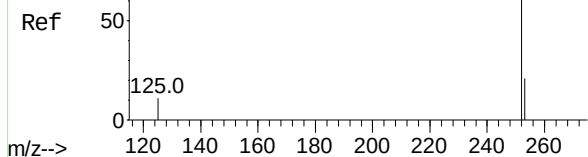





Tgt Ion	Ratio	Lower	Upper
252	100		
253	22.3	17.9	26.9
125	11.0	9.4	14.2

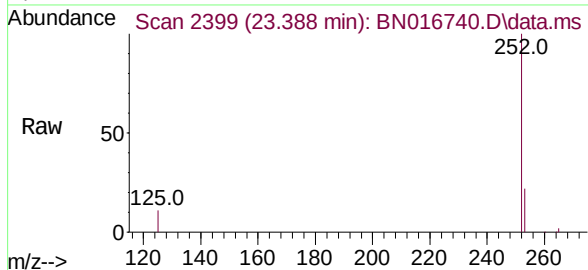


Abundance Scan 3103 (25.798 min): BN016710.D\data.ms (-3074) (-)

Dibenzo(a,h)anthracene
Concen: 0.467 ng
RT: 25.791 min Scan# 3101
Delta R.T. -0.007 min
Lab File: BN016740.D
Acq: 05 Oct 2021 10:36

Tgt Ion	Ratio	Lower	Upper
278	100		
139	17.2	13.1	19.7
279	24.0	19.3	28.9

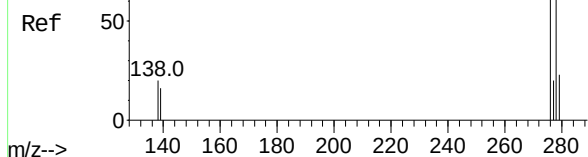


Abundance Scan 3301 (26.476 min): BN016710.D\data.ms (-32743) (-)



Benzo(g,h,i)perylene
Concen: 0.447 ng
RT: 26.469 min Scan# 3299
Delta R.T. -0.007 min
Lab File: BN016740.D
Acq: 05 Oct 2021 10:36

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Abundance Scan 3299 (26.469 min): BN016740.D\data.ms

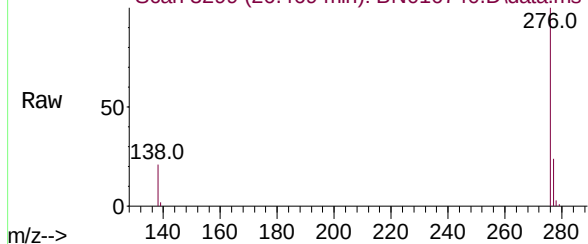

Tgt Ion:276 Resp: 141791
Ion Ratio Lower Upper
276 100
277 24.0 19.0 28.4
138 21.1 17.0 25.6

Abundance Scan 3299 (26.469 min): BN016740.D\data.ms (-3243) (-)

