

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100421\
 Data File : BN016764.D
 Acq On : 06 Oct 2021 05:05
 Operator : CG/JU
 Sample : M3915-16
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 RE109D2-20210922

Quant Time: Oct 06 06:57:49 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN100421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 04 17:52:33 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.642	152	26506	0.400	ng	0.00
7) Naphthalene-d8	10.407	136	121345	0.400	ng	# 0.00
13) Acenaphthene-d10	14.269	164	64549	0.400	ng	0.00
19) Phenanthrene-d10	17.017	188	123291	0.400	ng	#-0.01
29) Chrysene-d12	21.227	240	122525	0.400	ng	#-0.01
35) Perylene-d12	23.481	264	122898	0.400	ng	-0.01
System Monitoring Compounds						
4) 2-Fluorophenol	5.273	112	7726	0.114	ng	0.02
5) Phenol-d6	6.831	99	4786	0.064	ng	0.00
8) Nitrobenzene-d5	8.784	82	18740	0.220	ng	0.00
11) 2-Methylnaphthalene-d10	12.003	152	52061	0.288	ng	0.00
14) 2,4,6-Tribromophenol	15.766	330	6114	0.281	ng	-0.01
15) 2-Fluorobiphenyl	12.886	172	66138	0.256	ng	-0.01
27) Fluoranthene-d10	19.068	212	127966	0.379	ng	0.00
31) Terphenyl-d14	19.678	244	101652	0.371	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.253	88	36825	2.977	ng	# 69
3) n-Nitrosodimethylamine	3.502	42	1288	0.065	ng	# 1
20) 4,6-Dinitro-2-methylph...	15.398	198	2	0.266	ng	# 1
24) Pentachlorophenol	16.689	266	40	0.339	ng	# 86
34) Bis(2-ethylhexyl)phtha...	21.164	149	17746	0.077	ng	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100421\
Data File : BN016764.D
Acq On : 06 Oct 2021 05:05
Operator : CG/JU
Sample : M3915-16
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
RE109D2-20210922

Quant Time: Oct 06 06:57:49 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN100421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 04 17:52:33 2021
Response via : Initial Calibration



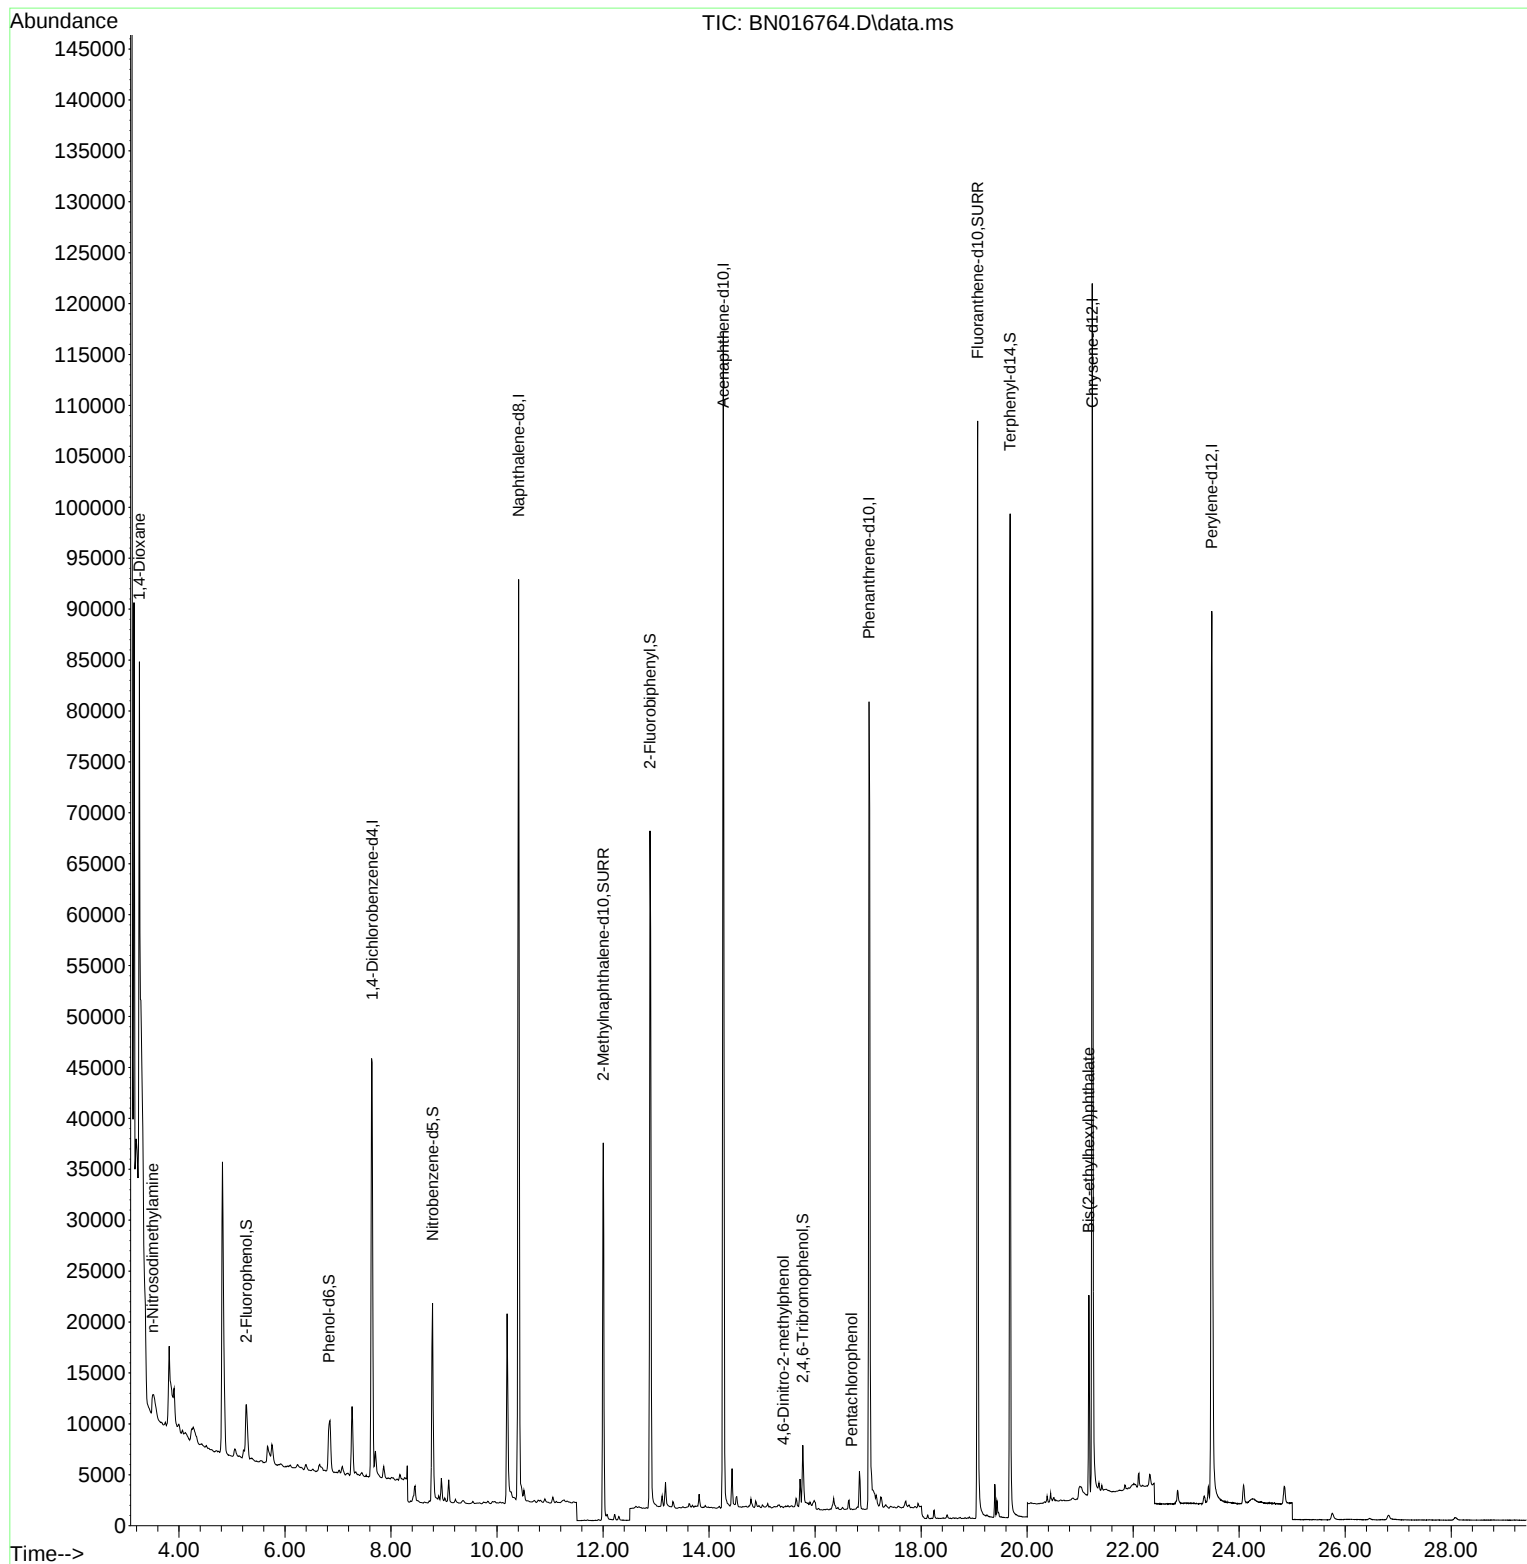




#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.642 min Scan# 495
 Delta R.T. 0.000 min
 Lab File: BN016764.D
 Acq: 06 Oct 2021 05:05




Instrument :
 BNA_N
 ClientSampleId :
 RE109D2-20210922


Tgt Ion:152 Resp: 26506
 Ion Ratio Lower Upper
 152 100
 150 153.1 123.3 184.9
 115 56.6 47.0 70.6

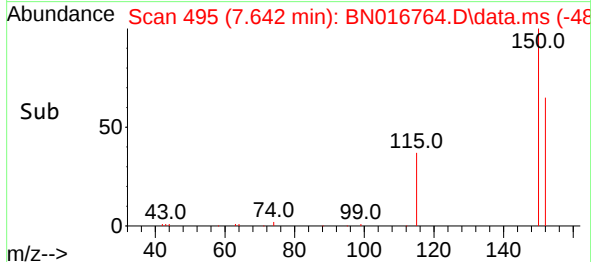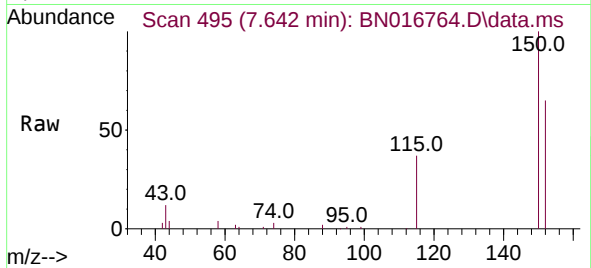

#2
 1,4-Dioxane
 Concen: 2.977 ng
 RT: 3.253 min Scan# 19
 Delta R.T. 0.000 min
 Lab File: BN016764.D
 Acq: 06 Oct 2021 05:05

Tgt Ion: 88 Resp: 36825
 Ion Ratio Lower Upper
 88 100
 43 26.4 61.7 92.5#
 58 74.3 62.2 93.2


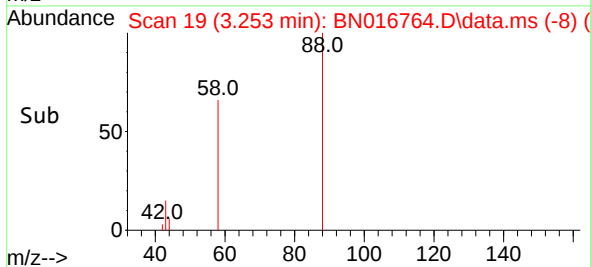

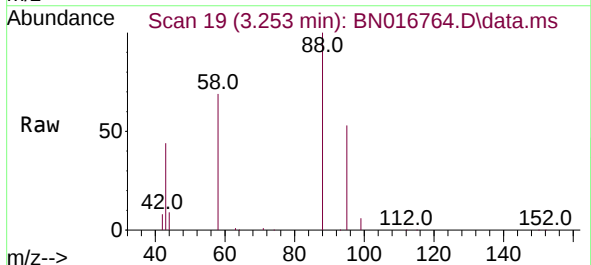


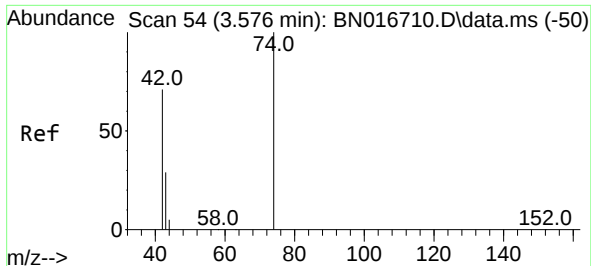

#3
n-Nitrosodimethylamine
Concen: 0.065 ng
RT: 3.502 min Scan# 46
Delta R.T. -0.073 min
Lab File: BN016764.D
Acq: 06 Oct 2021 05:05




Instrument :
BNA_N
ClientSampleId :
RE109D2-20210922


Tgt Ion: 42 Resp: 1288
Ion Ratio Lower Upper
42 100
74 0.0 124.0 186.0#
44 123.5 5.6 8.4#

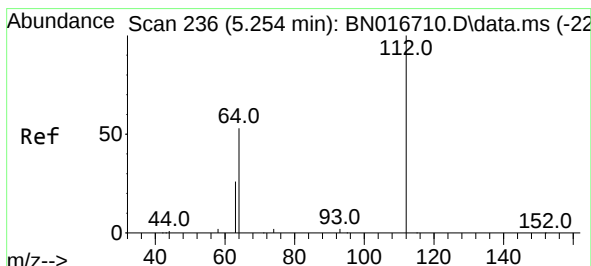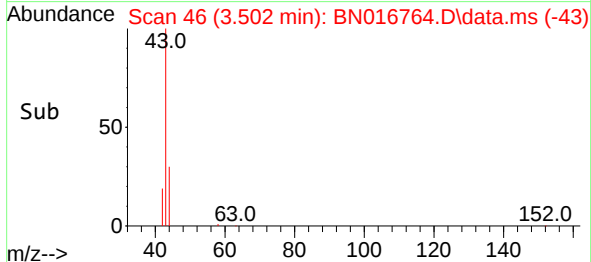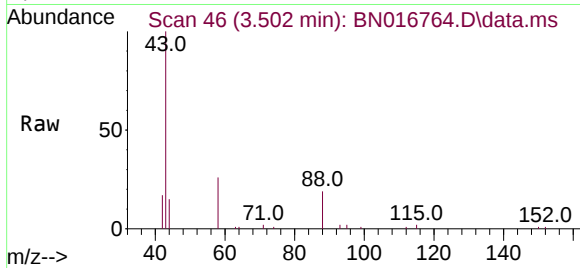

#4
2-Fluorophenol
Concen: 0.114 ng
RT: 5.273 min Scan# 238
Delta R.T. 0.019 min
Lab File: BN016764.D
Acq: 06 Oct 2021 05:05

Tgt Ion: 112 Resp: 7726
Ion Ratio Lower Upper
112 100
64 54.2 42.9 64.3
63 27.5 21.5 32.3


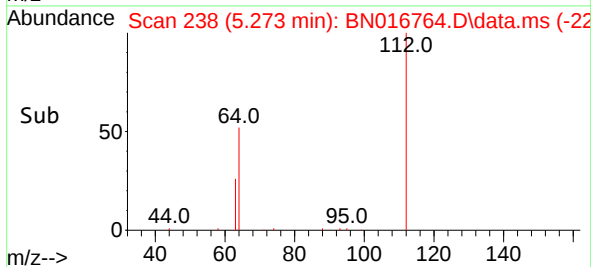

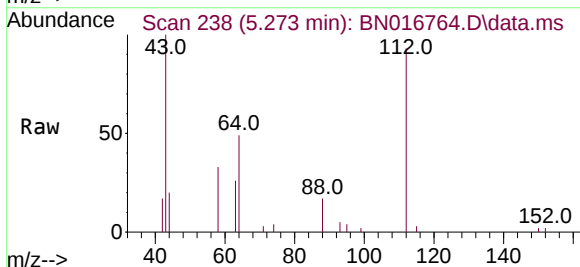


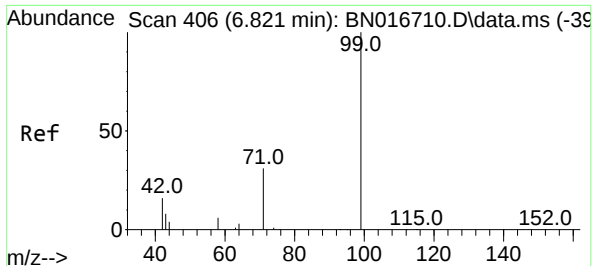

#5
Phenol-d6
Concen: 0.064 ng
RT: 6.831 min Scan# 407
Delta R.T. 0.010 min
Lab File: BN016764.D
Acq: 06 Oct 2021 05:05




Instrument :
BNA_N
ClientSampleId :
RE109D2-20210922


Tgt Ion: 99 Resp: 4786
Ion Ratio Lower Upper
99 100
42 21.7 13.4 20.2#
71 34.3 24.0 36.0

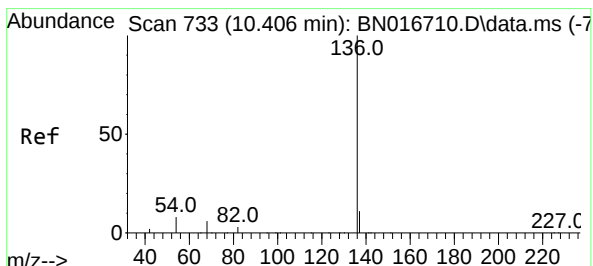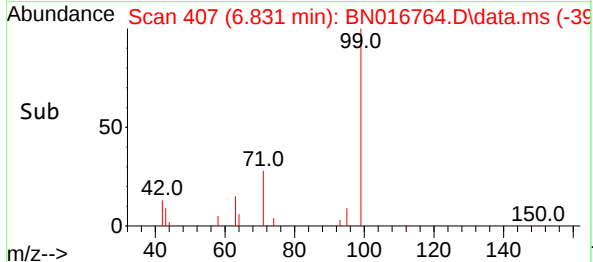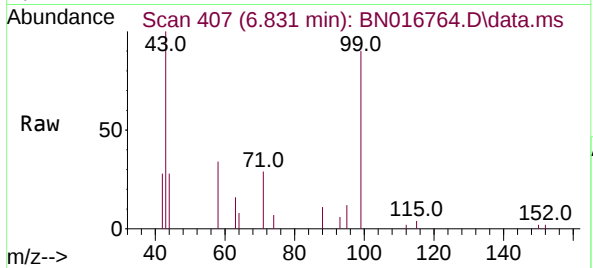

#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.407 min Scan# 733
Delta R.T. 0.000 min
Lab File: BN016764.D
Acq: 06 Oct 2021 05:05

Tgt Ion: 136 Resp: 121345
Ion Ratio Lower Upper
136 100
137 11.0 8.9 13.3
54 6.2 6.5 9.7#
68 5.2 5.3 7.9#


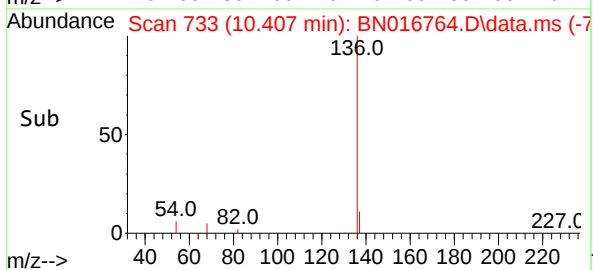

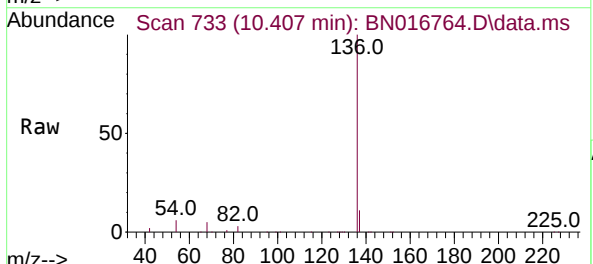


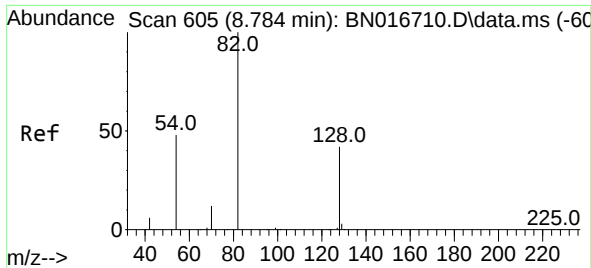

#8
Nitrobenzene-d5
Concen: 0.220 ng
RT: 8.784 min Scan# 605
Delta R.T. 0.000 min
Lab File: BN016764.D
Acq: 06 Oct 2021 05:05




Instrument :
BNA_N
ClientSampleId :
RE109D2-20210922


Tgt Ion: 82 Resp: 18740
Ion Ratio Lower Upper
82 100
128 44.5 33.8 50.6
54 46.5 38.5 57.7

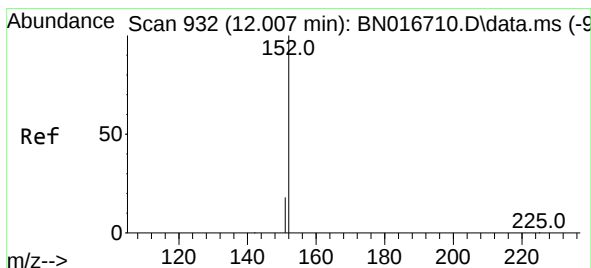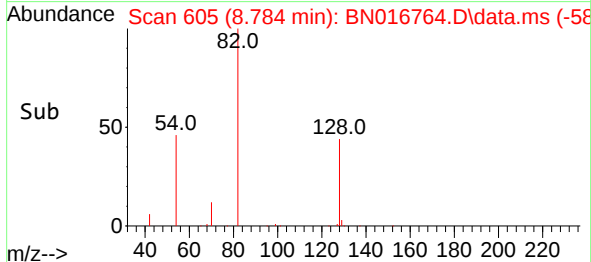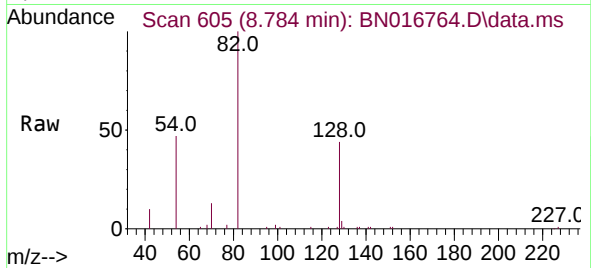

#11
2-Methylnaphthalene-d10
Concen: 0.288 ng
RT: 12.003 min Scan# 931
Delta R.T. -0.004 min
Lab File: BN016764.D
Acq: 06 Oct 2021 05:05

Tgt Ion: 152 Resp: 52061
Ion Ratio Lower Upper
152 100
151 20.4 16.2 24.4


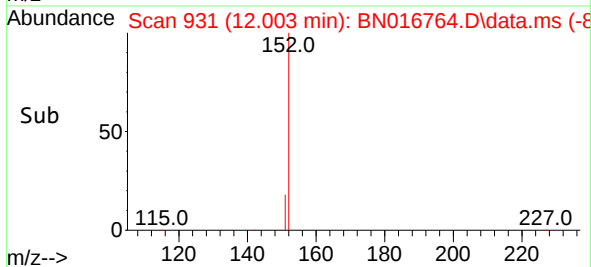

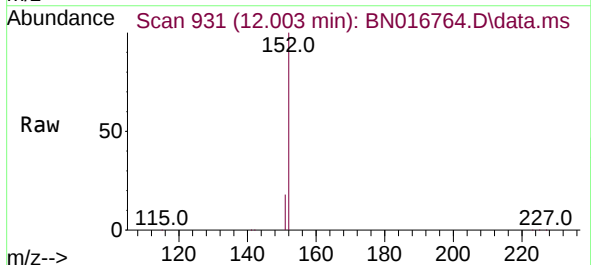


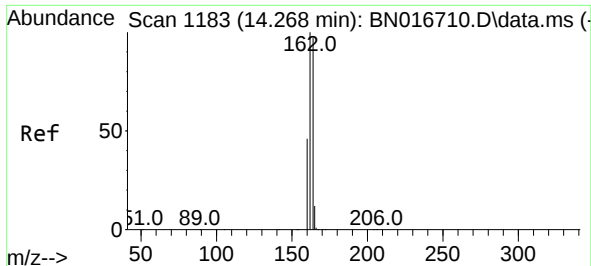

#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.269 min Scan# 1183
Delta R.T. 0.000 min
Lab File: BN016764.D
Acq: 06 Oct 2021 05:05




Instrument :
BNA_N
ClientSampleId :
RE109D2-20210922


Tgt Ion:164 Resp: 64549
Ion Ratio Lower Upper
164 100
162 101.0 82.6 124.0
160 45.4 38.2 57.2

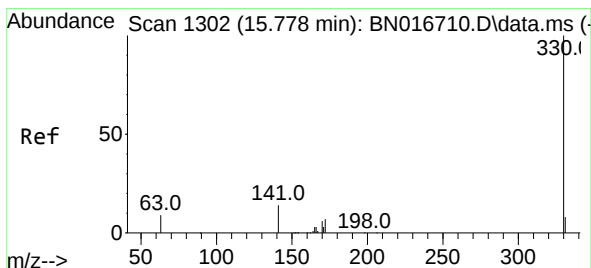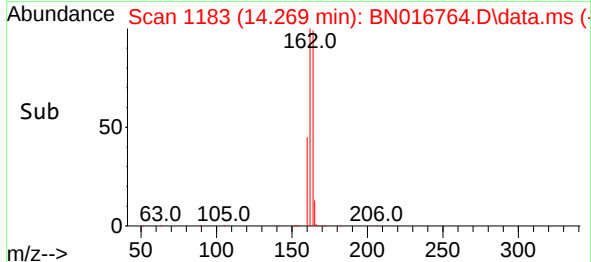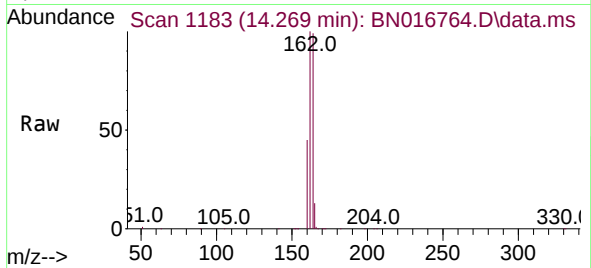

#14
2,4,6-Tribromophenol
Concen: 0.281 ng
RT: 15.766 min Scan# 1301
Delta R.T. -0.012 min
Lab File: BN016764.D
Acq: 06 Oct 2021 05:05

Tgt Ion:330 Resp: 6114
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 29.2 24.2 36.2


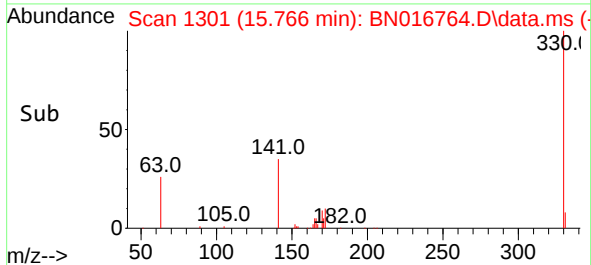

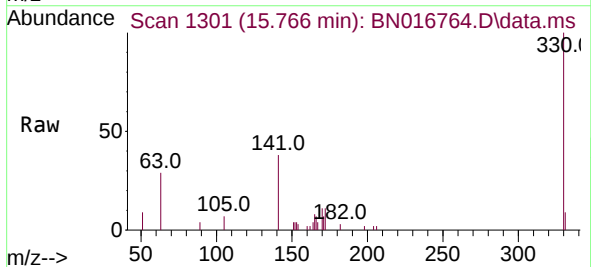


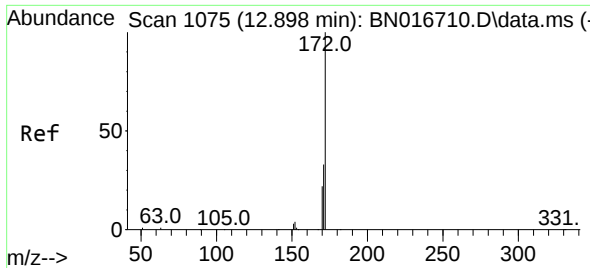

#15
2-Fluorobiphenyl
Concen: 0.256 ng
RT: 12.886 min Scan# 1074
Delta R.T. -0.012 min
Lab File: BN016764.D
Acq: 06 Oct 2021 05:05




Instrument :
BNA_N
ClientSampleId :
RE109D2-20210922


Tgt Ion:	172	Resp:	66138
Ion Ratio	Lower	Upper	
172	100		
171	35.5	26.9	40.3
170	24.5	17.4	26.0

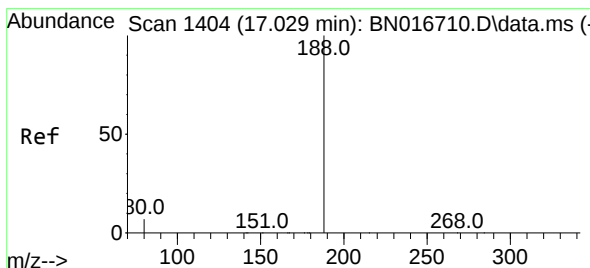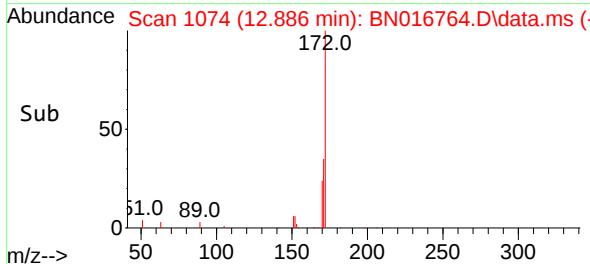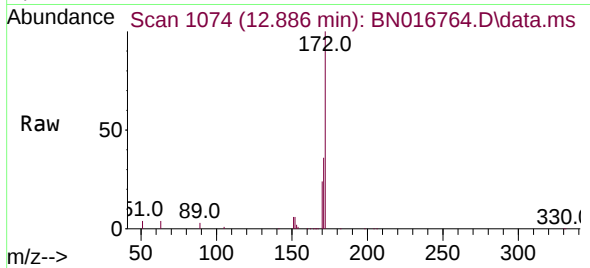

#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.017 min Scan# 1403
Delta R.T. -0.012 min
Lab File: BN016764.D
Acq: 06 Oct 2021 05:05

Tgt Ion:	188	Resp:	123291
Ion Ratio	Lower	Upper	
188	100		
94	0.0	0.0	0.0
80	12.4	5.8	8.8#


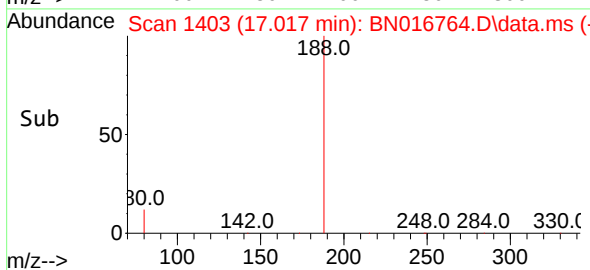

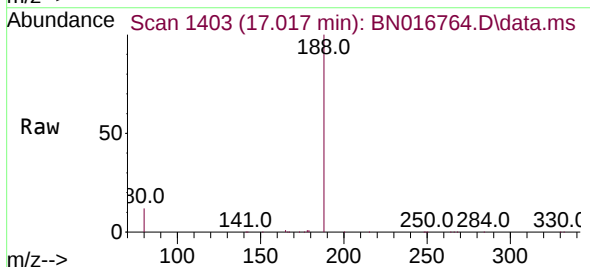


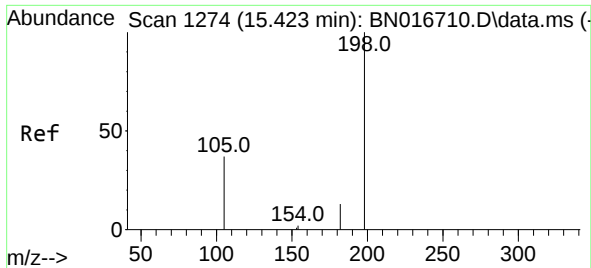

#20
4,6-Dinitro-2-methylphenol
Concen: 0.266 ng
RT: 15.398 min Scan# 1272
Delta R.T. -0.025 min
Lab File: BN016764.D
Acq: 06 Oct 2021 05:05




Instrument :
BNA_N
ClientSampleId :
RE109D2-20210922


Tgt Ion:198 Resp: 2
Ion Ratio Lower Upper
198 100
182 116.3 26.2 39.2#
77 0.0 0.0 0.0

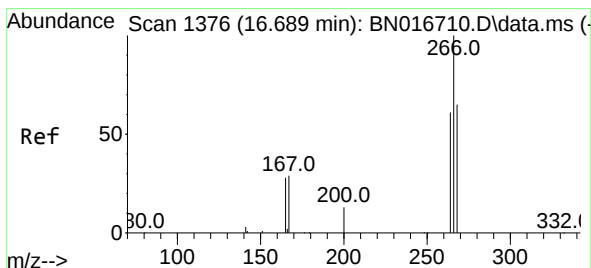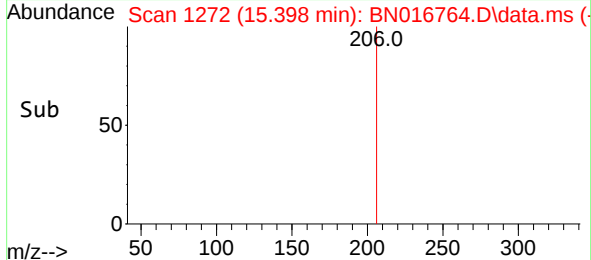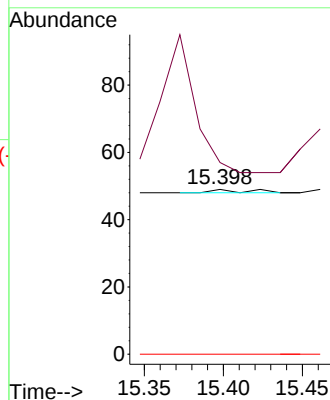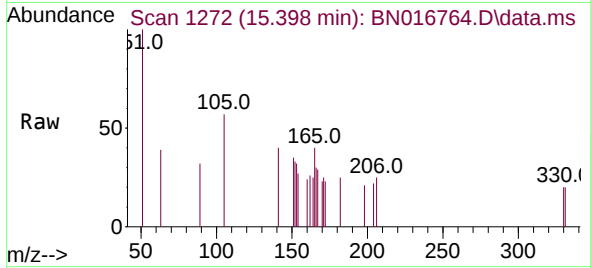

#24
Pentachlorophenol
Concen: 0.339 ng
RT: 16.689 min Scan# 1376
Delta R.T. -0.000 min
Lab File: BN016764.D
Acq: 06 Oct 2021 05:05

Tgt Ion:266 Resp: 40
Ion Ratio Lower Upper
266 100
264 65.0 49.3 73.9
268 82.5 51.8 77.8#


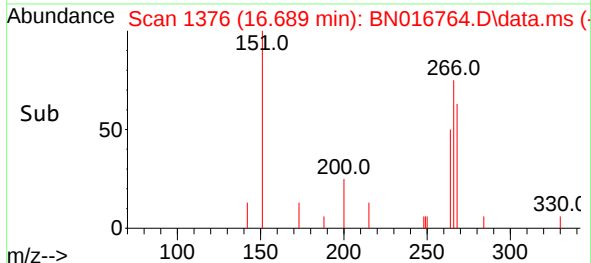
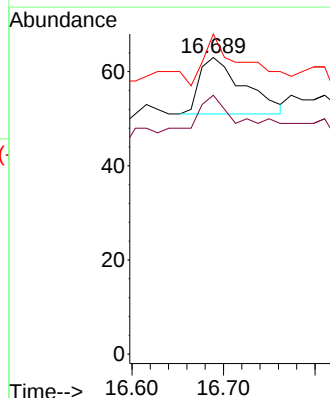
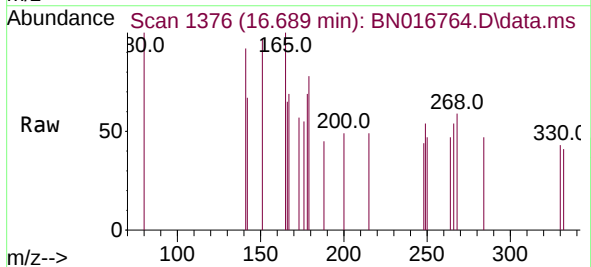


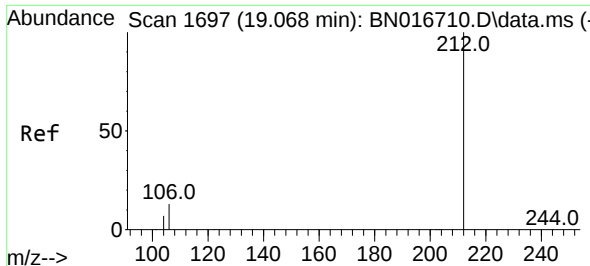

#27
Fluoranthene-d10
Concen: 0.379 ng
RT: 19.068 min Scan# 1697
Delta R.T. 0.000 min
Lab File: BN016764.D
Acq: 06 Oct 2021 05:05




Instrument :
BNA_N
ClientSampleId :
RE109D2-20210922


Tgt Ion:212 Resp: 127966
Ion Ratio Lower Upper
212 100
106 13.2 10.6 16.0
104 7.3 5.8 8.8

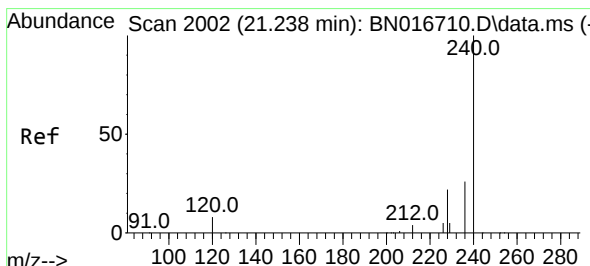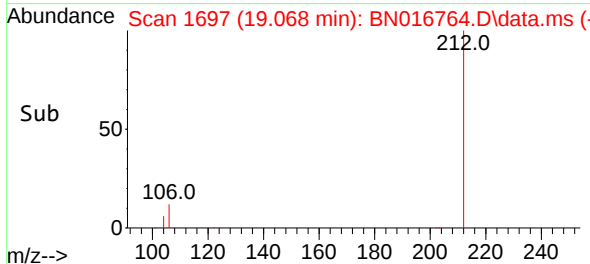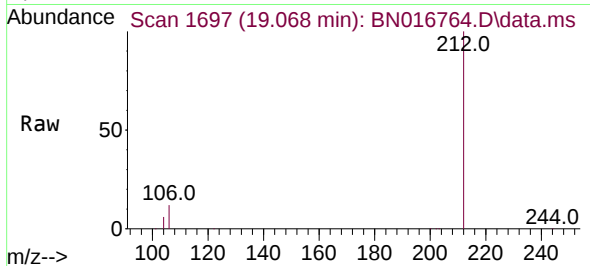

#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.227 min Scan# 2001
Delta R.T. -0.010 min
Lab File: BN016764.D
Acq: 06 Oct 2021 05:05

Tgt Ion:240 Resp: 122525
Ion Ratio Lower Upper
240 100
120 12.4 6.6 10.0#
236 26.5 20.7 31.1


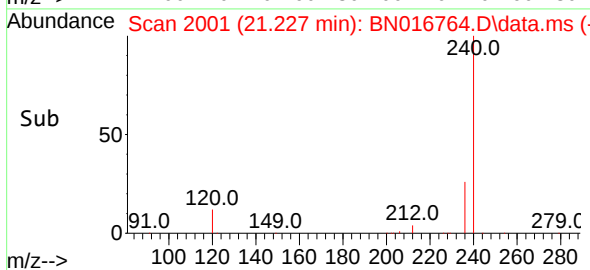

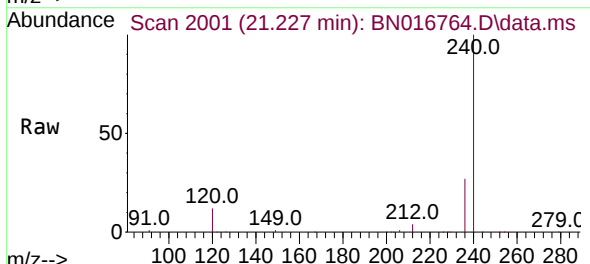


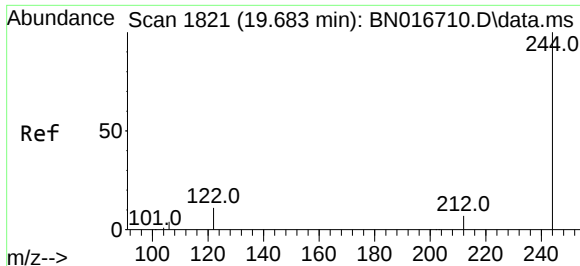

#31
Terphenyl-d14
Concen: 0.371 ng
RT: 19.678 min Scan# 1820
Delta R.T. -0.005 min
Lab File: BN016764.D
Acq: 06 Oct 2021 05:05




Instrument :
BNA_N
ClientSampleId :
RE109D2-20210922


Tgt Ion:244 Resp: 101652
Ion Ratio Lower Upper
244 100
212 7.1 5.8 8.6
122 11.5 8.9 13.3

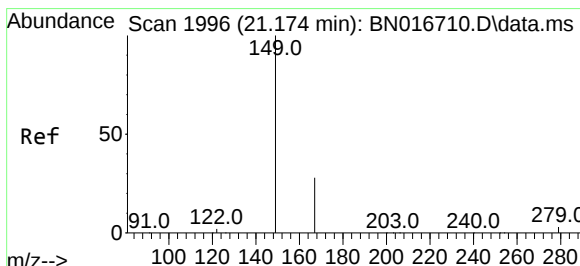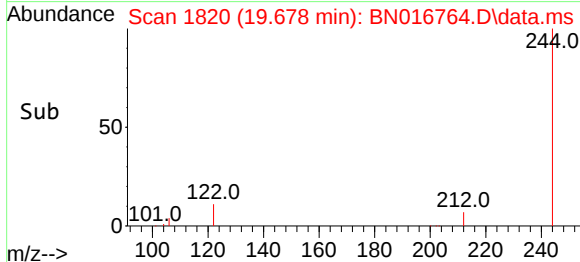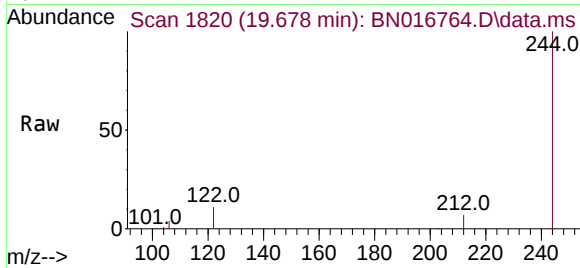

#34
Bis(2-ethylhexyl)phthalate
Concen: 0.077 ng
RT: 21.164 min Scan# 1995
Delta R.T. -0.010 min
Lab File: BN016764.D
Acq: 06 Oct 2021 05:05


Tgt Ion:149 Resp: 17746
Ion Ratio Lower Upper
149 100
167 27.3 22.2 33.4
279 4.2 3.4 5.2

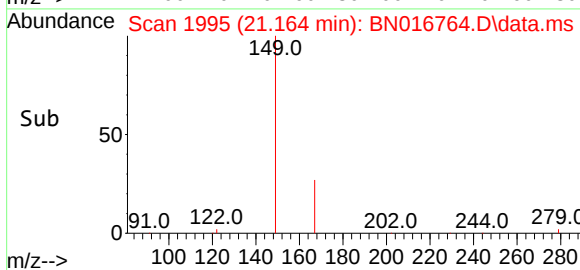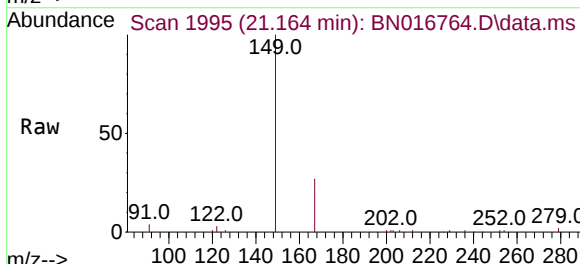

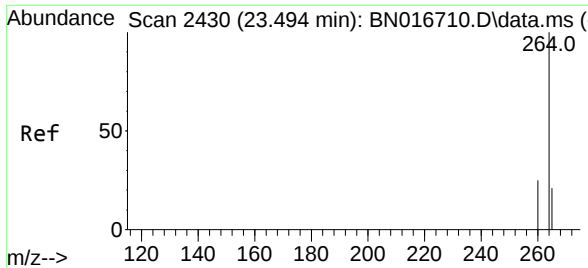

#35
Perylene-d12
Concen: 0.400 ng
RT: 23.481 min Scan# 2426
Delta R.T. -0.013 min
Lab File: BN016764.D
Acq: 06 Oct 2021 05:05

Instrument :
BNA_N
ClientSampleId :
RE109D2-20210922

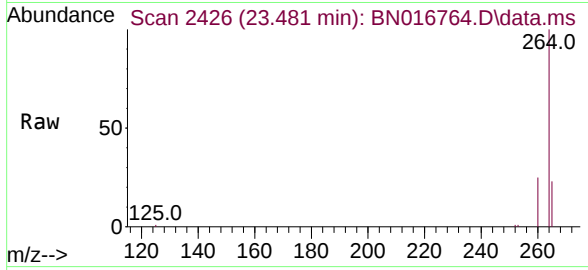

Tgt Ion:264 Resp: 122898

Ion	Ratio	Lower	Upper
264	100		
260	24.9	19.8	29.6
265	23.0	20.3	30.5

