
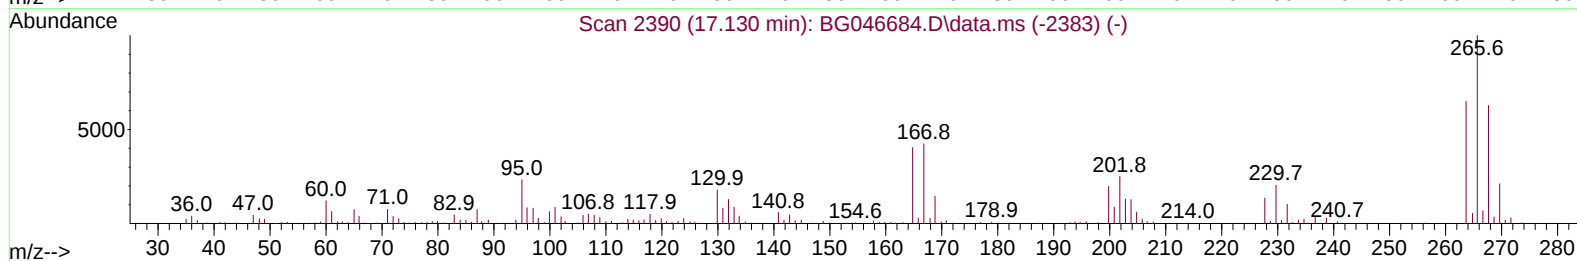
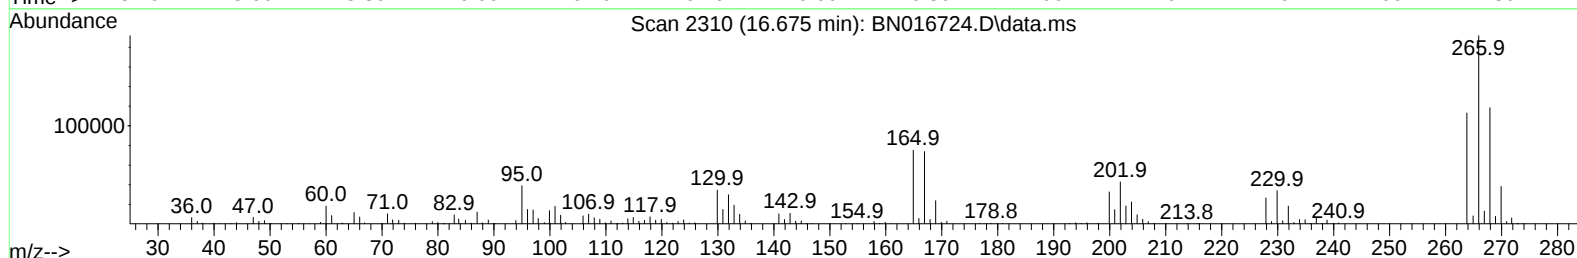


Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN100421\  
Data File : BN016724.D  
Acq On : 05 Oct 2021 01:01  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 05 04:48:14 2021  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Sep 30 18:14:09 2021  
Response via : Initial Calibration

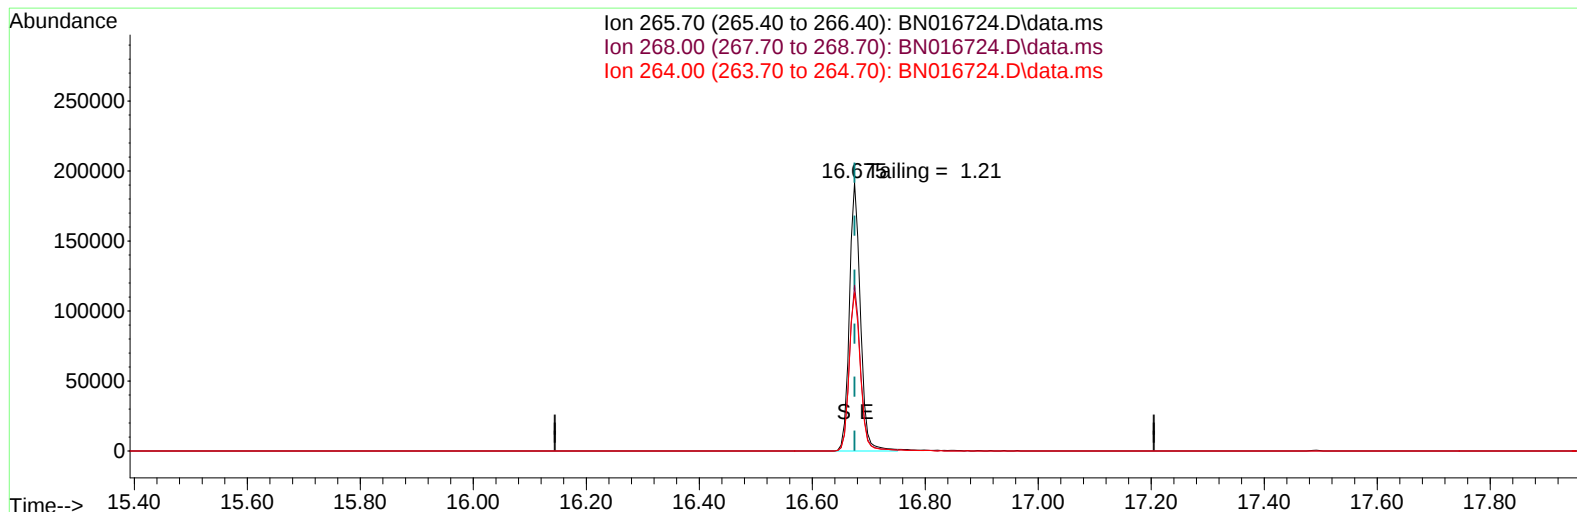

TIC: BN016724.D\data.ms

**(70) Pentachlorophenol (C)**




16.675min (-0.000) 27652.09 ng

response 262795

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 62.20  | 61.76  |
| 264.00 | 61.60  | 58.98  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN100421\  
Data File : BN016724.D  
Acq On : 05 Oct 2021 01:01  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 05 04:48:14 2021  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Sep 30 18:14:09 2021  
Response via : Initial Calibration

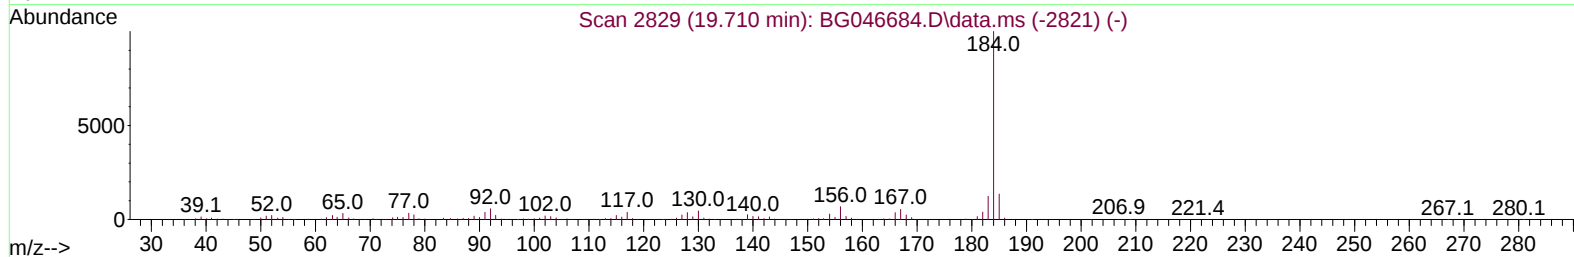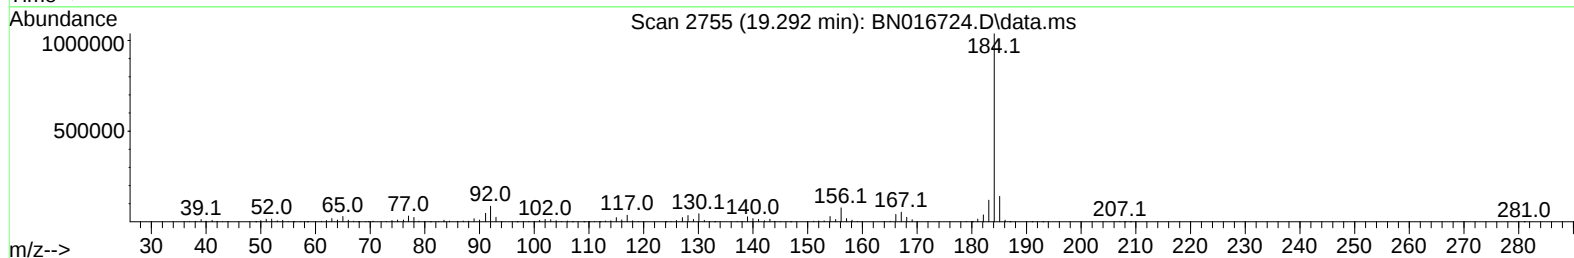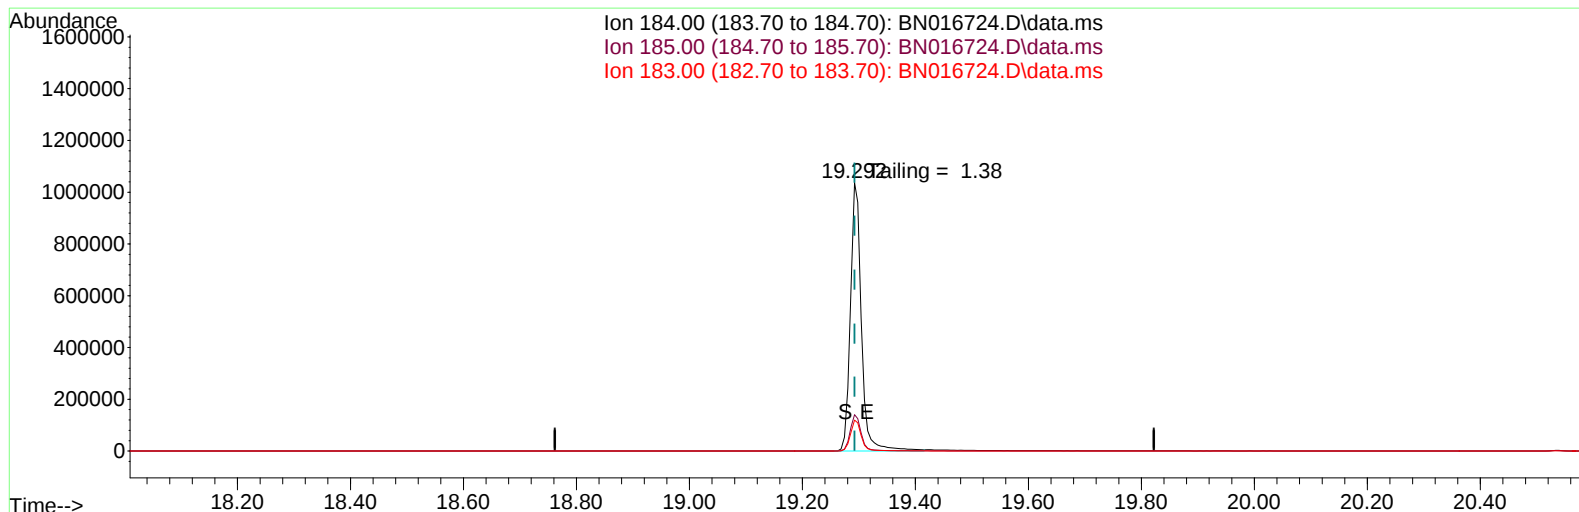

TIC: BN016724.D\data.ms

**(77) Benzidine**

19.292min (-0.000) 0.00 ng m

response 1403909

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.50  | 13.53  |
| 183.00 | 13.20  | 11.54  |
| 0.00   | 0.00   | 0.00   |