
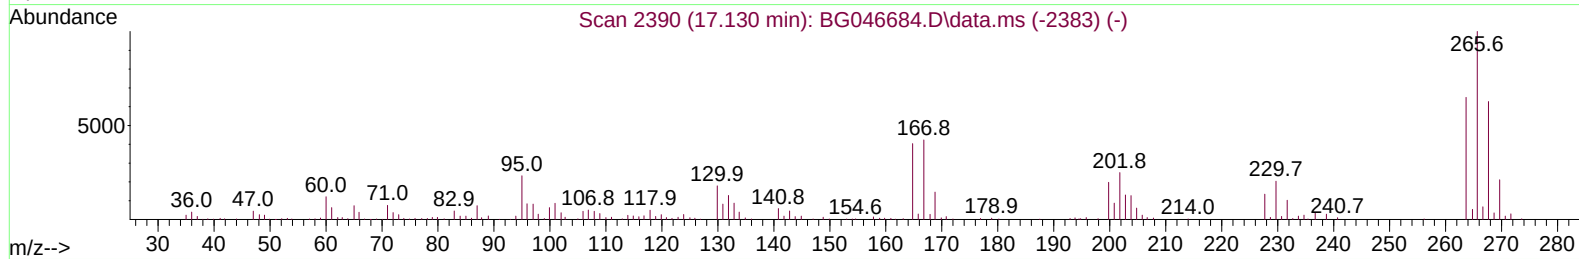
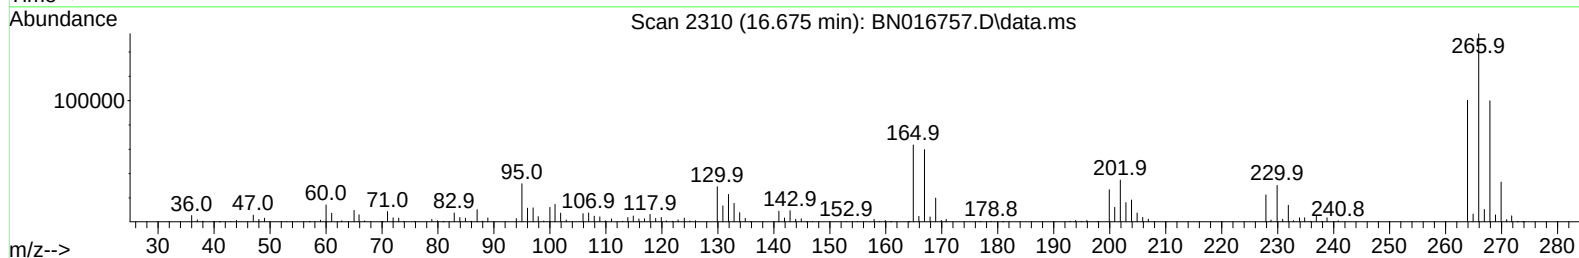


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100421\
Data File : BN016757.D
Acq On : 06 Oct 2021 00:51
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 06 04:41:44 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 30 18:14:09 2021
Response via : Initial Calibration

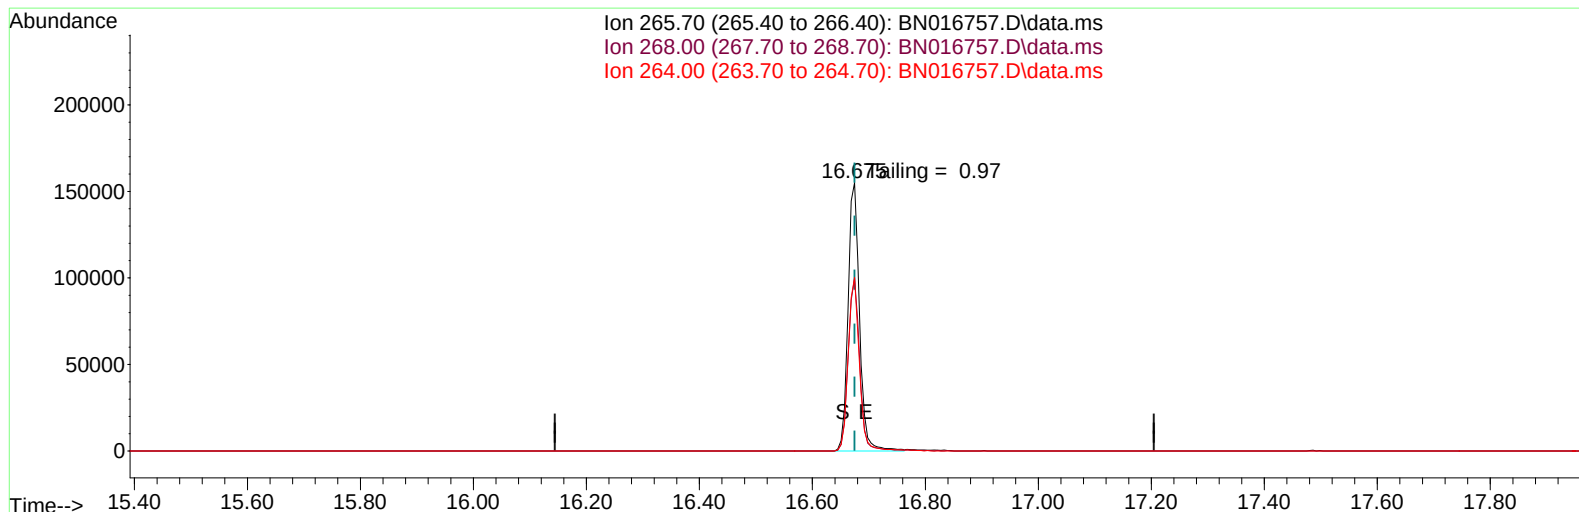

TIC: BN016757.D\data.ms

(70) Pentachlorophenol (C)




16.675min (-0.000) 22795.26 ng

response 220931

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.40
264.00	61.60	64.66
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN100421\
Data File : BN016757.D
Acq On : 06 Oct 2021 00:51
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 06 04:41:44 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 30 18:14:09 2021
Response via : Initial Calibration

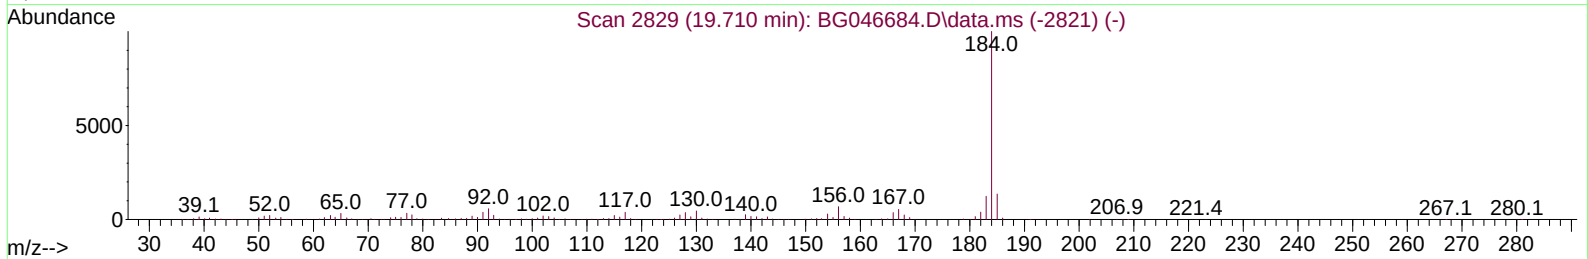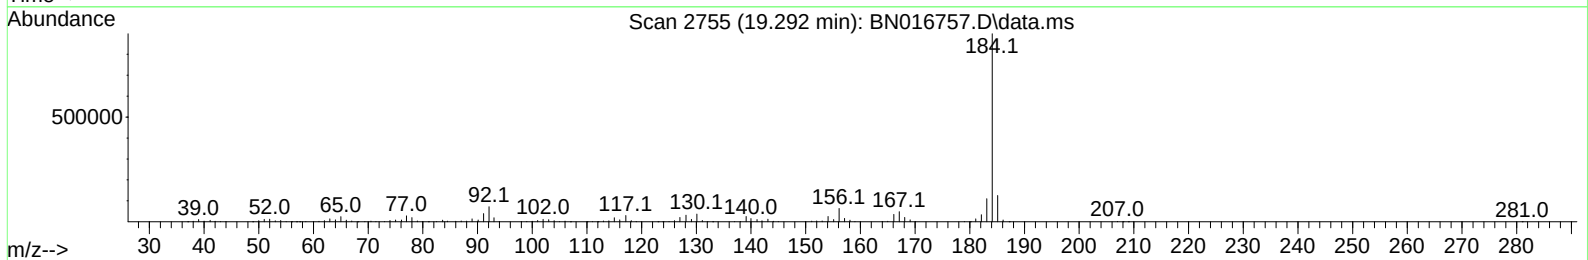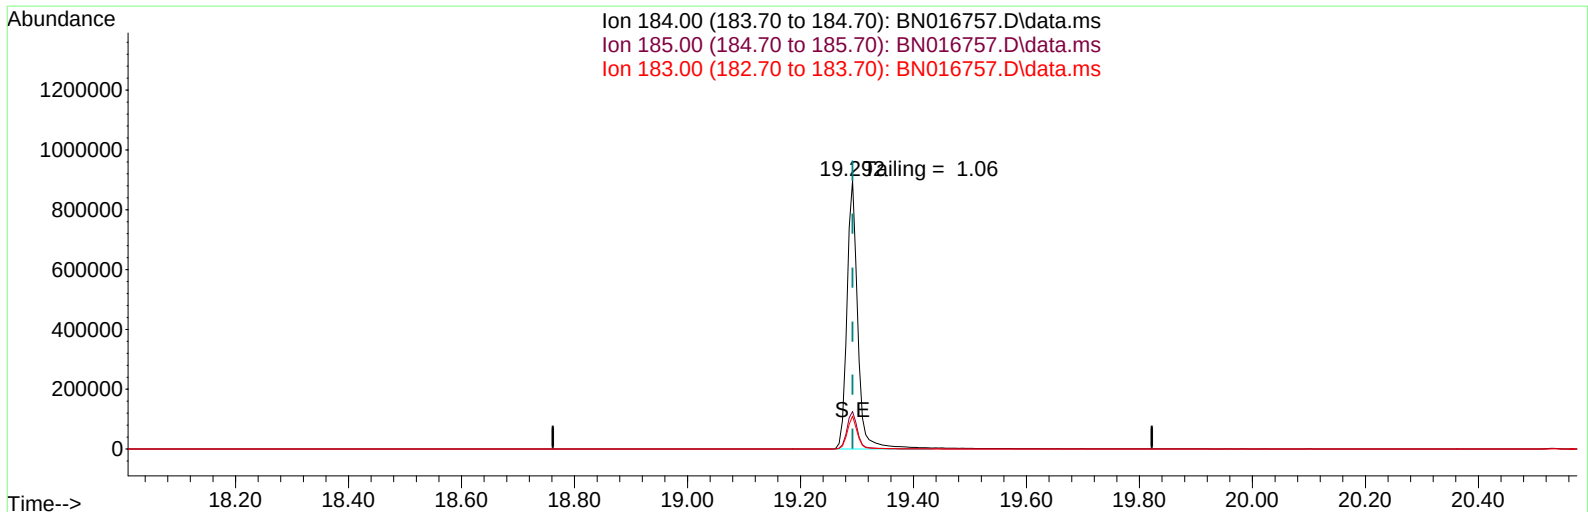

TIC: BN016757.D\data.ms

(77) Benzidine

19.292min (-0.000) 0.00 ng

response 1203109

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.99
183.00	13.20	12.28
0.00	0.00	0.00